

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031323\
 Data File : BN024272.D
 Acq On : 14 Mar 2023 09:26
 Operator : CG/JU
 Sample : 01843-04
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 RE132D4-20230306

Quant Time: Mar 15 01:42:53 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN031323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 14 03:11:52 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.047	152	8651	0.400	ng	0.00
7) Naphthalene-d8	10.866	136	25028	0.400	ng	0.00
13) Acenaphthene-d10	14.675	164	12607	0.400	ng	0.00
19) Phenanthrene-d10	17.425	188	27285	0.400	ng	0.00
29) Chrysene-d12	21.619	240	20924	0.400	ng	0.00
35) Perylene-d12	24.123	264	17507	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.584	112	2986	0.156	ng	0.00
5) Phenol-d6	7.195	99	2263	0.092	ng	0.00
8) Nitrobenzene-d5	9.211	82	6323	0.378	ng	0.00
11) 2-Methylnaphthalene-d10	12.441	152	10744	0.349	ng	0.00
14) 2,4,6-Tribromophenol	16.159	330	1788	0.277	ng	0.00
15) 2-Fluorobiphenyl	13.307	172	17059	0.358	ng	0.00
27) Fluoranthene-d10	19.450	212	28343	0.490	ng	0.00
31) Terphenyl-d14	20.043	244	16928	0.480	ng	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.432	88	58068	6.169	ng	99
3) n-Nitrosodimethylamine	3.685	42	733	0.053	ng	# 1
20) 4,6-Dinitro-2-methylph...	15.774	198	11	0.180	ng	# 1
24) Pentachlorophenol	17.065	266	16	0.130	ng	# 61
34) Bis(2-ethylhexyl)phtha...	21.511	149	2562	0.078	ng	# 95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031323\
Data File : BN024272.D
Acq On : 14 Mar 2023 09:26
Operator : CG/JU
Sample : 01843-04
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
RE132D4-20230306


Quant Time: Mar 15 01:42:53 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN031323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 14 03:11:52 2023
Response via : Initial Calibration

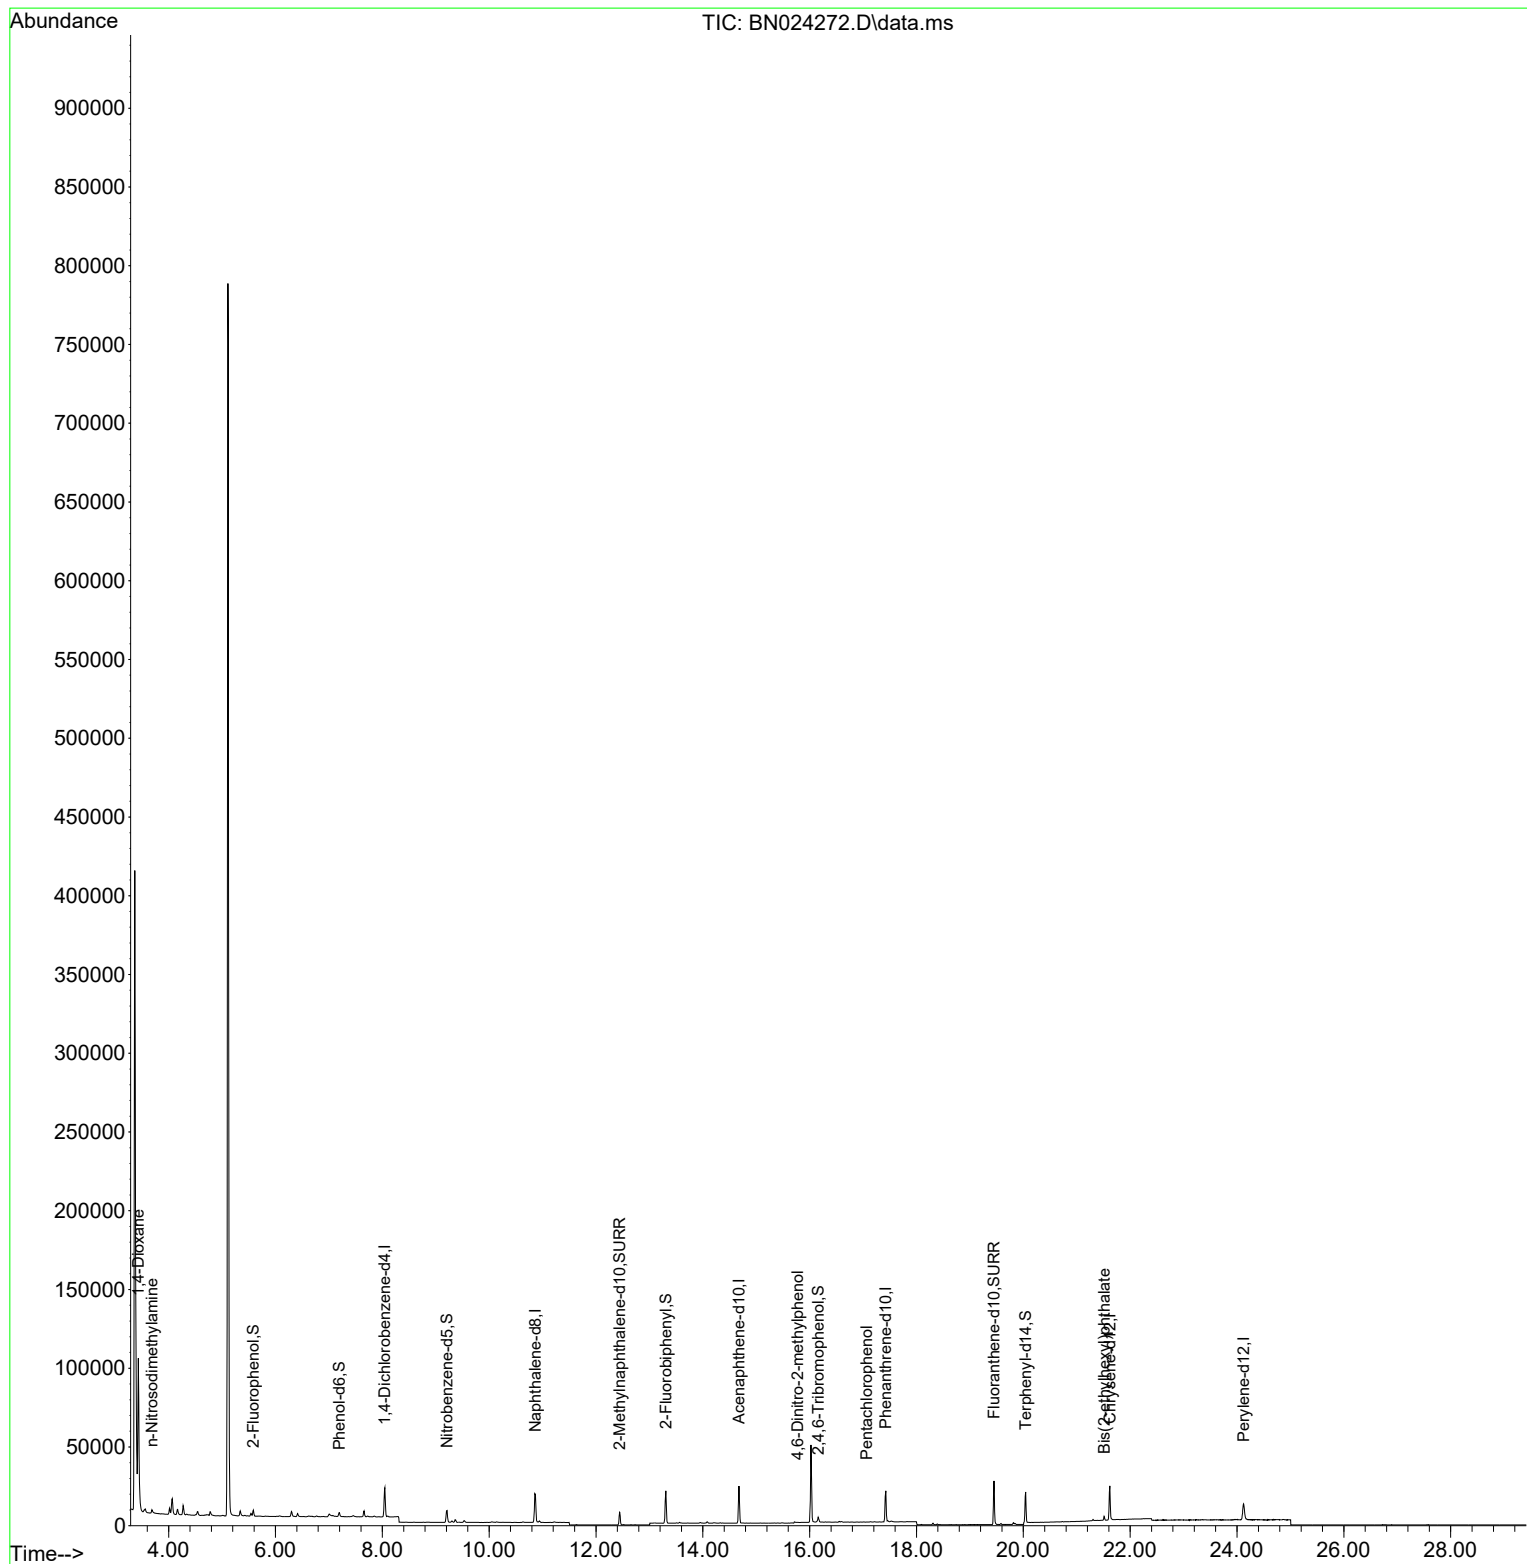



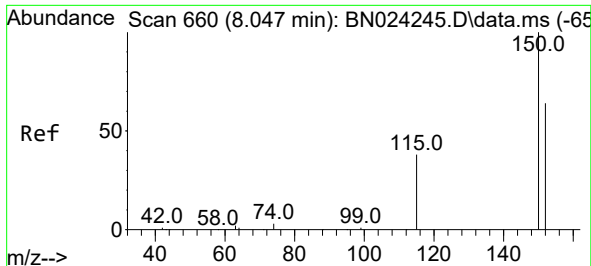


#1
1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 8.047 min Scan# 60
Delta R.T. 0.000 min
Lab File: BN024272.D
Acq: 14 Mar 2023 09:26


Instrument :
BNA_N
ClientSampleId :
RE132D4-20230306

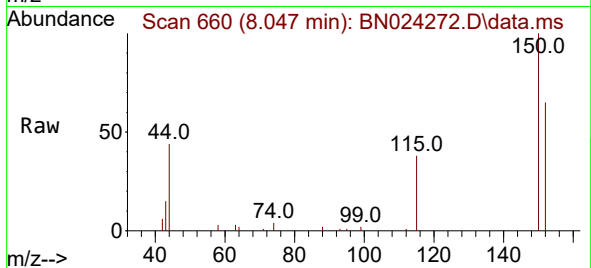



Tgt Ion:152 Resp: 8651
Ion Ratio Lower Upper
152 100
150 152.9 124.7 187.1
115 58.8 49.1 73.7

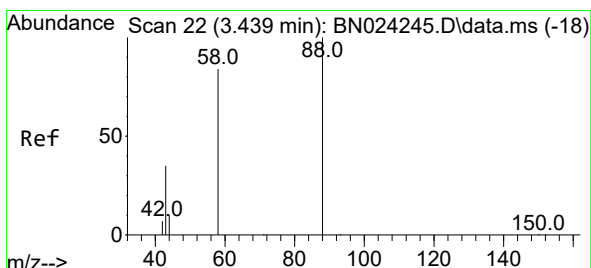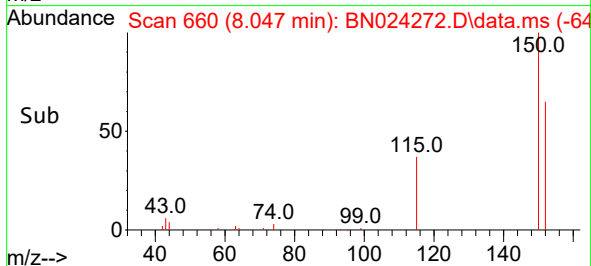


#2
1,4-Dioxane
Concen: 6.169 ng
RT: 3.432 min Scan# 21
Delta R.T. -0.007 min
Lab File: BN024272.D
Acq: 14 Mar 2023 09:26

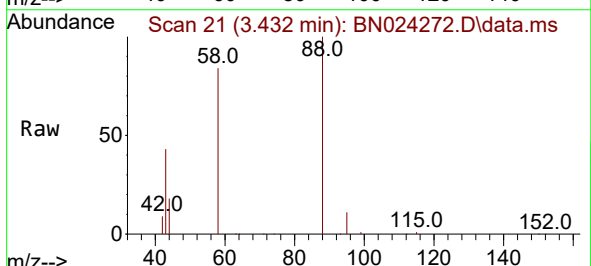

Tgt Ion: 88 Resp: 58068
Ion Ratio Lower Upper
88 100
43 36.4 29.0 43.4
58 83.0 67.3 100.9



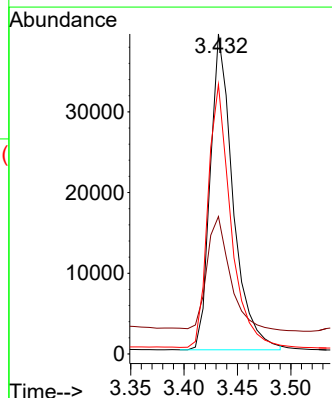
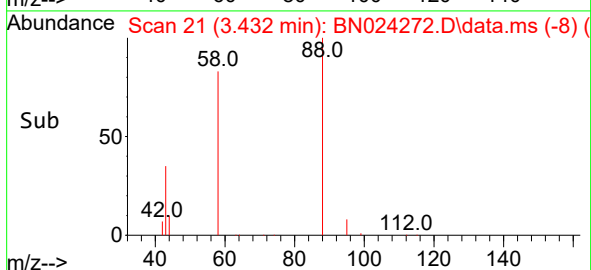


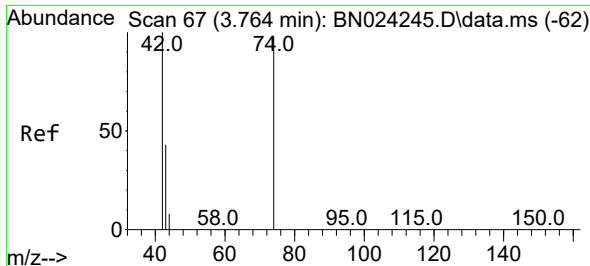

#3
n-Nitrosodimethylamine
Concen: 0.053 ng
RT: 3.685 min Scan# 50
Delta R.T. -0.079 min
Lab File: BN024272.D
Acq: 14 Mar 2023 09:26




Instrument :
BNA_N
ClientSampleId :
RE132D4-20230306


Tgt Ion: 42 Resp: 733
Ion Ratio Lower Upper
42 100
74 2.9 81.6 122.4#
44 94.3 7.3 10.9#

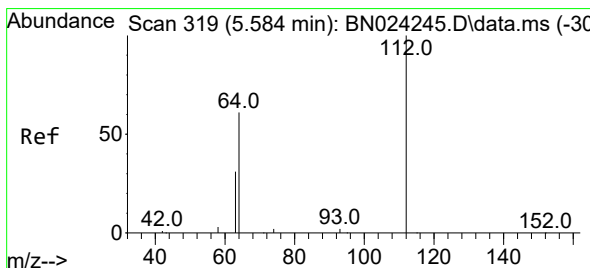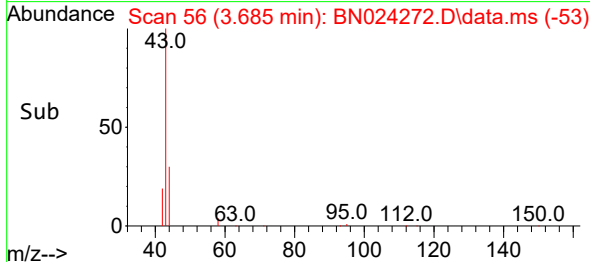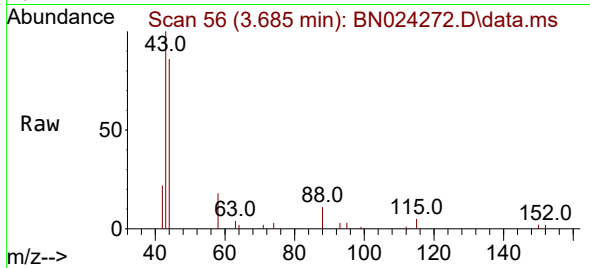

#4
2-Fluorophenol
Concen: 0.156 ng
RT: 5.584 min Scan# 319
Delta R.T. 0.000 min
Lab File: BN024272.D
Acq: 14 Mar 2023 09:26

Tgt Ion: 112 Resp: 2986
Ion Ratio Lower Upper
112 100
64 62.1 49.0 73.6
63 32.3 25.7 38.5


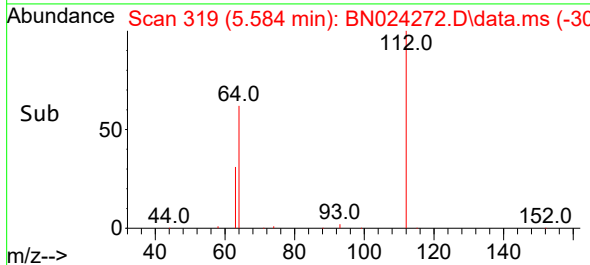

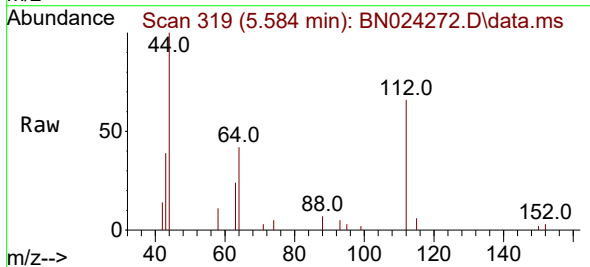


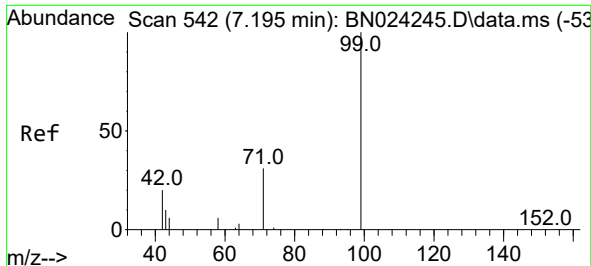

#5
Phenol-d6
Concen: 0.092 ng
RT: 7.195 min Scan# 542
Delta R.T. 0.000 min
Lab File: BN024272.D
Acq: 14 Mar 2023 09:26




Instrument :
BNA_N
ClientSampleId :
RE132D4-20230306


Tgt Ion: 99 Resp: 2263
Ion Ratio Lower Upper
99 100
42 28.8 20.1 30.1
71 37.9 25.8 38.8

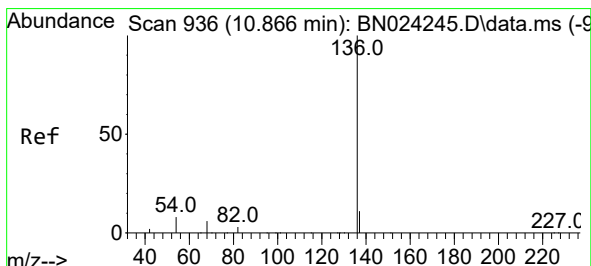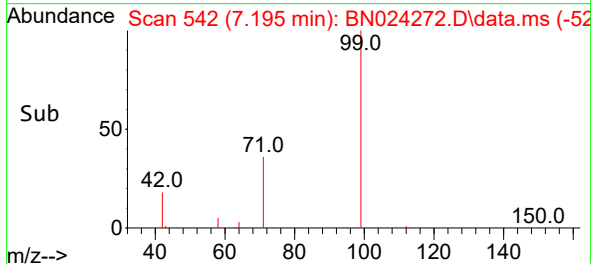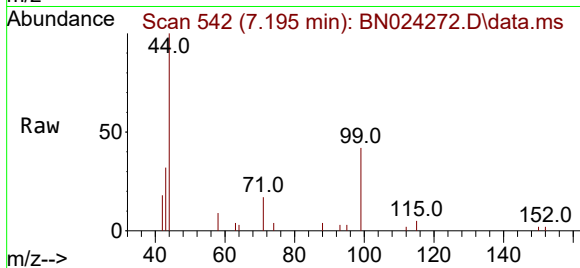

#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.866 min Scan# 936
Delta R.T. 0.000 min
Lab File: BN024272.D
Acq: 14 Mar 2023 09:26

Tgt Ion: 136 Resp: 25028
Ion Ratio Lower Upper
136 100
137 11.3 8.9 13.3
54 7.8 7.1 10.7
68 6.1 5.3 7.9


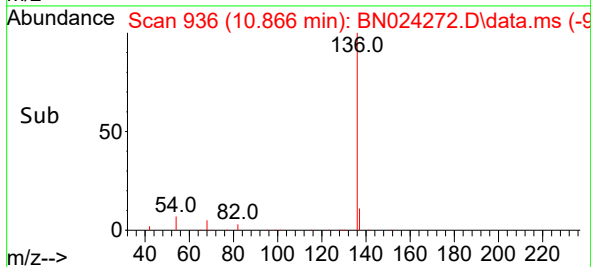

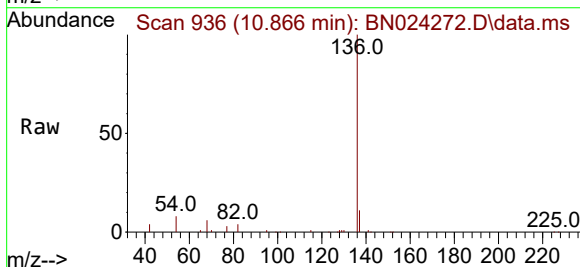


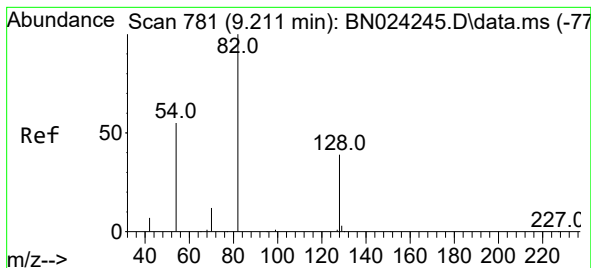

#8
Nitrobenzene-d5
Concen: 0.378 ng
RT: 9.211 min Scan# 781
Delta R.T. 0.000 min
Lab File: BN024272.D
Acq: 14 Mar 2023 09:26




Instrument :
BNA_N
ClientSampleId :
RE132D4-20230306


Tgt Ion: 82 Resp: 6323
Ion Ratio Lower Upper
82 100
128 43.5 32.4 48.6
54 55.7 45.2 67.8

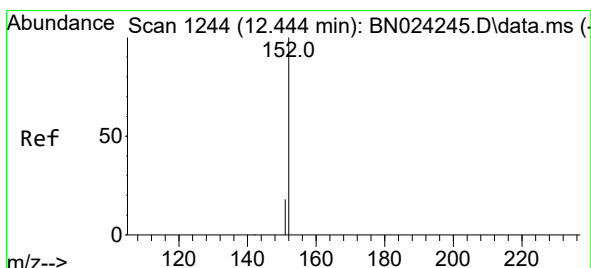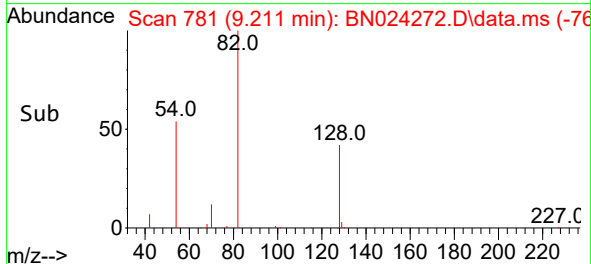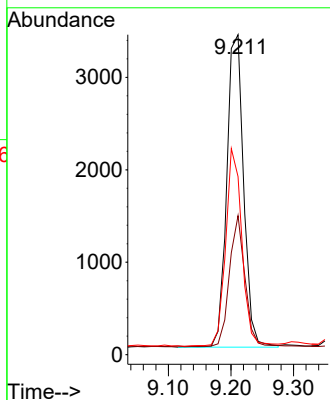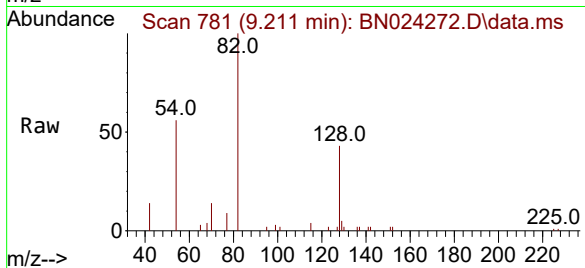

#11
2-Methylnaphthalene-d10
Concen: 0.349 ng
RT: 12.441 min Scan# 1243
Delta R.T. -0.004 min
Lab File: BN024272.D
Acq: 14 Mar 2023 09:26

Tgt Ion: 152 Resp: 10744
Ion Ratio Lower Upper
152 100
151 20.7 16.8 25.2


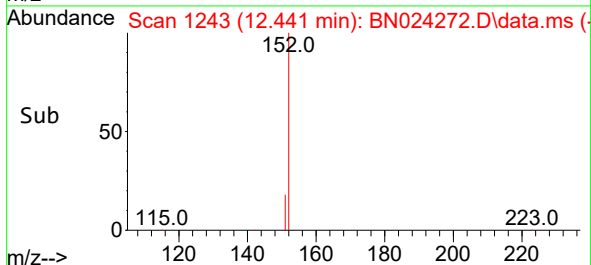
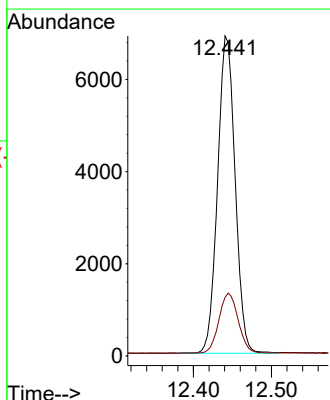
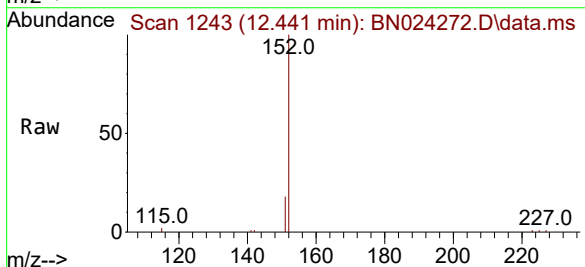


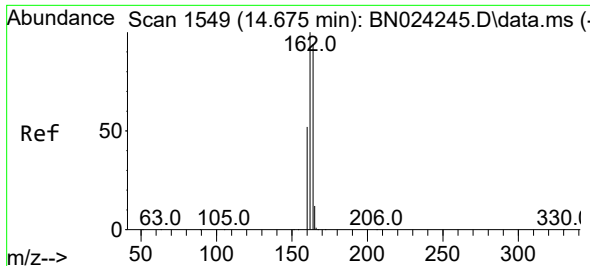

#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.675 min Scan# 1549
Delta R.T. 0.000 min
Lab File: BN024272.D
Acq: 14 Mar 2023 09:26




Instrument :
BNA_N
ClientSampleId :
RE132D4-20230306


Tgt Ion:164 Resp: 12607
Ion Ratio Lower Upper
164 100
162 105.6 84.7 127.1
160 55.2 44.6 66.8

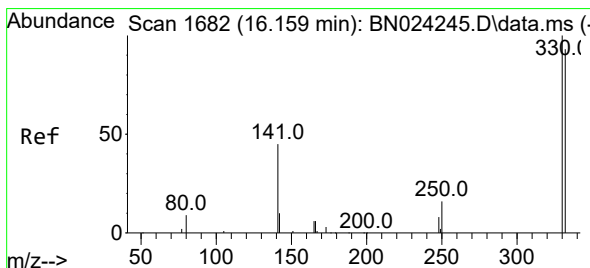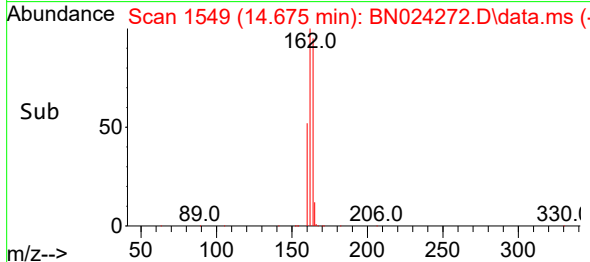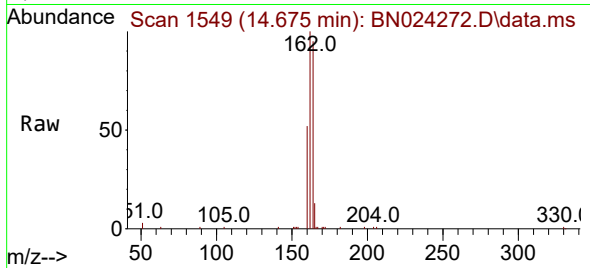

#14
2,4,6-Tribromophenol
Concen: 0.277 ng
RT: 16.159 min Scan# 1682
Delta R.T. 0.000 min
Lab File: BN024272.D
Acq: 14 Mar 2023 09:26

Tgt Ion:330 Resp: 1788
Ion Ratio Lower Upper
330 100
332 96.2 78.0 117.0
141 40.1 30.8 46.2


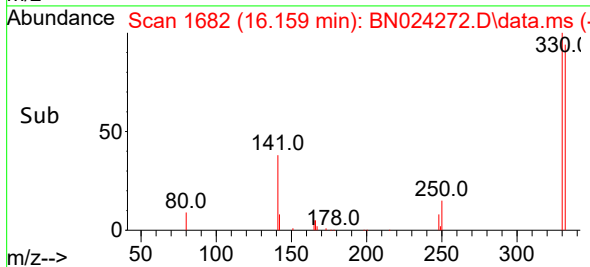

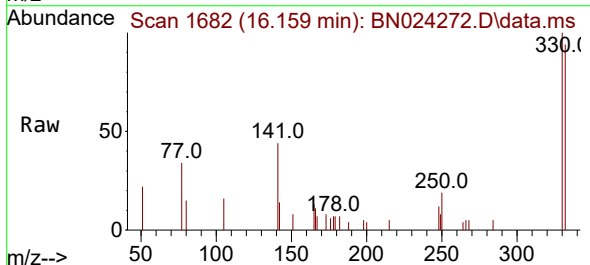


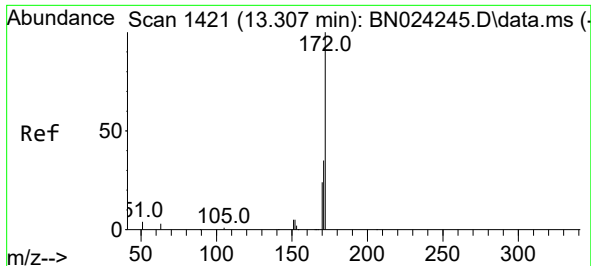

#15
2-Fluorobiphenyl
Concen: 0.358 ng
RT: 13.307 min Scan# 1421
Delta R.T. 0.000 min
Lab File: BN024272.D
Acq: 14 Mar 2023 09:26




Instrument :
BNA_N
ClientSampleId :
RE132D4-20230306


Tgt Ion:	172	Resp:	17059
Ion Ratio	Lower	Upper	
172	100		
171	34.3	27.8	41.8
170	23.3	19.0	28.6

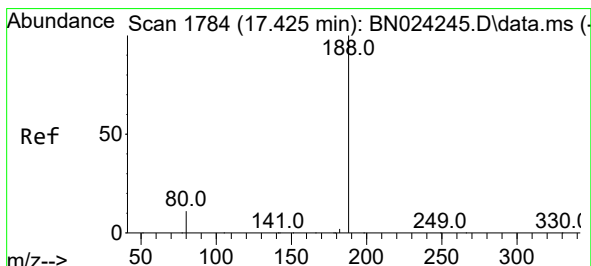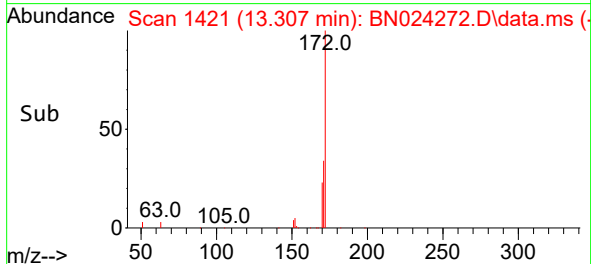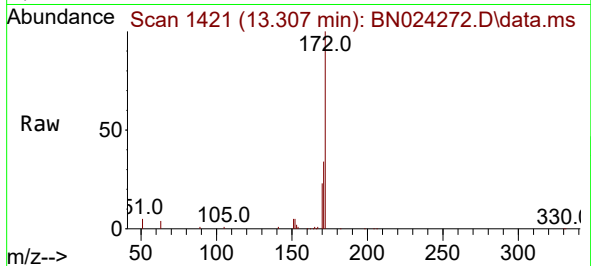

#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.425 min Scan# 1784
Delta R.T. 0.000 min
Lab File: BN024272.D
Acq: 14 Mar 2023 09:26

Tgt Ion:	188	Resp:	27285
Ion Ratio	Lower	Upper	
188	100		
94	0.0	0.0	0.0
80	10.4	8.9	13.3


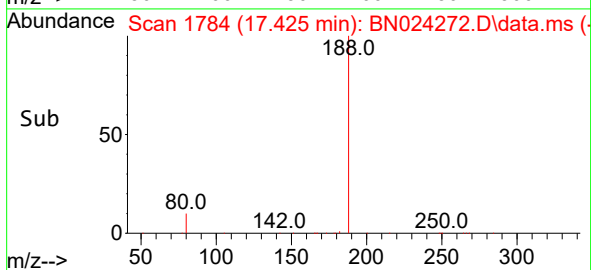

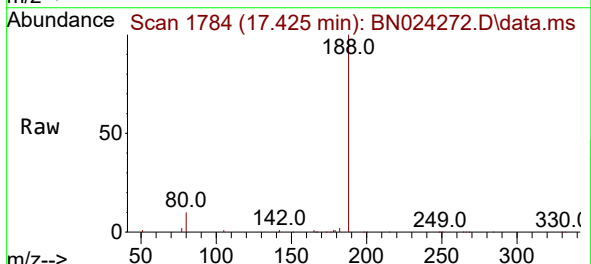


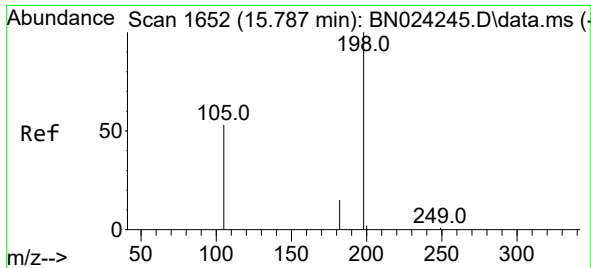

#20
4,6-Dinitro-2-methylphenol
Concen: 0.180 ng
RT: 15.774 min Scan# 1651
Delta R.T. -0.013 min
Lab File: BN024272.D
Acq: 14 Mar 2023 09:26




Instrument :
BNA_N
ClientSampleId :
RE132D4-20230306


Tgt Ion:198 Resp: 11
Ion Ratio Lower Upper
198 100
51 432.7 68.2 102.2#
105 238.8 51.6 77.4#

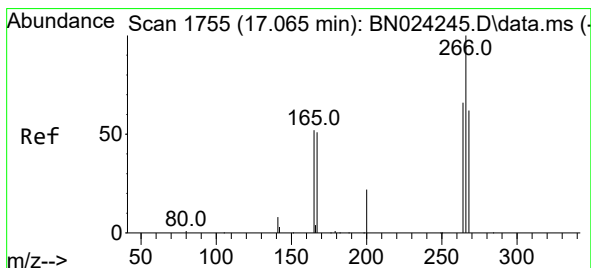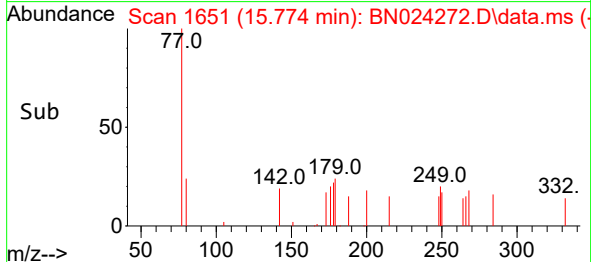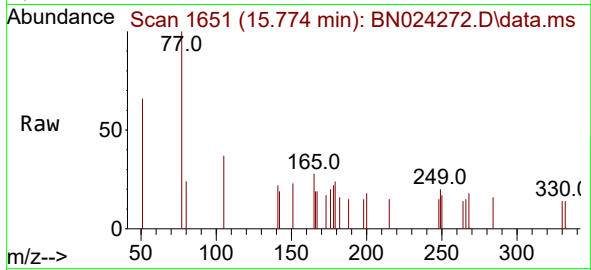

#24
Pentachlorophenol
Concen: 0.130 ng
RT: 17.065 min Scan# 1755
Delta R.T. 0.000 min
Lab File: BN024272.D
Acq: 14 Mar 2023 09:26

Tgt Ion:266 Resp: 16
Ion Ratio Lower Upper
266 100
264 43.8 51.1 76.7#
268 25.0 52.2 78.4#


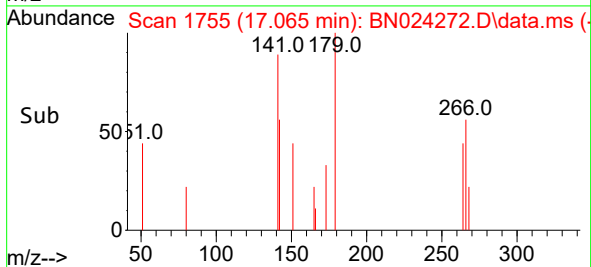

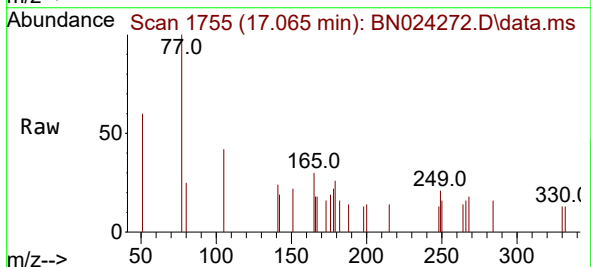


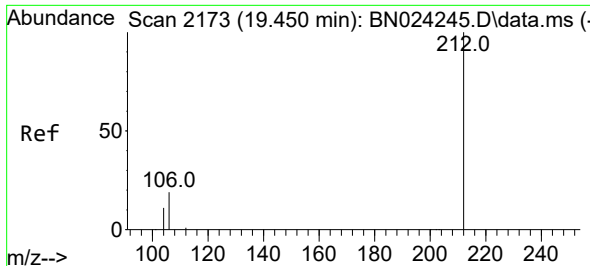

#27
Fluoranthene-d10
Concen: 0.490 ng
RT: 19.450 min Scan# 2173
Delta R.T. 0.000 min
Lab File: BN024272.D
Acq: 14 Mar 2023 09:26




Instrument :
BNA_N
ClientSampleId :
RE132D4-20230306


Tgt Ion:212 Resp: 28343
Ion Ratio Lower Upper
212 100
106 19.4 15.4 23.2
104 10.9 8.6 13.0

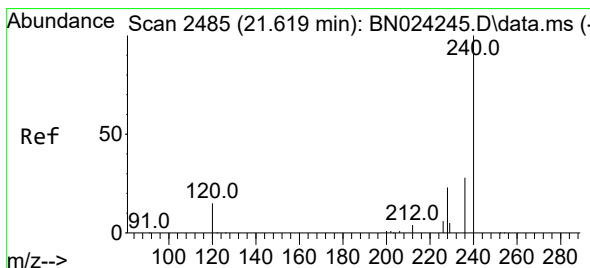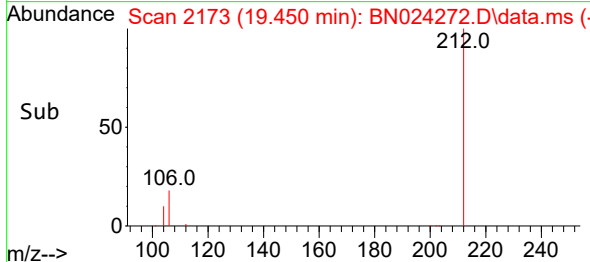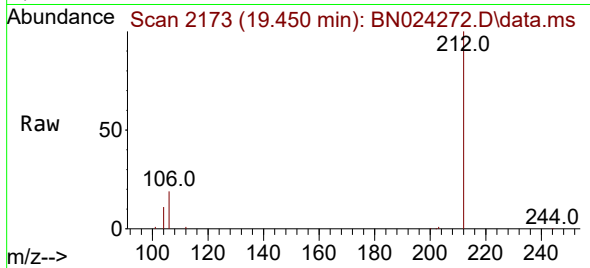

#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.619 min Scan# 2485
Delta R.T. 0.000 min
Lab File: BN024272.D
Acq: 14 Mar 2023 09:26

Tgt Ion:240 Resp: 20924
Ion Ratio Lower Upper
240 100
120 15.1 12.8 19.2
236 28.0 22.5 33.7

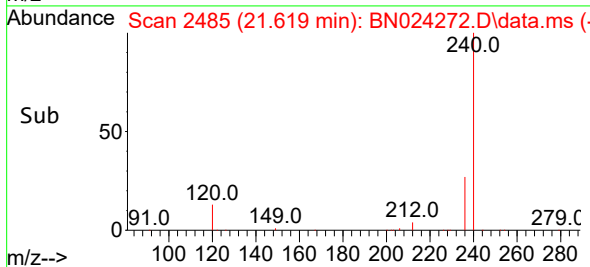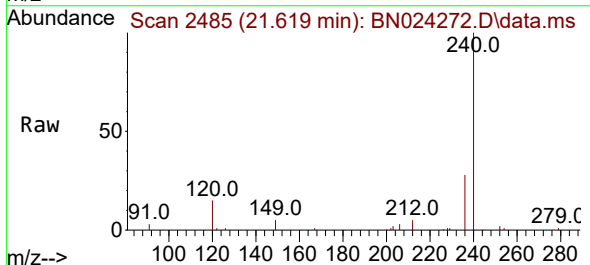

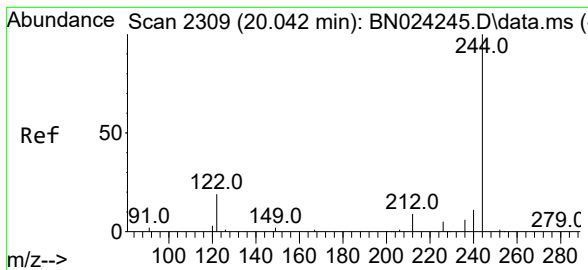

#31

Terphenyl-d14

Concen: 0.480 ng

RT: 20.043 min Scan# 21

Delta R.T. 0.000 min

Lab File: BN024272.D

Acq: 14 Mar 2023 09:26

Instrument :

BNA_N

ClientSampleId :

RE132D4-20230306





Tgt Ion:244 Resp: 16928

Ion Ratio Lower Upper

244 100

212 8.7 7.6 11.4

122 14.4 15.1 22.7#

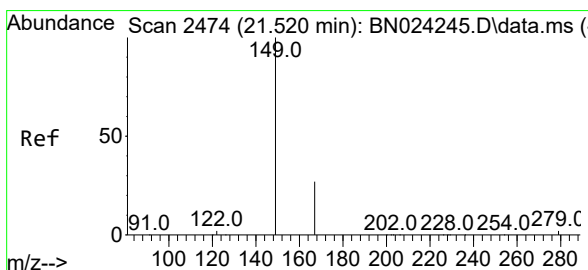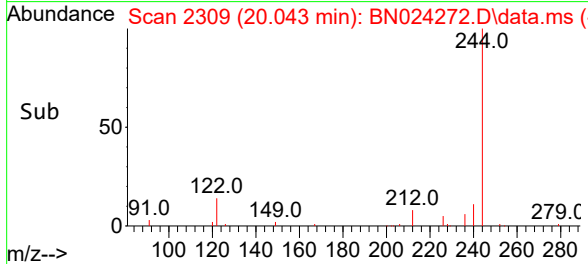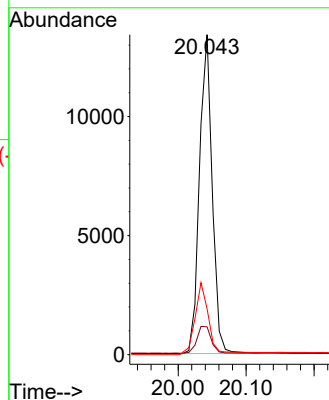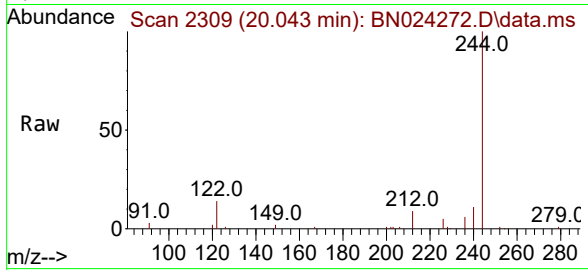

#34

Bis(2-ethylhexyl)phthalate

Concen: 0.078 ng

RT: 21.511 min Scan# 2473

Delta R.T. -0.009 min

Lab File: BN024272.D

Acq: 14 Mar 2023 09:26




Tgt Ion:149 Resp: 2562


Ion Ratio Lower Upper

149 100

167 24.0 21.2 31.8


279 3.2 1.8 2.8#

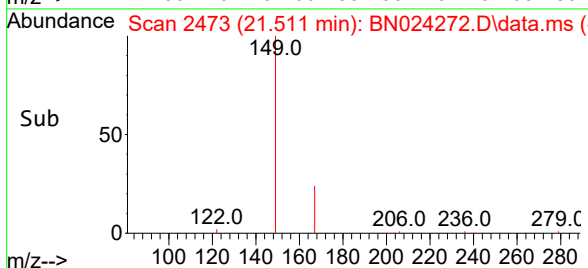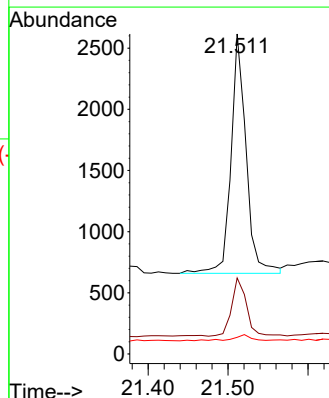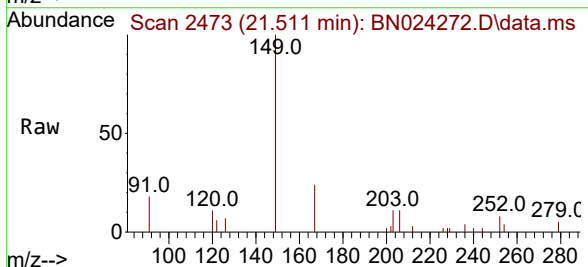

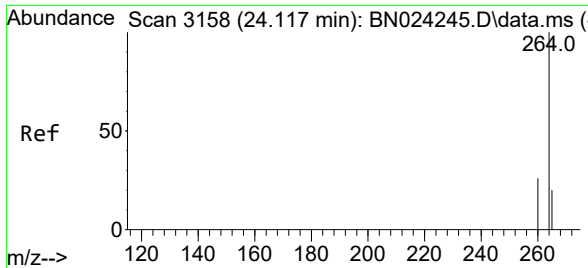

#35
Perylene-d12
Concen: 0.400 ng
RT: 24.123 min Scan# 31
Delta R.T. 0.006 min
Lab File: BN024272.D
Acq: 14 Mar 2023 09:26

Instrument :
BNA_N
ClientSampleId :
RE132D4-20230306

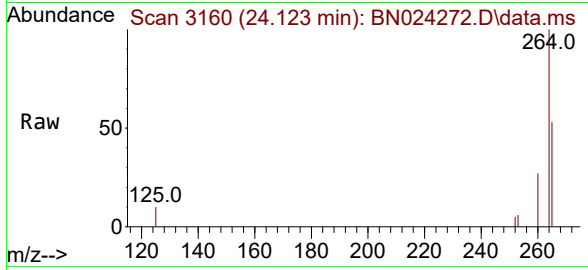

Tgt Ion:264 Resp: 17507

Ion	Ratio	Lower	Upper
264	100		
260	27.2	21.4	32.2
265	52.7	35.7	53.5

