
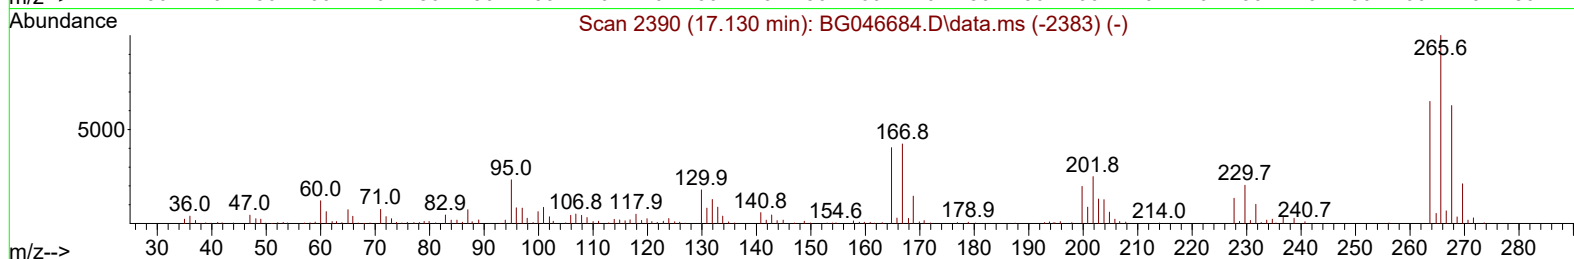
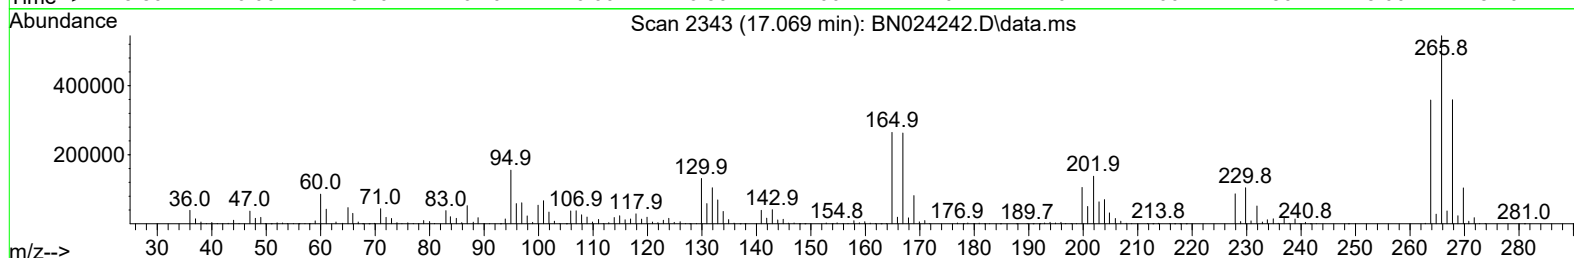


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031323\
Data File : BN024242.D
Acq On : 13 Mar 2023 11:57
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 14 06:35:39 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 14 06:35:35 2023
Response via : Initial Calibration

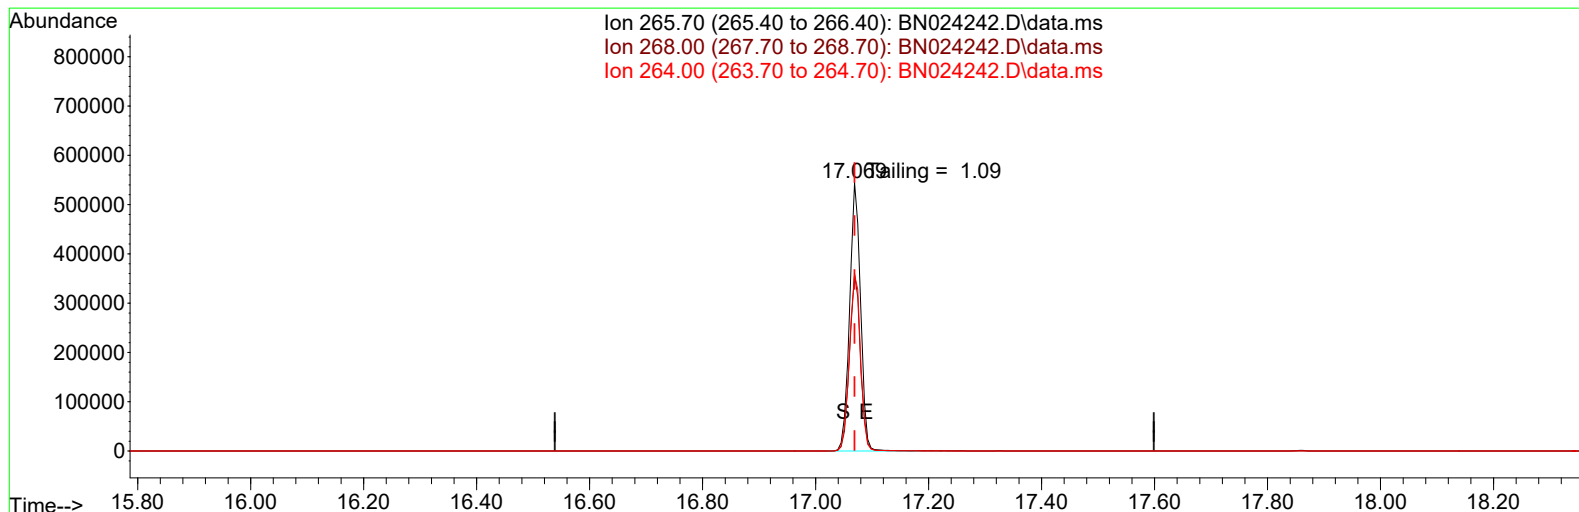

TIC: BN024242.D\data.ms

(70) Pentachlorophenol (C)




17.069min (0.000) 27355.37 ng

response 734843

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.99
264.00	61.60	65.79
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031323\
 Data File : BN024242.D
 Acq On : 13 Mar 2023 11:57
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 14 06:35:39 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 14 06:35:35 2023
 Response via : Initial Calibration

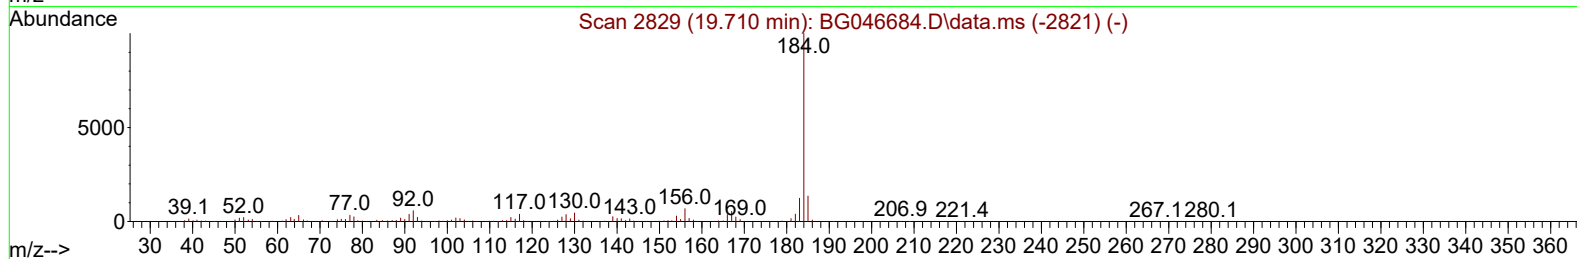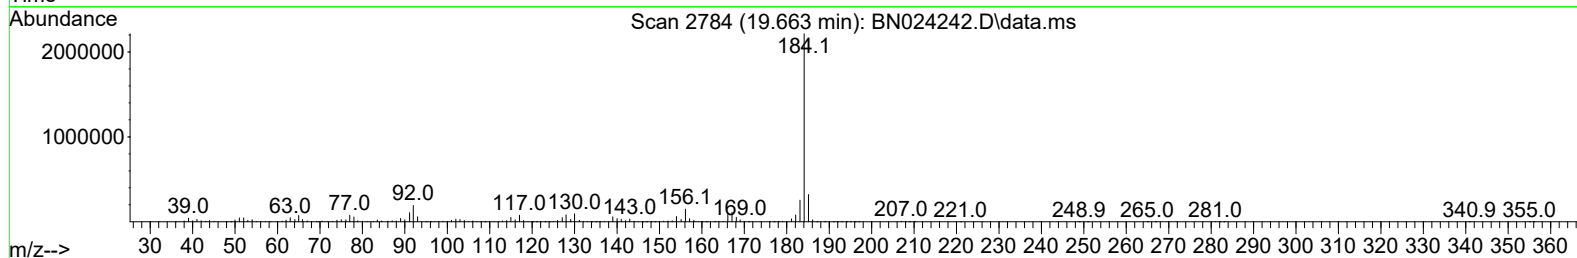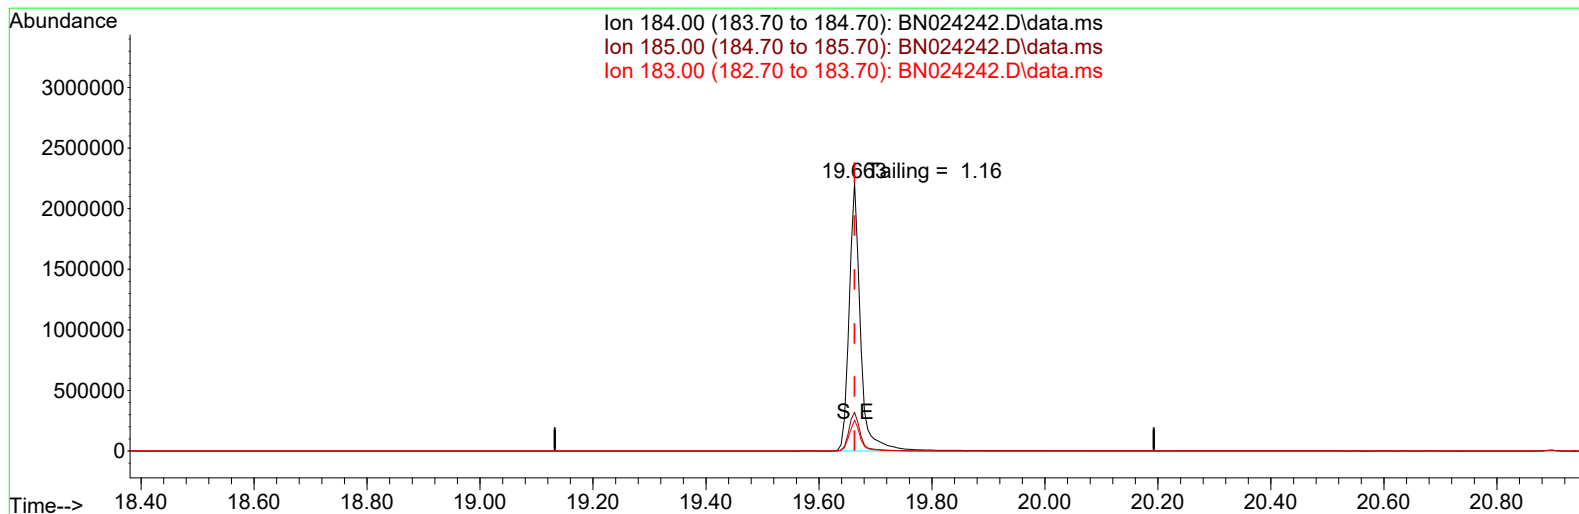

TIC: BN024242.D\data.ms

(77) Benzidine

19.663min (0.000) 169364.97 ng

response 3048911

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.46
183.00	13.20	11.51
0.00	0.00	0.00