
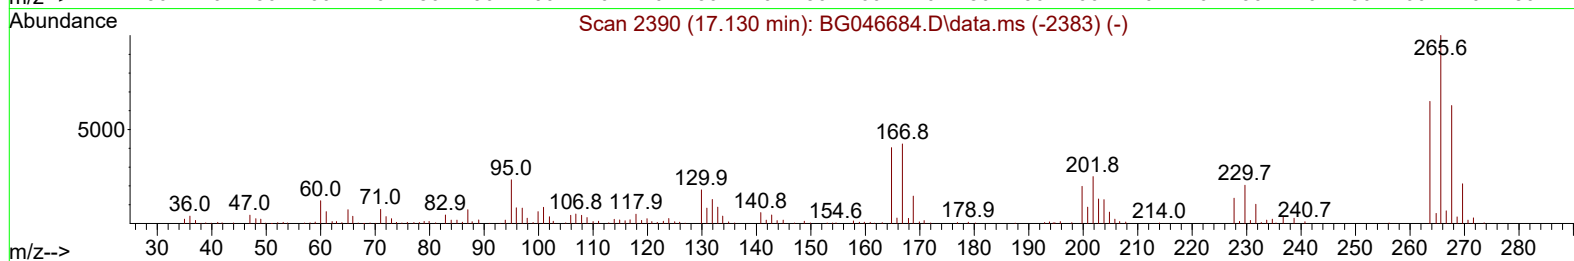
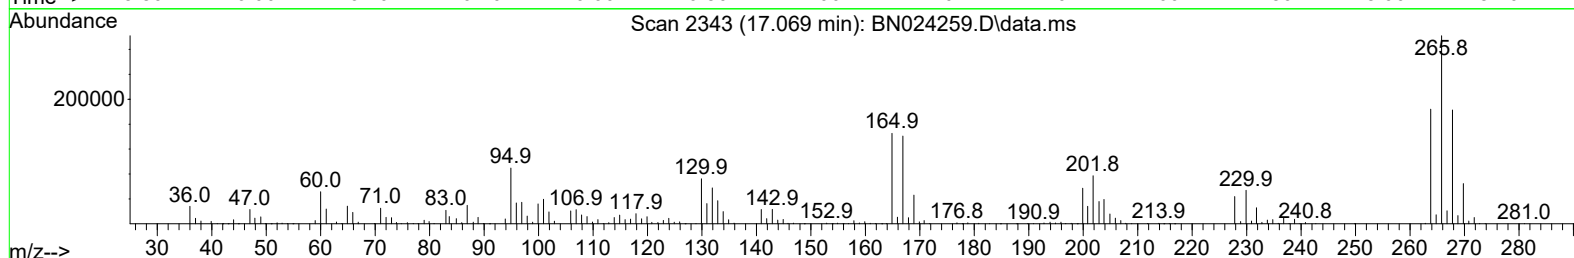


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031323\
Data File : BN024259.D
Acq On : 14 Mar 2023 00:53
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 14 06:36:50 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 14 06:35:35 2023
Response via : Initial Calibration

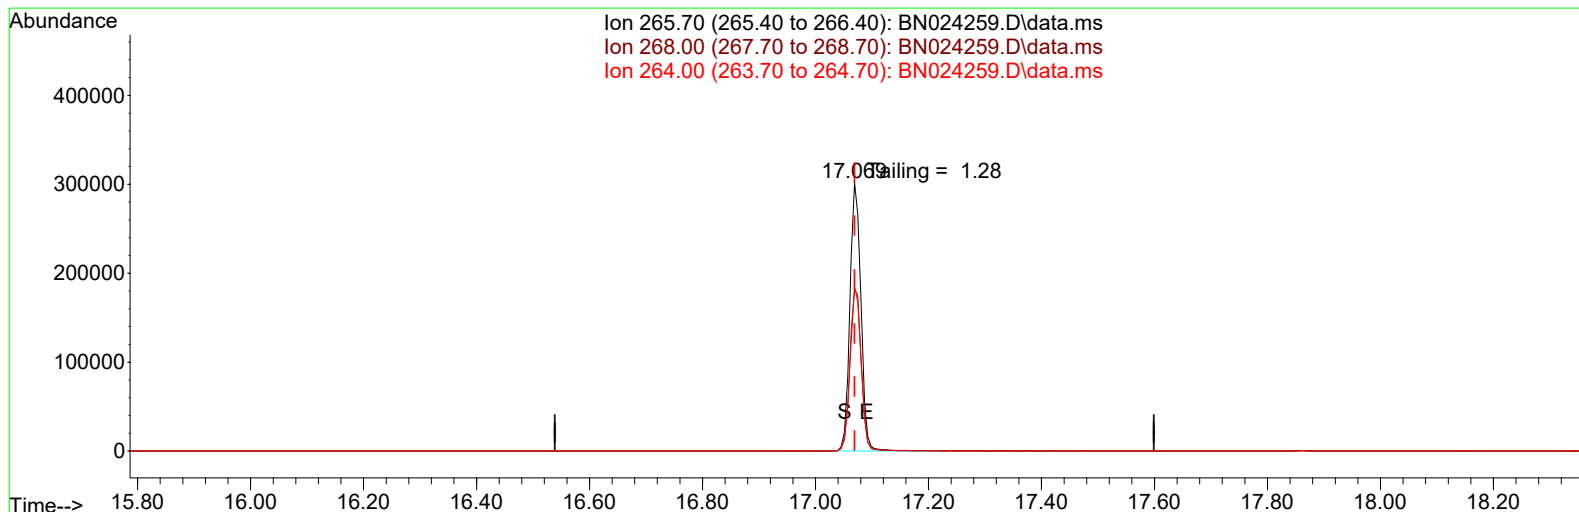

TIC: BN024259.D\data.ms

(70) Pentachlorophenol (C)




17.069min (+ 0.000) 27850.15 ng

response **410239**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	60.57
264.00	61.60	60.93
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031323\
Data File : BN024259.D
Acq On : 14 Mar 2023 00:53
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 14 06:36:50 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 14 06:35:35 2023
Response via : Initial Calibration

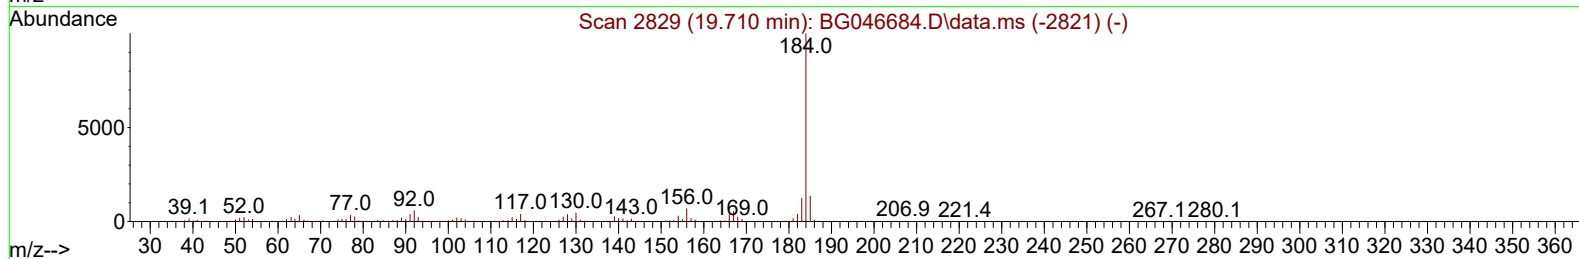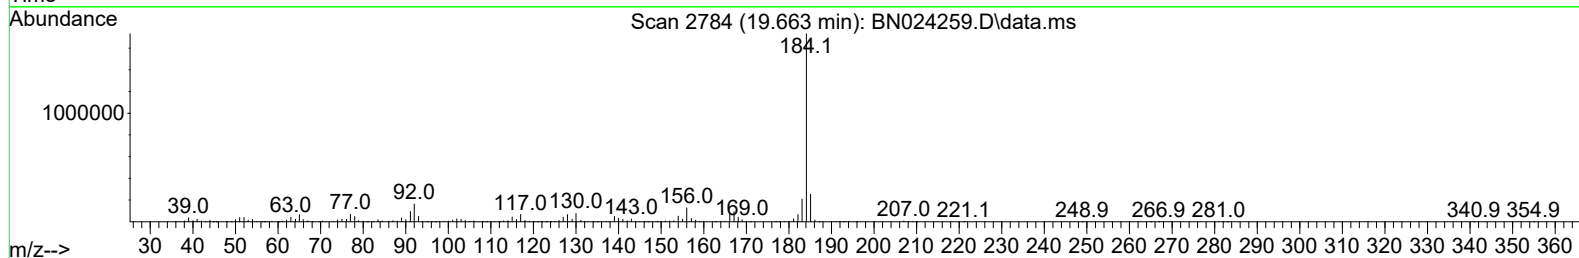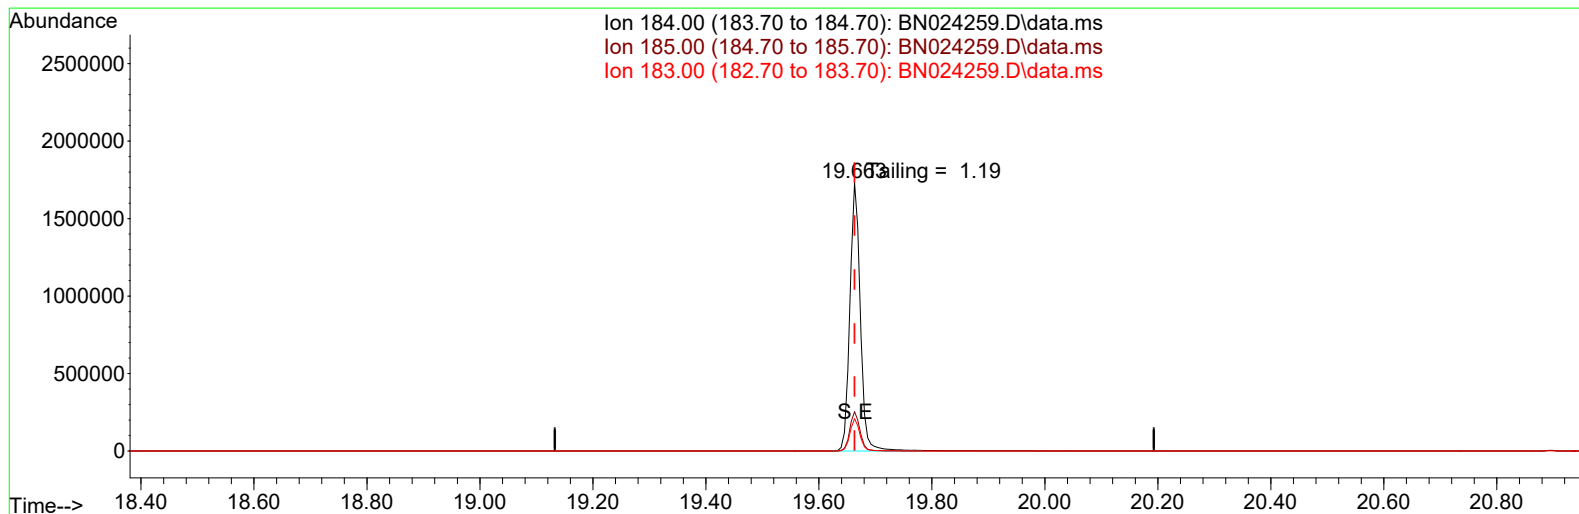

TIC: BN024259.D\data.ms

(77) Benzidine

19.663min (+ 0.000) 0.00 ng

response 2242401

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.68
183.00	13.20	12.08
0.00	0.00	0.00