
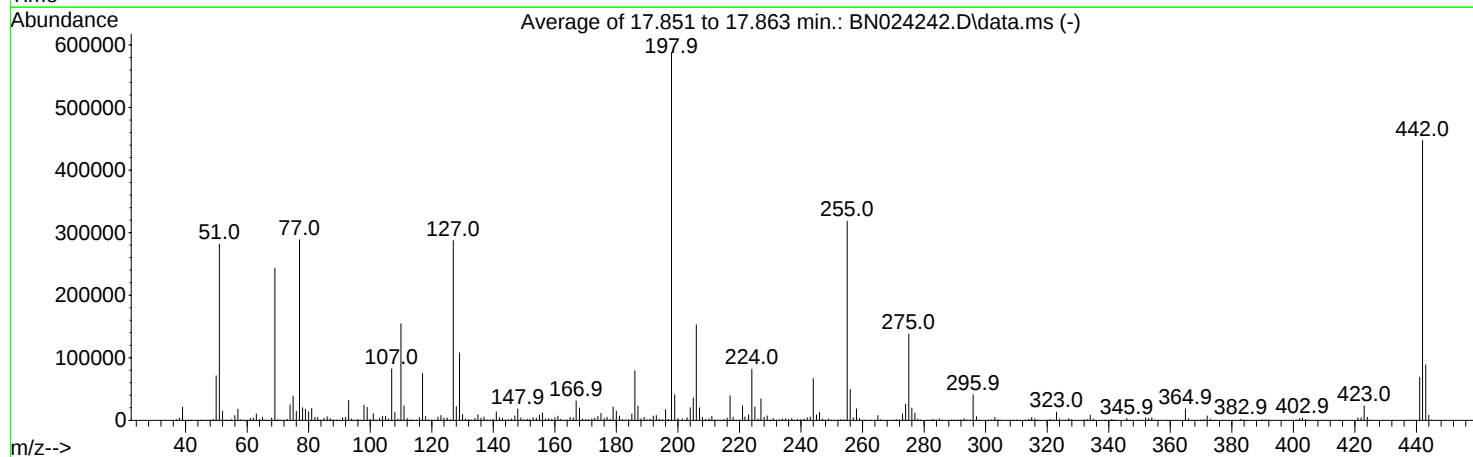


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031323\
Data File : BN024242.D
Acq On : 13 Mar 2023 11:57
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN031323.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Mar 14 03:11:52 2023

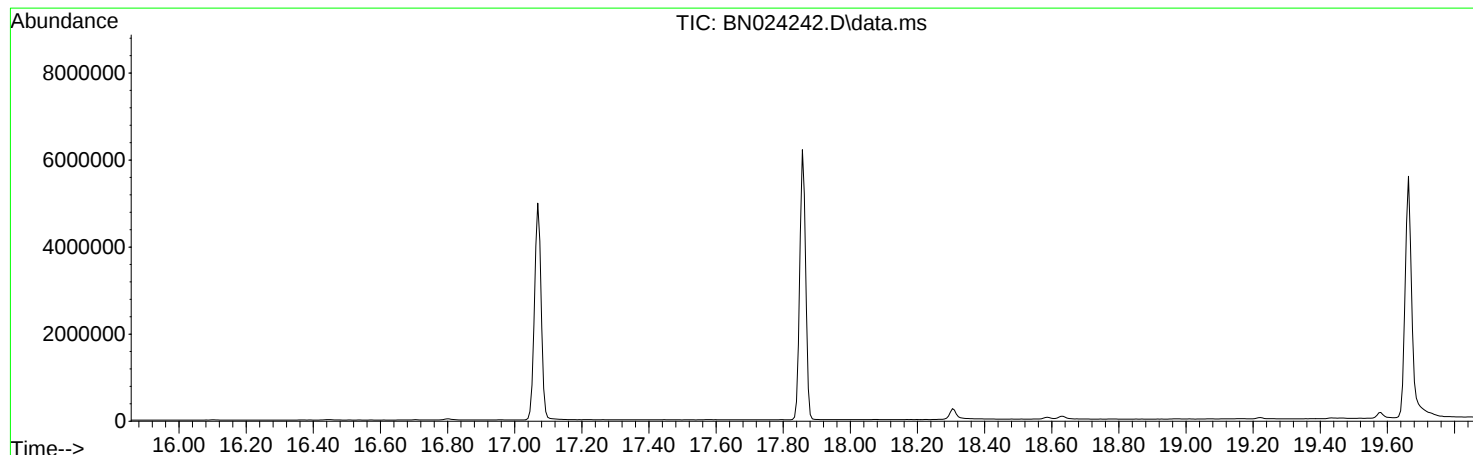




AutoFind: Scans 2476, 2477, 2478; Background Corrected with Scan 2469

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.9	281690	PASS
68	69	0.00	2	1.6	3858	PASS
69	198	0.00	100	41.4	243362	PASS
70	69	0.00	2	0.5	1251	PASS
127	198	10	80	48.9	287381	PASS
197	198	0.00	2	0.3	1736	PASS
198	198	100	100	100.0	588224	PASS
199	198	5	9	6.9	40717	PASS
275	198	10	60	23.4	137931	PASS
365	198	1	100	3.1	18404	PASS
441	198	0.01	100	11.7	69101	PASS
442	442	50	100	100.0	447424	PASS
443	442	15	24	19.8	88776	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031323\
Data File : BN024242.D
Acq On : 13 Mar 2023 11:57
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 14 06:35:39 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 14 06:35:35 2023
Response via : Initial Calibration

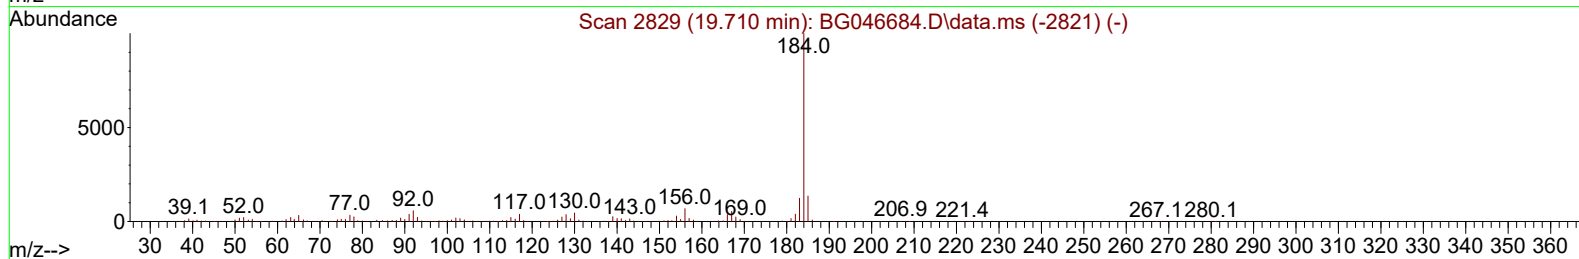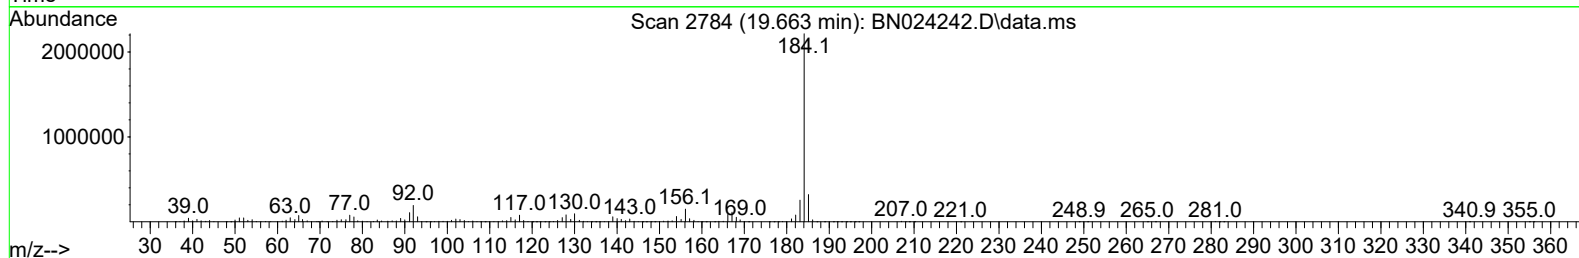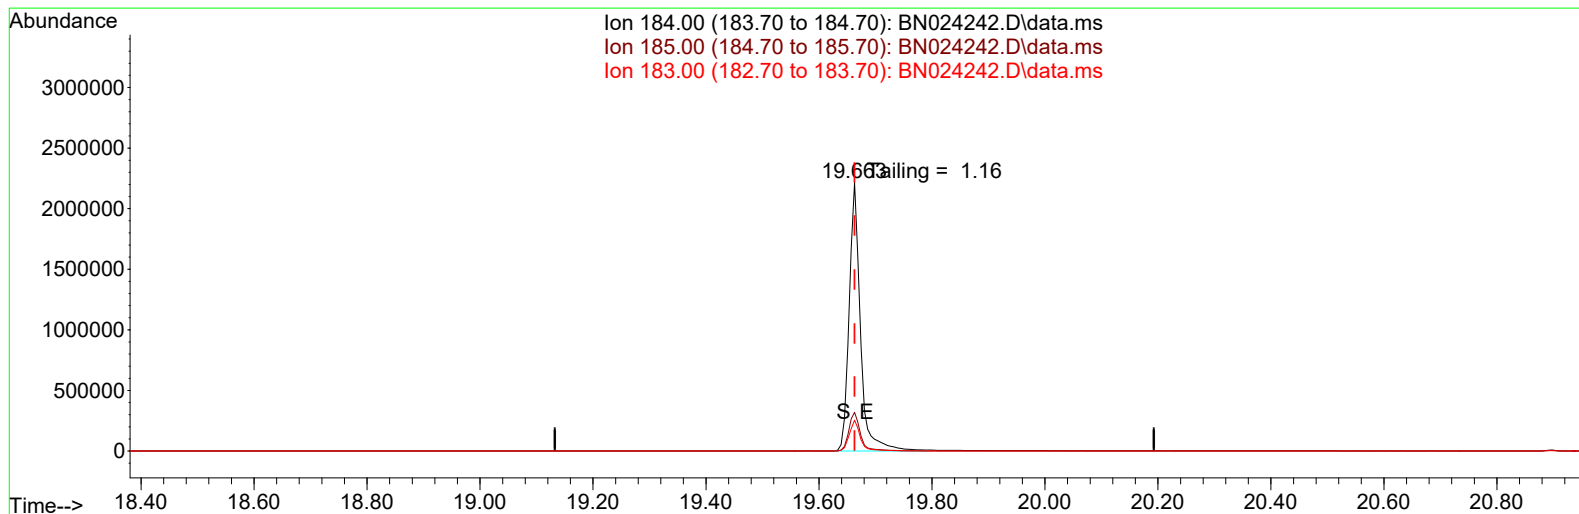

TIC: BN024242.D\data.ms

(77) Benzidine

19.663min (0.000) 169364.97 ng

response 3048911

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.46
183.00	13.20	11.51
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/13/2023	BNA_N	<u>BN024242.D</u>
Compound Name	Response	Retention Time
DDT	1869744	20.898
DDD	27700	20.451
DDE	941	19.945
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
28641	1898385	1.51

Instrument :
BNA_N
ClientSampleId :
DFTPP