
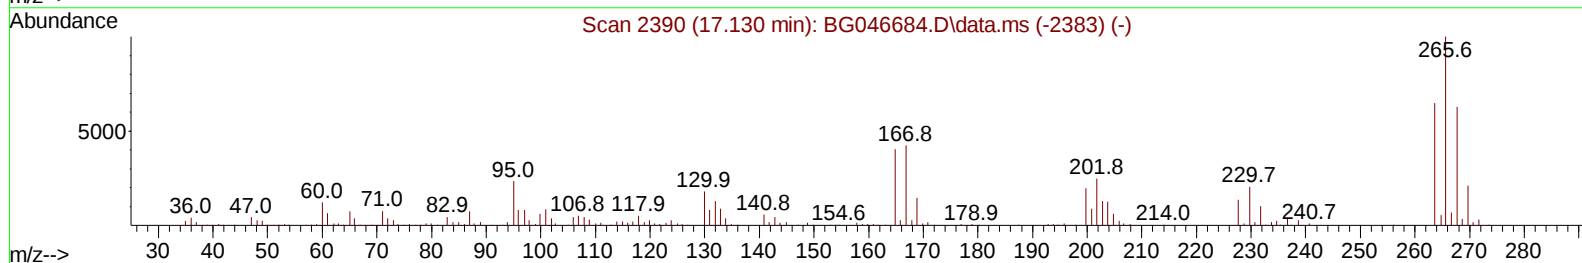
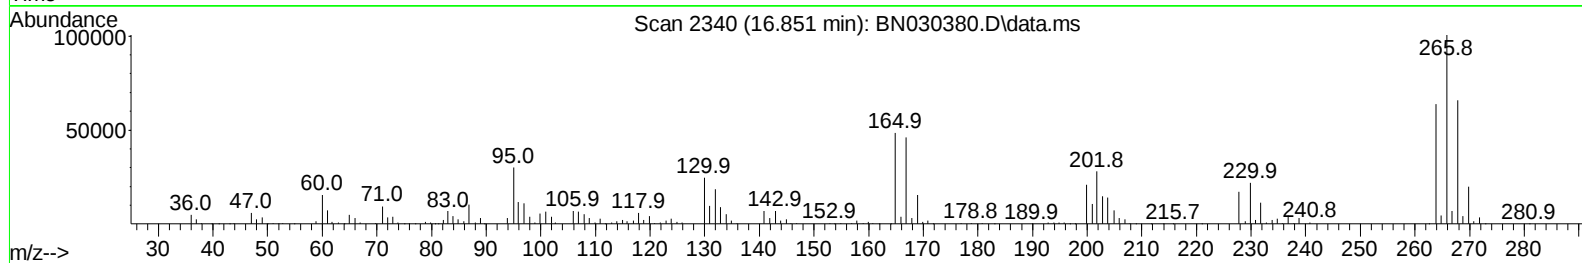


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031324\
Data File : BN030380.D
Acq On : 13 Mar 2024 13:57
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 14 04:53:07 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 08 04:34:38 2024
Response via : Initial Calibration

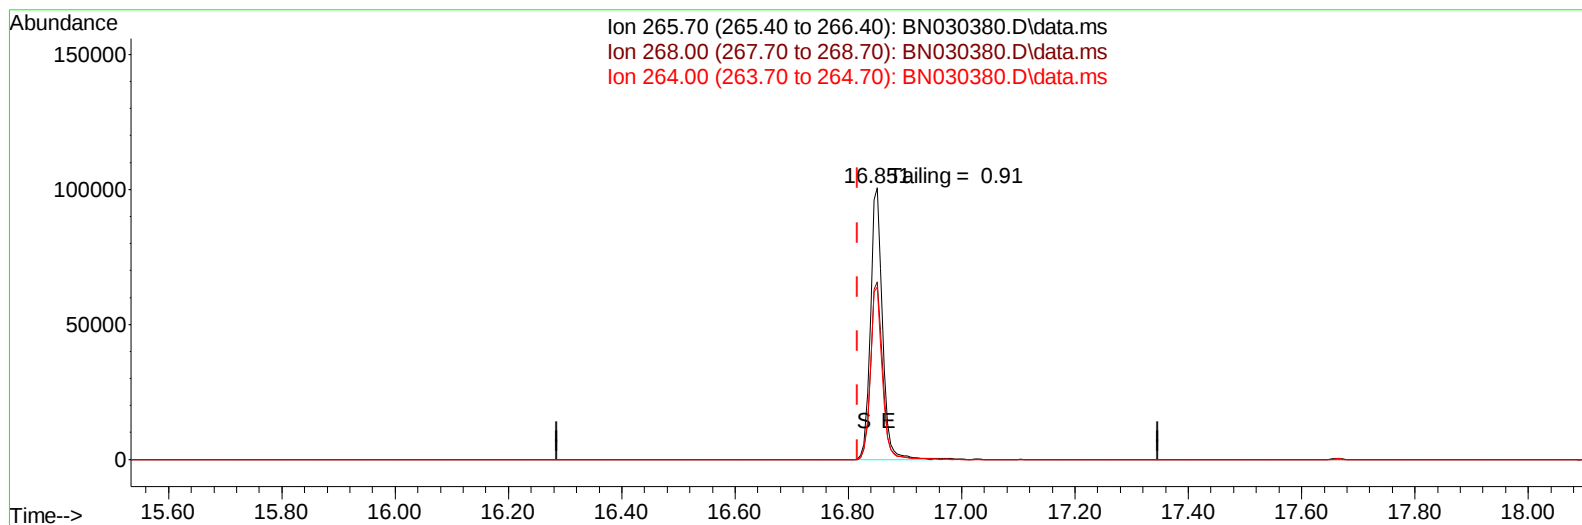




TIC: BN030380.D\data.ms

(70) Pentachlorophenol (C)**16.851min (+ 0.035) 22011.38 ng****response 148038**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.46
264.00	61.60	63.49
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031324\
Data File : BN030380.D
Acq On : 13 Mar 2024 13:57
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 14 04:53:07 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 08 04:34:38 2024
Response via : Initial Calibration

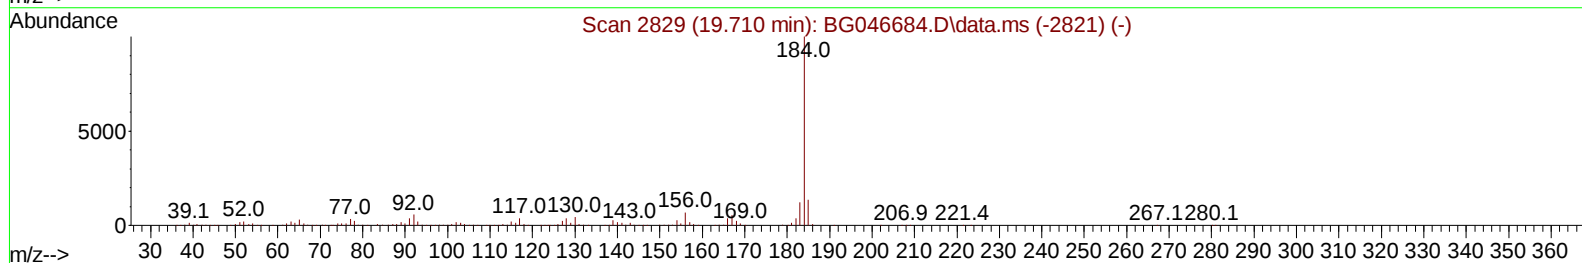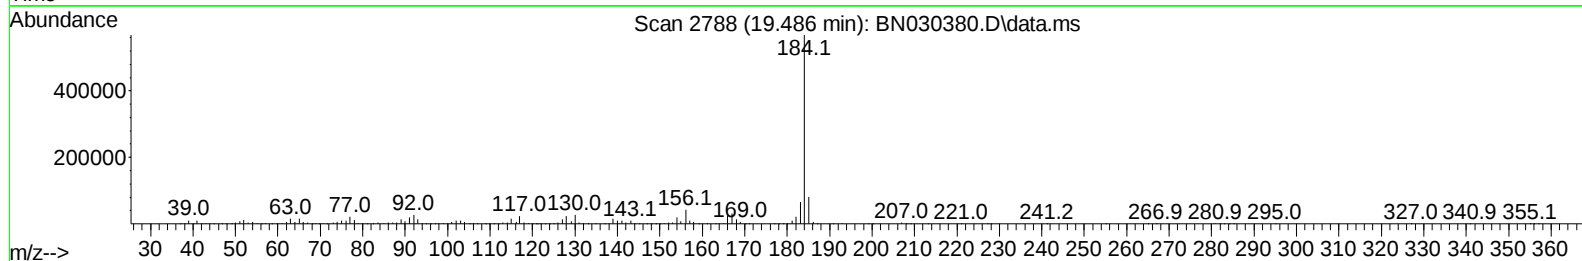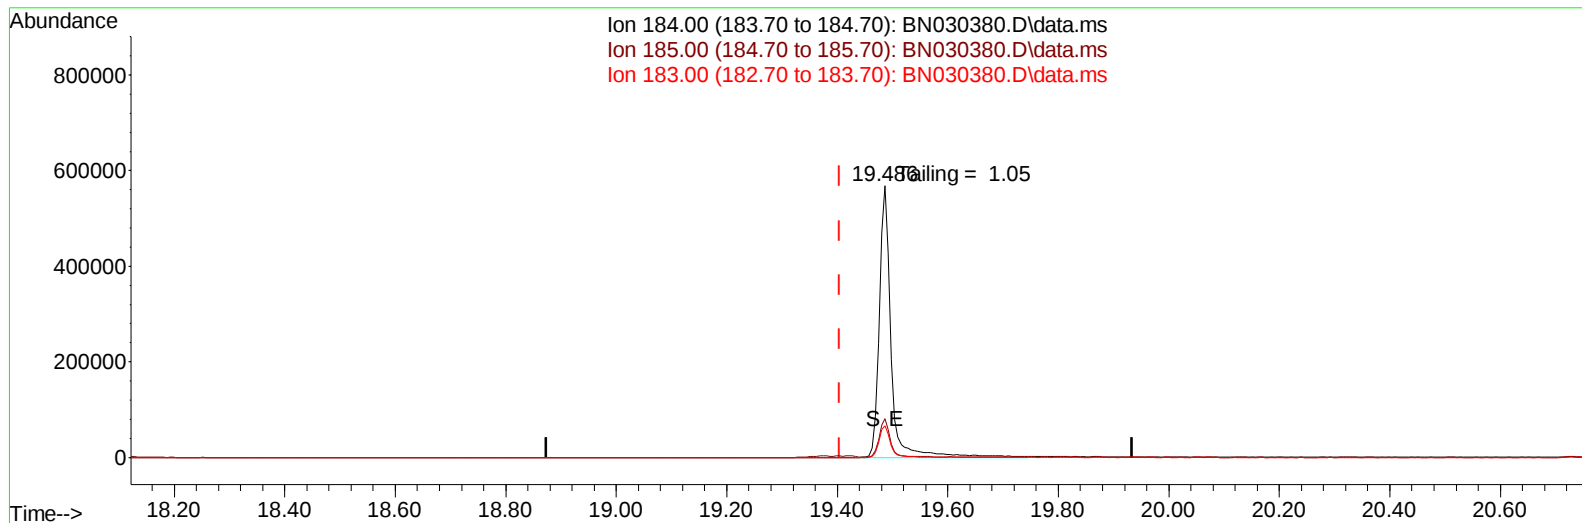

TIC: BN030380.D\data.ms

(77) Benzidine

19.486min (+ 0.082) 0.00 ng

response 854156

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.39
183.00	13.20	11.70
0.00	0.00	0.00