


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031324\
Data File : BN030380.D
Acq On : 13 Mar 2024 13:57
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN031324.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Mar 14 11:36:29 2024

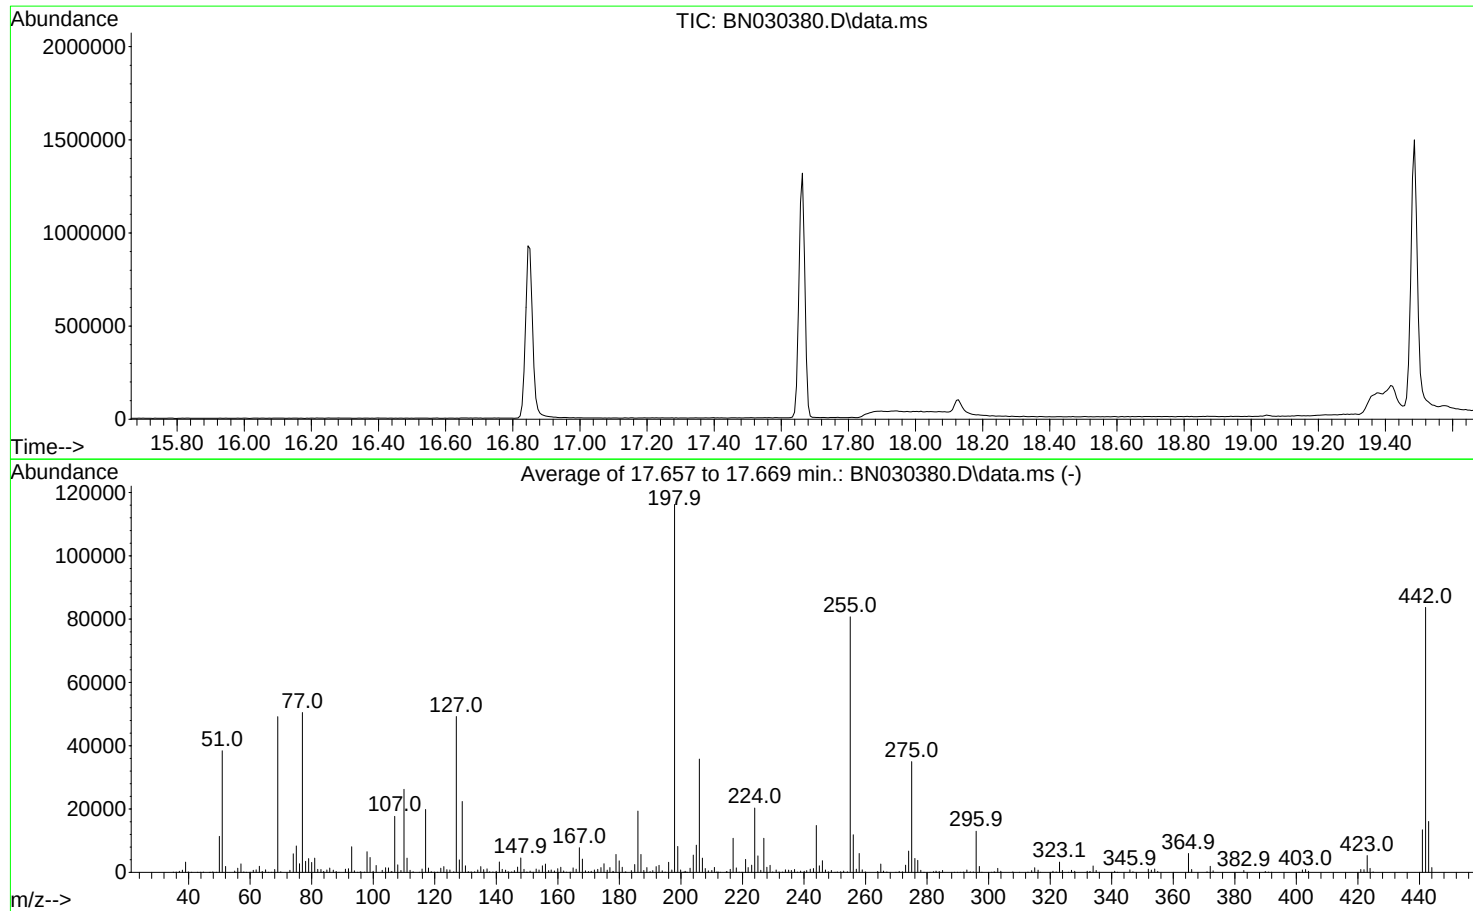




AutoFind: Scans 2477, 2478, 2479; Background Corrected with Scan 2470

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.1	38432	PASS
68	69	0.00	2	1.9	914	PASS
69	198	0.00	100	42.3	49189	PASS
70	69	0.00	2	0.4	192	PASS
127	198	10	80	42.4	49232	PASS
197	198	0.00	2	0.7	758	PASS
198	198	100	100	100.0	116221	PASS
199	198	5	9	7.1	8201	PASS
275	198	10	60	30.1	34976	PASS
365	198	1	100	5.1	5953	PASS
441	198	0.01	100	11.6	13446	PASS
442	442	50	100	100.0	83704	PASS
443	442	15	24	19.2	16093	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031324\
Data File : BN030380.D
Acq On : 13 Mar 2024 13:57
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 14 04:53:07 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 08 04:34:38 2024
Response via : Initial Calibration

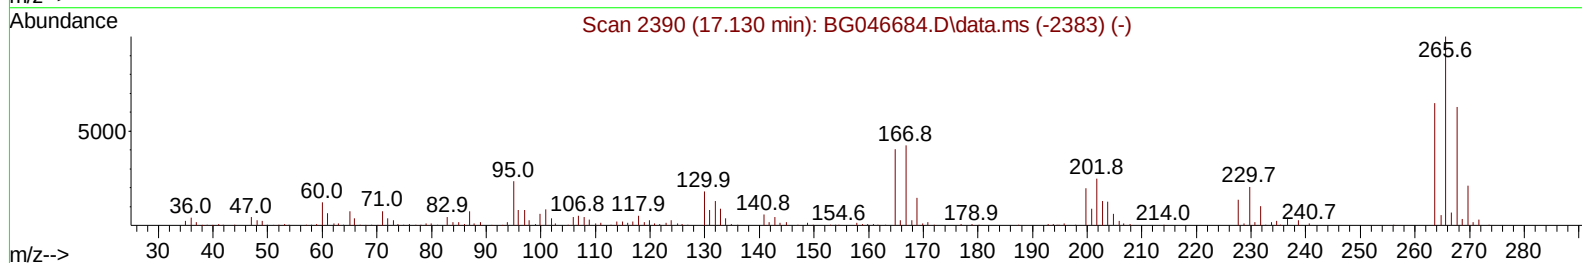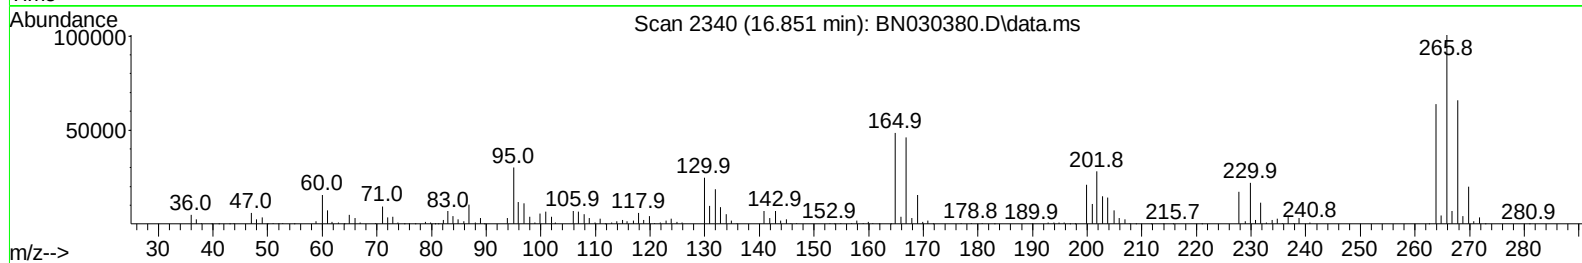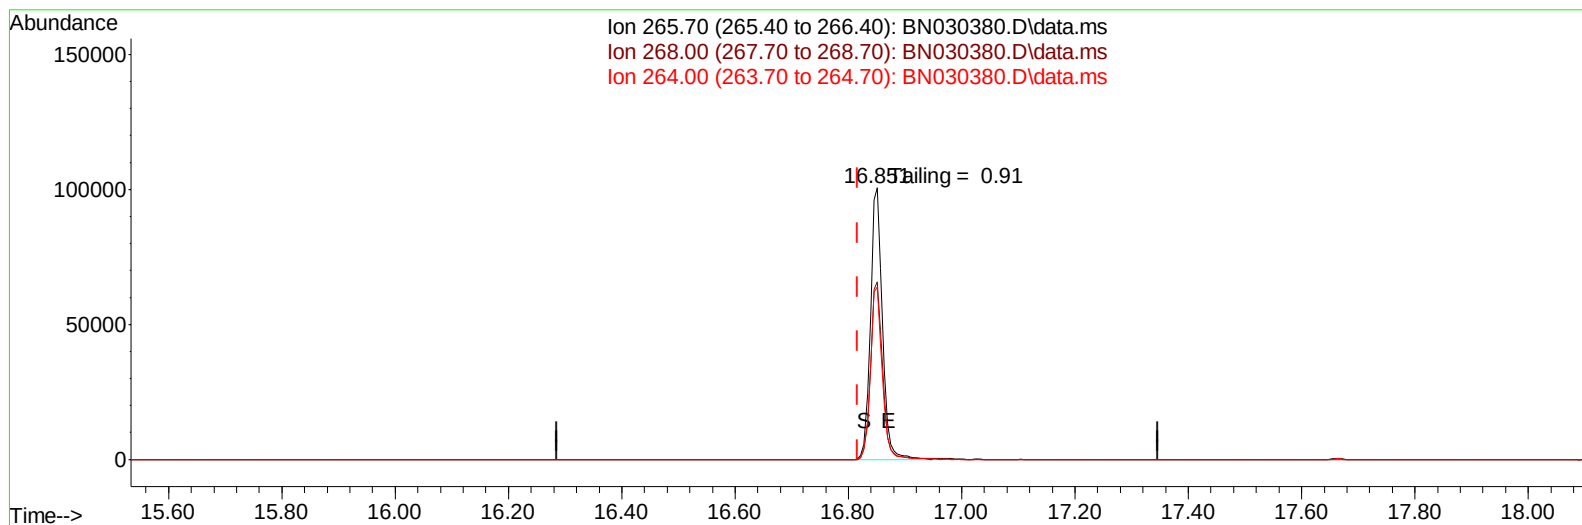

TIC: BN030380.D\data.ms

(70) Pentachlorophenol (C)

16.851min (+ 0.035) 22011.38 ng




response 148038

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.46
264.00	61.60	63.49
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031324\
Data File : BN030380.D
Acq On : 13 Mar 2024 13:57
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 14 04:53:07 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 08 04:34:38 2024
Response via : Initial Calibration

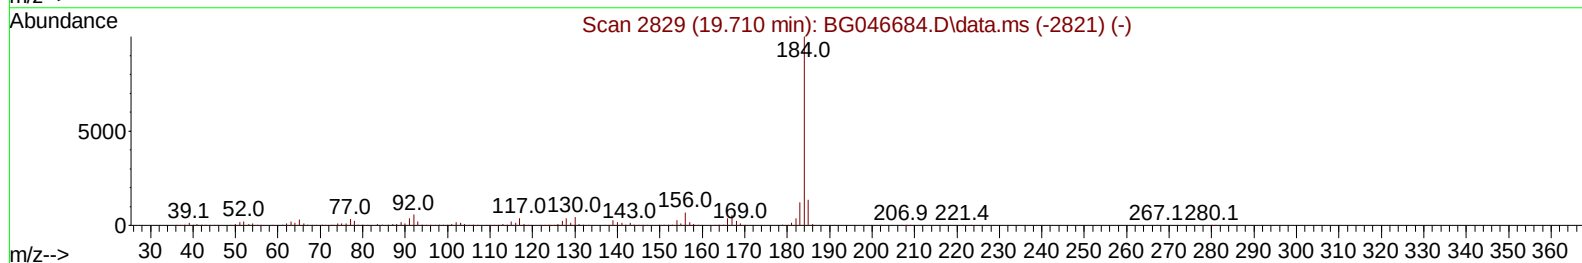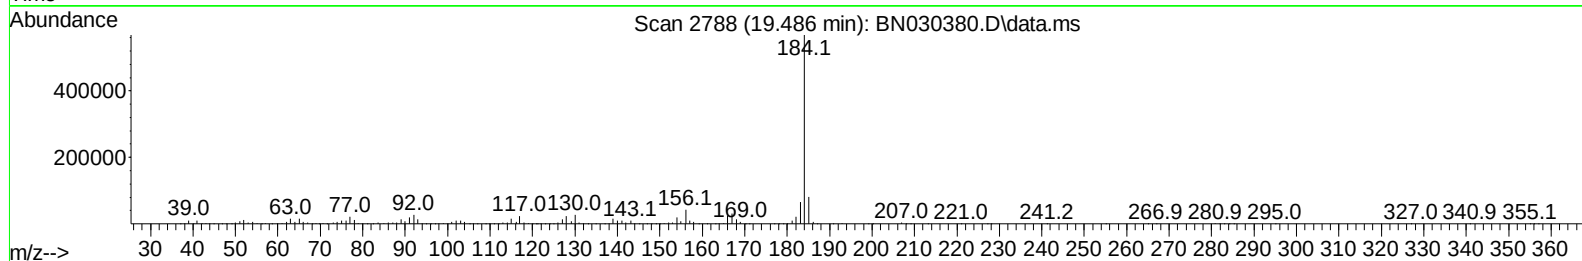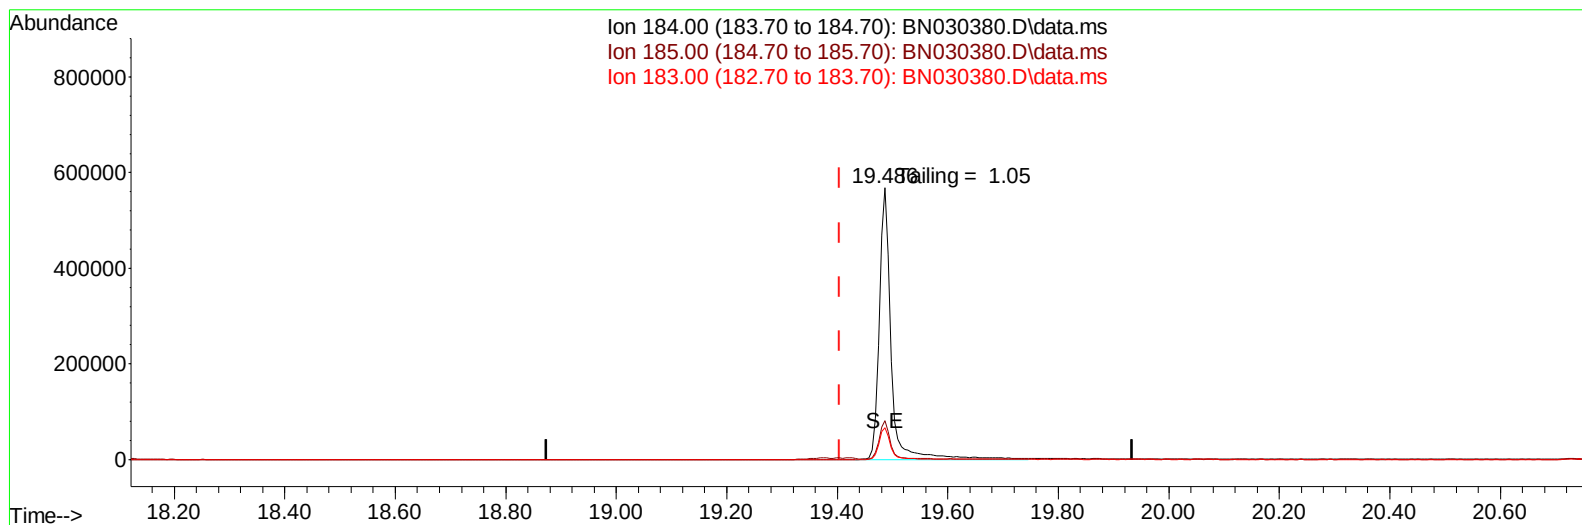

TIC: BN030380.D\data.ms

(77) Benzidine

19.486min (+ 0.082) 0.00 ng

response 854156

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.39
183.00	13.20	11.70
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/13/2024	BNA_N	<u>BN030380.D</u>
Compound Name	Response	Retention Time
DDT	414861	20.727
DDD	11371	20.286
DDE	541	19.775
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
11912	426773	2.79

Instrument :
BNA_N
ClientSampleId :
DFTPP