

Data Path : Z:\HPCHEM1\BNA_N\DATA\BN031418\
 Data File : BN000401.D
 Acq On : 15 Mar 2018 06:44
 Operator : JU/SJ
 Sample : J1845-20
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DAMD6

Manual Integrations
 APPROVED

Sohil
 3/15/2018 7:03:40 PM

Quant Time: Mar 15 08:16:59 2018
 Quant Method : Z:\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN030918MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 15 07:55:46 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.45	152	237140	20.00	ng/ul	0.00
2) Naphthalene-d8	11.29	136	1154233	20.00	ng/ul	0.00
6) Acenaphthene-d10	15.06	164	651923	20.00	ng/ul	0.00
12) Phenanthrene-d10	17.79	188	1422242	20.00	ng/ul	0.00
17) Chrysene-d12	21.90	240	1237737	20.00	ng/ul	0.00
22) Perylene-d12	24.40	264	1127165	20.00	ng/ul	0.00
System Monitoring Compounds						
7) Acenaphthylene-d8	14.76	160	1447043	22.36	ng/ul	0.00
10) Fluorene-d10	16.05	176	954129	21.78	ng/ul	0.00
14) Anthracene-d10	17.89	188	1480158	22.27	ng/ul	0.00
18) Pyrene-d10	20.14	212	1542071	25.47	ng/ul	0.00
25) Benzo(a)pyrene-d12	24.23	264	1147180	22.29	ng/ul	0.00
Target Compounds				Qvalue		
3) Naphthalene	11.34	128	68635	1.127	ng/ul	98
9) Acenaphthene	15.13	153	83039	1.835	ng/ul	95
11) Fluorene	16.10	166	84944	1.702	ng/ul	96
13) Phenanthrene	17.83	178	1596365	19.572	ng/ul	99
15) Anthracene	17.92	178	354272	4.281	ng/ul	99
16) Fluoranthene	19.81	202	2008942	22.796	ng/ul#	93
19) Pyrene	20.17	202	1594741	20.407	ng/ul#	91
20) Benzo(a)anthracene	21.89	228	707090	9.189	ng/ul	97
21) Chrysene	21.95	228	680500	9.319	ng/ul	97
23) Benzo(b)fluoranthene	23.64	252	781373m	11.625	ng/ul	
24) Benzo(k)fluoranthene	23.68	252	261144m	4.151	ng/ul	
26) Benzo(a)pyrene	24.29	252	498313	7.790	ng/ul#	93
27) Indeno(1,2,3-cd)pyrene	26.96	276	322011	4.669	ng/ul#	86
28) Dibenzo(a,h)anthracene	26.96	278	83657	1.480	ng/ul#	75
29) Benzo(g,h,i)perylene	27.76	276	266166	4.622	ng/ul#	87

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA_N\DATA\BN031418\
Data File : BN000401.D
Acq On : 15 Mar 2018 06:44
Operator : JU/SJ
Sample : J1845-20
Misc :
ALS Vial : 36 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampled :
DAMD6

Manual Integrations
APPROVED

Sohil
3/15/2018 7:03:40 PM

Quant Time: Mar 15 08:16:59 2018
Quant Method : Z:\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN030918MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 15 07:55:46 2018
Response via : Initial Calibration

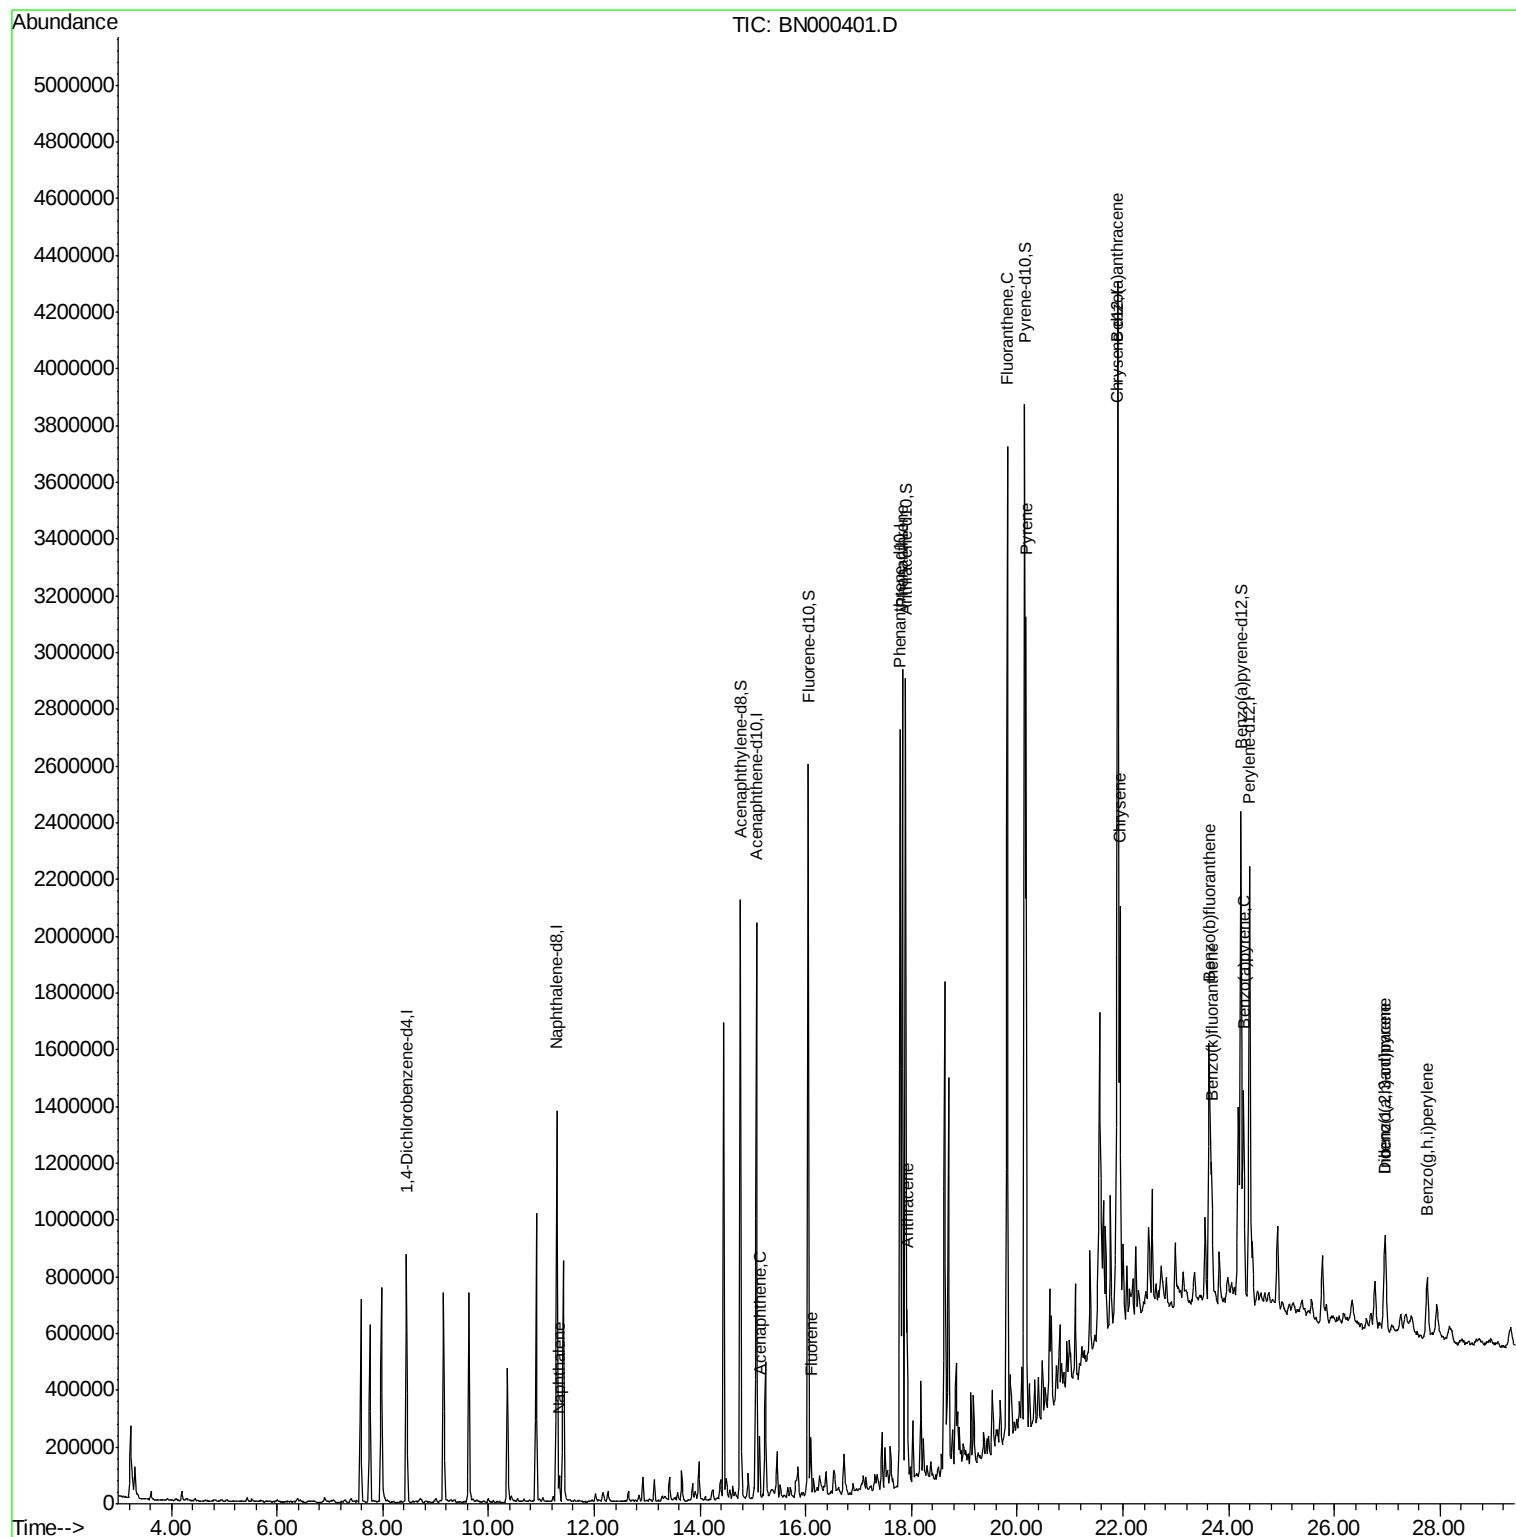



#3

Naphthalene

Concen: 1.127 ng/ul

RT: 11.34 min Scan# 1420

Delta R.T. -0.00 min

Lab File: BN000401.D

Acq: 15 Mar 2018 06:44

Instrument :

BNA_N





ClientSampled :

DAMD6

Tgt Ion:	128	Resp:	68635
Ion Ratio	Lower	Upper	
128	100		
129	11.7	8.7	13.1
127	12.8	10.6	16.0

Manual Integrations
APPROVED

Sohil
3/15/2018 7:03:40 PM

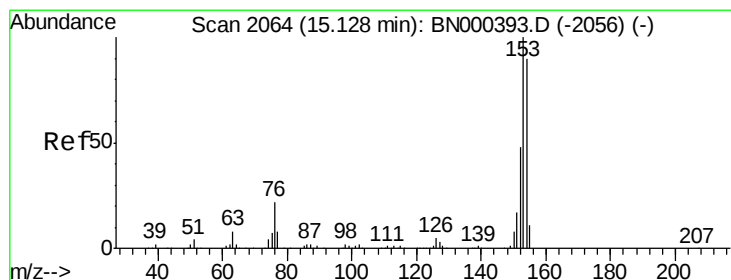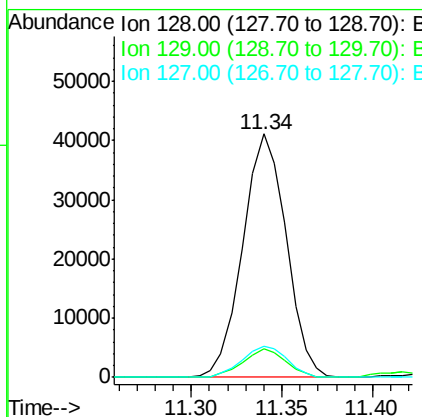

#9

Acenaphthene

Concen: 1.835 ng/ul




RT: 15.13 min Scan# 2064


Delta R.T. -0.00 min

Lab File: BN000401.D

Acq: 15 Mar 2018 06:44

Tgt Ion:	153	Resp:	83039
Ion Ratio	Lower	Upper	
153	100		
152	49.2	39.0	58.6
154	89.7	66.8	100.2

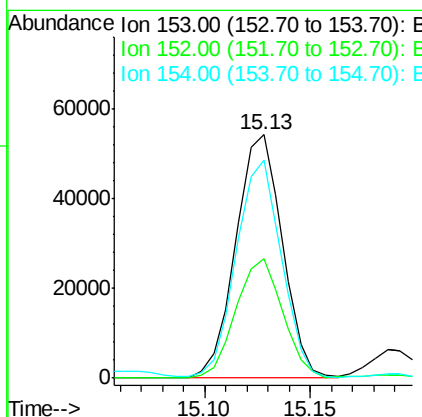




#11
 Fluorene
 Concen: 1.702 ng/ul
 RT: 16.10 min Scan# 2229
 Delta R.T. -0.00 min
 Lab File: BN000401.D
 Acq: 15 Mar 2018 06:44

Instrument :
 BNA_N
 ClientSampleId :
 DAMD6

Tgt Ion	Ratio	Lower	Upper
166	100		
165	100.0	83.8	125.8
167	15.0	11.5	17.3

Manual Integrations
 APPROVED

Sohil
 3/15/2018 7:03:40 PM



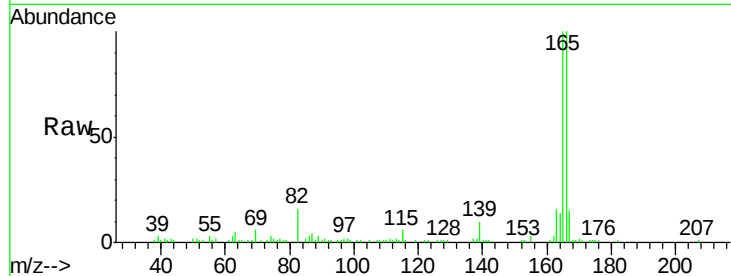


Abundance

Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

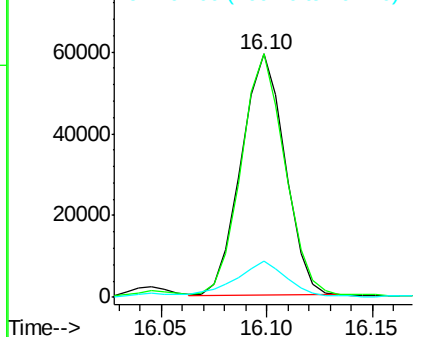

#13
 Phenanthrene
 Concen: 19.572 ng/ul
 RT: 17.83 min Scan# 2523
 Delta R.T. -0.00 min
 Lab File: BN000401.D
 Acq: 15 Mar 2018 06:44




Tgt Ion	Ratio	Lower	Upper
178	100		
179	15.7	12.3	18.5
176	19.3	15.1	22.7


Abundance

Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

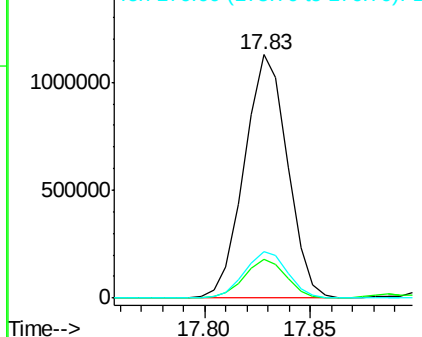







#15
 Anthracene
 Concen: 4.281 ng/ul
 RT: 17.92 min Scan# 2538
 Delta R.T. -0.00 min
 Lab File: BN000401.D
 Acq: 15 Mar 2018 06:44

Instrument :
 BNA_N
 ClientSampleId :
 DAMD6

Tgt Ion	Ratio	Lower	Upper
178	100		
179	15.7	11.8	17.8
176	18.7	15.2	22.8




Manual Integrations
 APPROVED


Sohil
 3/15/2018 7:03:40 PM

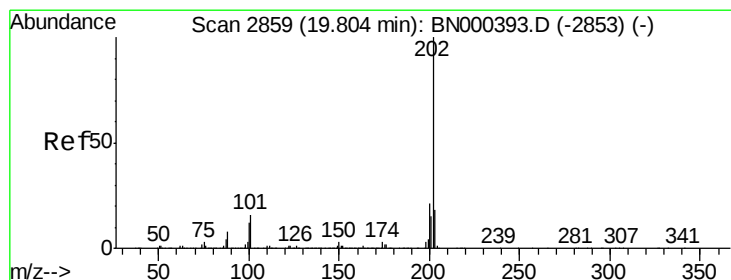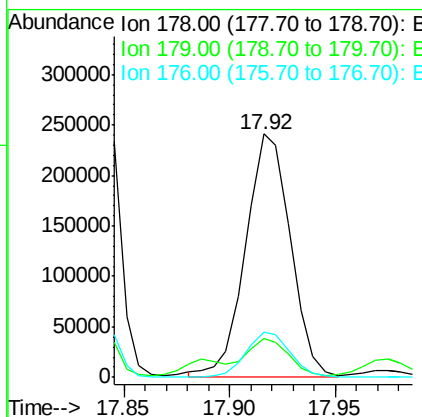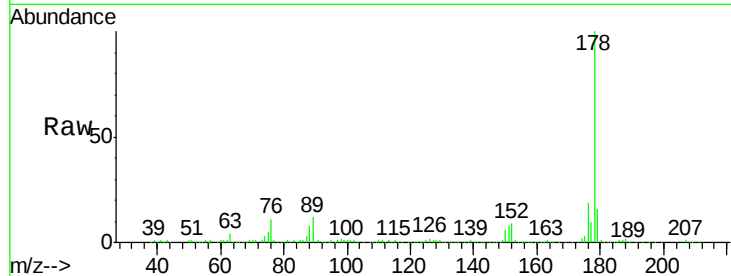

#16
 Fluoranthene
 Concen: 22.796 ng/ul
 RT: 19.81 min Scan# 2860
 Delta R.T. 0.01 min
 Lab File: BN000401.D
 Acq: 15 Mar 2018 06:44

Tgt Ion	Ratio	Lower	Upper
202	100		
101	15.3	9.9	14.9#
100	11.3	7.4	11.0#

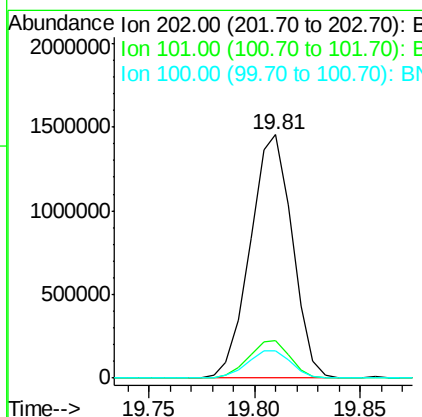







#19
Pyrene
Concen: 20.407 ng/ul
RT: 20.17 min Scan# 2921
Delta R.T. 0.01 min
Lab File: BN000401.D
Acq: 15 Mar 2018 06:44

Instrument :
BNA_N
ClientSampleId :
DAMD6

Tgt Ion	Ratio	Lower	Upper
202	100		
101	17.1	11.0	16.4#
100	13.9	8.1	12.1#




Manual Integrations
APPROVED


Sohil
3/15/2018 7:03:40 PM

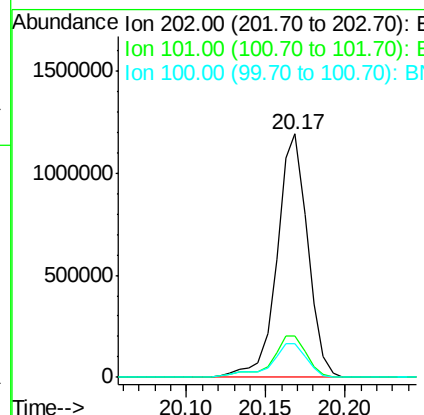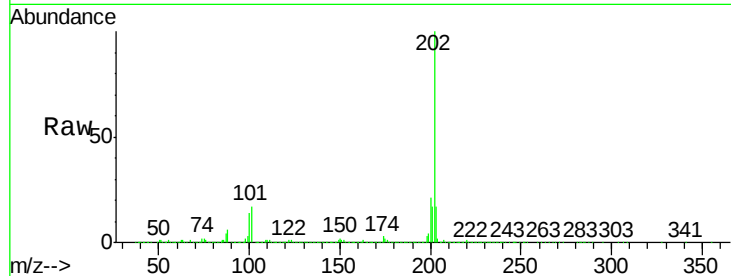

#20
Benzo(a)anthracene
Concen: 9.189 ng/ul
RT: 21.89 min Scan# 3214
Delta R.T. 0.01 min
Lab File: BN000401.D
Acq: 15 Mar 2018 06:44

Tgt Ion	Ratio	Lower	Upper
228	100		
229	21.2	15.7	23.5
226	27.6	21.1	31.7

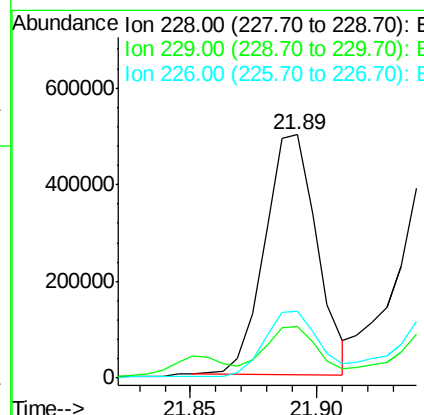



#21

Chrysene

Concen: 9.319 ng/ul

RT: 21.95 min Scan# 3223

Delta R.T. -0.00 min

Lab File: BN000401.D

Acq: 15 Mar 2018 06:44

Instrument :

BNA_N





ClientSampleId :

DAMD6

Tgt Ion:	228	Resp:	680500
Ion Ratio		Lower	Upper
228	100		
226	30.3	24.5	36.7
229	22.5	15.8	23.8

Manual Integrations
APPROVED

Sohil
3/15/2018 7:03:40 PM

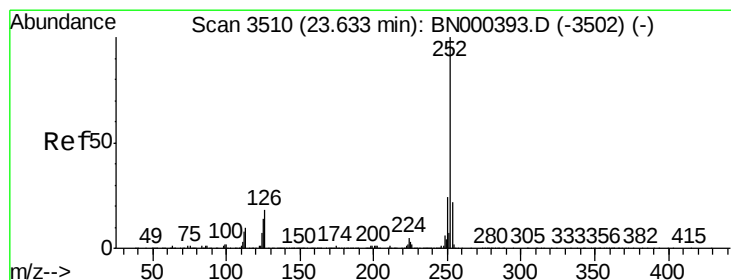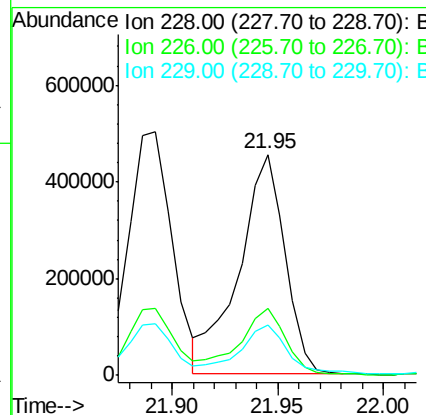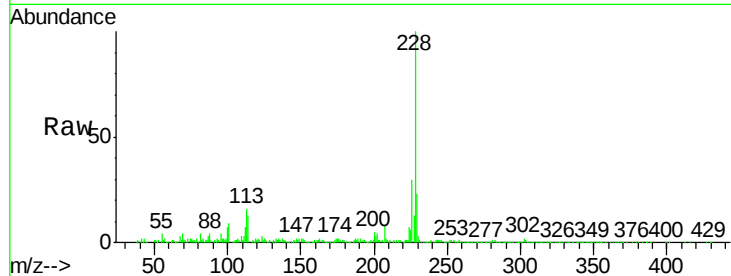

#23

Benzo(b)fluoranthene

Concen: 11.625 ng/ul m




RT: 23.64 min Scan# 3511


Delta R.T. 0.01 min

Lab File: BN000401.D

Acq: 15 Mar 2018 06:44

Tgt Ion:	252	Resp:	781373
Ion Ratio		Lower	Upper
252	100		
253	22.4	18.0	27.0
125	14.9	8.0	12.0#

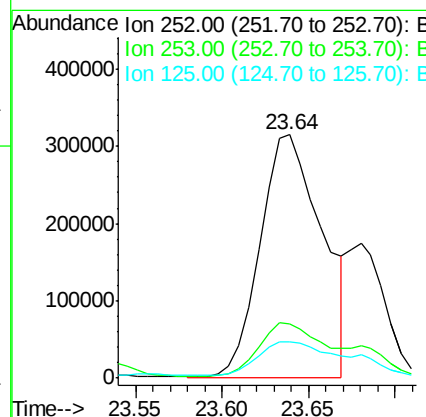







#24
Benzo(k)fluoranthene
Concen: 4.151 ng/ul m
RT: 23.68 min Scan# 3518
Delta R.T. -0.00 min
Lab File: BN000401.D
Acq: 15 Mar 2018 06:44

Instrument :
BNA_N
ClientSampleId :
DAMD6

Tgt Ion	Ratio	Lower	Upper
252	100		
253	23.7	18.0	27.0
125	17.0	8.1	12.1#




Manual Integrations
APPROVED


Sohil
3/15/2018 7:03:40 PM

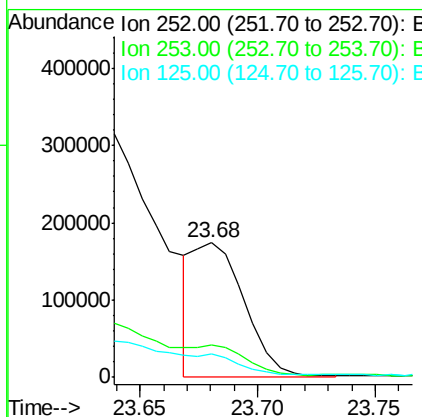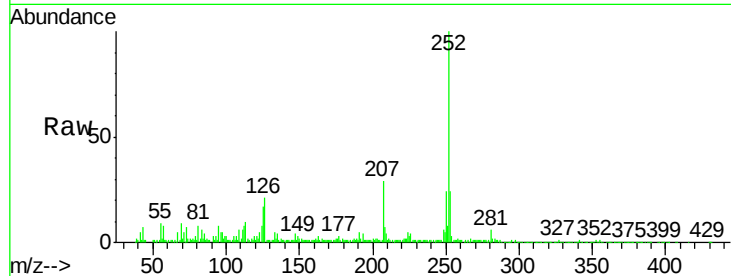

#26
Benzo(a)pyrene
Concen: 7.790 ng/ul
RT: 24.29 min Scan# 3621
Delta R.T. 0.01 min
Lab File: BN000401.D
Acq: 15 Mar 2018 06:44

Tgt Ion	Ratio	Lower	Upper
252	100		
253	23.0	17.2	25.8
125	16.3	8.2	12.4#

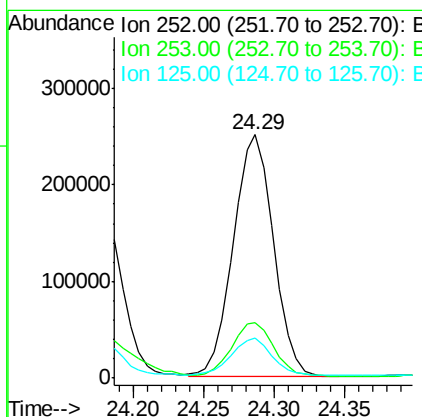



#27

Indeno(1,2,3-cd)pyrene

Concen: 4.669 ng/ul

RT: 26.96 min Scan# 4076

Delta R.T. -0.00 min

Lab File: BN000401.D





Acq: 15 Mar 2018 06:44

Instrument :
BNA_N
ClientSampled :
DAMD6

Tgt Ion	Ratio	Lower	Upper
276	100		
138	28.7	14.4	21.6#
277	25.1	18.0	27.0

Manual Integrations
APPROVED

Sohil
3/15/2018 7:03:40 PM

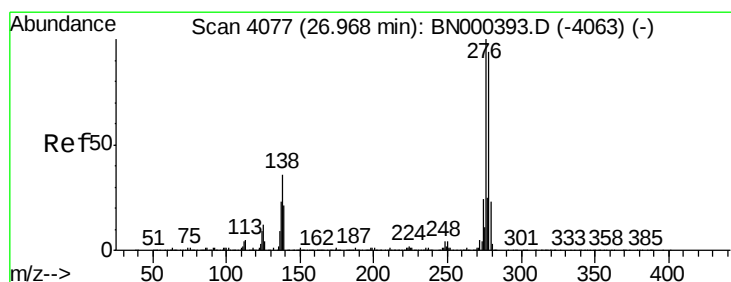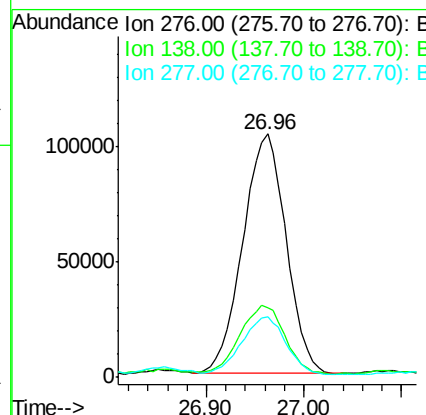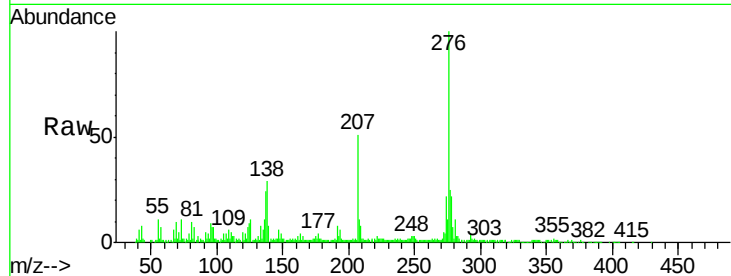

#28

Dibenzo(a,h)anthracene

Concen: 1.480 ng/ul




RT: 26.96 min Scan# 4076


Delta R.T. -0.01 min

Lab File: BN000401.D

Acq: 15 Mar 2018 06:44

Tgt Ion	Ratio	Lower	Upper
278	100		
139	34.3	12.2	18.4#
279	29.9	19.2	28.8#

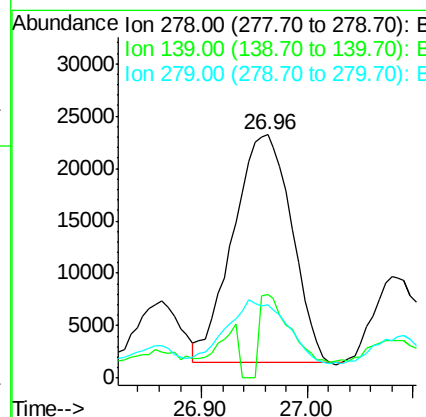



#29

Benzo(g,h,i)perylene

Concen: 4.622 ng/ul

RT: 27.76 min Scan# 4211

Delta R.T. -0.00 min

Lab File: BN000401.D


Acq: 15 Mar 2018 06:44

Instrument :

BNA_N

ClientSampleId :

DAMD6



Tgt	Ion	276	Resp:	266166
Ion	Ratio	100	Lower	Upper
138	30.5	15.3	22.9#	
277	24.9	19.0	28.4	

Manual Integrations
APPROVED

Sohil
3/15/2018 7:03:40 PM

