
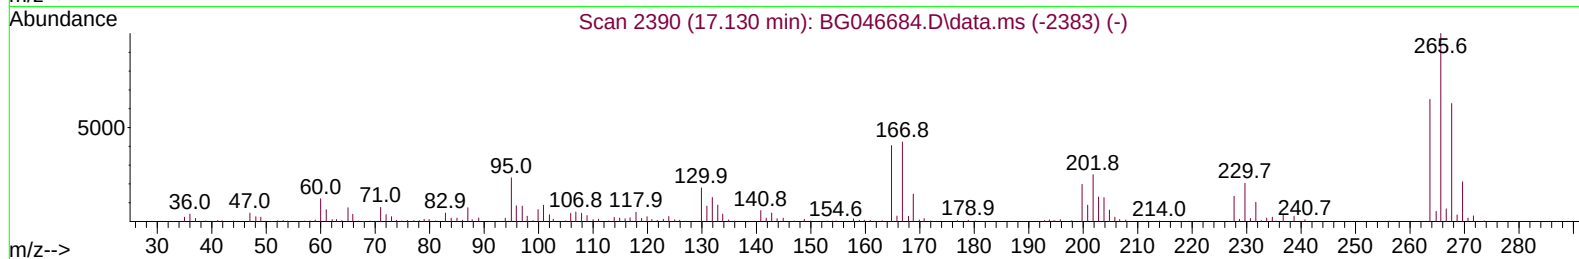
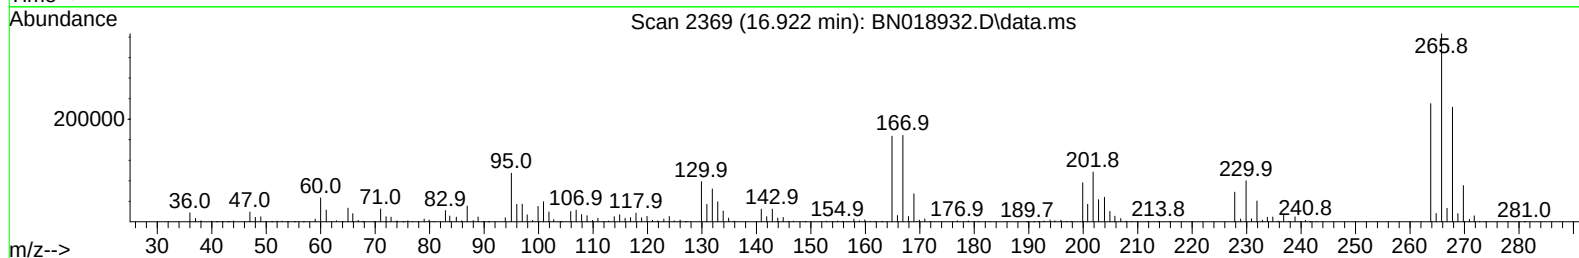


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031422\
Data File : BN018932.D
Acq On : 14 Mar 2022 12:22
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 14 15:12:09 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 14 15:11:57 2022
Response via : Initial Calibration

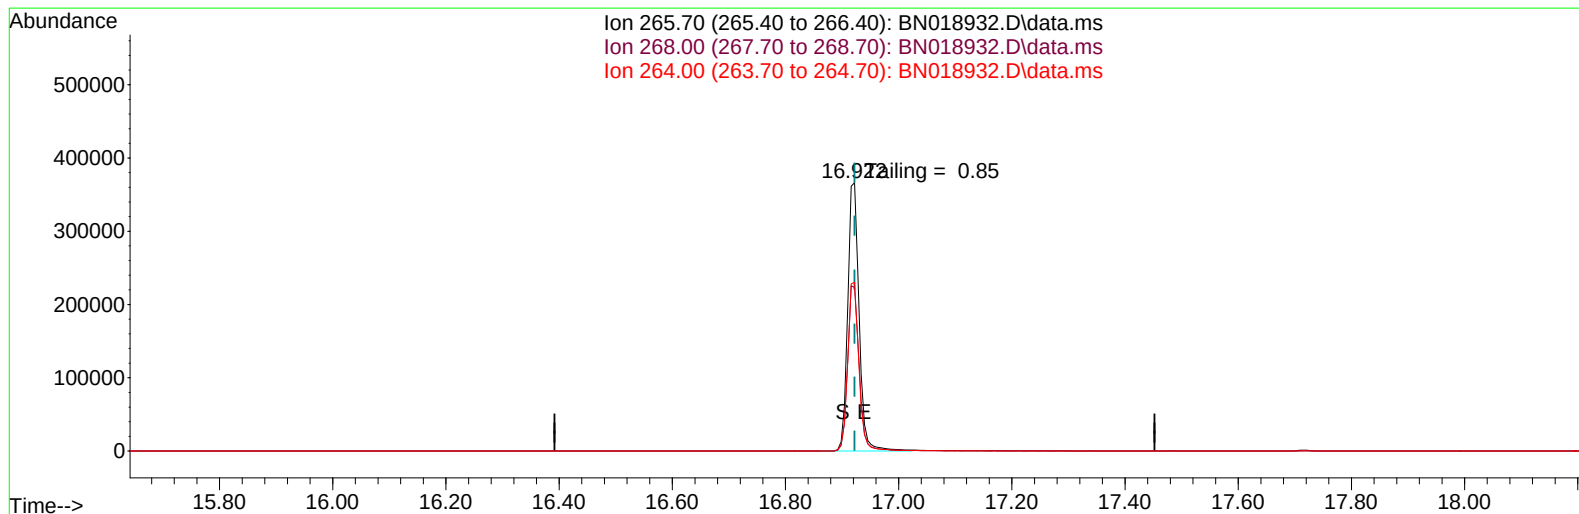

TIC: BN018932.D\data.ms

(70) Pentachlorophenol (C)




16.922min (0.000) 20473.02 ng

response 515902

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	60.93
264.00	61.60	62.83
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031422\
Data File : BN018932.D
Acq On : 14 Mar 2022 12:22
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 14 15:12:09 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 14 15:11:57 2022
Response via : Initial Calibration

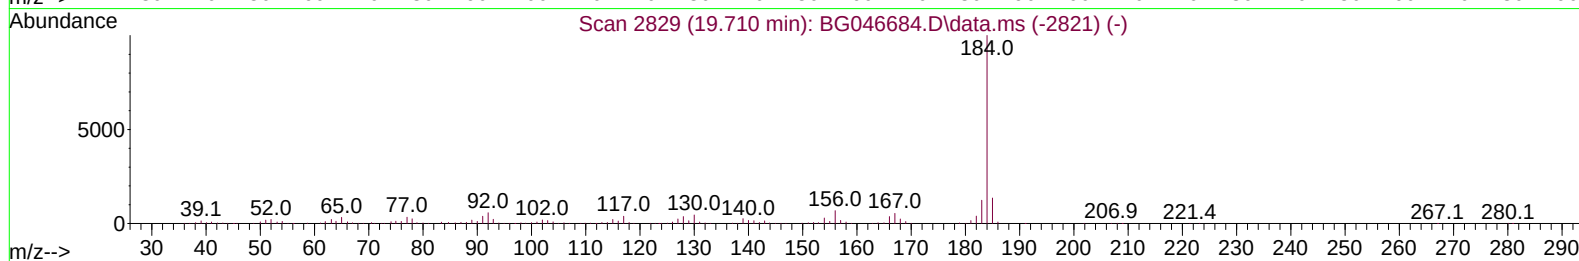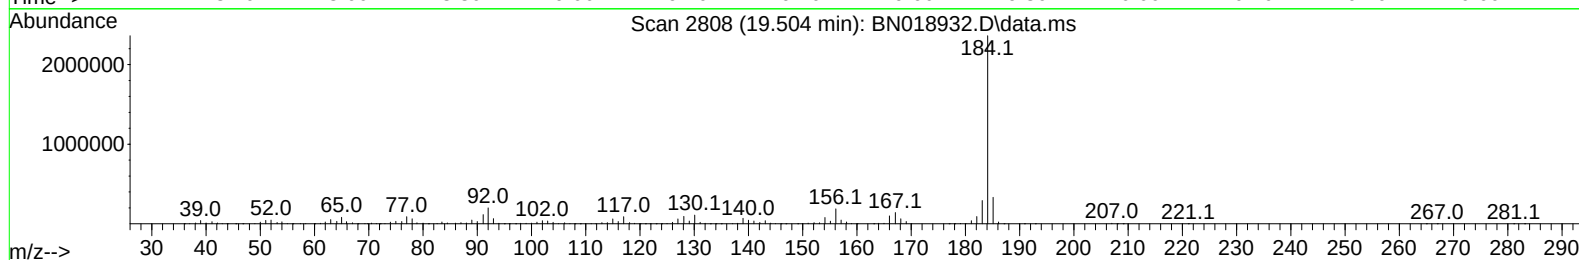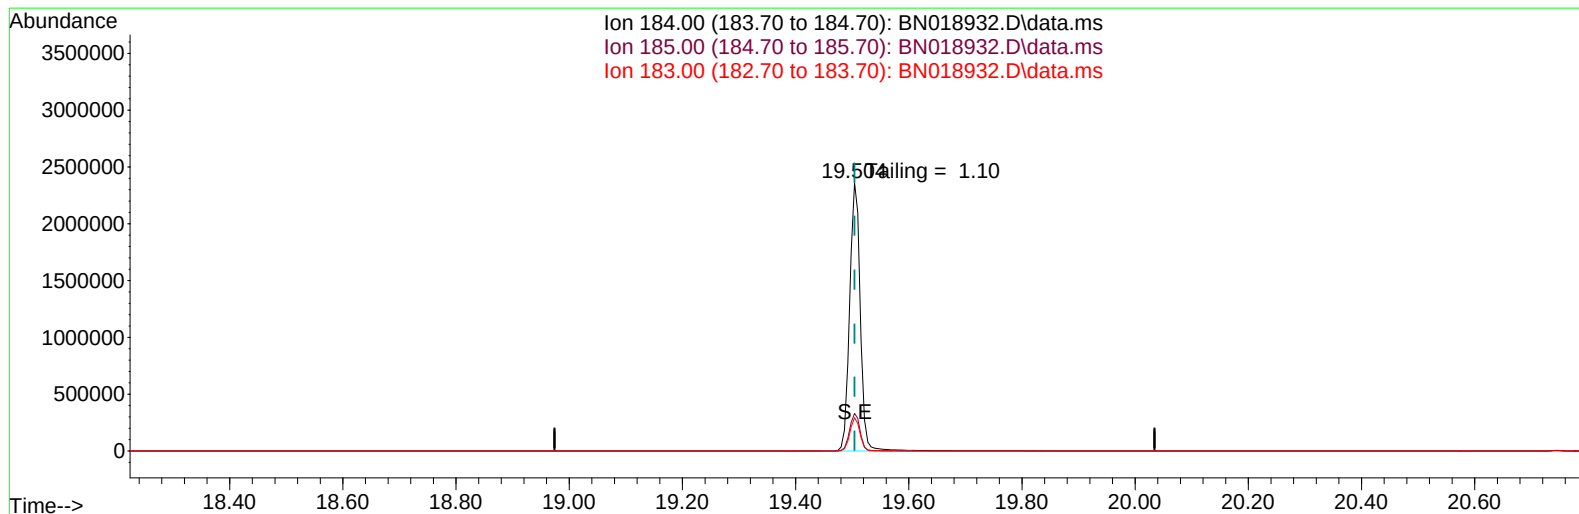

TIC: BN018932.D\data.ms

(77) Benzidine

19.504min (0.000) 0.00 ng

response 3094564

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.04
183.00	13.20	12.39
0.00	0.00	0.00