
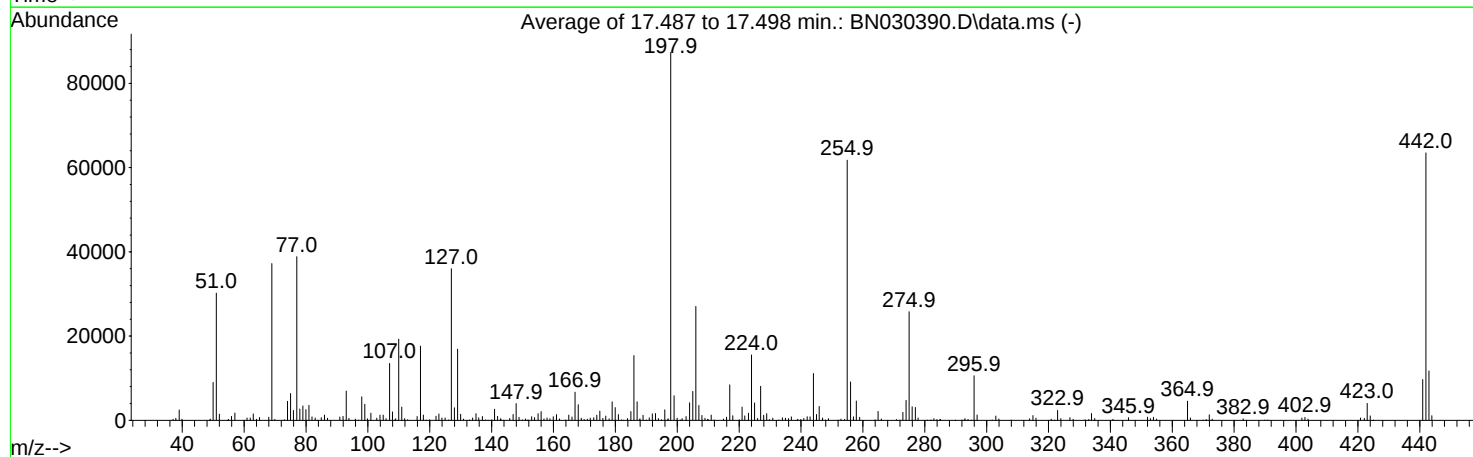


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031424\
Data File : BN030390.D
Acq On : 14 Mar 2024 10:32
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN031324.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Mar 14 11:36:29 2024

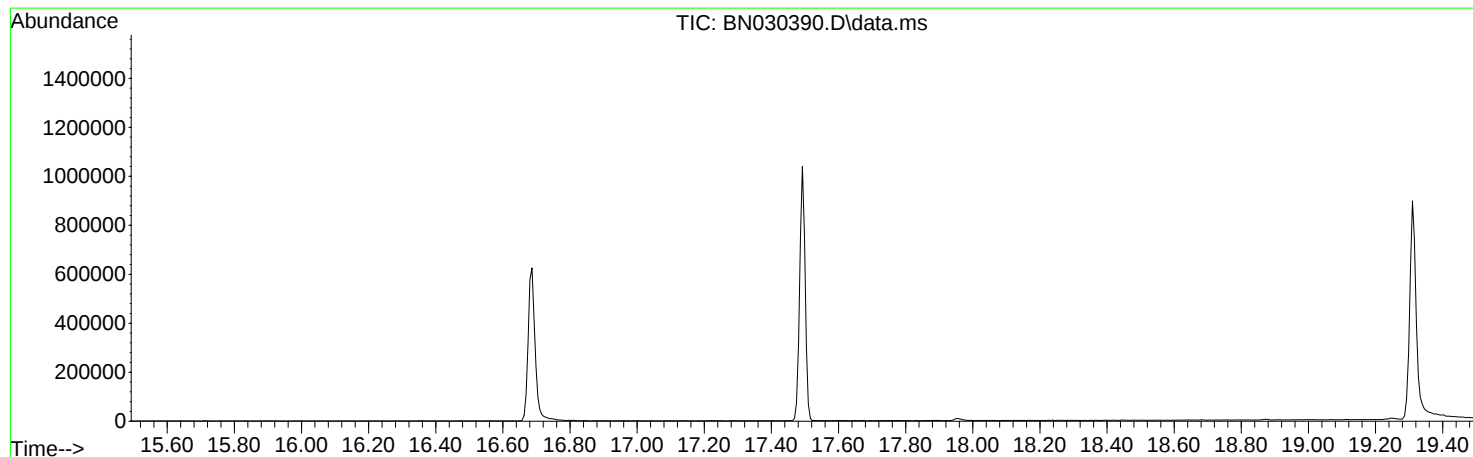




AutoFind: Scans 2448, 2449, 2450; Background Corrected with Scan 2442

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.6	30219	PASS
68	69	0.00	2	2.0	763	PASS
69	198	0.00	100	42.6	37229	PASS
70	69	0.00	2	0.6	226	PASS
127	198	10	80	41.2	36016	PASS
197	198	0.00	2	0.5	403	PASS
198	198	100	100	100.0	87328	PASS
199	198	5	9	6.7	5869	PASS
275	198	10	60	29.5	25805	PASS
365	198	1	100	5.2	4556	PASS
441	198	0.01	100	11.1	9699	PASS
442	442	50	100	100.0	63507	PASS
443	442	15	24	18.5	11736	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031424\
Data File : BN030390.D
Acq On : 14 Mar 2024 10:32
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 15 00:31:52 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 15 00:31:48 2024
Response via : Initial Calibration

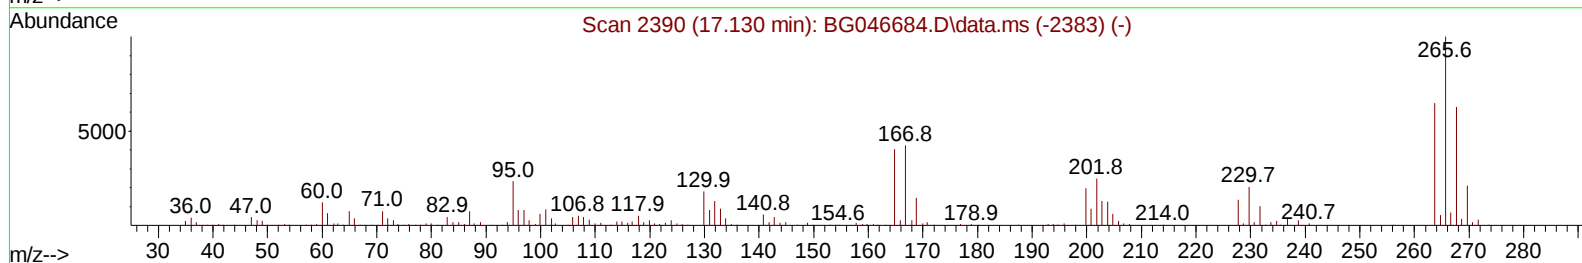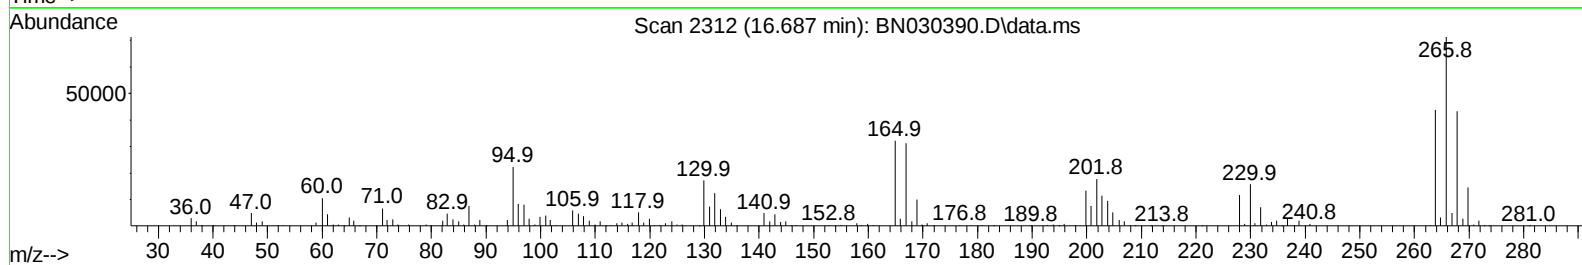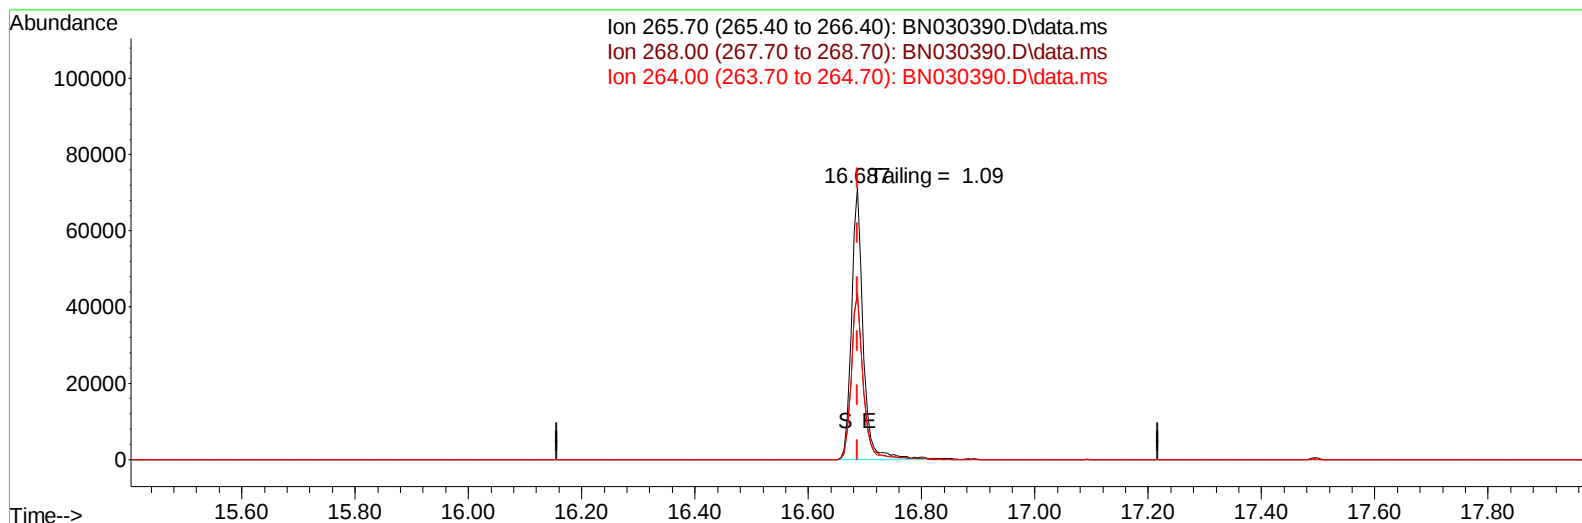

TIC: BN030390.D\data.ms

(70) Pentachlorophenol (C)

16.687min (0.000) 18203.02 ng




response 101854

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	60.62
264.00	61.60	61.51
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031424\
Data File : BN030390.D
Acq On : 14 Mar 2024 10:32
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 15 00:31:52 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 15 00:31:48 2024
Response via : Initial Calibration

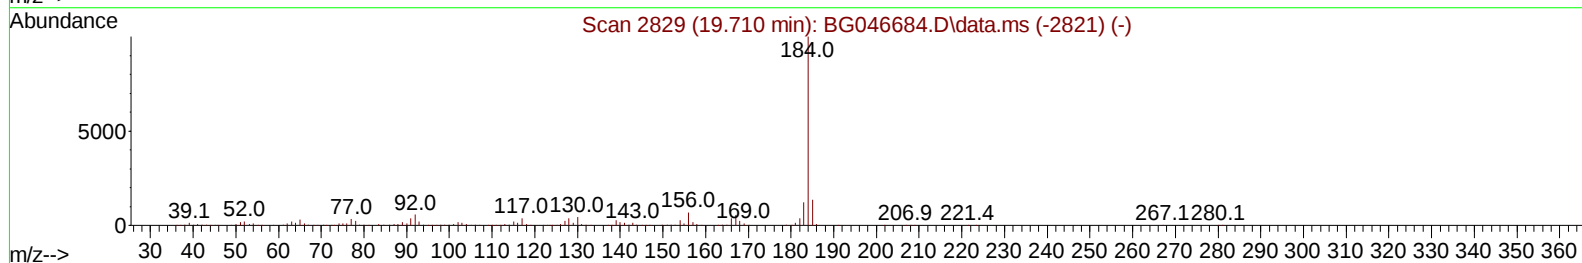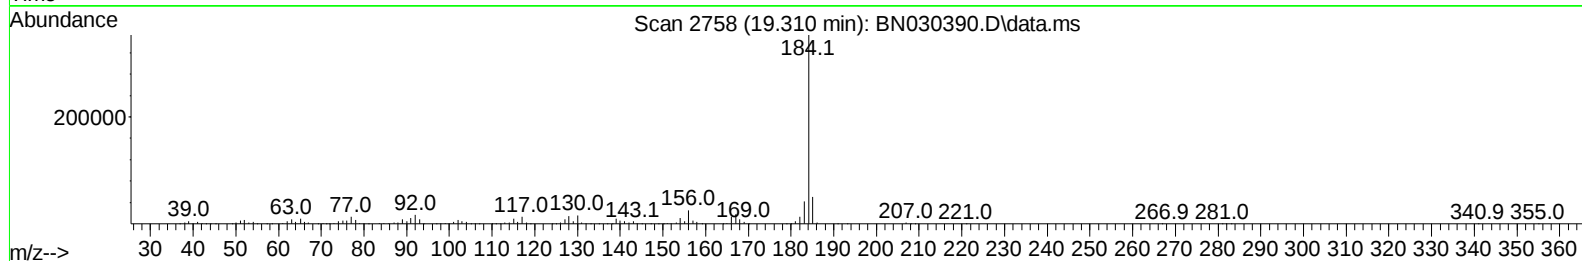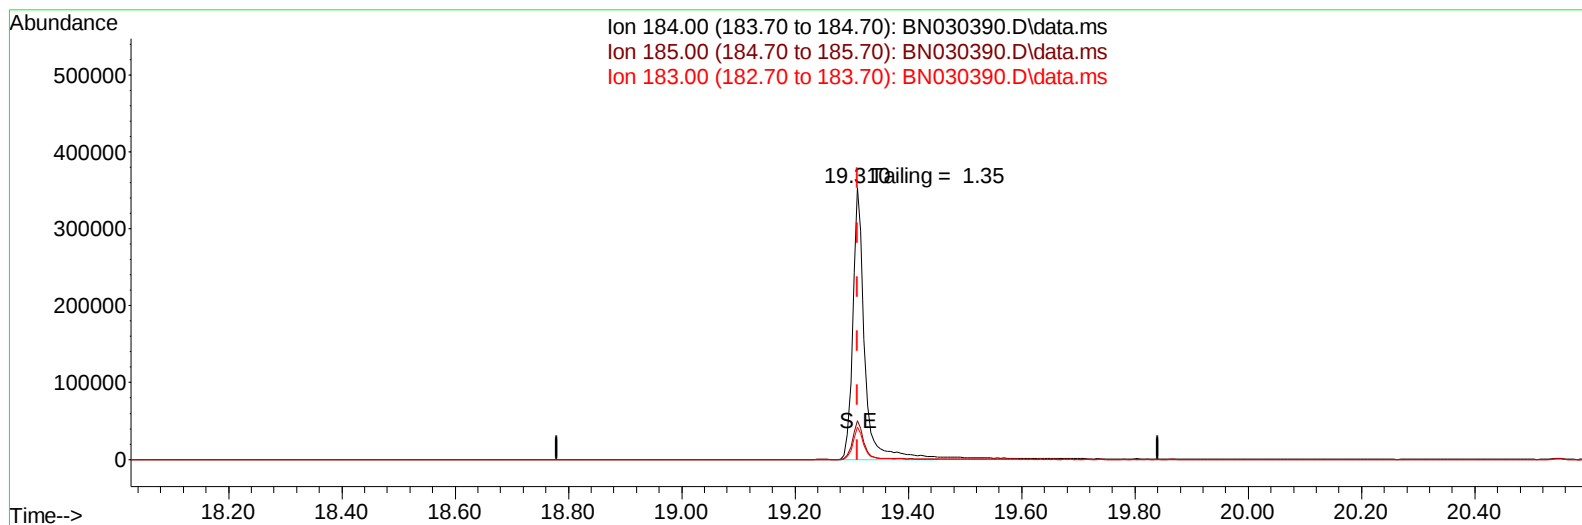

TIC: BN030390.D\data.ms

(77) Benzidine

19.310min (0.000) 0.00 ng

response 516687

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.23
183.00	13.20	11.91
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/14/2024	BNA_N	<u>BN030390.D</u>
Compound Name	Response	Retention Time
DDT	312058	20.551
DDD	6829	20.11
DDE	186	19.592
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7015	319073	2.20

Instrument :
BNA_N
ClientSampleId :
DFTPP