
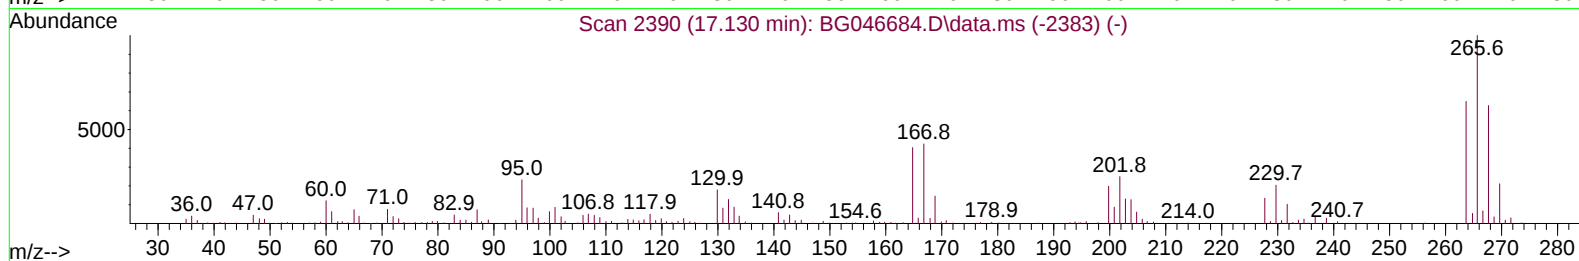
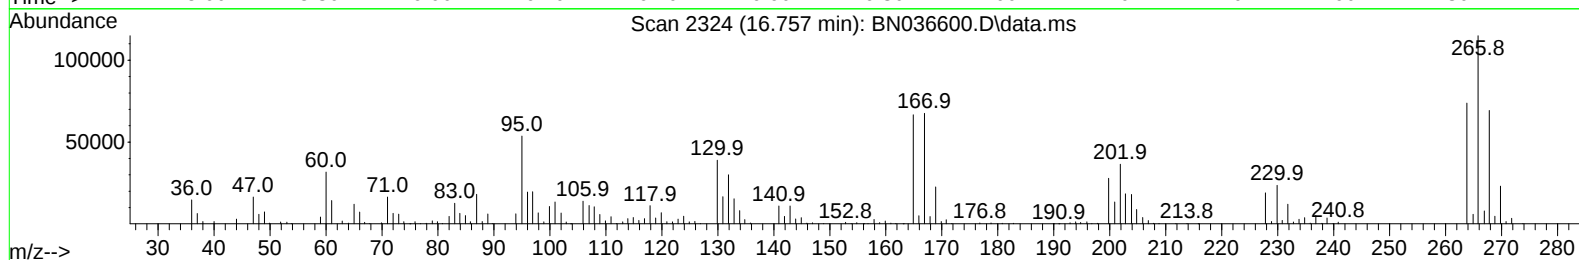


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031425\
Data File : BN036600.D
Acq On : 14 Mar 2025 09:30
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 15 00:26:41 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 15 00:26:30 2025
Response via : Initial Calibration

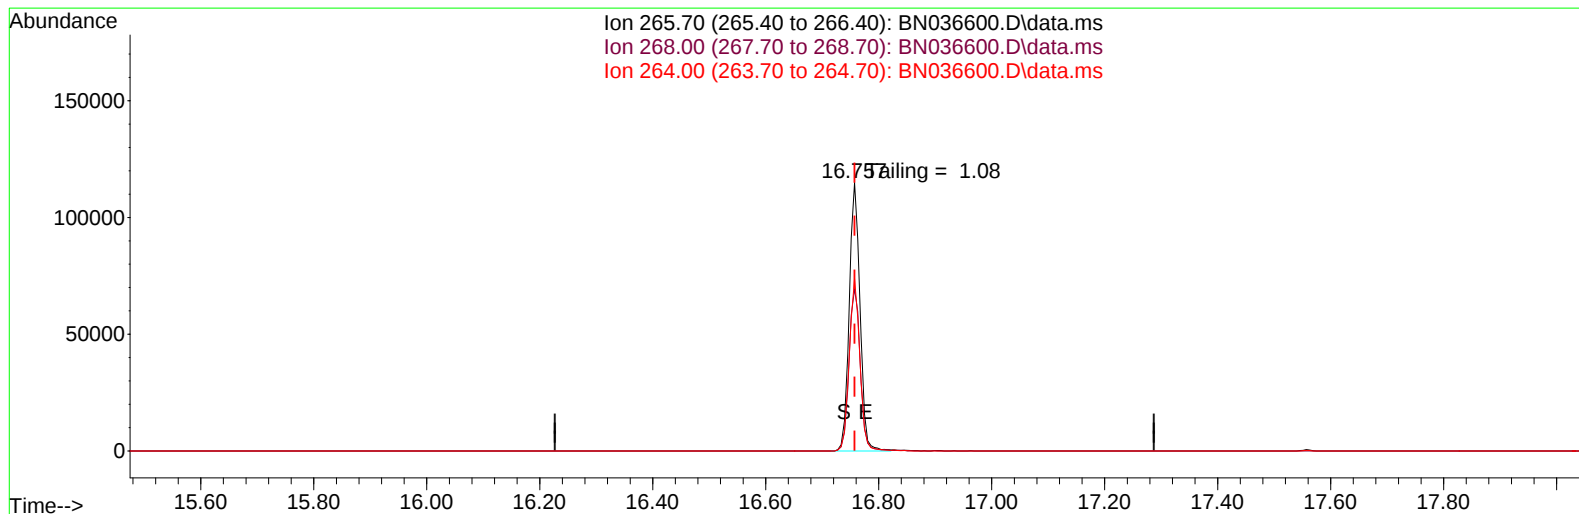

TIC: BN036600.D\data.ms

(70) Pentachlorophenol (C)




16.757min (0.000) 18451.01 ng

response 152618

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	60.30
264.00	61.60	64.18
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031425\
Data File : BN036600.D
Acq On : 14 Mar 2025 09:30
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 15 00:26:41 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 15 00:26:30 2025
Response via : Initial Calibration

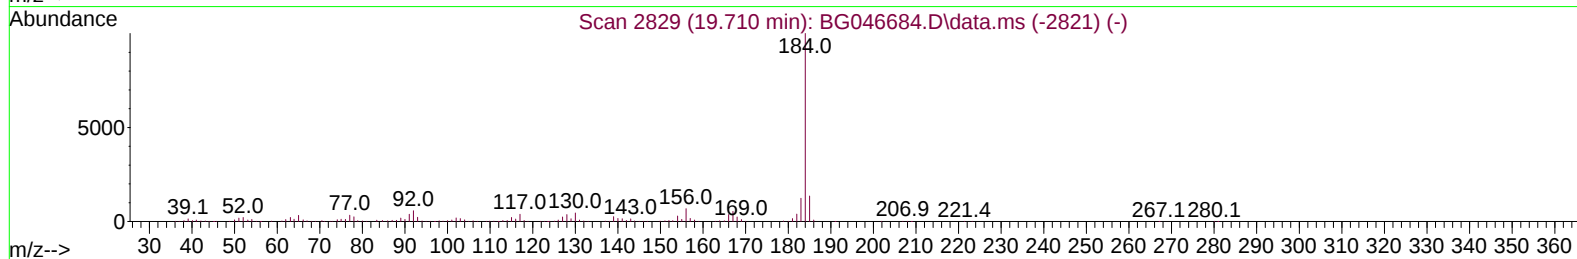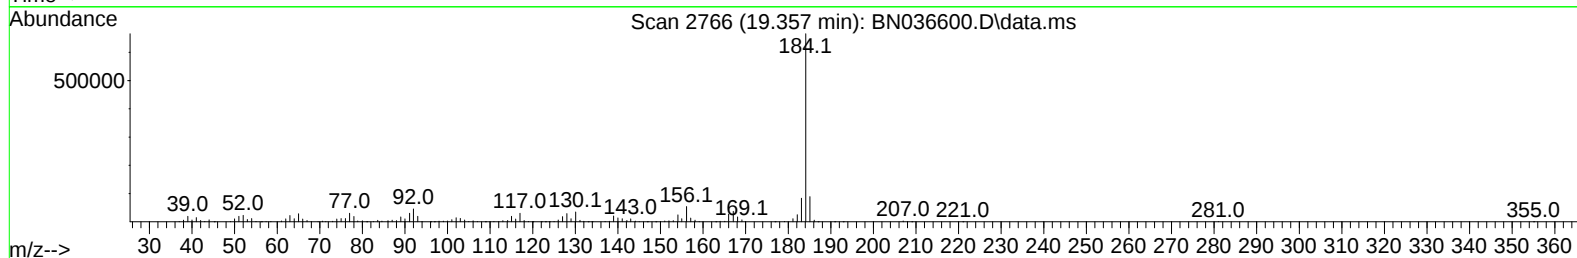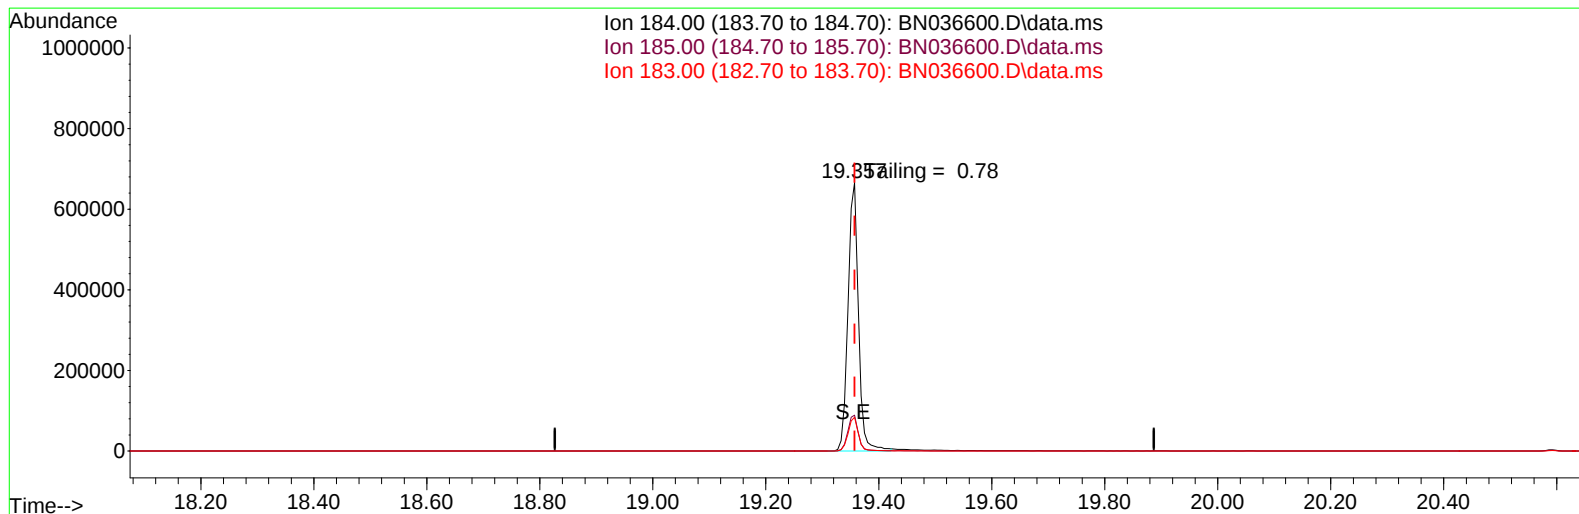

TIC: BN036600.D\data.ms

(77) Benzidine

19.357min (0.000) 0.00 ng

response 868744

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.38
183.00	13.20	12.57
0.00	0.00	0.00