
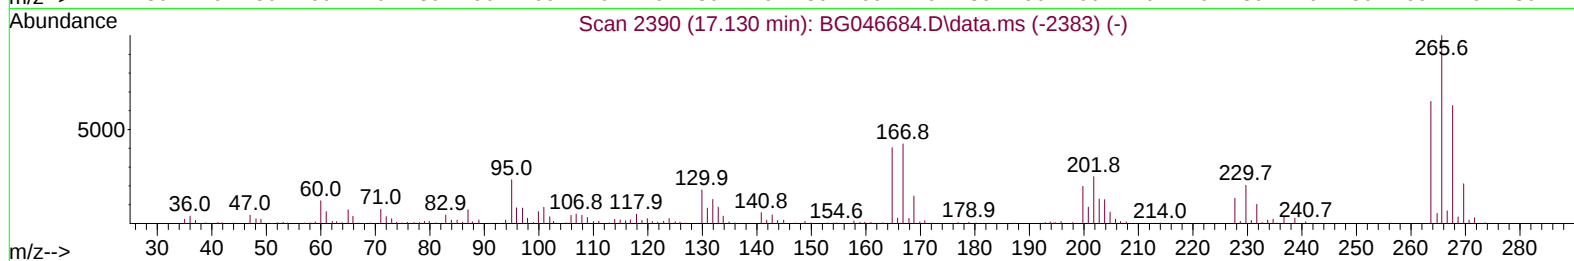
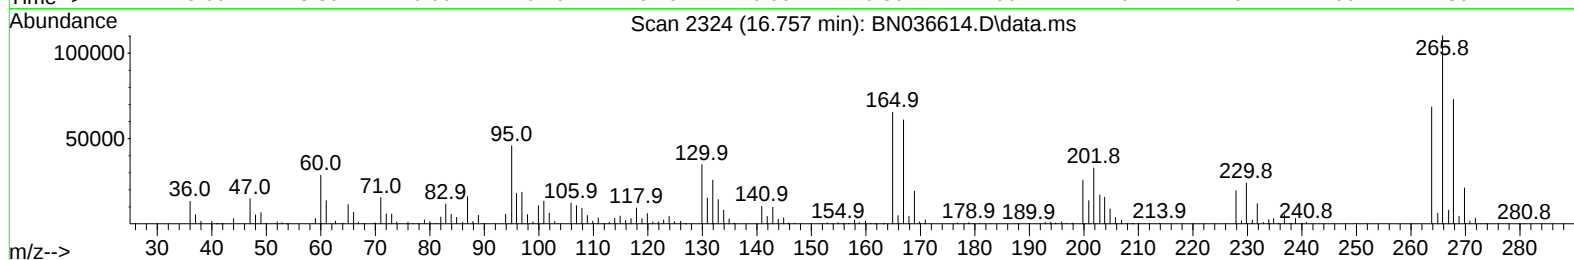


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031425\
Data File : BN036614.D
Acq On : 14 Mar 2025 19:51
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 8 Sample Multiplier: 1

Quant Time: Mar 15 00:28:19 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 15 00:26:30 2025
Response via : Initial Calibration

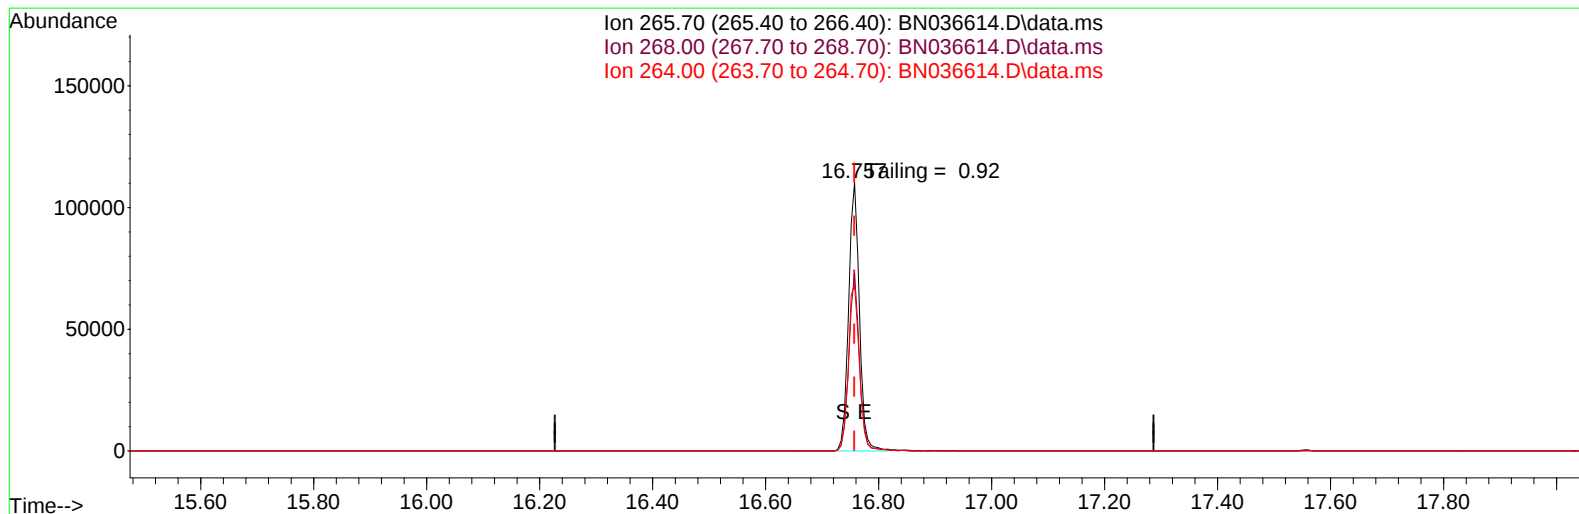

TIC: BN036614.D\data.ms

(70) Pentachlorophenol (C)




16.757min (+ 0.000) 16591.40 ng

response 147262

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	66.06
264.00	61.60	62.07
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031425\
Data File : BN036614.D
Acq On : 14 Mar 2025 19:51
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 8 Sample Multiplier: 1

Quant Time: Mar 15 00:28:19 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 15 00:26:30 2025
Response via : Initial Calibration

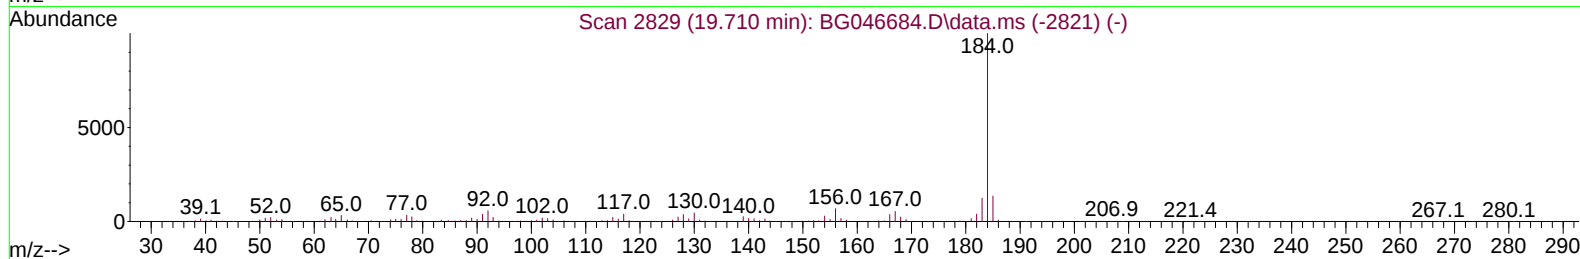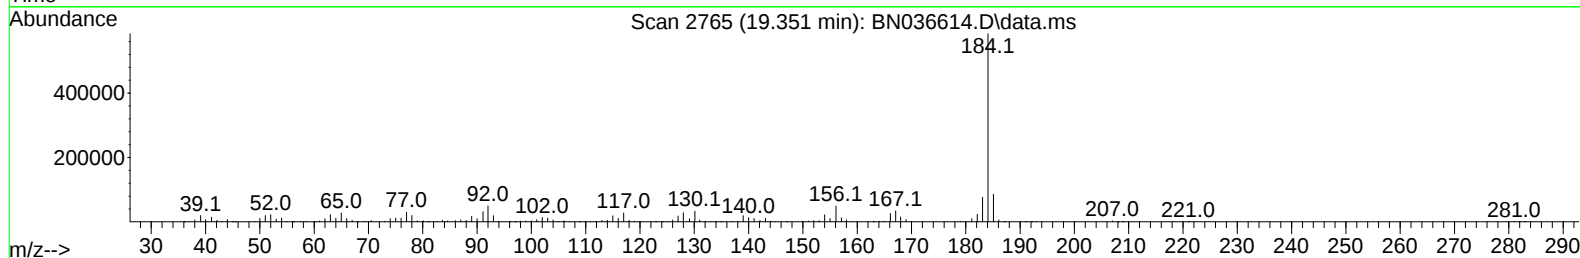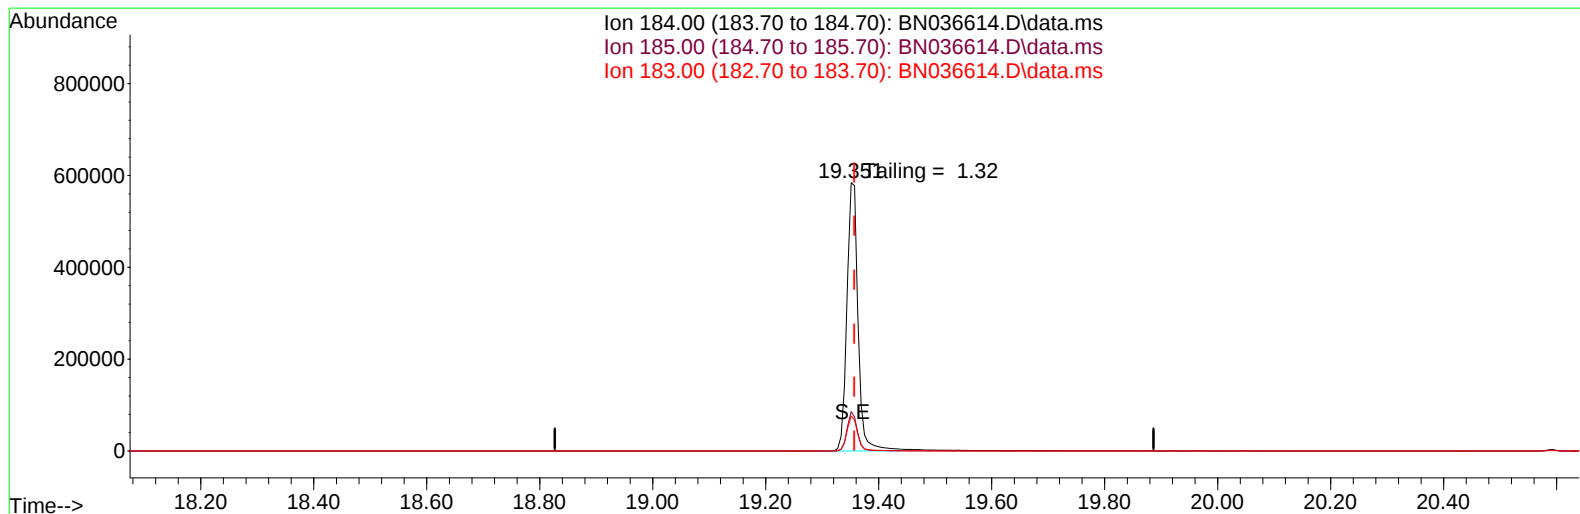

TIC: BN036614.D\data.ms

(77) Benzidine

19.351min (-0.006) 0.00 ng

response 817261

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.66
183.00	13.20	13.06
0.00	0.00	0.00