
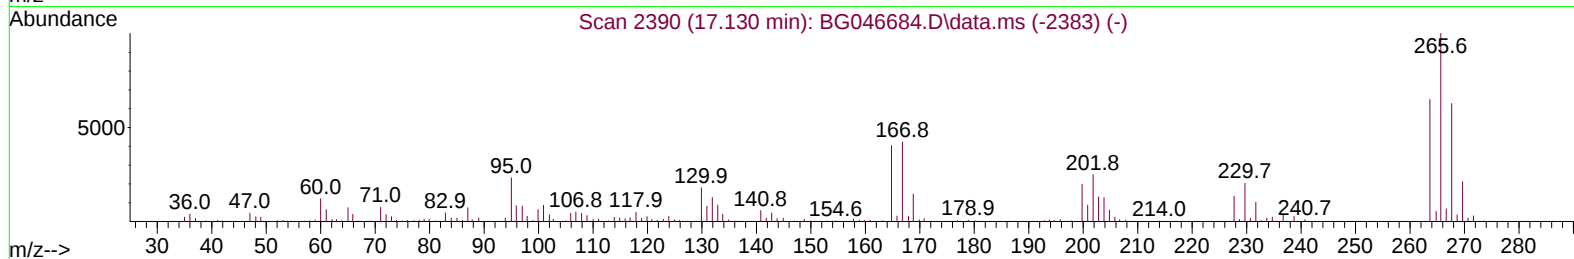
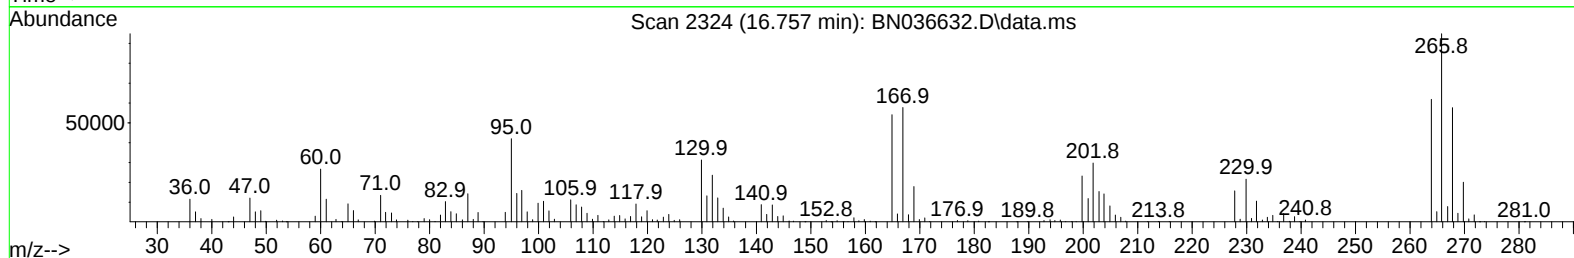


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031425\
Data File : BN036632.D
Acq On : 15 Mar 2025 06:41
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 26 Sample Multiplier: 1

Quant Time: Mar 17 01:20:19 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 17 01:20:13 2025
Response via : Initial Calibration

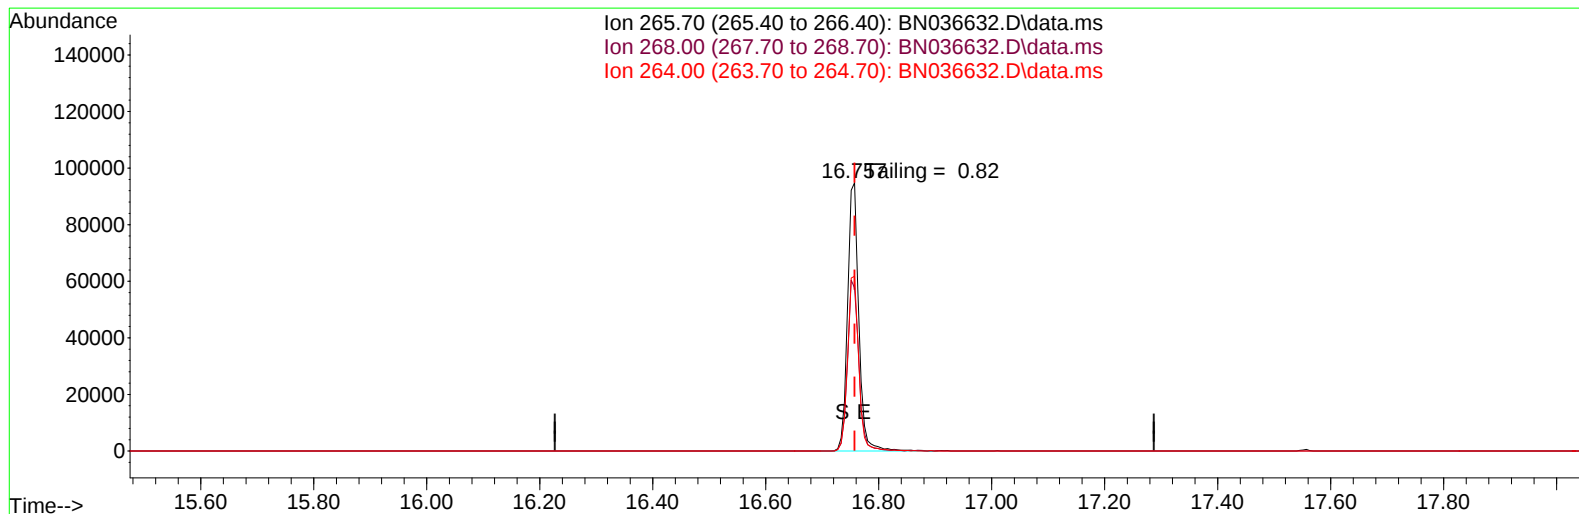

TIC: BN036632.D\data.ms

(70) Pentachlorophenol (C)




16.757min (0.000) 18589.43 ng

response 130859

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	60.74
264.00	61.60	65.13
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031425\
Data File : BN036632.D
Acq On : 15 Mar 2025 06:41
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 26 Sample Multiplier: 1

Quant Time: Mar 17 01:20:19 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 17 01:20:13 2025
Response via : Initial Calibration

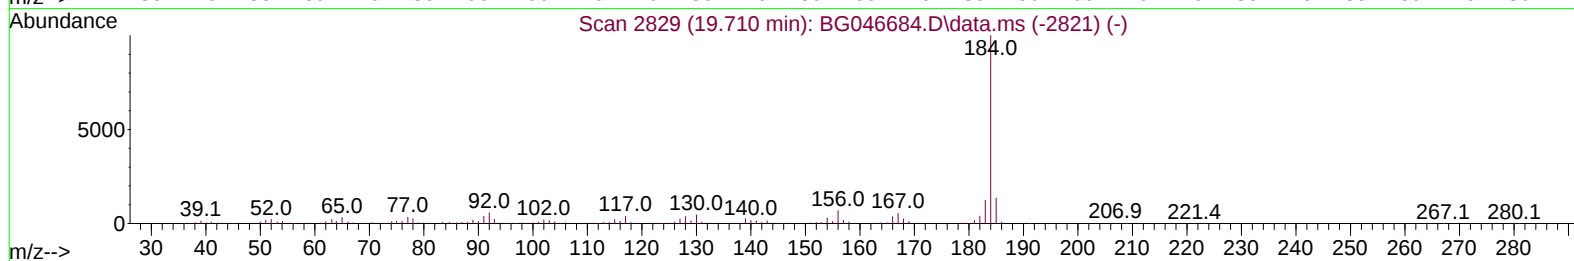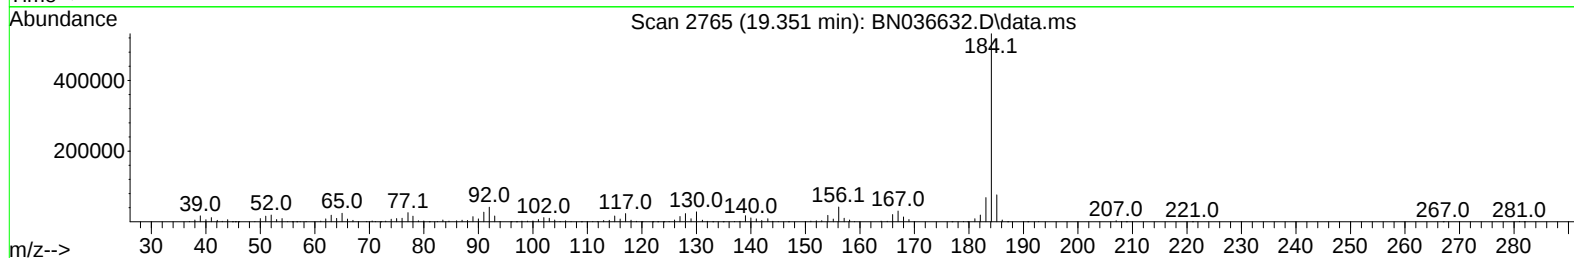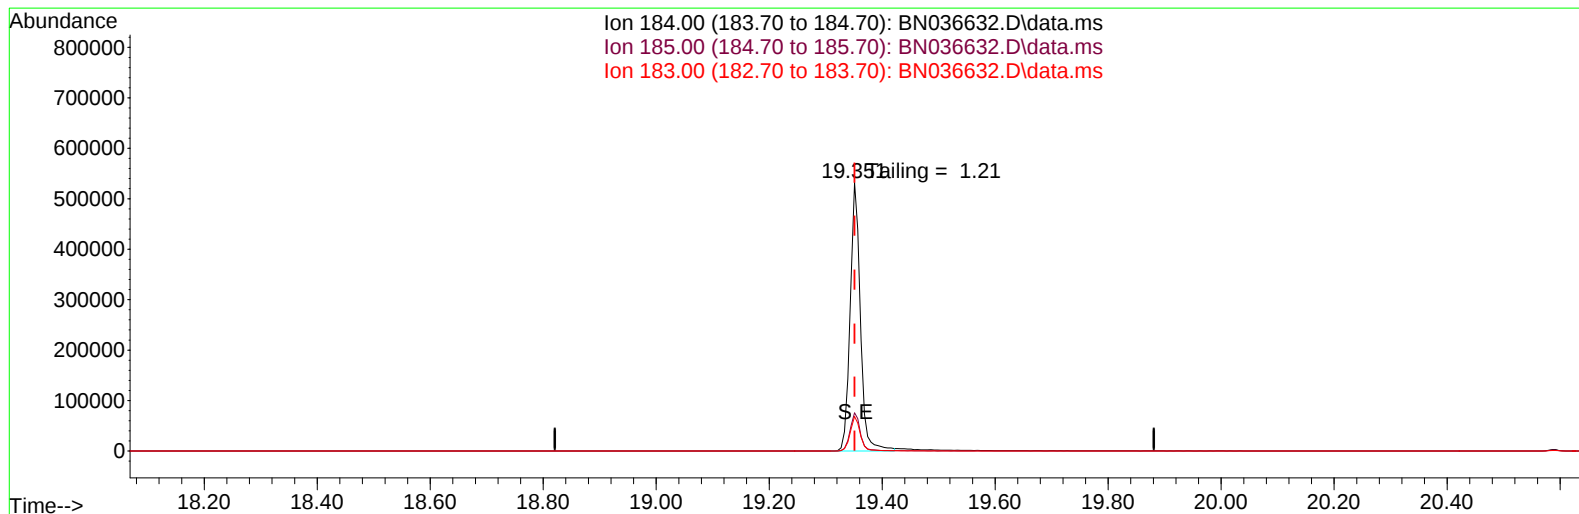

TIC: BN036632.D\data.ms

(77) Benzidine

19.351min (0.000) 0.00 ng

response 681752

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.29
183.00	13.20	12.92
0.00	0.00	0.00