

Data Path : Z:\HPCHEM1\BNA N\DATA\BN031518\
 Data File : BN000419.D
 Acq On : 15 Mar 2018 17:10
 Operator : JU/SJ
 Sample : J1865-14
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Mar 16 06:48:05 2018
 Quant Method : Z:\HPCHEM1\BNA N\METHODS\SOM-EPA-BN030918MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 16 06:47:18 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.45	152	164255	20.00	ng/ul	0.00
2) Naphthalene-d8	11.29	136	803743	20.00	ng/ul	0.00
6) Acenaphthene-d10	15.07	164	465743	20.00	ng/ul	0.00
12) Phenanthrene-d10	17.79	188	1067667	20.00	ng/ul	0.00
17) Chrysene-d12	21.91	240	989888	20.00	ng/ul	0.00
22) Perylene-d12	24.41	264	950644	20.00	ng/ul	0.00
System Monitoring Compounds						
7) Acenaphthylene-d8	14.77	160	2031996	43.96	ng/ul	0.00
10) Fluorene-d10	16.05	176	1348305	43.07	ng/ul	0.00
14) Anthracene-d10	17.89	188	2133916	42.78	ng/ul	0.00
18) Pyrene-d10	20.14	212	2307243	47.64	ng/ul	0.00
25) Benzo(a)pyrene-d12	24.25	264	1859039	42.82	ng/ul	0.00
Target Compounds				Ovalue		
3) Naphthalene	11.34	128	52959	1.249	ng/ul	97
4) 2-Methylnaphthalene	12.92	142	31473	1.054	ng/ul	98
8) Acenaphthylene	14.80	152	122441	2.636	ng/ul	98
13) Phenanthrene	17.83	178	561259	9.166	ng/ul	99
15) Anthracene	17.92	178	223900	3.604	ng/ul	99
16) Fluoranthene	19.81	202	1820165	27.513	ng/ul#	93
19) Pyrene	20.17	202	1673652	26.780	ng/ul#	88
20) Benzo(a)anthracene	21.90	228	1182399	19.214	ng/ul	97
21) Chrysene	21.95	228	1207160	20.671	ng/ul	97
23) Benzo(b)fluoranthene	23.65	252	2204992	38.897	ng/ul#	96
24) Benzo(k)fluoranthene	23.65	252	2204992	41.555	ng/ul#	96
26) Benzo(a)pyrene	24.30	252	1393324	25.825	ng/ul#	93
27) Indeno(1,2,3-cd)pyrene	26.98	276	1120643	19.264	ng/ul#	85
28) Dibenzo(a,h)anthracene	26.98	278	294268	6.172	ng/ul#	81
29) Benzo(g,h,i)perylene	27.78	276	965574	19.879	ng/ul#	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA N\DATA\BN031518\
Data File : BN000419.D
Acq On : 15 Mar 2018 17:10
Operator : JU/SJ
Sample : J1865-14
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Mar 16 06:48:05 2018
Quant Method : Z:\HPCHEM1\BNA N\METHODS\SOM-EPA-BN030918MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 16 06:47:18 2018
Response via : Initial Calibration

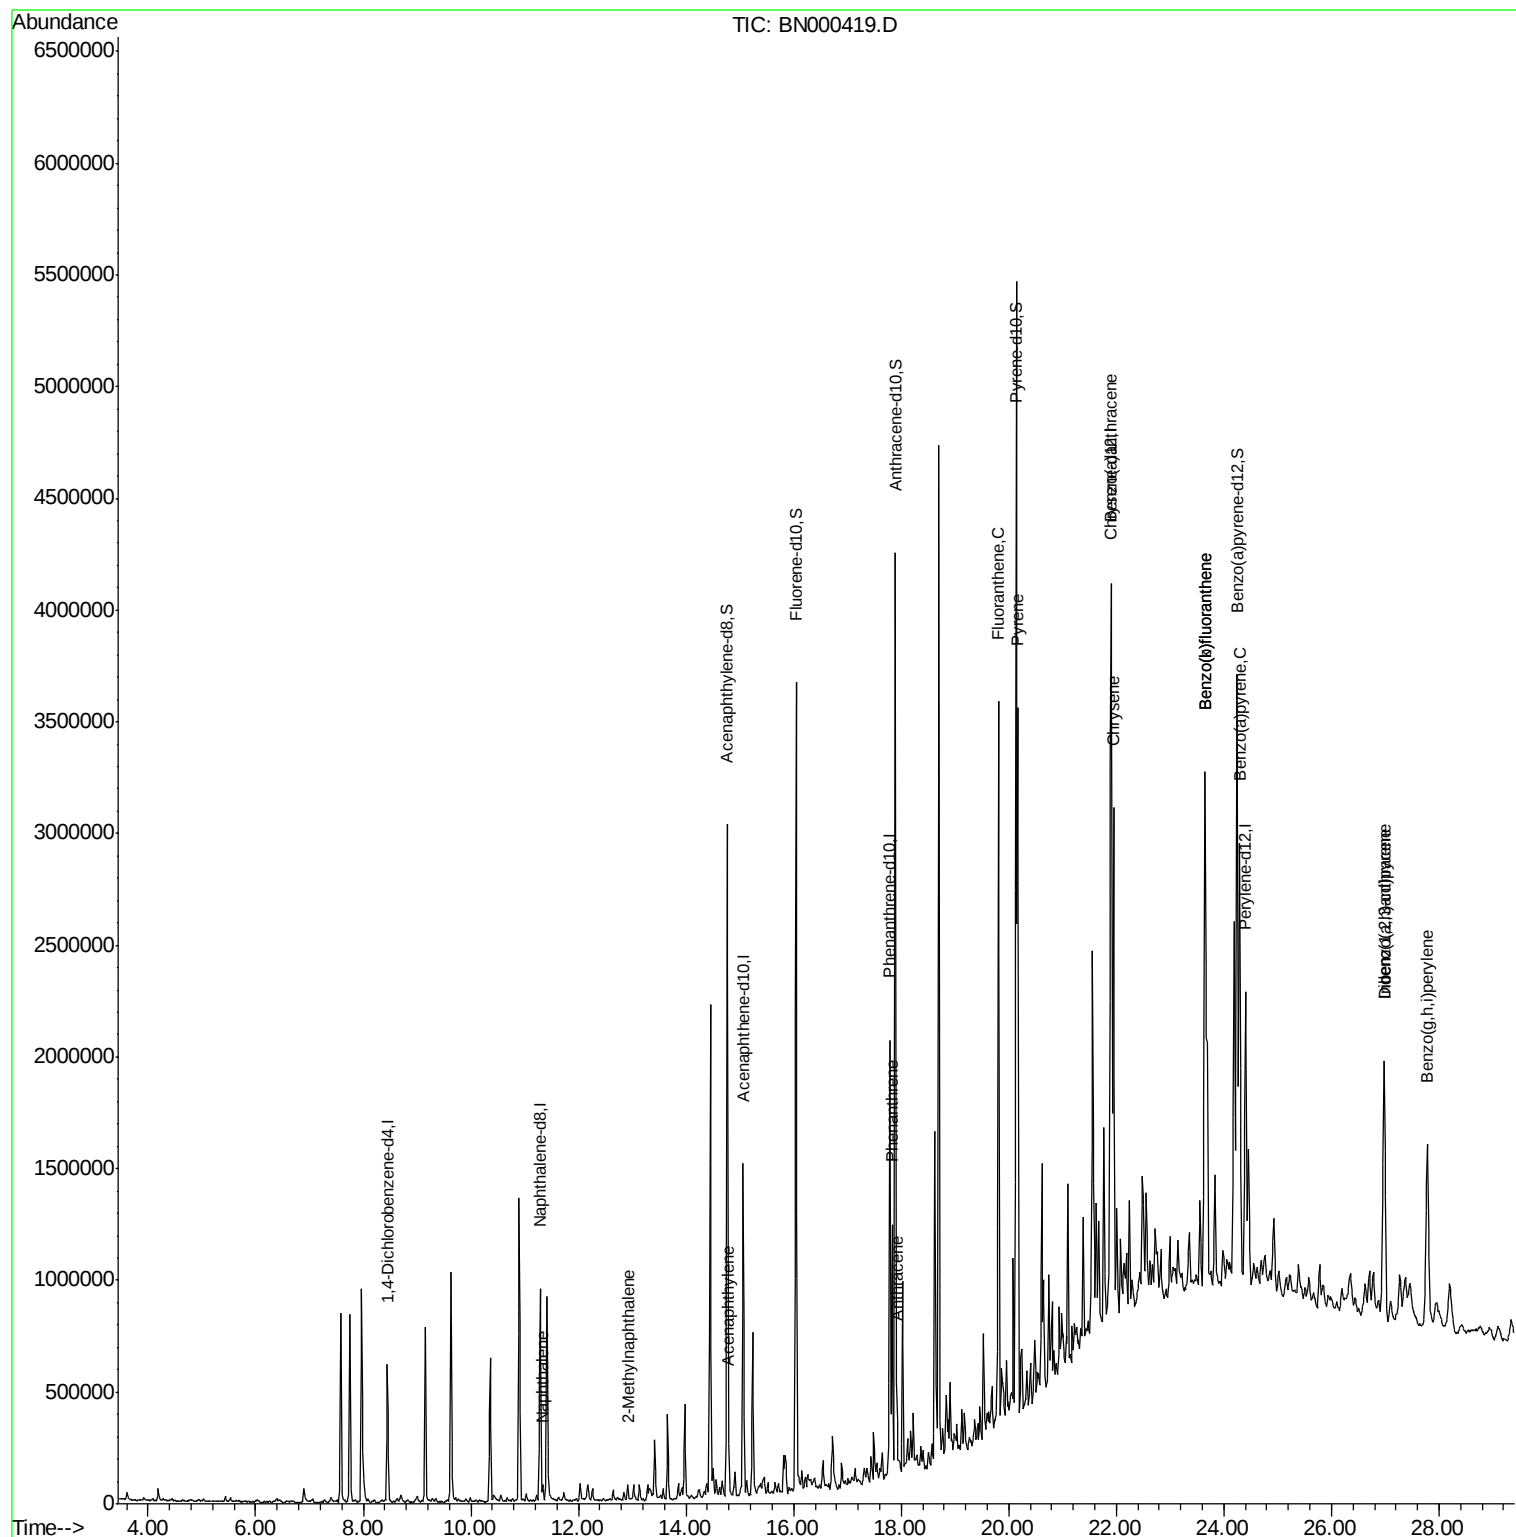

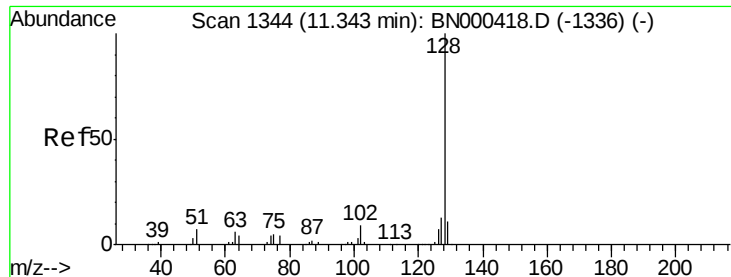

#3

Naphthalene

Concen: 1.249 ng/ul

RT: 11.34 min Scan# 1344

Delta R.T. 0.00 min

Lab File: BN000419.D

Acq: 15 Mar 2018 17:10


Instrument :

BNA_N

ClientSampleId :

Tot Ion:128 Resp: 52959




Ion	Ratio	Lower	Upper
128	100		
129	12.2	8.7	13.1
127	12.0	10.6	16.0

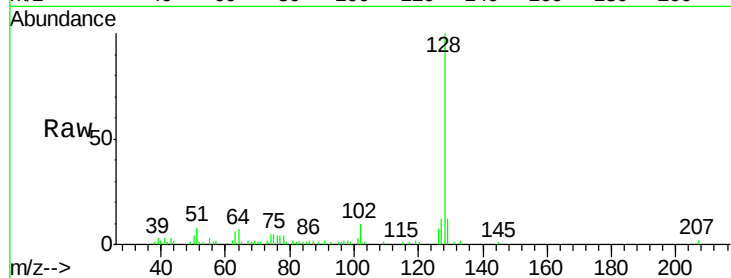

Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

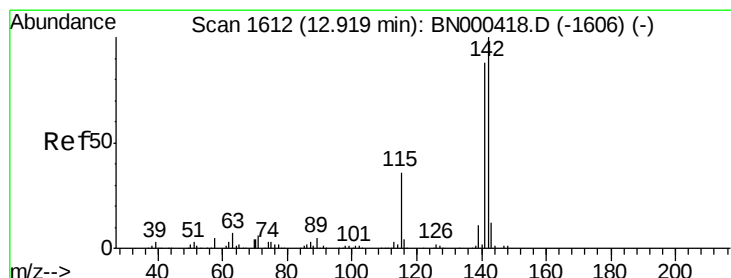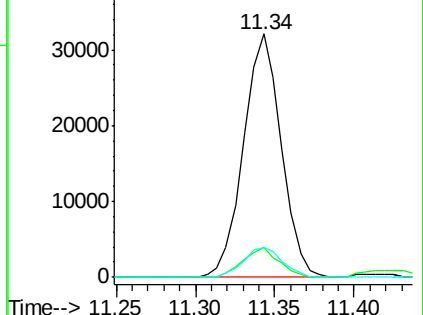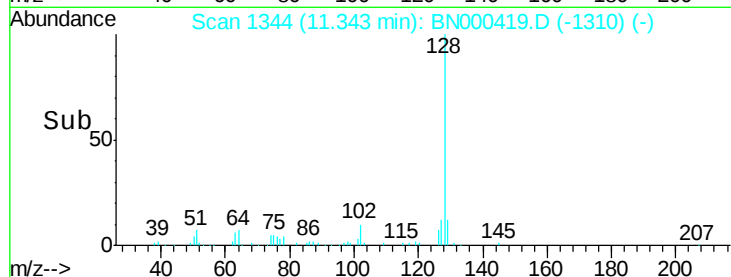

#4

2-Methylnaphthalene

Concen: 1.054 ng/ul

RT: 12.92 min Scan# 1612


Delta R.T. 0.00 min

Lab File: BN000419.D

Acq: 15 Mar 2018 17:10



Tgt Ion:142 Resp: 31473


Ion	Ratio	Lower	Upper
142	100		
141	89.4	72.7	109.1

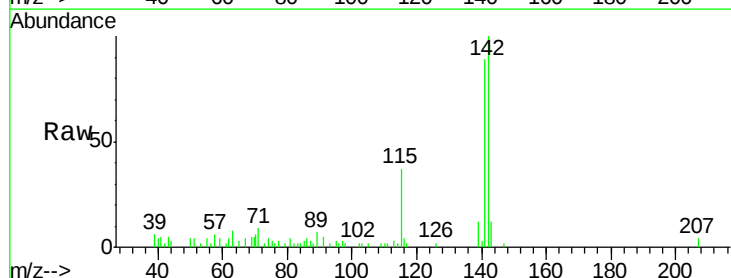

Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

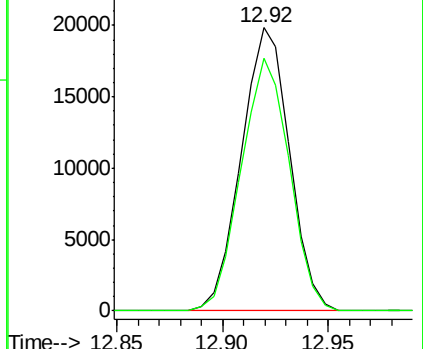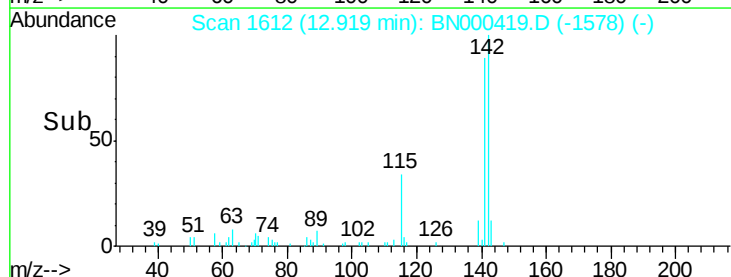

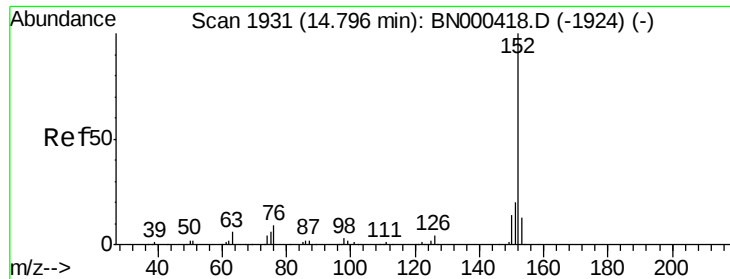

#8

Acenaphthylene

Concen: 2.636 ng/ul

RT: 14.80 min Scan# 1931

Delta R.T. 0.00 min

Lab File: BN000419.D

Acq: 15 Mar 2018 17:10

Instrument :

BNA_N

ClientSampleId :


Tot Ion:152 Resp: 122441

Ion Ratio Lower Upper




152 100

151 20.5 16.7 25.1

153 14.2 10.2 15.4

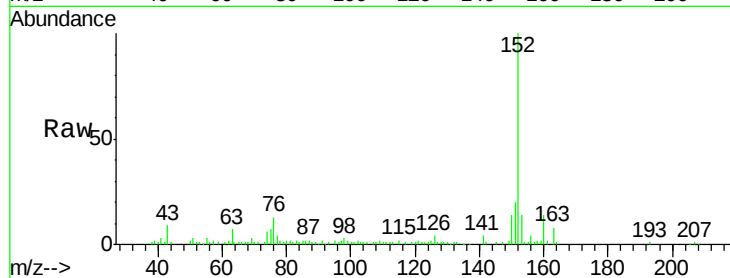

Abundance Ion 152.00 (151.70 to 152.70): E
Ion 151.00 (150.70 to 151.70): E
Ion 153.00 (152.70 to 153.70): E

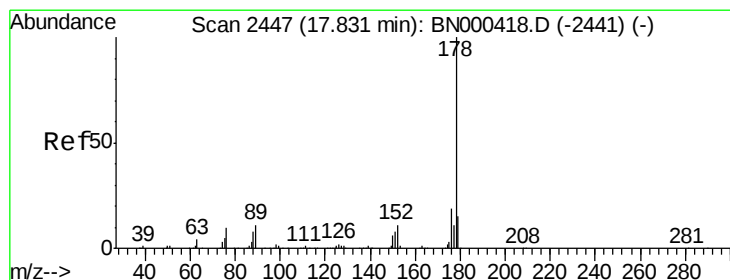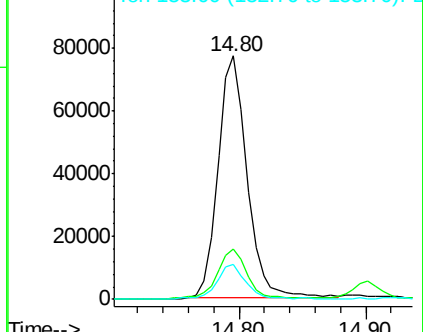

#13

Phenanthrene

Concen: 9.166 ng/ul

RT: 17.83 min Scan# 2447

Delta R.T. 0.00 min

Lab File: BN000419.D

Acq: 15 Mar 2018 17:10


Tgt Ion:178 Resp: 561259

Ion Ratio Lower Upper



178 100


179 15.5 12.3 18.5

176 19.5 15.1 22.7

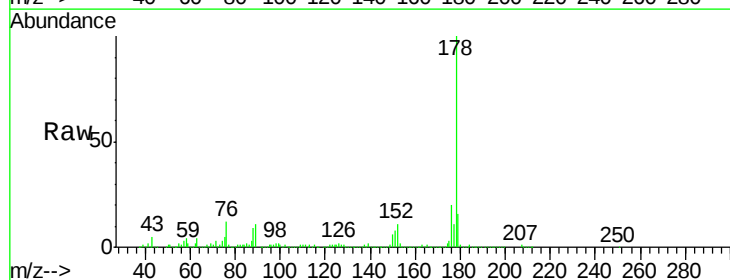

Abundance Ion 178.00 (177.70 to 178.70): E
Ion 179.00 (178.70 to 179.70): E
Ion 176.00 (175.70 to 176.70): E




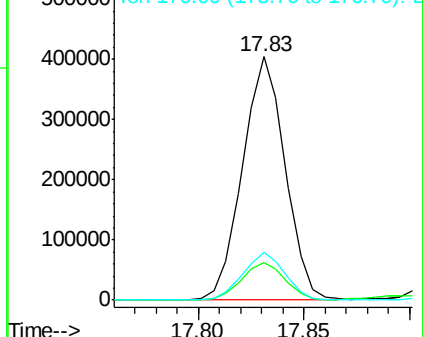




#15
 Anthracene
 Concen: 3.604 ng/ul
 RT: 17.92 min Scan# 2462
 Delta R.T. -0.01 min
 Lab File: BN000419.D
 Acq: 15 Mar 2018 17:10




Instrument :
 BNA_N
 ClientSampleId :


Tot Ion:178 Resp: 223900
 Ion Ratio Lower Upper
 178 100
 179 15.3 11.8 17.8
 176 18.9 15.2 22.8

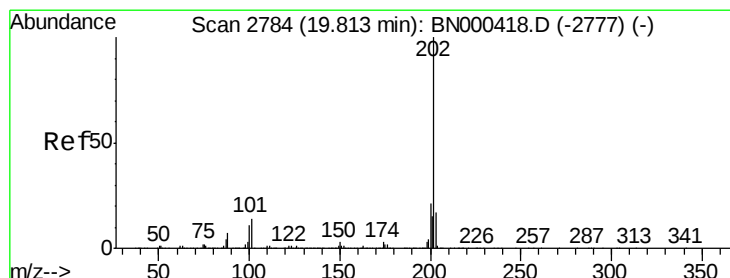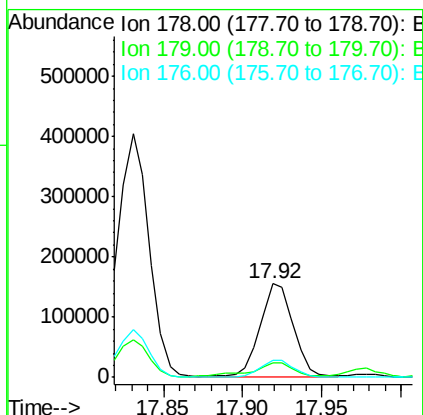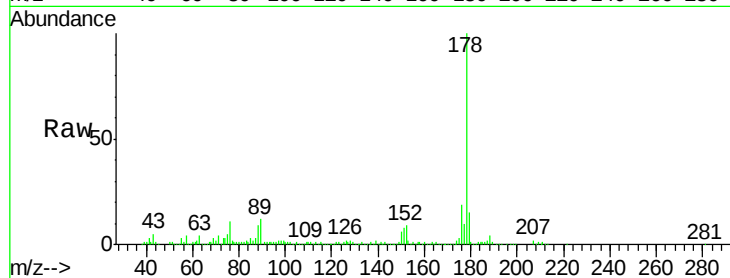

#16
 Fluoranthene
 Concen: 27.513 ng/ul
 RT: 19.81 min Scan# 2784
 Delta R.T. 0.00 min
 Lab File: BN000419.D
 Acq: 15 Mar 2018 17:10

Tgt Ion:202 Resp: 1820165
 Ion Ratio Lower Upper
 202 100
 101 15.5 9.9 14.9#
 100 11.5 7.4 11.0#

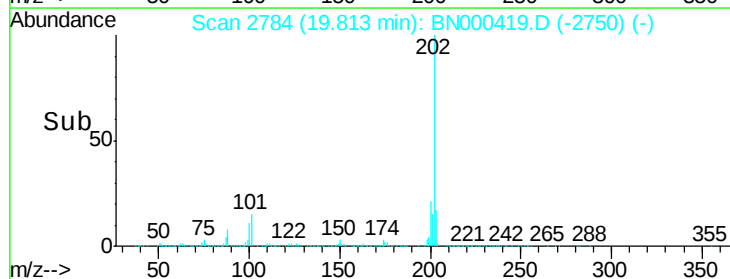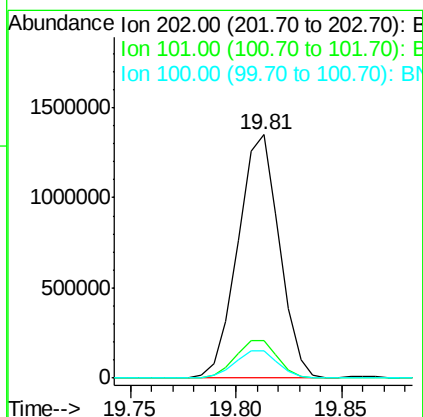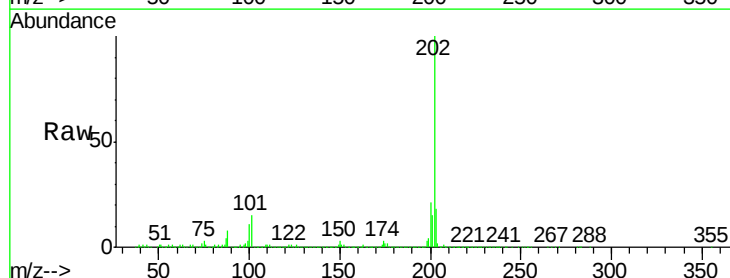



#19

Pvrene

Concen: 26.780 ng/ul

RT: 20.17 min Scan# 2845

Delta R.T. 0.00 min

Lab File: BN000419.D

Acq: 15 Mar 2018 17:10

Instrument :

BNA_N

ClientSampleId :


Tot Ion:202 Resp: 1673652

Ion Ratio Lower Upper

202 100

101 18.1 11.0 16.4#




100 15.4 8.1 12.1#

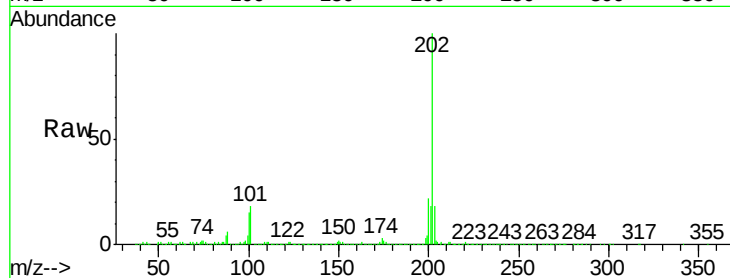

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

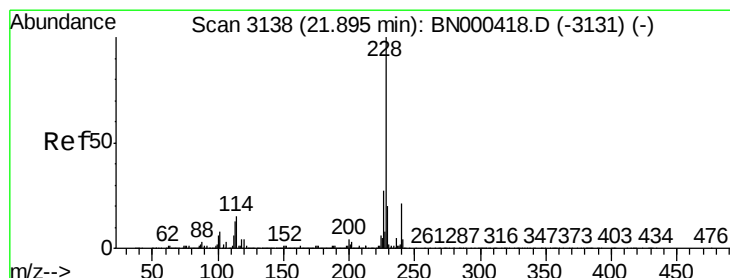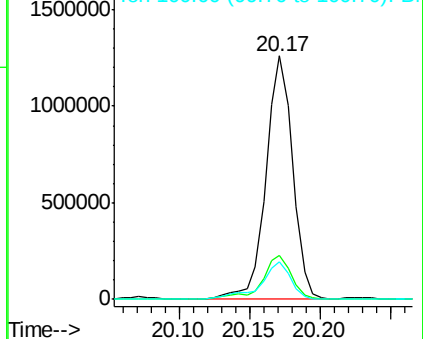

#20

Benzo(a)anthracene

Concen: 19.214 ng/ul

RT: 21.90 min Scan# 3138

Delta R.T. 0.00 min

Lab File: BN000419.D

Acq: 15 Mar 2018 17:10


Tgt Ion:228 Resp: 1182399

Ion Ratio Lower Upper

228 100

229 20.8 15.7 23.5



226 28.0 21.1 31.7

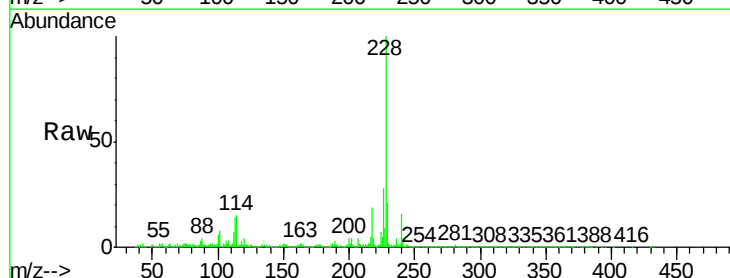


Abundance Ion 228.00 (227.70 to 228.70): E

Ion 229.00 (228.70 to 229.70): E

Ion 226.00 (225.70 to 226.70): E

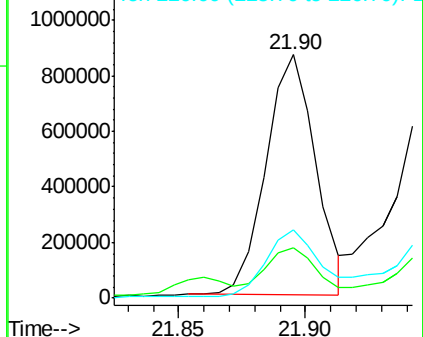

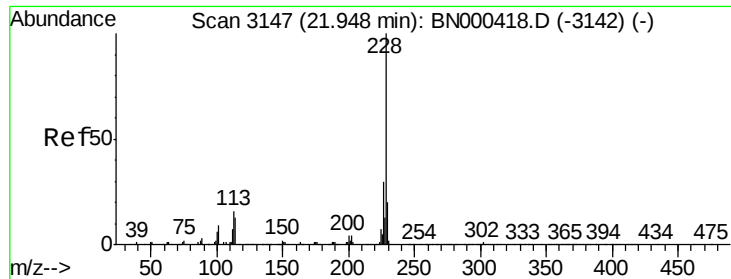

#21

Chrysene

Concen: 20.671 ng/ul

RT: 21.95 min Scan# 3147

Delta R.T. 0.00 min

Lab File: BN000419.D

Acq: 15 Mar 2018 17:10


Instrument :

BNA_N

ClientSampled :

Tot Ion:228 Resp: 1207160

Ion	Ratio	Lower	Upper
228	100		
226	30.2	24.5	36.7
229	23.0	15.8	23.8



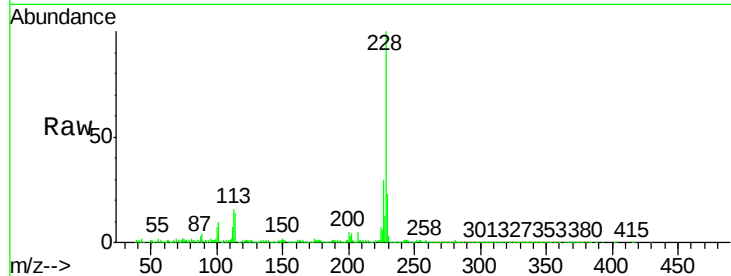


Abundance

Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

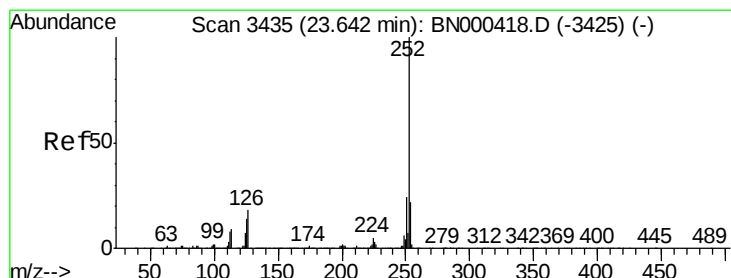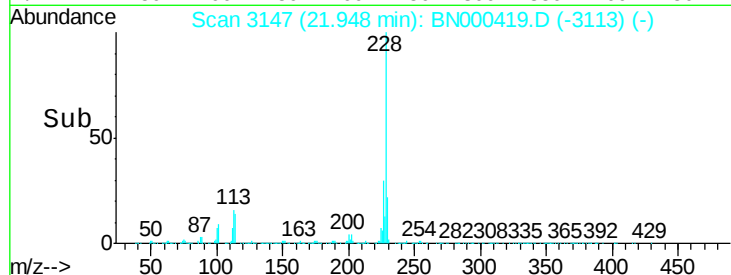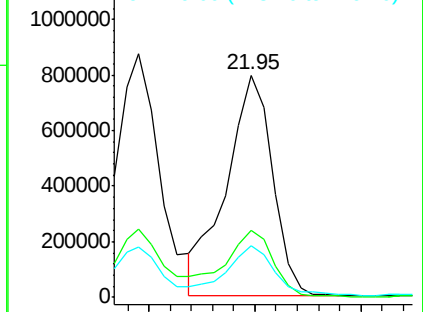

#23

Benzo(b)fluoranthene

Concen: 38.897 ng/ul

RT: 23.65 min Scan# 3436


Delta R.T. 0.01 min

Lab File: BN000419.D

Acq: 15 Mar 2018 17:10

Tgt Ion:252 Resp: 2204992

Ion	Ratio	Lower	Upper
252	100		
253	22.6	18.0	27.0
125	15.2	8.0	12.0


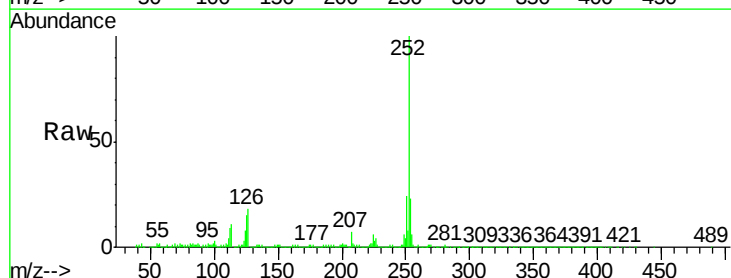



Abundance

Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E



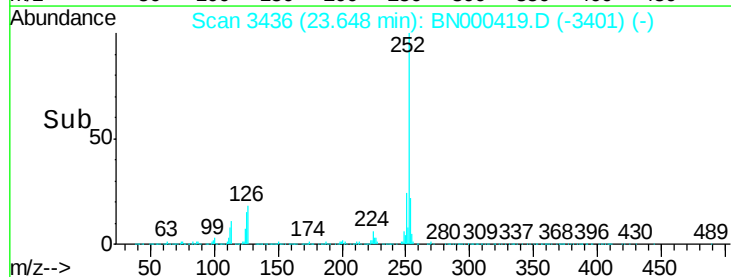
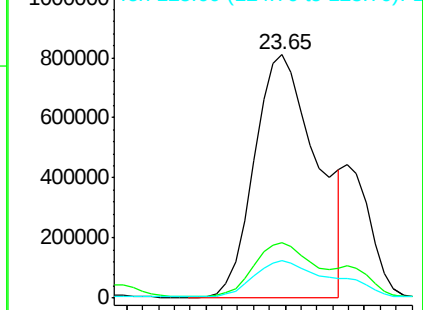




#24
Benzo(k)fluoranthene
Concen: 41.555 ng/ul
RT: 23.65 min Scan# 3436
Delta R.T. -0.04 min
Lab File: BN000419.D
Acq: 15 Mar 2018 17:10




Instrument :
BNA_N
ClientSampled :


Tot Ion:252 Resp: 2204992
Ion Ratio Lower Upper
252 100
253 22.6 18.0 27.0
125 15.2 8.1 12.1#

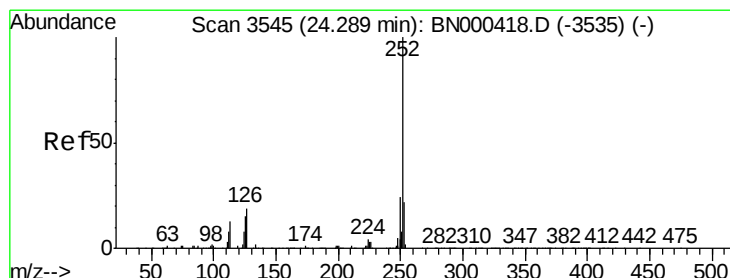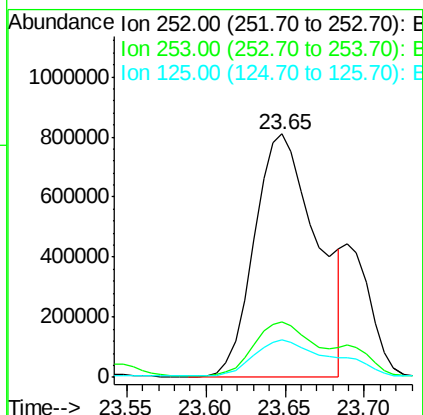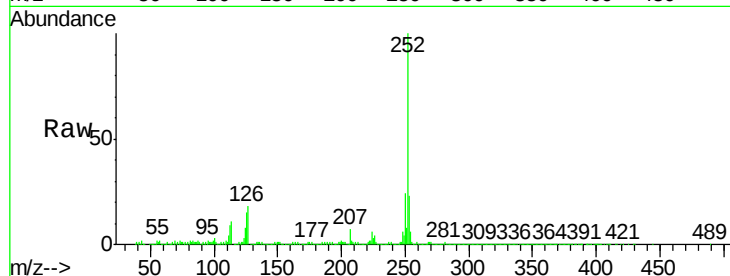

#26
Benzo(a)pyrene
Concen: 25.825 ng/ul
RT: 24.30 min Scan# 3546
Delta R.T. 0.01 min
Lab File: BN000419.D
Acq: 15 Mar 2018 17:10

Tgt Ion:252 Resp: 1393324
Ion Ratio Lower Upper
252 100
253 23.1 17.2 25.8
125 15.8 8.2 12.4#

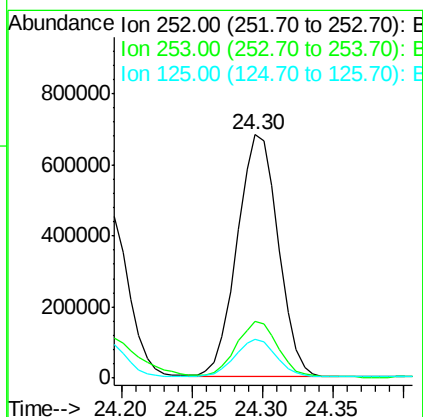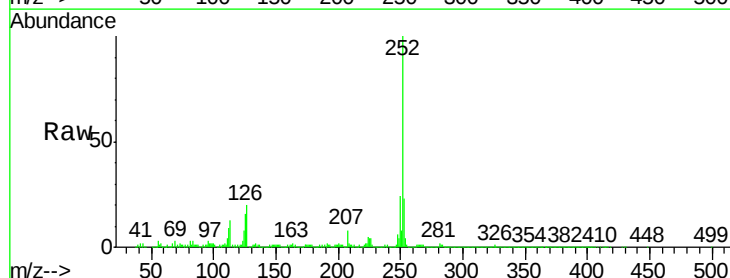

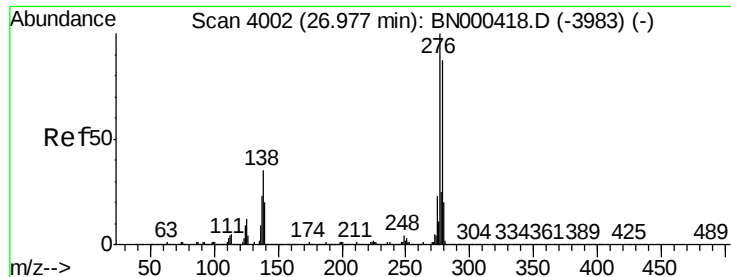


#27




Indeno(1,2,3-cd)pyrene
Concen: 19.264 ng/ul
RT: 26.98 min Scan# 4003
Delta R.T. 0.01 min
Lab File: BN000419.D
Acq: 15 Mar 2018 17:10

Instrument :
BNA_N
ClientSampled :

Tot Ion:276 Resp: 1120643
Ion Ratio Lower Upper
276 100
138 29.3 14.4 21.6#
277 25.2 18.0 27.0

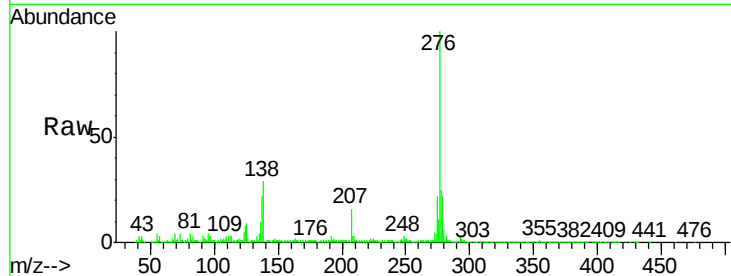


Abundance Ion 276.00 (275.70 to 276.70): E
Ion 138.00 (137.70 to 138.70): E
Ion 277.00 (276.70 to 277.70): E

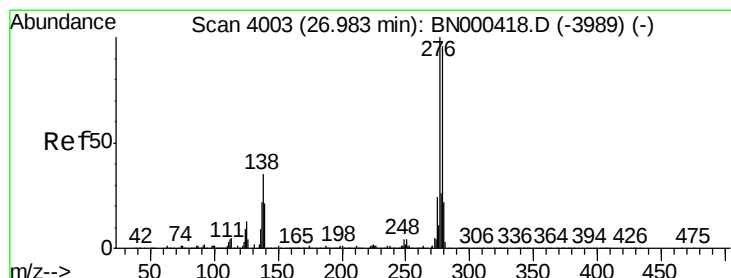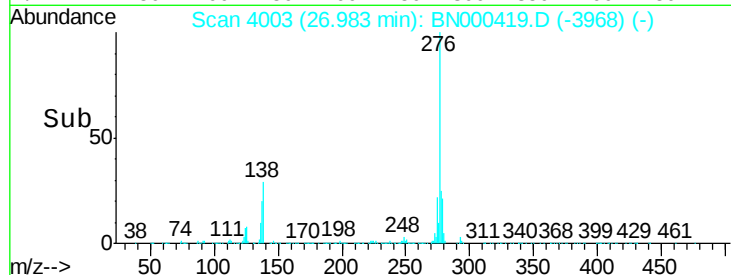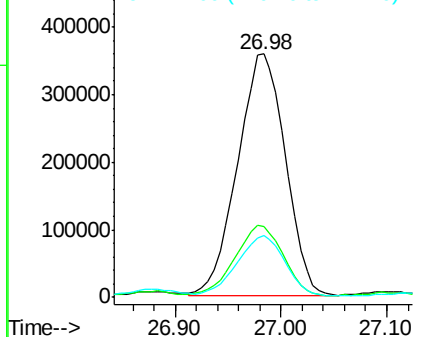



#28


Dibenzo(a,h)anthracene
Concen: 6.172 ng/ul
RT: 26.98 min Scan# 4002
Delta R.T. -0.01 min
Lab File: BN000419.D
Acq: 15 Mar 2018 17:10

Tgt Ion:278 Resp: 294268
Ion Ratio Lower Upper
278 100
139 0.0 12.2 18.4#
279 27.5 19.2 28.8

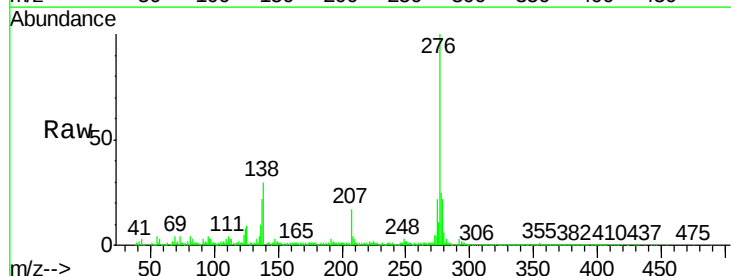

Abundance Ion 278.00 (277.70 to 278.70): E
Ion 139.00 (138.70 to 139.70): E
Ion 279.00 (278.70 to 279.70): E

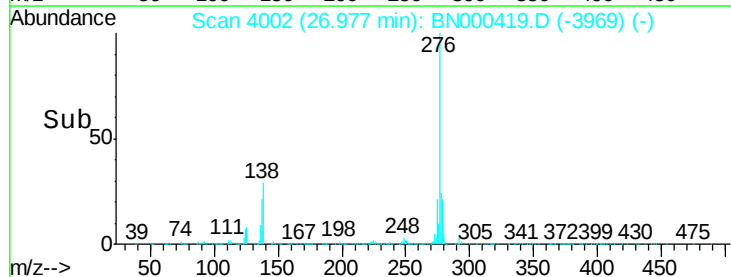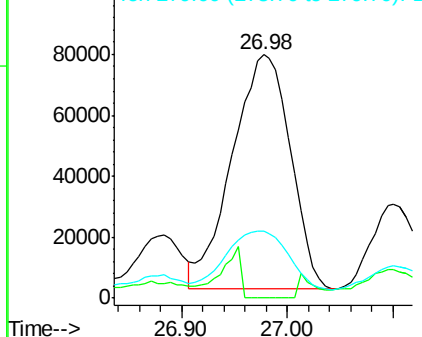

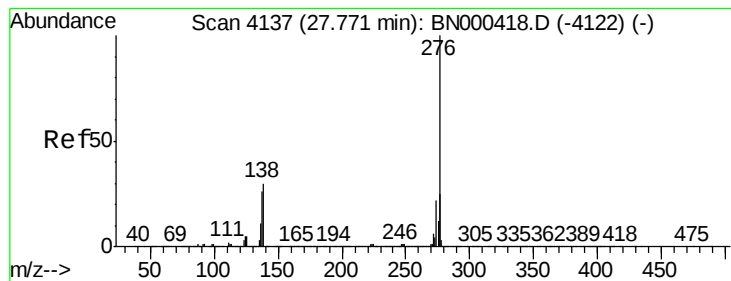

#29

Benzo(a,h,i)perylene

Concen: 19.879 ng/ul

RT: 27.78 min Scan# 4139

Delta R.T. 0.01 min

Lab File: BN000419.D

Acq: 15 Mar 2018 17:10

Instrument :

BNA_N

ClientSampleId :


Tot Ion:276 Resp: 965574

Ion Ratio Lower Upper

276 100

138 30.2 15.3 22.9#

277 24.9 19.0 28.4

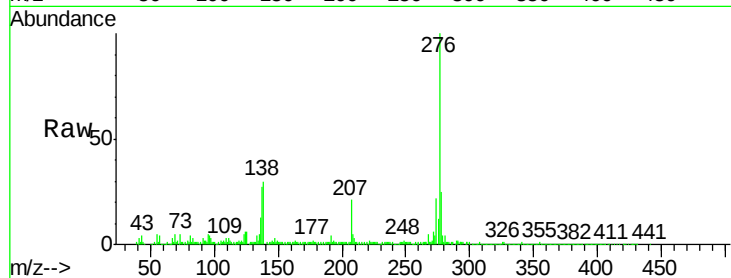

Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

