

Data Path : Z:\HPCHEM1\BNA N\DATA\BN031518\
 Data File : BN000431.D
 Acq On : 16 Mar 2018 00:05
 Operator : JU/SJ
 Sample : J1865-06
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DAMB9

Manual Integrations
 APPROVED

Sohil
 3/16/2018 12:12:06 PM

Quant Time: Mar 16 07:24:15 2018
 Quant Method : Z:\HPCHEM1\BNA N\METHODS\SOM-EPA-BN030918MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 16 06:47:18 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.45	152	211449	20.00	ng/ul	0.00
2) Naphthalene-d8	11.30	136	987510	20.00	ng/ul	0.00
6) Acenaphthene-d10	15.07	164	557965	20.00	ng/ul	0.00
12) Phenanthrene-d10	17.80	188	1223177	20.00	ng/ul	0.00
17) Chrysene-d12	21.92	240	959592	20.00	ng/ul	0.01
22) Perylene-d12	24.42	264	889838	20.00	ng/ul	0.02
System Monitoring Compounds						
7) Acenaphthylene-d8	14.77	160	1949020	35.19	ng/ul	0.00
10) Fluorene-d10	16.05	176	1290359	34.41	ng/ul	0.00
14) Anthracene-d10	17.90	188	2013996	35.24	ng/ul	0.00
18) Pyrene-d10	20.15	212	1953332	41.61	ng/ul	0.00
25) Benzo(a)pyrene-d12	24.26	264	1451896	35.73	ng/ul	0.02
Target Compounds						
13) Phenanthrene	17.84	178	124892	1.780	ng/ul	98
16) Fluoranthene	19.82	202	370375	4.887	ng/ul#	93
19) Pyrene	20.18	202	335909	5.544	ng/ul#	89
20) Benzo(a)anthracene	21.90	228	212797	3.567	ng/ul	95
21) Chrysene	21.95	228	256919m	4.538	ng/ul	
23) Benzo(b)fluoranthene	23.65	252	428514	8.076	ng/ul#	84
24) Benzo(k)fluoranthene	23.70	252	101888m	2.051	ng/ul	
26) Benzo(a)pyrene	24.31	252	255919	5.068	ng/ul#	80
27) Indeno(1,2,3-cd)pyrene	27.01	276	225529	4.142	ng/ul#	78
28) Dibenzo(a,h)anthracene	27.01	278	67743	1.518	ng/ul#	36
29) Benzo(g,h,i)perylene	27.82	276	219772	4.834	ng/ul#	79

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA N\DATA\BN031518\
Data File : BN000431.D
Acq On : 16 Mar 2018 00:05
Operator : JU/SJ
Sample : J1865-06
Misc :
ALS Vial : 25 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampled :
DAMB9

Manual Integrations
APPROVED

Sohil
3/16/2018 12:12:06 PM

Quant Time: Mar 16 07:24:15 2018
Quant Method : Z:\HPCHEM1\BNA N\METHODS\SOM-EPA-BN030918MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 16 06:47:18 2018
Response via : Initial Calibration

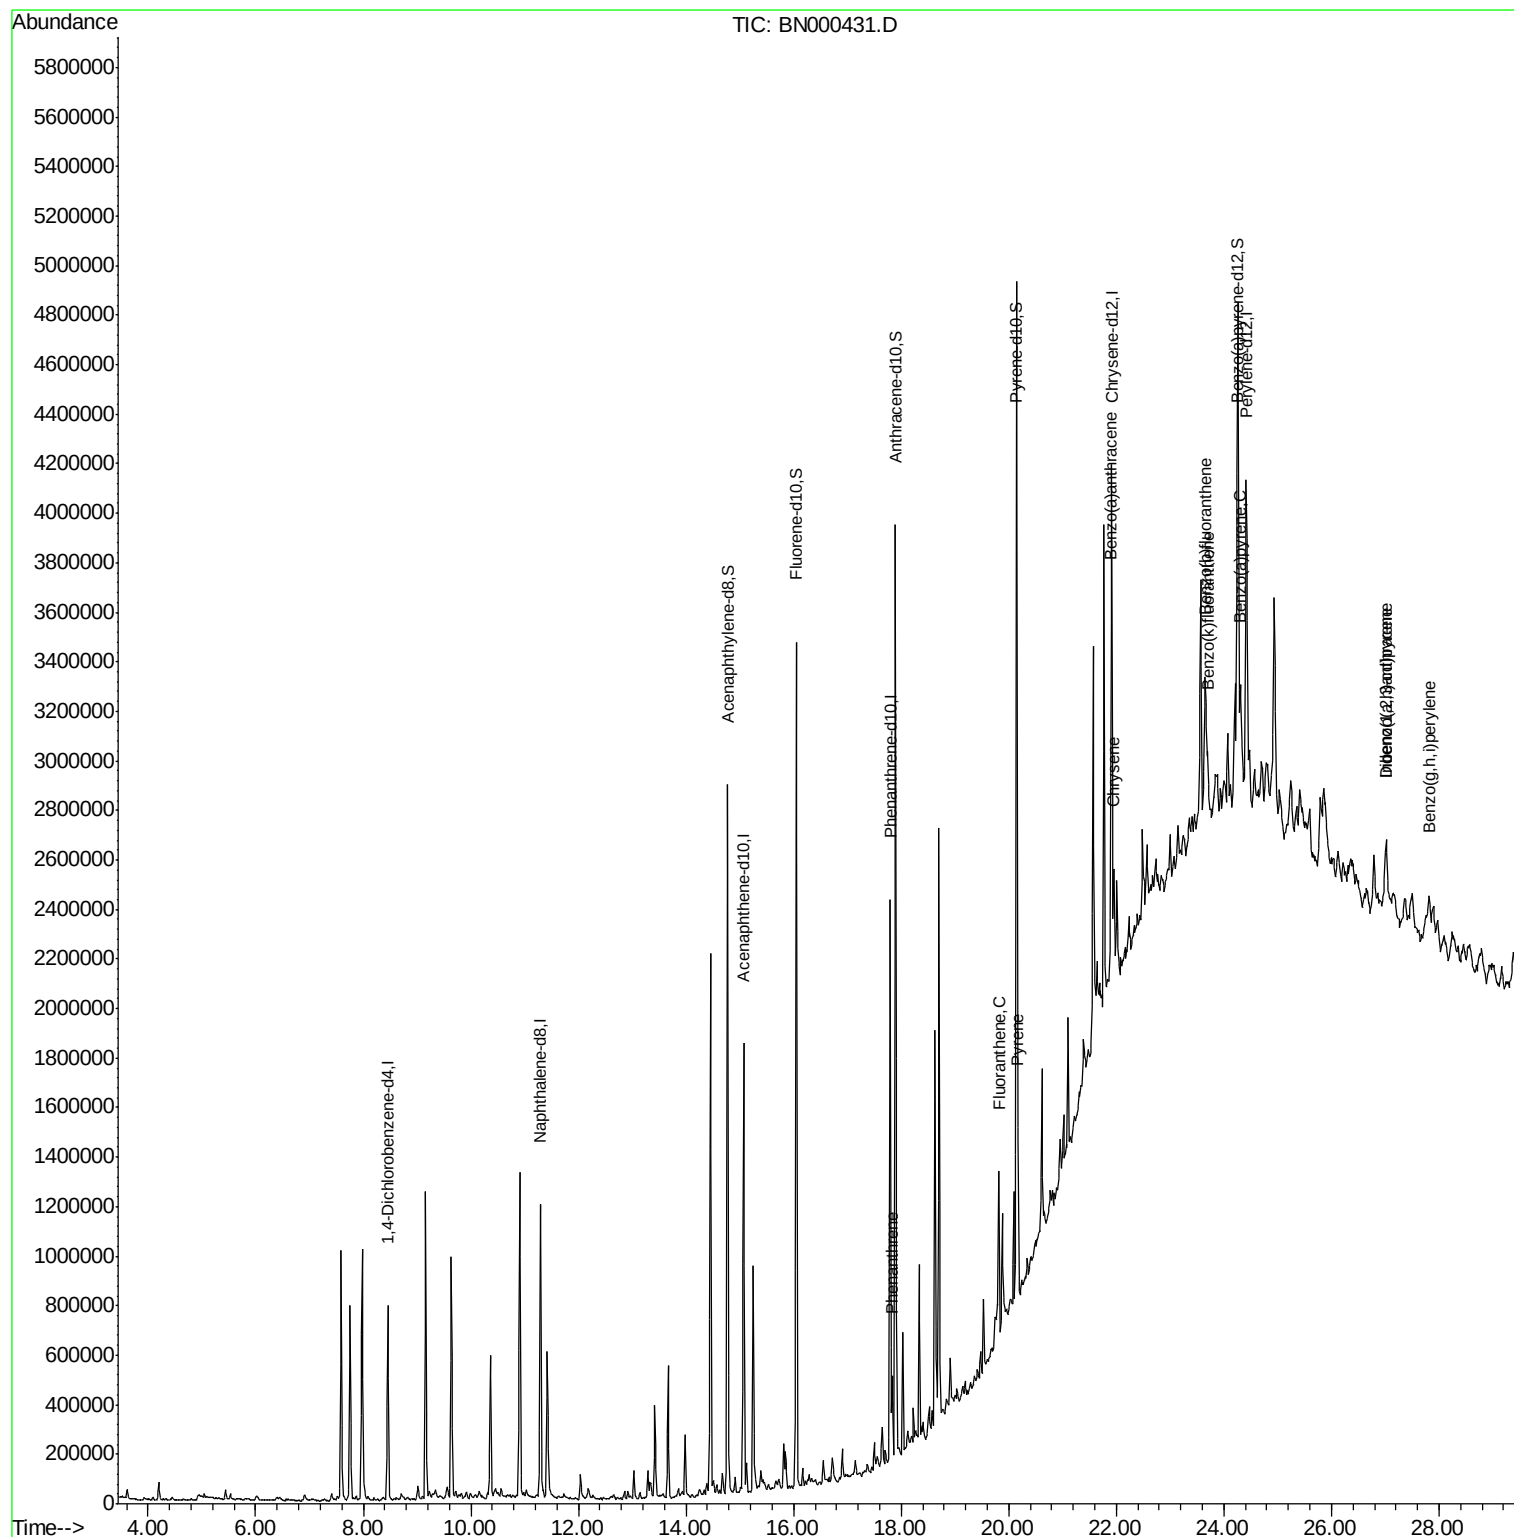

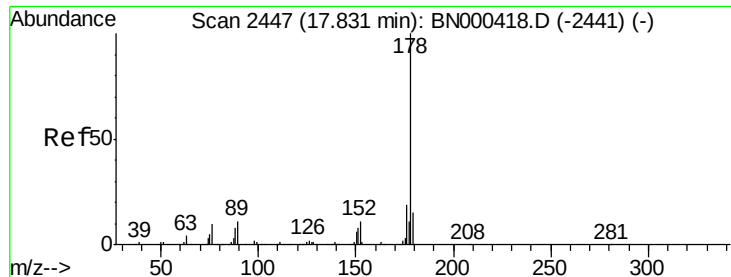

#13

Phenanthrene

Concen: 1.780 ng/ul

RT: 17.84 min Scan# 2448

Delta R.T. 0.01 min

Lab File: BN000431.D

Acq: 16 Mar 2018 00:05

Instrument :

BNA_N





ClientSampleId :

DAMB9

Tot Ion:	178	Resp:	124892
Ion Ratio	Lower	Upper	
178	100		
179	16.8	12.3	18.5
176	18.8	15.1	22.7

Manual Integrations
APPROVED

Sohil
3/16/2018 12:12:06 PM

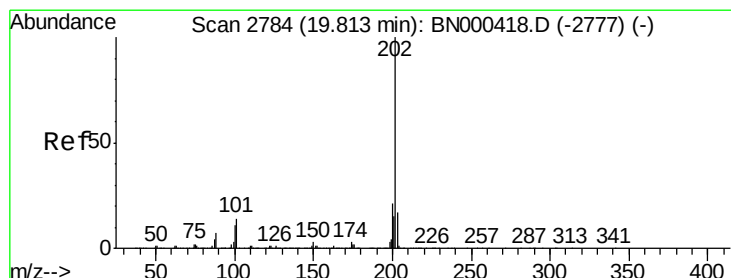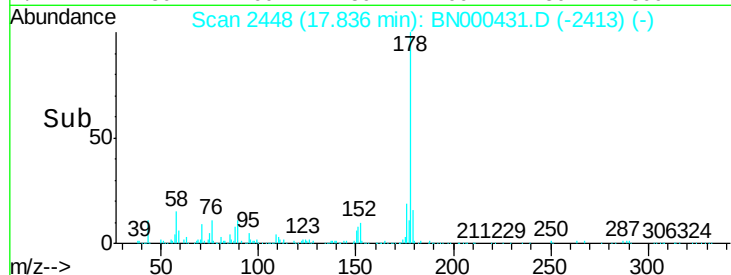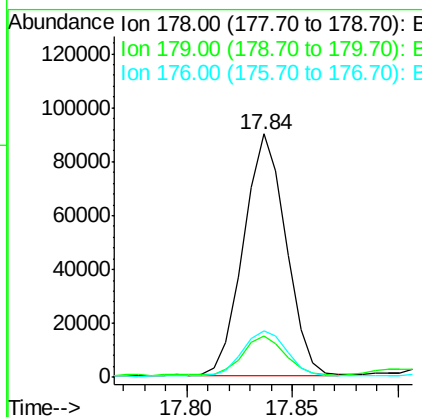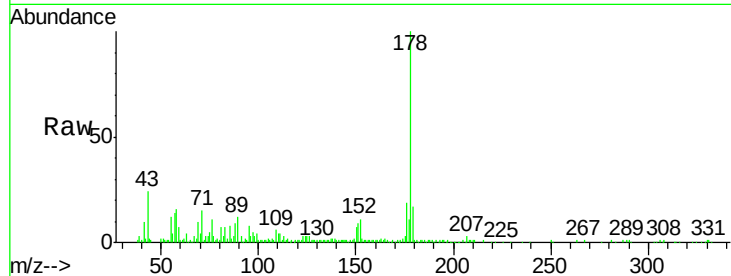

#16

Fluoranthene

Concen: 4.887 ng/ul




RT: 19.82 min Scan# 2785


Delta R.T. 0.01 min

Lab File: BN000431.D

Acq: 16 Mar 2018 00:05

Tgt Ion:	202	Resp:	370375
Ion Ratio	Lower	Upper	
202	100		
101	15.4	9.9	14.9#
100	11.6	7.4	11.0#

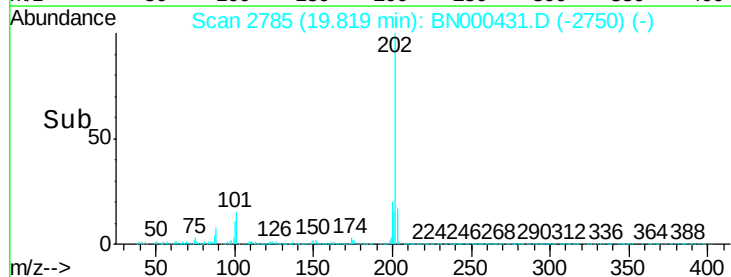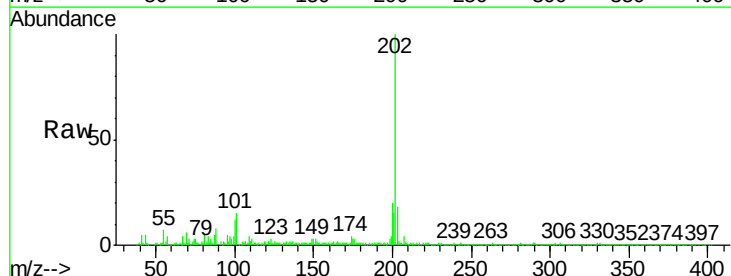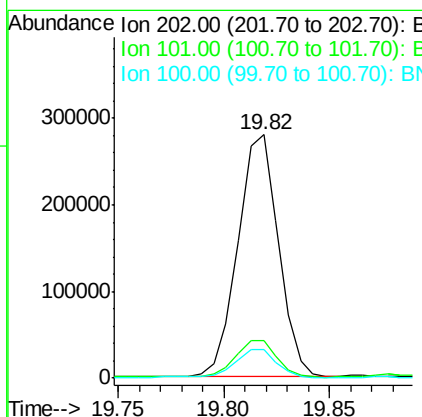

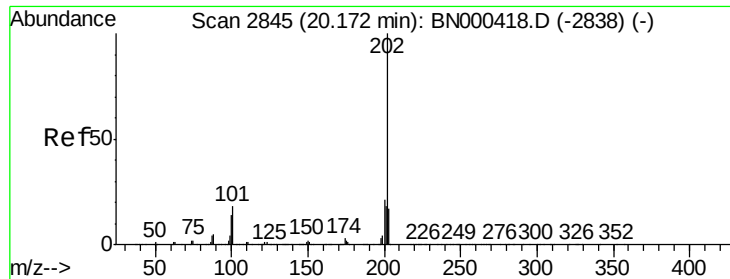

#19

Pvrene

Concen: 5.544 ng/ul

RT: 20.18 min Scan# 2846

Delta R.T. 0.01 min

Lab File: BN000431.D

Acq: 16 Mar 2018 00:05

Instrument :

BNA_N





ClientSampleId :

DAMB9

Tot Ion:	202	Resp:	335909
Ion Ratio	Lower	Upper	
202	100		
101	18.1	11.0	16.4#
100	14.3	8.1	12.1#

Manual Integrations
APPROVED

Sohil
3/16/2018 12:12:06 PM

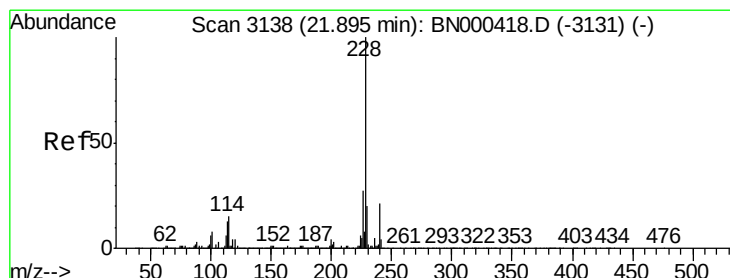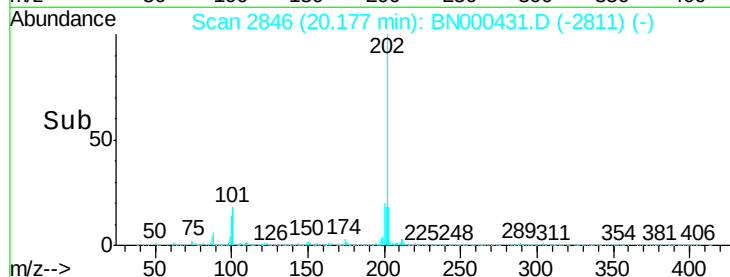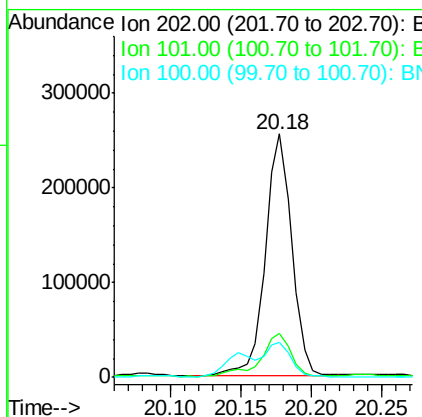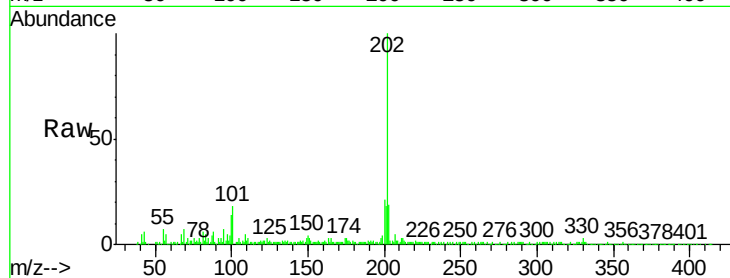

#20

Benzo(a)anthracene

Concen: 3.567 ng/ul




RT: 21.90 min Scan# 3139


Delta R.T. 0.01 min

Lab File: BN000431.D

Acq: 16 Mar 2018 00:05

Tgt Ion:	228	Resp:	212797
Ion Ratio	Lower	Upper	
228	100		
229	22.9	15.7	23.5
226	28.2	21.1	31.7

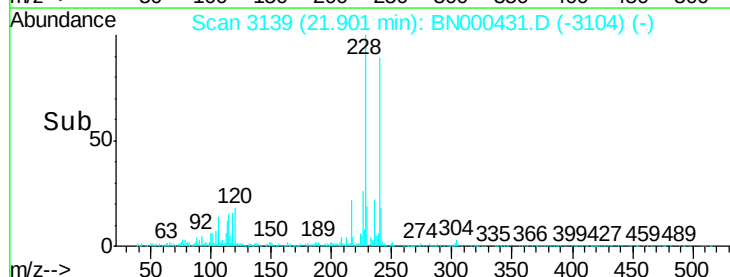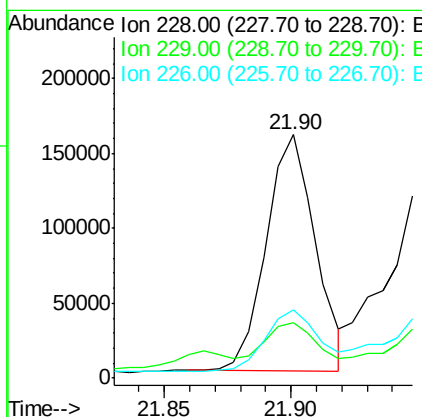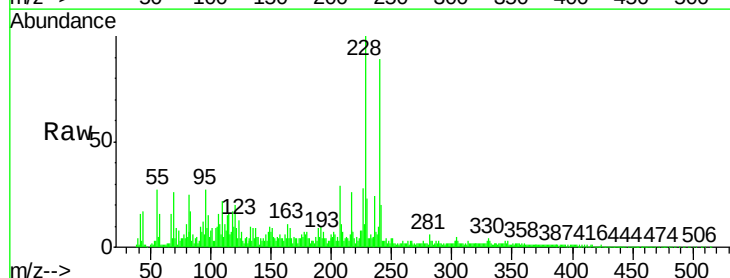

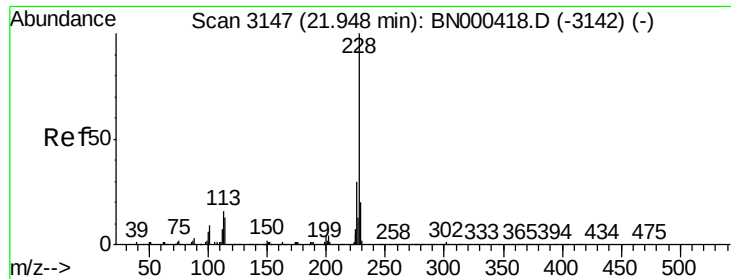

#21

Chrysene

Concen: 4.538 ng/ul m

RT: 21.95 min Scan# 3148

Delta R.T. 0.01 min

Lab File: BN000431.D

Acq: 16 Mar 2018 00:05

Instrument :

BNA_N





ClientSampled :

DAMB9

Tot Ion:	228	Resp:	256919
Ion Ratio	Lower	Upper	
228	100		
226	31.2	24.5	36.7
229	25.2	15.8	23.8#

Manual Integrations
APPROVED

Sohil
3/16/2018 12:12:06 PM

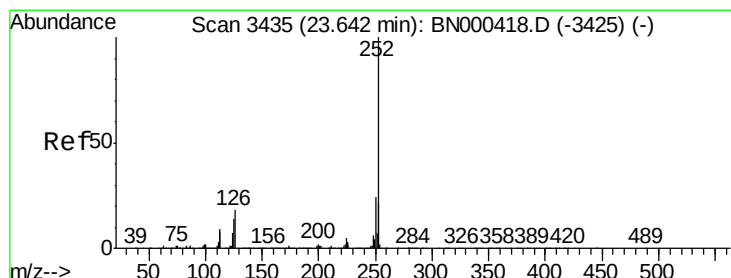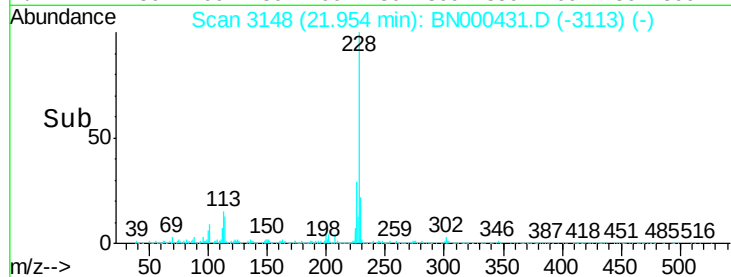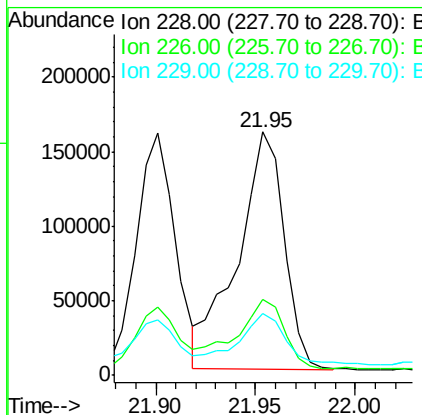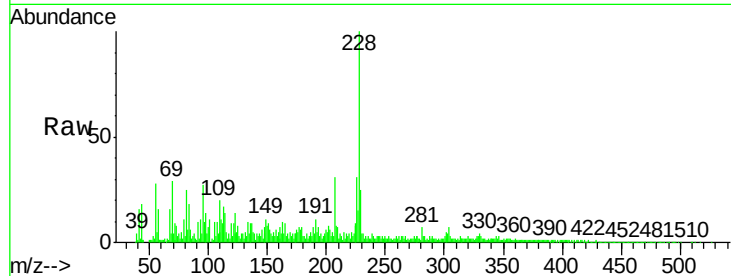

#23

Benzo(b)fluoranthene

Concen: 8.076 ng/ul




RT: 23.65 min Scan# 3437


Delta R.T. 0.01 min

Lab File: BN000431.D

Acq: 16 Mar 2018 00:05

Tgt Ion:	252	Resp:	428514
Ion Ratio	Lower	Upper	
252	100		
253	26.0	18.0	27.0
125	22.9	8.0	12.0#

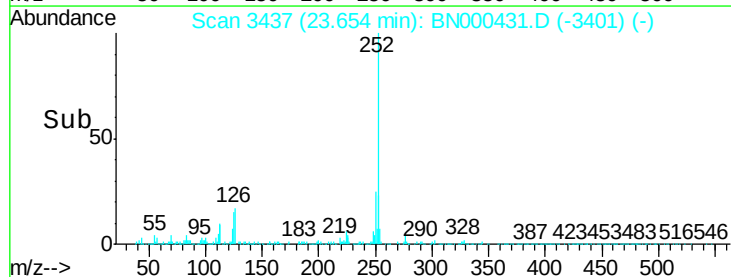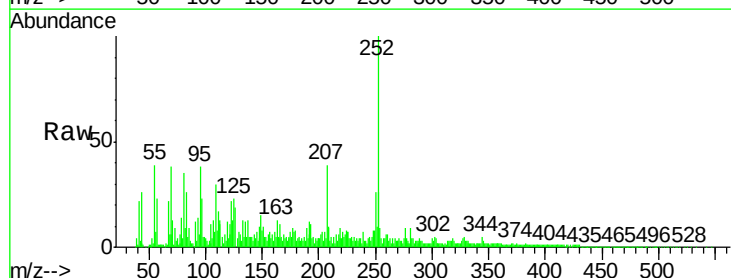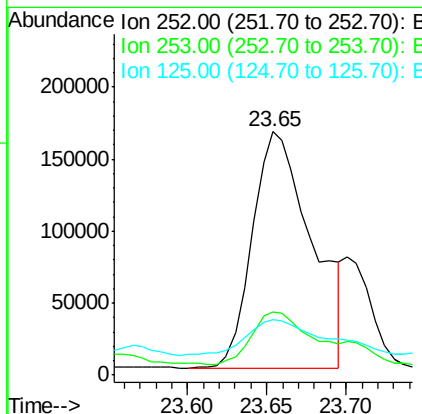

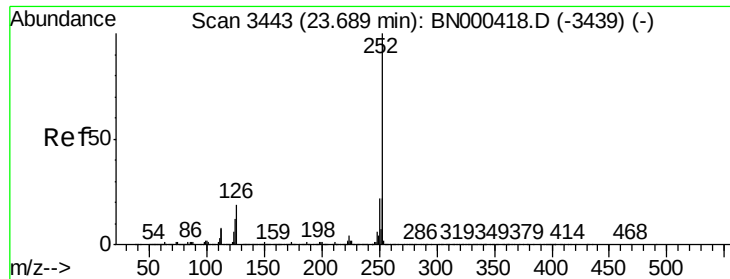

#24

Benzo(k)fluoranthene

Concen: 2.051 ng/ul m

RT: 23.70 min Scan# 3445

Delta R.T. 0.01 min

Lab File: BN000431.D

Acq: 16 Mar 2018 00:05

Instrument :

BNA_N





ClientSampleId :

DAMB9

Tot Ion:	252	Resp:	101888
Ion Ratio	Lower	Upper	
252	100		
253	28.9	18.0	27.0#
125	29.4	8.1	12.1#

Manual Integrations
APPROVED

Sohil
3/16/2018 12:12:06 PM

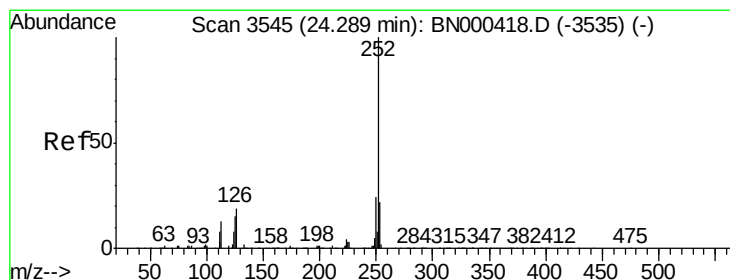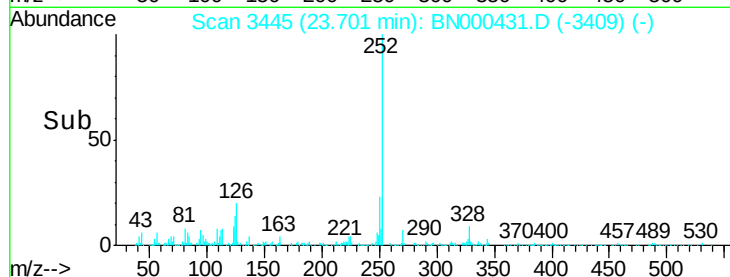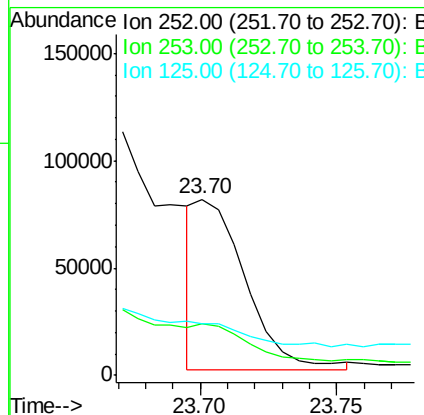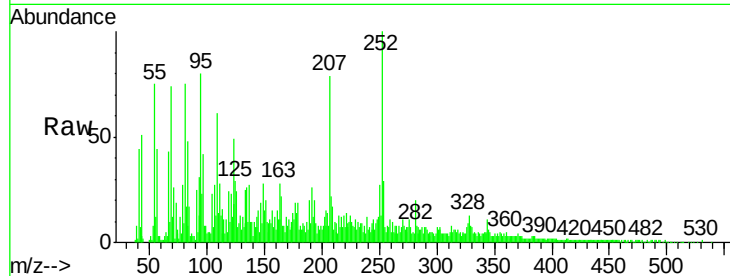

#26

Benzo(a)pyrene

Concen: 5.068 ng/ul




RT: 24.31 min Scan# 3549


Delta R.T. 0.02 min

Lab File: BN000431.D

Acq: 16 Mar 2018 00:05

Tgt Ion:	252	Resp:	255919
Ion Ratio	Lower	Upper	
252	100		
253	26.2	17.2	25.8#
125	25.3	8.2	12.4#

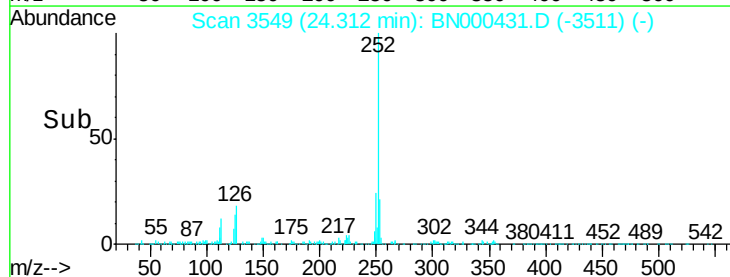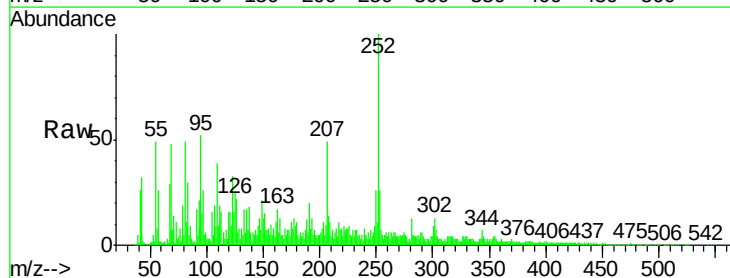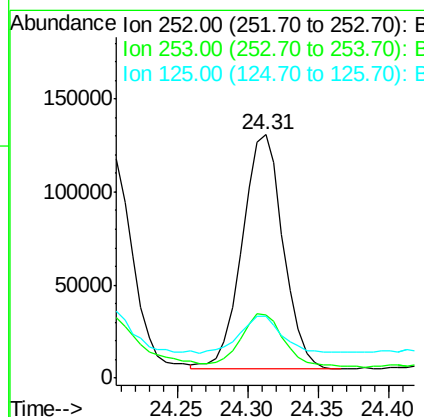

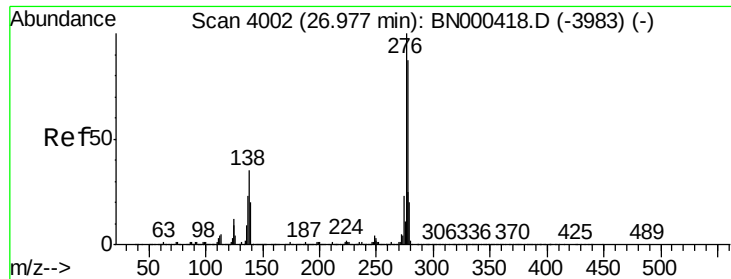

#27

Indeno(1,2,3-cd)pyrene

Concen: 4.142 ng/ul

RT: 27.01 min Scan# 4008

Delta R.T. 0.04 min

Lab File: BN000431.D

Acq: 16 Mar 2018 00:05

Instrument :

BNA_N





ClientSampled :

DAMB9

Tot Ion:	276	Resp:	225529
Ion Ratio	Lower	Upper	
276	100		
138	33.1	14.4	21.6#
277	28.6	18.0	27.0#

Manual Integrations
APPROVED

Sohil
3/16/2018 12:12:06 PM

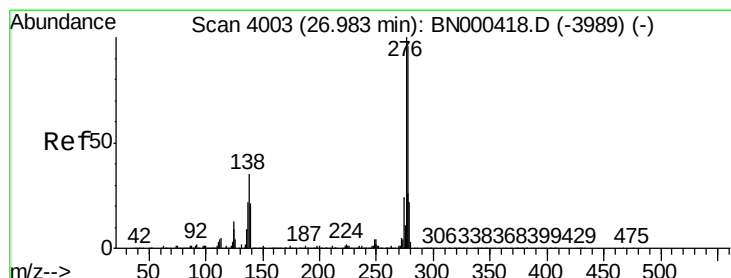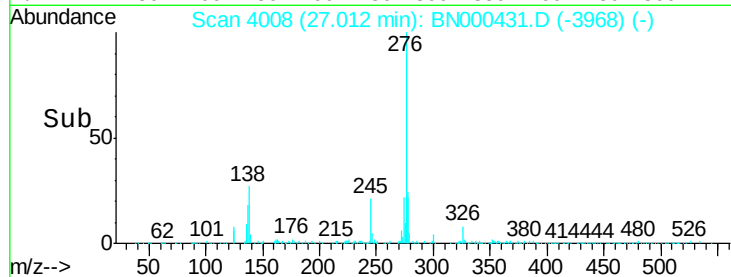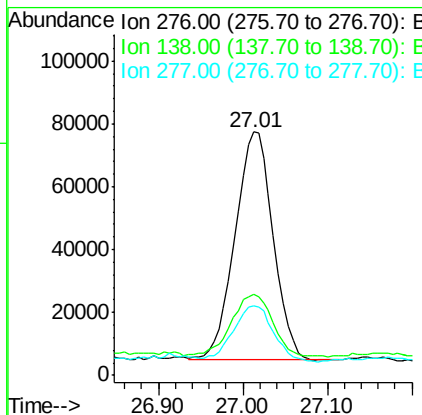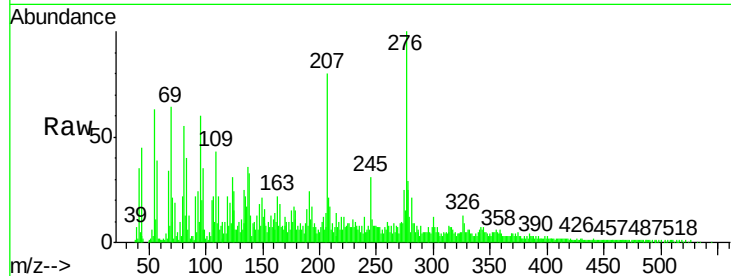

#28

Dibenzo(a,h)anthracene

Concen: 1.518 ng/ul




RT: 27.01 min Scan# 4008


Delta R.T. 0.03 min

Lab File: BN000431.D

Acq: 16 Mar 2018 00:05

Tgt Ion:	278	Resp:	67743
Ion Ratio	Lower	Upper	
278	100		
139	51.5	12.2	18.4#
279	48.5	19.2	28.8#

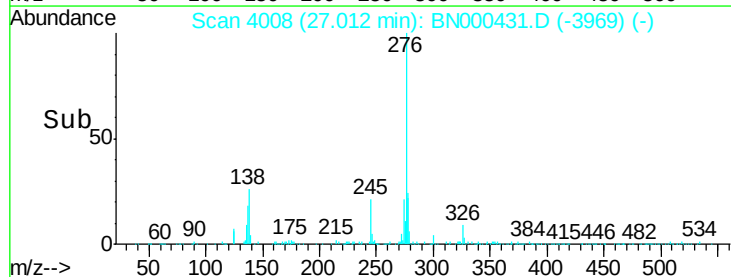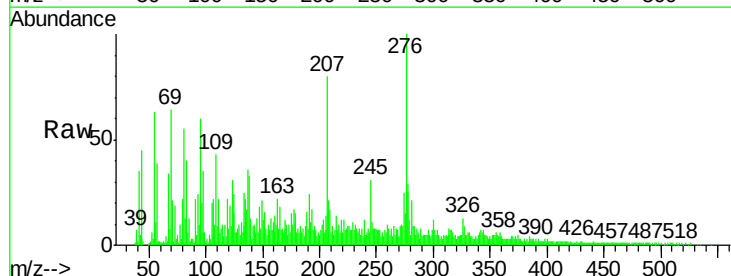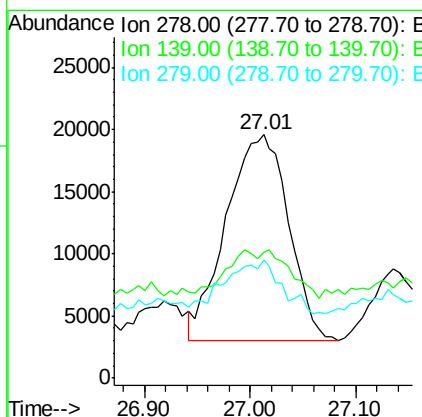

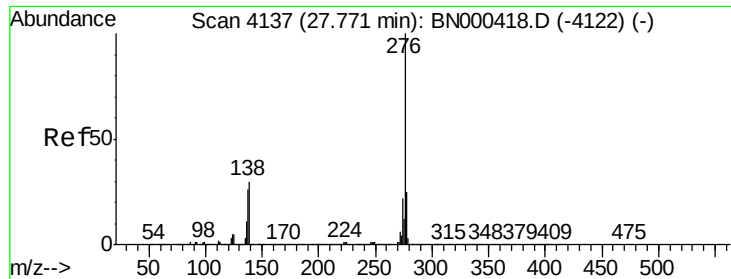

#29

Benzo(a,h,i)perylene

Concen: 4.834 ng/ul

RT: 27.82 min Scan# 4145

Delta R.T. 0.05 min

Lab File: BN000431.D

Acq: 16 Mar 2018 00:05

Instrument :

BNA_N

ClientSampled :

DAMB9

Tot Ion	Ion	Ratio	Lower	Upper
276	100			
138	34.6	15.3	22.9#	
277	28.6	19.0	28.4#	

Manual Integrations
APPROVED

Sohil
3/16/2018 12:12:06 PM

