

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031522\
 Data File : BN018975.D
 Acq On : 16 Mar 2022 08:07
 Operator : CG/JU
 Sample : N1818-01
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBSE7

Quant Time: Mar 16 08:39:07 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN031522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Mar 15 15:17:15 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.893	152	229779	20.000	ng/u1	0.00
20) Naphthalene-d8	10.699	136	979478	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.528	164	642337	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.263	188	1260252	20.000	ng/u1	0.00
79) Chrysene-d12	21.445	240	951987	20.000	ng/u1	0.00
88) Perylene-d12	23.833	264	772437	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.264	96	32429	5.884	ng/uL	0.00
4) Pyridine-d5	3.681	84	321319	21.929	ng/u1	0.00
7) Phenol-d5	7.046	99	574997	29.190	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.211	67	379821	31.040	ng/u1	0.00
11) 2-Chlorophenol-d4	7.416	132	456367	30.386	ng/u1	0.00
15) 4-Methylphenol-d8	8.593	113	477504	30.226	ng/u1	0.00
21) Nitrobenzene-d5	9.052	128	228074	30.463	ng/u1	0.00
24) 2-Nitrophenol-d4	9.775	143	265740	31.955	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.316	165	457952	30.297	ng/u1	0.00
31) 4-Chloroaniline-d4	10.828	131	655048	31.439	ng/u1	0.00
46) Dimethylphthalate-d6	13.934	166	1509399	31.850	ng/u1	0.00
49) Acenaphthylene-d8	14.222	160	1867982	31.938	ng/u1	0.00
54) 4-Nitrophenol-d4	14.704	143	205972	23.676	ng/u1	0.00
60) Fluorene-d10	15.516	176	1262163	31.834	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.628	200	197867	25.582	ng/u1	0.00
73) Anthracene-d10	17.363	188	1890691	32.372	ng/u1	0.00
81) Pyrene-d10	19.657	212	1950544	32.865	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.680	264	1283287	32.574	ng/u1	0.00
Target Compounds						
					Qvalue	
8) Phenol	7.075	94	44458	2.243	ng/u1	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031522\
Data File : BN018975.D
Acq On : 16 Mar 2022 08:07
Operator : CG/JU
Sample : N1818-01
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBSE7


Quant Time: Mar 16 08:39:07 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN031522.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Mar 15 15:17:15 2022
Response via : Initial Calibration

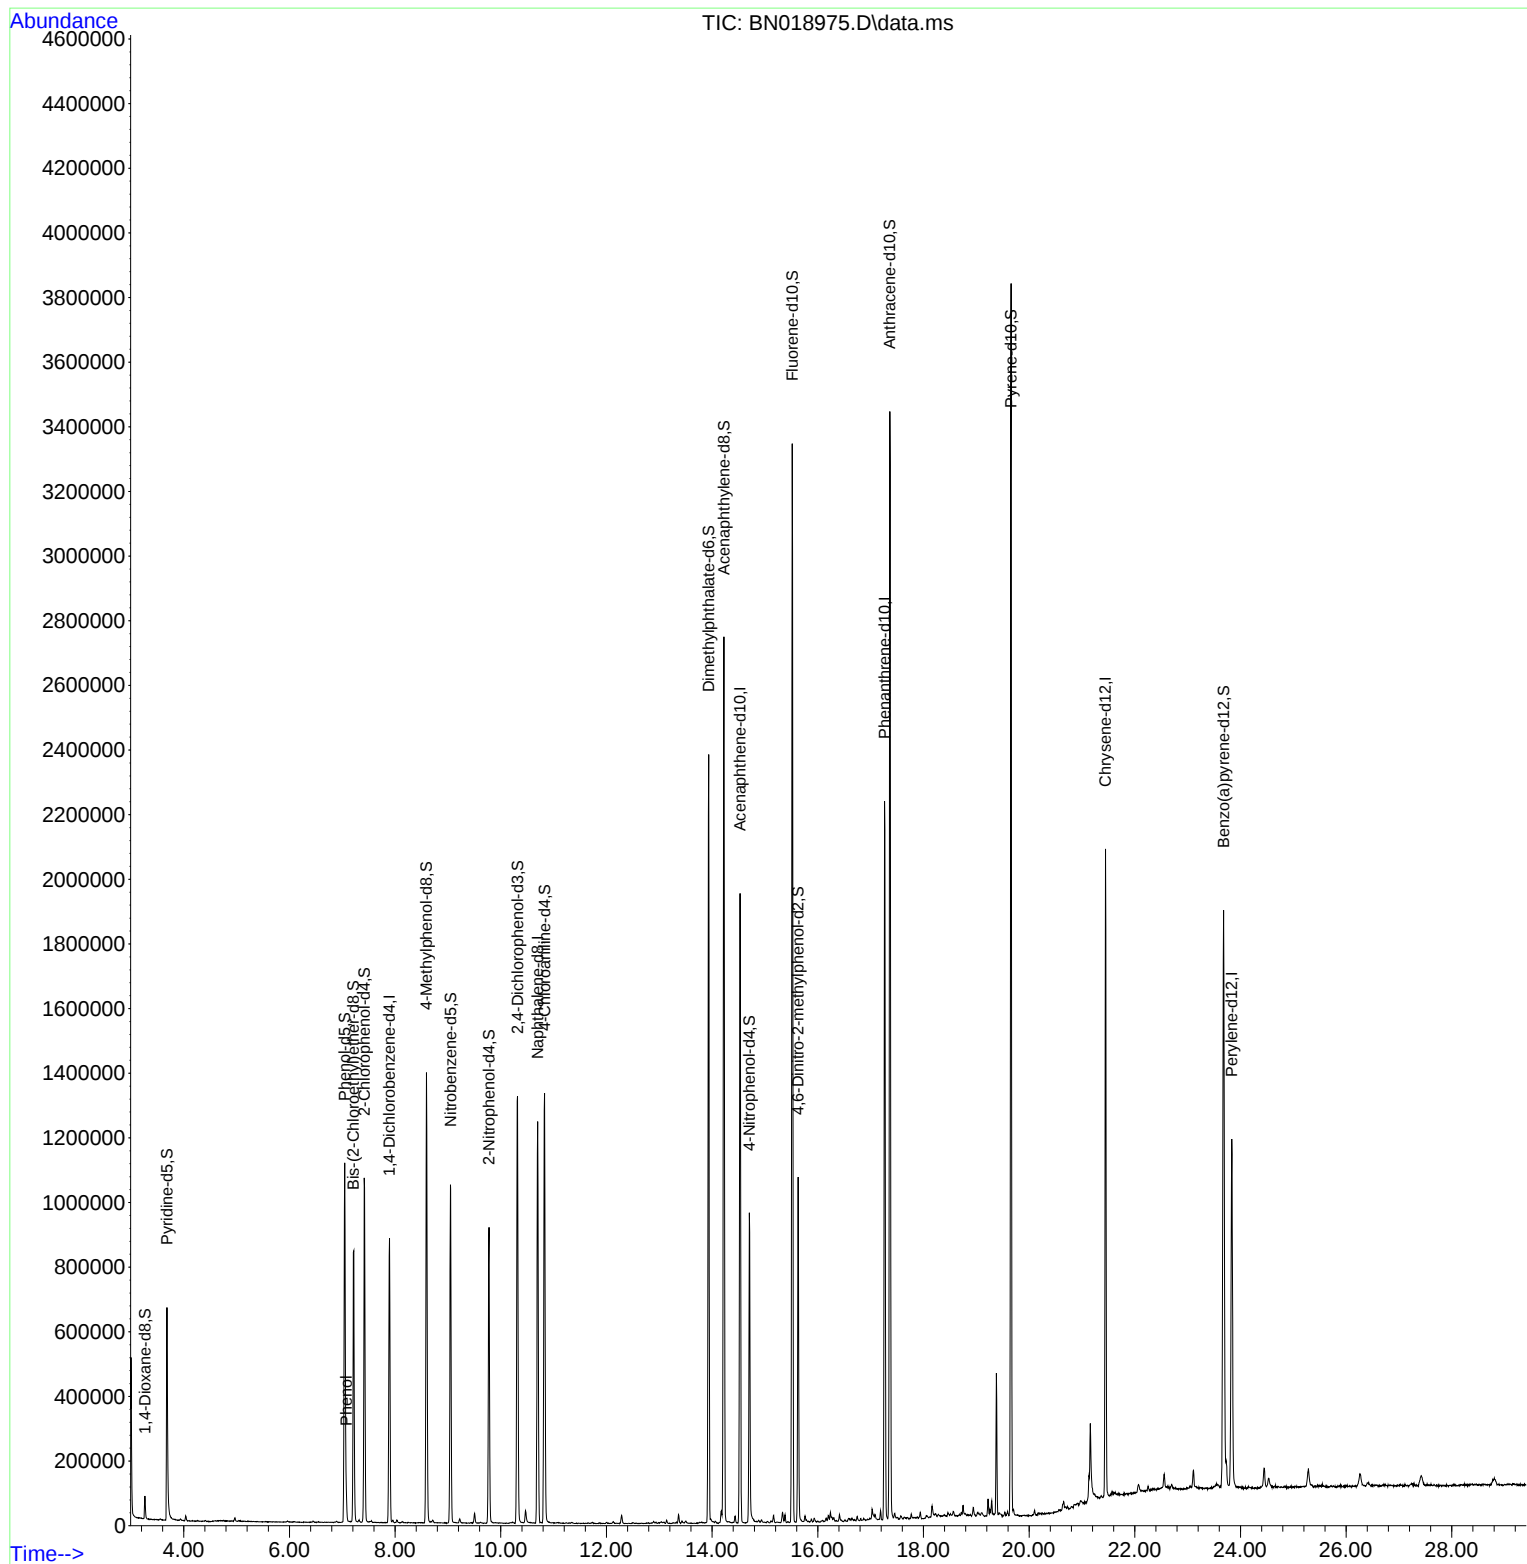

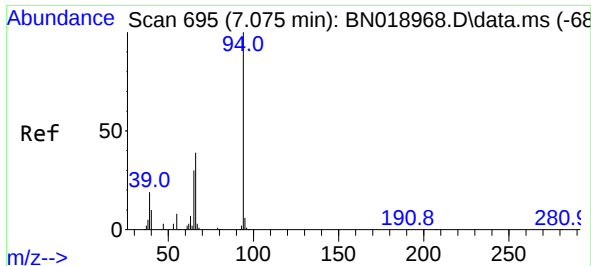

#8
Phenol
Concen: 2.243 ng/ul
RT: 7.075 min Scan# 61
Delta R.T. 0.000 min
Lab File: BN018975.D
Acq: 16 Mar 2022 08:07

Instrument :
BNA_N
ClientSampleId :
DBSE7

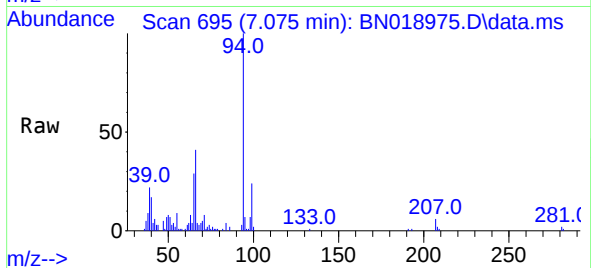

Tgt Ion: 94 Resp: 44458
Ion Ratio Lower Upper
94 100
65 28.8 23.6 35.4
66 41.2 31.2 46.8

