

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031522\
 Data File : BN018982.D
 Acq On : 16 Mar 2022 13:57
 Operator : CG/JU
 Sample : N1693-04
 Misc : GC/MS CONFIRMATION
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BGZM7

Quant Time: Mar 17 01:50:33 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN031522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 17 01:47:21 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.852	152	240884	20.000	ng/ul	-0.04
20) Naphthalene-d8	10.663	136	960242	20.000	ng/ul	-0.04
38) Acenaphthene-d10	14.498	164	646240	20.000	ng/ul	-0.03
64) Phenanthrene-d10	17.234	188	1220335	20.000	ng/ul	-0.04
79) Chrysene-d12	21.416	240	702987	20.000	ng/ul	-0.04
88) Perylene-d12	23.780	264	502496	20.000	ng/ul	-0.05
System Monitoring Compounds						
3) 1,4-Dioxane-d8	0.000	96	0d	0.000	ng/uL	
4) Pyridine-d5	0.000	84	0d	0.000	ng/ul	
7) Phenol-d5	0.000	99	0	0.000	ng/ul	
9) Bis-(2-Chloroethyl)eth...	0.000	67	0d	0.000	ng/ul	
11) 2-Chlorophenol-d4	0.000	132	0	0.000	ng/ul	
15) 4-Methylphenol-d8	0.000	113	0	0.000	ng/ul	
21) Nitrobenzene-d5	0.000	128	0	0.000	ng/ul	
24) 2-Nitrophenol-d4	0.000	143	0	0.000	ng/ul	
28) 2,4-Dichlorophenol-d3	0.000	165	0	0.000	ng/ul	
31) 4-Chloroaniline-d4	0.000	131	0d	0.000	ng/ul	
46) Dimethylphthalate-d6	0.000	166	0	0.000	ng/ul	
49) Acenaphthylene-d8	0.000	160	0	0.000	ng/ul	
54) 4-Nitrophenol-d4	0.000	143	0d	0.000	ng/ul	
60) Fluorene-d10	0.000	176	0	0.000	ng/ul	
65) 4,6-Dinitro-2-methylph...	0.000	200	0	0.000	ng/ul	
73) Anthracene-d10	0.000	188	0d	0.000	ng/ul	
81) Pyrene-d10	0.000	212	0d	0.000	ng/ul	
92) Benzo(a)pyrene-d12	0.000	264	0d	0.000	ng/ul	
Target Compounds						
					Qvalue	
80) Fluoranthene	19.292	202	84714	1.669	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031522\
Data File : BN018982.D
Acq On : 16 Mar 2022 13:57
Operator : CG/JU
Sample : N1693-04
Misc : GC/MS CONFIRMATION
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGZM7

Quant Time: Mar 17 01:50:33 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN031522.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 17 01:47:21 2022
Response via : Initial Calibration

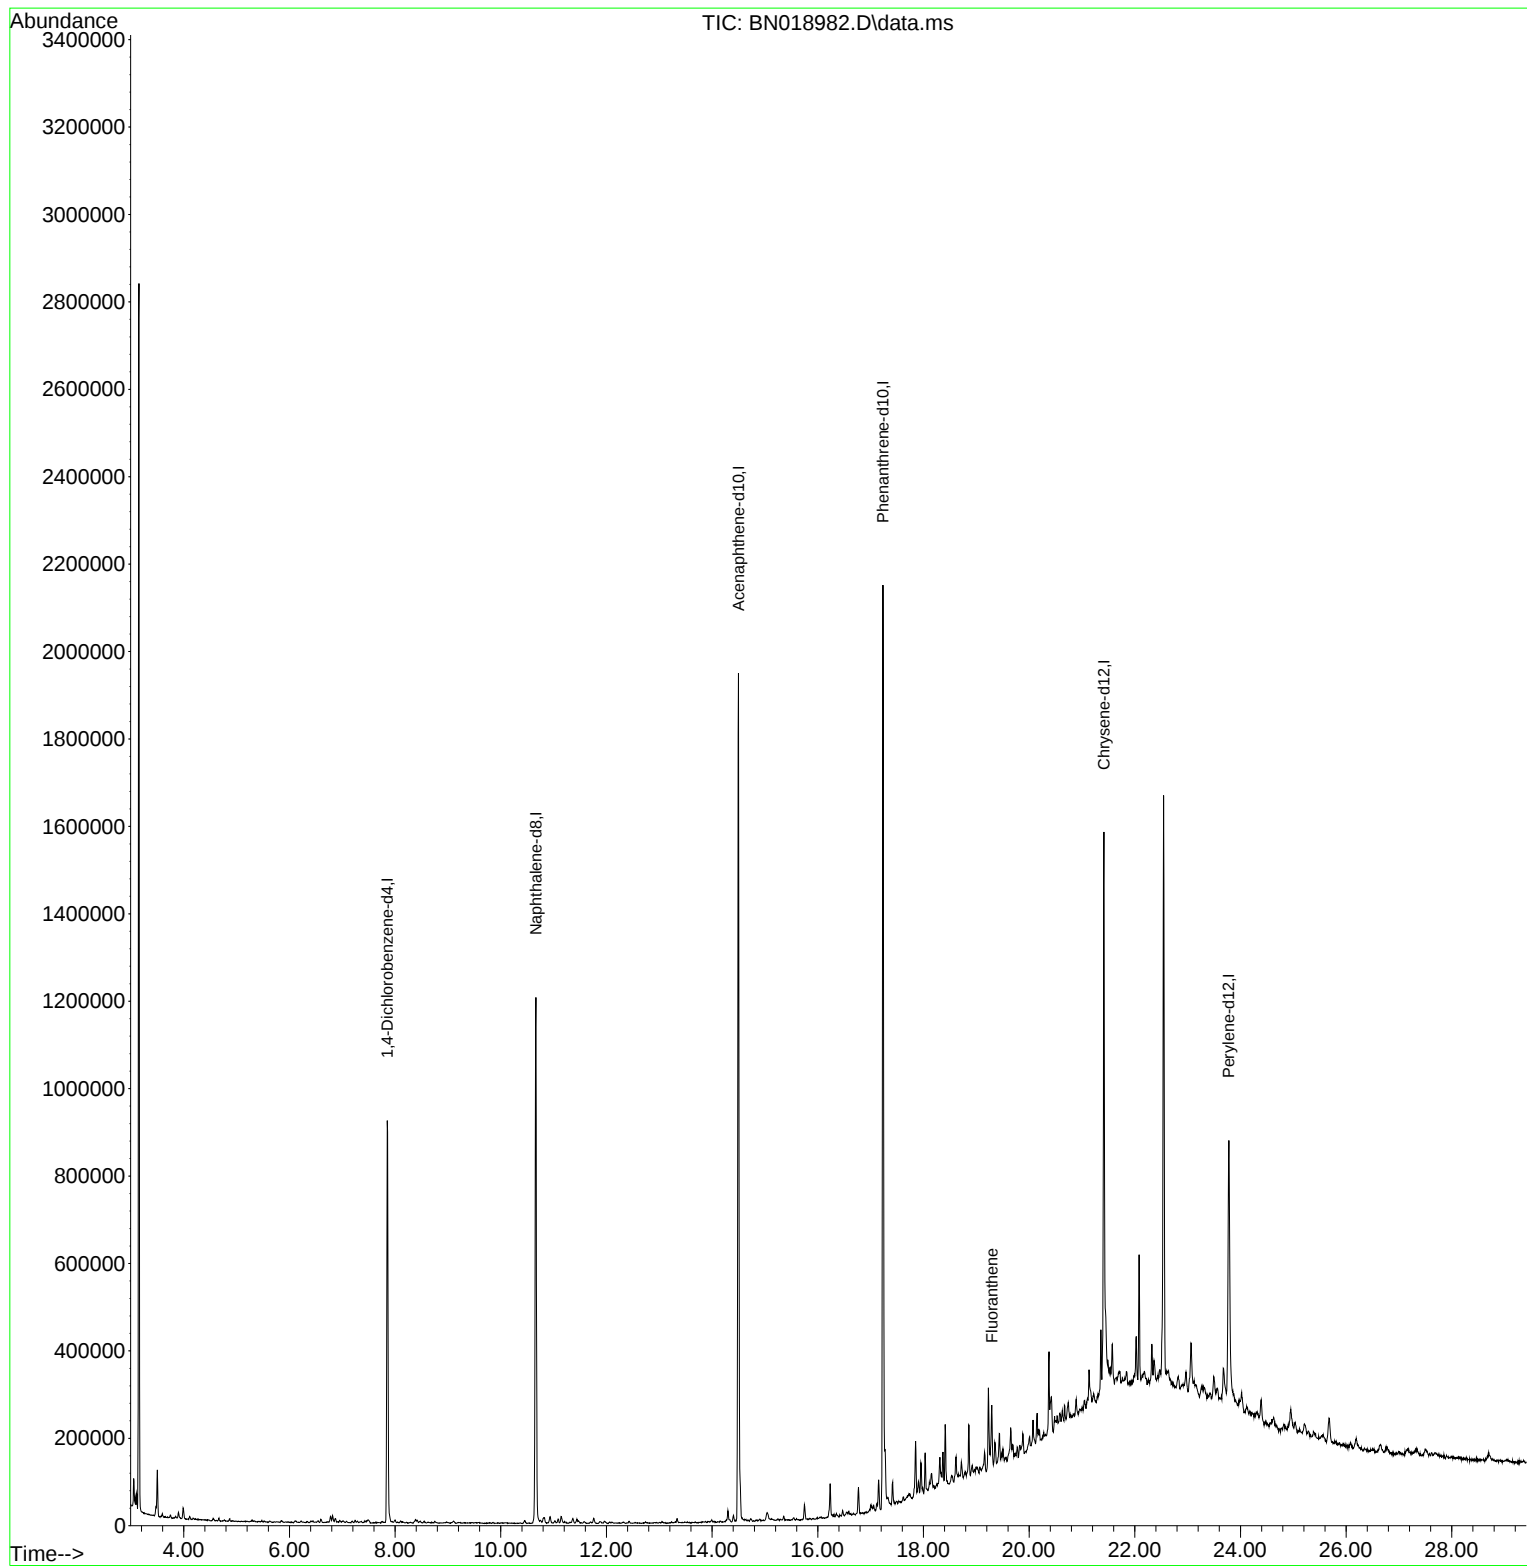

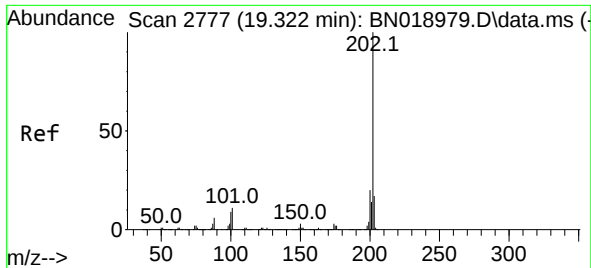

#80
 Fluoranthene
 Concen: 1.669 ng/ul
 RT: 19.292 min Scan# 21
 Delta R.T. -0.029 min
 Lab File: BN018982.D
 Acq: 16 Mar 2022 13:57

Instrument :
 BNA_N
 ClientSampleId :
 BGZM7

Tgt Ion:202 Resp: 84714
 Ion Ratio Lower Upper
 202 100
 101 10.1 8.9 13.3
 100 8.8 6.7 10.1

