

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031522\
 Data File : BN018952.D
 Acq On : 15 Mar 2022 17:44
 Operator : CG/JU
 Sample : PB143210BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK210

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN031522.M
 Title : SVOA CALIBRATION

Signal : TIC: BN018952.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.264	43	47	55	rVB	58879	78820	1.47%	0.139%
2	3.681	114	118	141	rBV	719655	1104737	20.57%	1.944%
3	4.034	174	178	184	rVB2	14067	20380	0.38%	0.036%
4	7.046	683	690	700	rBV	949213	1451849	27.03%	2.555%
5	7.216	712	719	728	rBB	733582	1157957	21.56%	2.038%
6	7.422	747	754	764	rBV	917771	1464128	27.26%	2.576%
7	7.893	827	834	845	rBV	753976	1177570	21.92%	2.072%
8	8.593	946	953	963	rBV	1130188	1811757	33.73%	3.188%
9	9.051	1023	1031	1041	rBV	923409	1483457	27.62%	2.610%
10	9.775	1147	1154	1163	rBV	792838	1279376	23.82%	2.251%
11	10.316	1239	1246	1258	rBV	1160211	1894613	35.27%	3.334%
12	10.698	1303	1311	1320	rBV	1075240	1778222	33.11%	3.129%
13	10.828	1325	1333	1345	rBV	1176099	1976034	36.79%	3.477%
14	12.287	1576	1581	1588	rBV2	18808	30069	0.56%	0.053%
15	13.934	1854	1861	1867	rBV	2141682	2915628	54.28%	5.131%
16	14.222	1903	1910	1928	rBV	2497681	3541635	65.94%	6.232%
17	14.528	1955	1962	1970	rBV	1646090	2457548	45.75%	4.325%
18	14.710	1986	1993	2014	rBV	1026484	1421100	26.46%	2.501%
19	15.522	2123	2131	2140	rBV	2976234	4265897	79.42%	7.507%
20	15.633	2143	2150	2163	rBV	997219	1381760	25.72%	2.431%
21	15.757	2168	2171	2176	rVB	13901	19219	0.36%	0.034%
22	17.057	2385	2392	2395	rBV4	7697	13088	0.24%	0.023%
23	17.269	2421	2428	2438	rBV	2059586	2940226	54.74%	5.174%
24	17.369	2438	2445	2458	rVV	3314049	4621054	86.03%	8.132%
25	19.222	2756	2760	2767	rVB2	41586	54986	1.02%	0.097%
26	19.292	2767	2772	2778	rBV	41330	57855	1.08%	0.102%
27	19.657	2828	2834	2849	rBV	3787431	5371399	100.00%	9.452%
28	20.657	3000	3004	3008	rBV3	23327	28451	0.53%	0.050%
29	21.445	3133	3138	3150	rBV	2373094	3138731	58.43%	5.523%
30	22.063	3240	3243	3248	rVB4	24960	33522	0.62%	0.059%
31	22.557	3324	3327	3332	rVB2	53277	74734	1.39%	0.132%
32	23.110	3417	3421	3428	rVB	89908	142357	2.65%	0.251%
33	23.686	3510	3519	3525	rBV2	2135584	4375042	81.45%	7.699%
34	23.839	3537	3545	3557	rVB2	1318442	2629319	48.95%	4.627%
35	24.451	3643	3649	3657	rVB3	101890	217687	4.05%	0.383%
36	25.286	3786	3791	3801	rVB2	99970	228039	4.25%	0.401%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031522\
Data File : BN018952.D
Acq On : 15 Mar 2022 17:44
Operator : CG/JU
Sample : PB143210BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK210

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN031522.M
Title : SVOA CALIBRATION

37	26.268	3952	3958	3967	rVB4	70316	190158	3.54%	0.335%
----	--------	------	------	------	------	-------	--------	-------	--------




Sum of corrected areas: 56828404

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031522\
Data File : BN018952.D
Acq On : 15 Mar 2022 17:44
Operator : CG/JU
Sample : PB143210BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK210

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN031522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

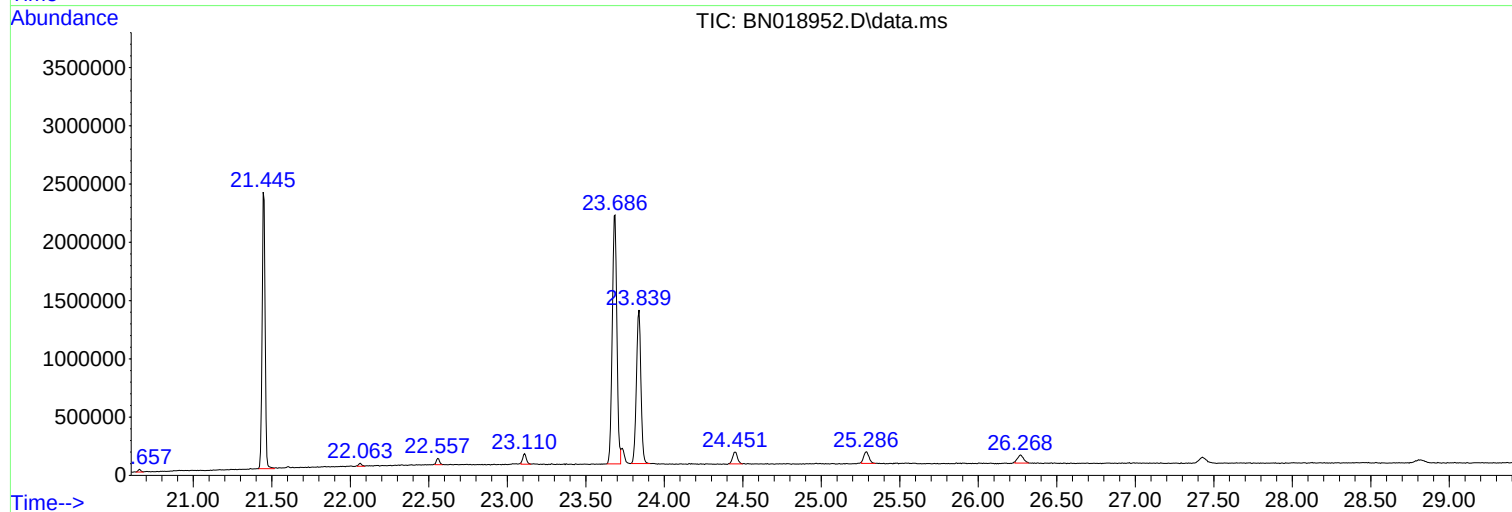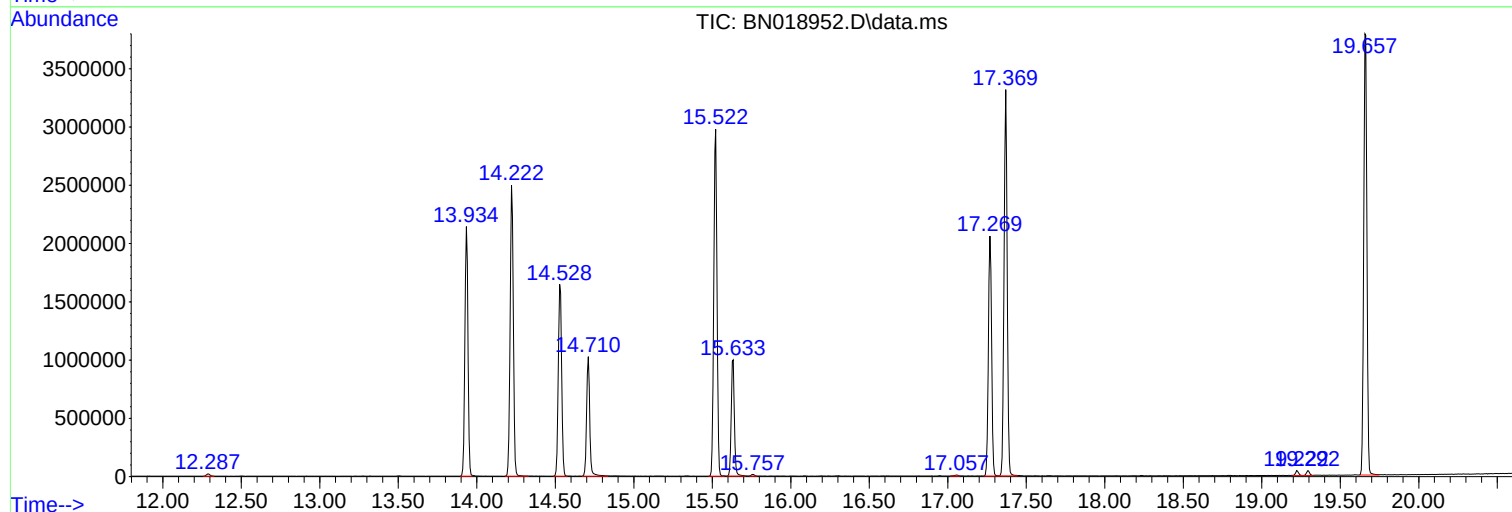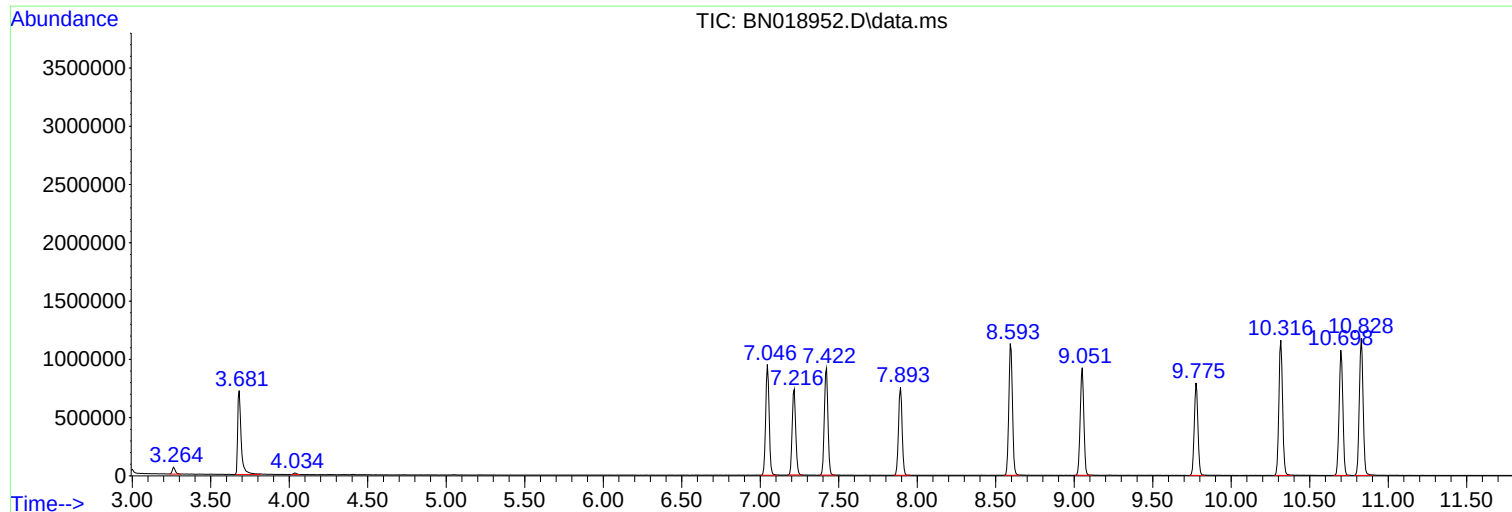

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031522\
Data File : BN018952.D
Acq On : 15 Mar 2022 17:44
Operator : CG/JU
Sample : PB143210BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK210

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN031522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031522\
Data File : BN018952.D
Acq On : 15 Mar 2022 17:44
Operator : CG/JU
Sample : PB143210BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK210

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN031522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------