

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031522\
 Data File : BN018956.D
 Acq On : 15 Mar 2022 20:09
 Operator : CG/JU
 Sample : N1818-19
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBSG7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN031522.M
 Title : SVOA CALIBRATION

Signal : TIC: BN018956.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.264	43	47	60	rVB	57096	80392	1.36%	0.131%
2	3.540	91	94	103	rBV	53664	80639	1.37%	0.131%
3	3.681	114	118	140	rBV	684438	1049931	17.79%	1.706%
4	4.034	174	178	185	rVB	10949	17169	0.29%	0.028%
5	4.405	237	241	250	rVB3	11629	18970	0.32%	0.031%
6	4.969	332	337	341	rBV2	12507	18409	0.31%	0.030%
7	5.199	371	376	381	rBV4	4624	8087	0.14%	0.013%
8	5.963	502	506	509	rVB3	5227	6191	0.10%	0.010%
9	7.046	683	690	703	rBV	1025830	1591712	26.97%	2.586%
10	7.216	712	719	727	rBV	794469	1247168	21.13%	2.026%
11	7.422	746	754	762	rBV	969041	1563770	26.50%	2.540%
12	7.487	762	765	770	rVV2	4952	7522	0.13%	0.012%
13	7.893	827	834	841	rBV	755379	1163892	19.72%	1.891%
14	7.957	841	845	852	rVB4	6310	11550	0.20%	0.019%
15	8.599	946	954	966	rBV	1202192	1986363	33.66%	3.227%
16	8.710	970	973	981	rVB4	5447	9204	0.16%	0.015%
17	9.051	1023	1031	1041	rBV	985301	1572205	26.64%	2.554%
18	9.222	1055	1060	1068	rVB8	7979	13732	0.23%	0.022%
19	9.504	1101	1108	1113	rVB2	13385	19637	0.33%	0.032%
20	9.775	1144	1154	1162	rBV	837406	1353187	22.93%	2.198%
21	10.316	1239	1246	1260	rBV	1285073	2046928	34.68%	3.325%
22	10.469	1266	1272	1289	rBV	209462	336909	5.71%	0.547%
23	10.698	1304	1311	1321	rVB	1041910	1756550	29.76%	2.854%
24	10.828	1324	1333	1344	rBV	1265450	2085185	35.33%	3.388%
25	12.287	1576	1581	1591	rBV2	22404	35830	0.61%	0.058%
26	12.892	1680	1684	1690	rBV5	4074	7058	0.12%	0.011%
27	13.145	1722	1727	1730	rBV2	5543	7555	0.13%	0.012%
28	13.369	1761	1765	1769	rBV2	7253	8898	0.15%	0.014%
29	13.428	1771	1775	1780	rBV4	8342	12653	0.21%	0.021%
30	13.498	1784	1787	1792	rVB4	4345	6400	0.11%	0.010%
31	13.934	1855	1861	1867	rBV	2310627	3090859	52.37%	5.021%
32	14.222	1903	1910	1923	rVB	2601487	3753428	63.59%	6.098%
33	14.434	1942	1946	1951	rVB3	7843	9985	0.17%	0.016%
34	14.528	1954	1962	1972	rBV	1643237	2427280	41.13%	3.943%
35	14.710	1983	1993	2008	rBV	1080043	1536257	26.03%	2.496%
36	14.892	2019	2024	2028	rVB7	4138	7462	0.13%	0.012%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031522\
 Data File : BN018956.D
 Acq On : 15 Mar 2022 20:09
 Operator : CG/JU
 Sample : N1818-19
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBSG7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN031522.M
 Title : SVOA CALIBRATION

37	14.939	2028	2032	2037	rBV7	7052	9874	0.17%	0.016%
38	15.116	2057	2062	2065	rBV6	4283	6899	0.12%	0.011%
39	15.339	2094	2100	2103	rBV3	8053	13231	0.22%	0.021%
40	15.381	2103	2107	2112	rVB2	12166	15443	0.26%	0.025%
41	15.522	2124	2131	2140	rBV	3162330	4569150	77.42%	7.423%
42	15.628	2143	2149	2165	rBV	1040736	1431797	24.26%	2.326%
43	15.757	2167	2171	2176	rBV	15008	23295	0.39%	0.038%
44	15.939	2198	2202	2203	rBV2	5265	6148	0.10%	0.010%
45	15.963	2203	2206	2209	rVB4	7297	9403	0.16%	0.015%
46	16.210	2241	2248	2252	rBV	26061	41778	0.71%	0.068%
47	16.298	2260	2263	2270	rVB7	7519	11469	0.19%	0.019%
48	16.416	2279	2283	2288	rBB6	6243	7684	0.13%	0.012%
49	17.033	2382	2388	2389	rBV5	7928	11165	0.19%	0.018%
50	17.057	2389	2392	2395	rVB3	6209	6998	0.12%	0.011%
51	17.269	2421	2428	2438	rBV	2088345	2921818	49.50%	4.747%
52	17.369	2438	2445	2456	rVV	3475828	4948460	83.84%	8.039%
53	17.451	2456	2459	2464	rVB7	18311	27365	0.46%	0.044%
54	17.639	2488	2491	2497	rVB2	6004	8372	0.14%	0.014%
55	17.945	2537	2543	2547	rBV	45722	56218	0.95%	0.091%
56	18.163	2575	2580	2588	rBV2	36752	62365	1.06%	0.101%
57	18.592	2649	2653	2658	rBV3	15754	18534	0.31%	0.030%
58	19.116	2737	2742	2747	rBV7	19496	27954	0.47%	0.045%
59	19.221	2755	2760	2767	rBV2	46406	68676	1.16%	0.112%
60	19.292	2767	2772	2776	rBV	49669	69727	1.18%	0.113%
61	19.439	2793	2797	2802	rBV7	12842	21081	0.36%	0.034%
62	19.657	2828	2834	2840	rBV	4473313	5902100	100.00%	9.588%
63	20.169	2918	2921	2923	rBV3	7266	8571	0.15%	0.014%
64	20.657	3000	3004	3007	rBV2	23284	28565	0.48%	0.046%
65	21.151	3084	3088	3098	rBV	164780	239595	4.06%	0.389%
66	21.445	3133	3138	3148	rBV	2622715	3207977	54.35%	5.212%
67	22.557	3322	3327	3332	rVB3	50164	82891	1.40%	0.135%
68	23.104	3417	3420	3426	rVB2	73489	108921	1.85%	0.177%
69	23.680	3510	3518	3534	rVB2	2687520	5429132	91.99%	8.820%
70	23.833	3536	3544	3555	rVB2	1416720	2851821	48.32%	4.633%
71	24.445	3643	3648	3655	rVB2	84755	172482	2.92%	0.280%
72	25.286	3785	3791	3802	rVB2	76183	178057	3.02%	0.289%


Sum of corrected areas: 61553983

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031522\
Data File : BN018956.D
Acq On : 15 Mar 2022 20:09
Operator : CG/JU
Sample : N1818-19
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBSG7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN031522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

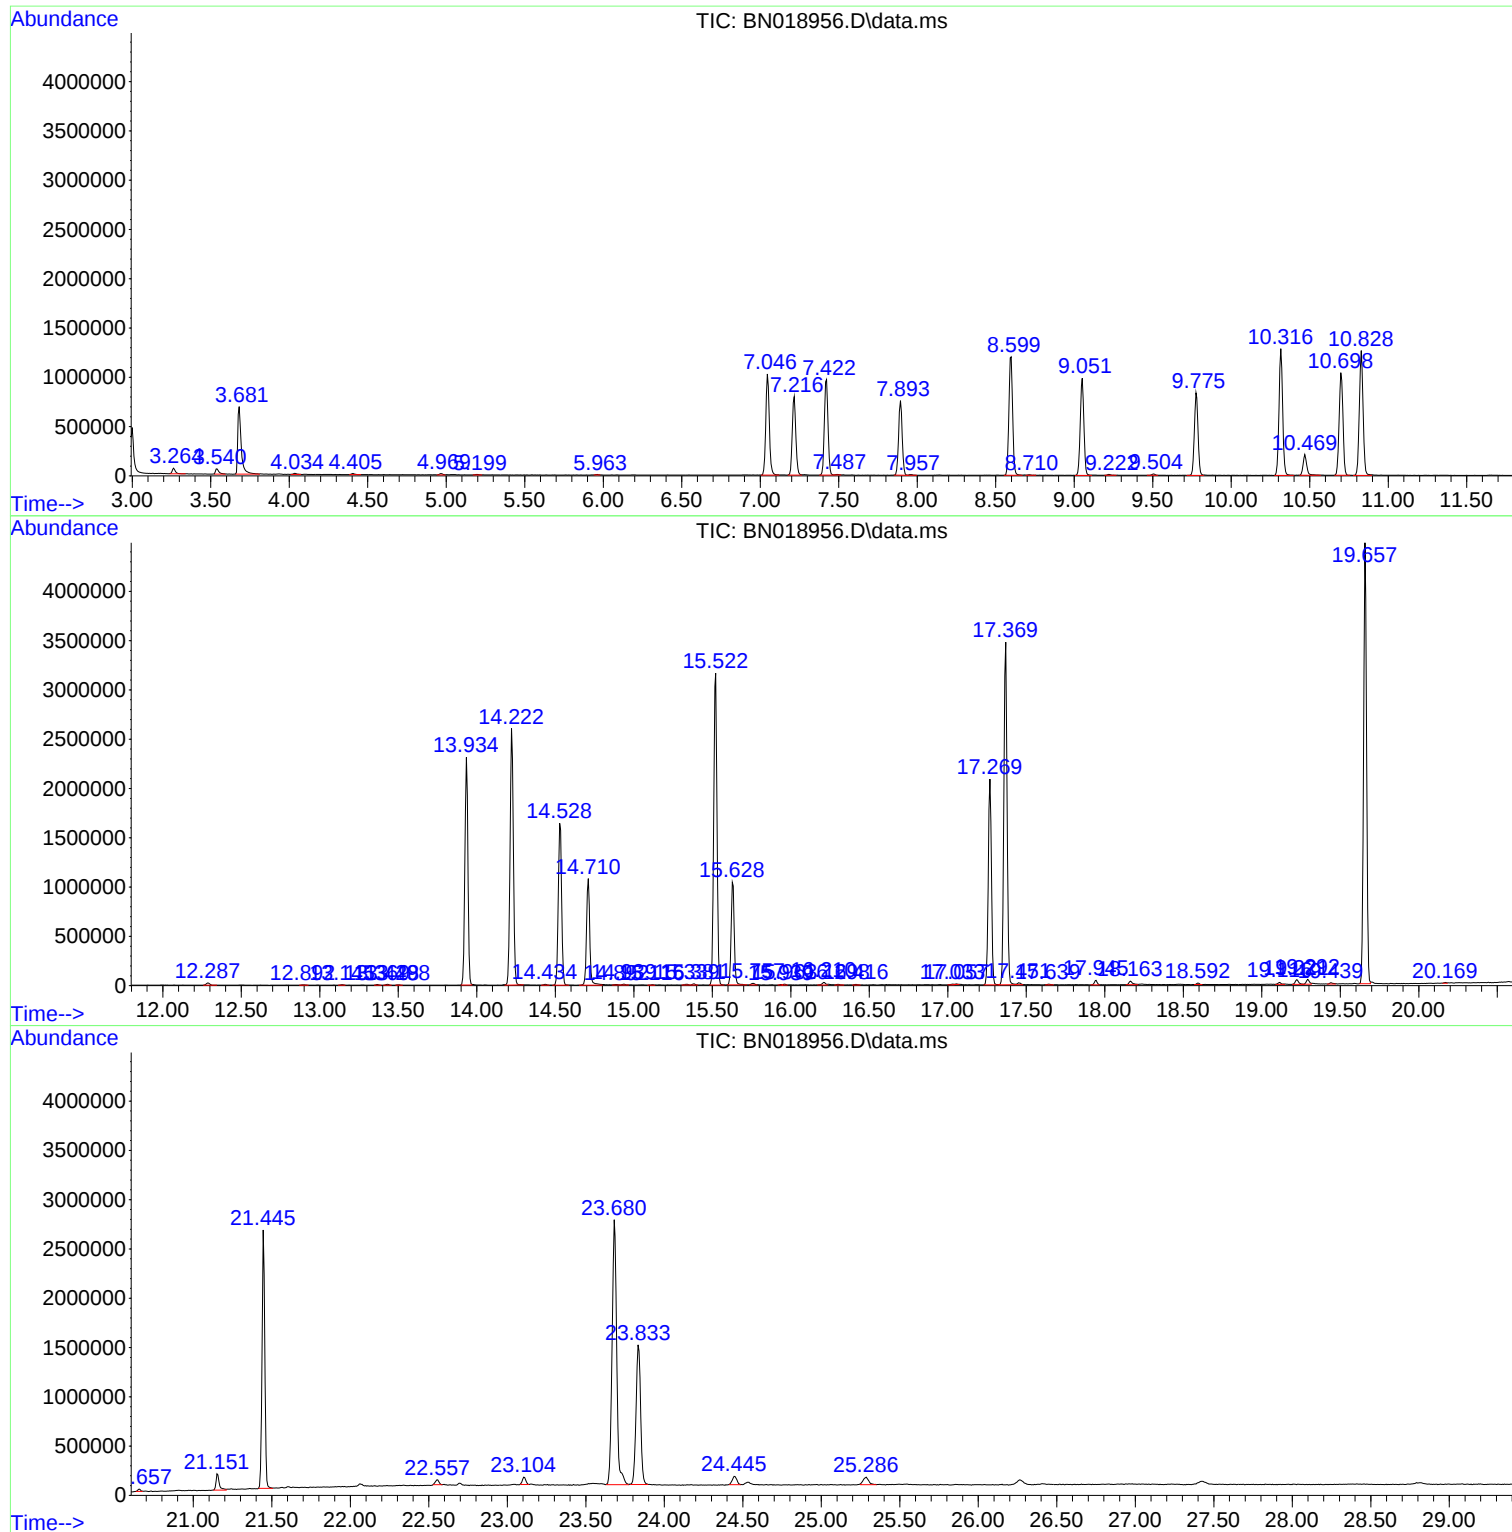

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031522\
Data File : BN018956.D
Acq On : 15 Mar 2022 20:09
Operator : CG/JU
Sample : N1818-19
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBSG7










Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN031522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Ethanol, 2-(2-butoxyethoxy)- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
10.469	3.84 ng/ul	336909	Naphthalene-d8	10.698

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	90
2			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	90
3			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	90
4			Ethanol, 1-(2-butoxyethoxy)-	162	C8H18O3	054446-78-5	83
5			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	72

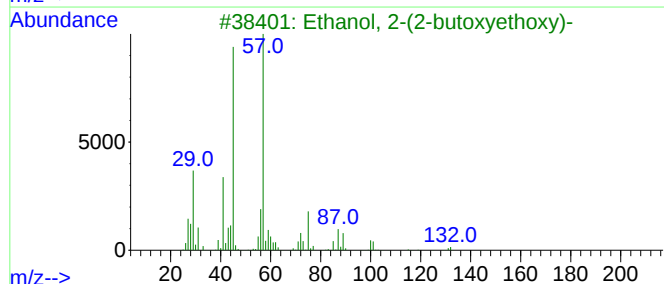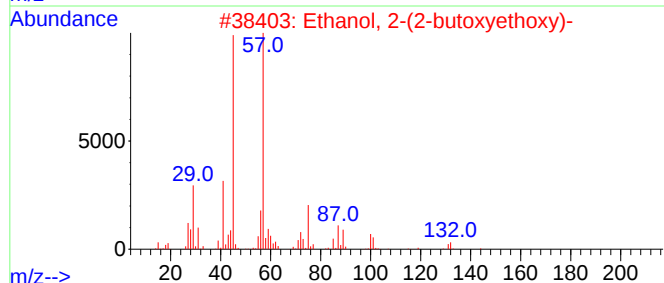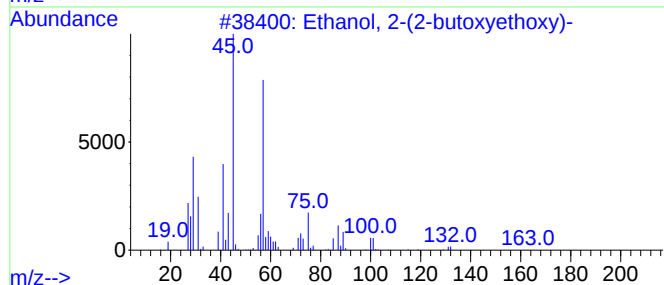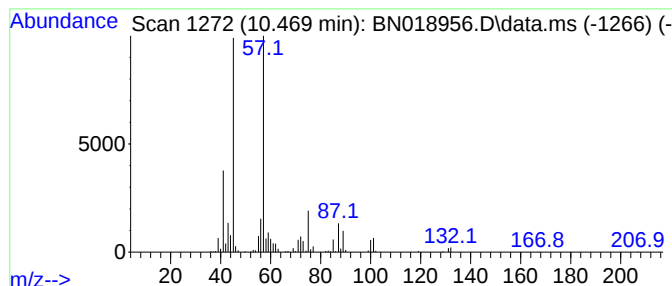

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031522\
Data File : BN018956.D
Acq On : 15 Mar 2022 20:09
Operator : CG/JU
Sample : N1818-19
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBSG7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN031522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Ethanol, 2-(2-b...	10.469	3.8	ng/u1	336909	2	10.698	1756550	20.0