

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031522\
 Data File : BN018959.D
 Acq On : 15 Mar 2022 21:57
 Operator : CG/JU
 Sample : N1818-06
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBSF2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN031522.M
 Title : SVOA CALIBRATION

Signal : TIC: BN018959.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.264	43	47	54	rVB	68263	85118	1.41%	0.128%
2	3.540	90	94	103	rBV	52968	70723	1.17%	0.106%
3	3.681	114	118	137	rBV	769954	1067657	17.65%	1.605%
4	4.034	175	178	186	rVB	16433	23984	0.40%	0.036%
5	4.964	332	336	343	rVB2	13844	22743	0.38%	0.034%
6	5.193	371	375	382	rBV3	7089	12431	0.21%	0.019%
7	6.187	540	544	552	rVB4	6719	12924	0.21%	0.019%
8	7.046	683	690	701	rBV	1120000	1728978	28.58%	2.599%
9	7.216	712	719	727	rBV	948310	1487041	24.58%	2.236%
10	7.422	746	754	765	rBV	1163396	1839861	30.42%	2.766%
11	7.522	765	771	776	rVB7	4849	9271	0.15%	0.014%
12	7.893	827	834	842	rBV	913227	1438393	23.78%	2.162%
13	7.958	842	845	851	rVB2	7211	12436	0.21%	0.019%
14	8.140	870	876	880	rBV7	3285	6365	0.11%	0.010%
15	8.593	946	953	967	rBV	1427495	2293736	37.92%	3.448%
16	9.052	1023	1031	1038	rBV	1175226	1886587	31.19%	2.836%
17	9.222	1054	1060	1067	rVB6	7775	13807	0.23%	0.021%
18	9.505	1103	1108	1116	rVB2	14295	22544	0.37%	0.034%
19	9.775	1146	1154	1162	rBV	998630	1609547	26.61%	2.420%
20	10.316	1238	1246	1258	rBV	1469113	2412722	39.89%	3.627%
21	10.469	1266	1272	1281	rBV	76054	127190	2.10%	0.191%
22	10.699	1303	1311	1322	rBV	1291281	2149825	35.54%	3.232%
23	10.828	1324	1333	1345	rBV	1500506	2504156	41.40%	3.765%
24	12.287	1576	1581	1587	rBV2	28808	43885	0.73%	0.066%
25	12.899	1679	1685	1691	rVB5	3928	7269	0.12%	0.011%
26	13.146	1723	1727	1732	rVB2	4508	7316	0.12%	0.011%
27	13.369	1761	1765	1770	rBV3	7206	10124	0.17%	0.015%
28	13.428	1770	1775	1782	rVV3	10564	16506	0.27%	0.025%
29	13.499	1782	1787	1795	rVB5	5109	10014	0.17%	0.015%
30	13.934	1852	1861	1867	rBV	2697791	3643962	60.24%	5.478%
31	14.222	1903	1910	1925	rVB	2926910	4400678	72.75%	6.616%
32	14.434	1943	1946	1950	rVB5	6967	8593	0.14%	0.013%
33	14.528	1954	1962	1973	rBV	1958776	2899225	47.93%	4.359%
34	14.710	1981	1993	2014	rBV	827239	1218807	20.15%	1.832%
35	14.881	2018	2022	2027	rVB7	4250	8497	0.14%	0.013%
36	14.940	2027	2032	2035	rBV4	10793	14759	0.24%	0.022%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031522\
 Data File : BN018959.D
 Acq On : 15 Mar 2022 21:57
 Operator : CG/JU
 Sample : N1818-06
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBSF2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN031522.M
 Title : SVOA CALIBRATION

37	15.122	2058	2063	2067	rBV6	3844	6993	0.12%	0.011%
38	15.334	2092	2099	2104	rBV3	11334	20772	0.34%	0.031%
39	15.381	2104	2107	2112	rVB	19576	24387	0.40%	0.037%
40	15.522	2124	2131	2143	rVB	3590389	5276401	87.23%	7.933%

41	15.628	2143	2149	2164	rBV	910780	1241894	20.53%	1.867%
42	15.757	2167	2171	2176	rBV	18707	25974	0.43%	0.039%
43	15.875	2187	2191	2196	rBV5	4254	7170	0.12%	0.011%
44	15.934	2198	2201	2203	rVV4	5613	7421	0.12%	0.011%
45	15.957	2203	2205	2209	rVB4	5383	7221	0.12%	0.011%

46	16.210	2242	2248	2251	rBV3	26419	38312	0.63%	0.058%
47	16.240	2251	2253	2256	rVV2	8540	9870	0.16%	0.015%
48	16.298	2260	2263	2269	rVB8	6597	10756	0.18%	0.016%
49	16.410	2278	2282	2287	rVB6	6408	11265	0.19%	0.017%
50	16.945	2370	2373	2377	rBV5	4732	6328	0.10%	0.010%

51	17.034	2383	2388	2390	rBV4	11746	19736	0.33%	0.030%
52	17.269	2421	2428	2436	rBV	2399216	3377318	55.83%	5.077%
53	17.369	2438	2445	2456	rVV	3849138	5579101	92.23%	8.388%
54	17.451	2456	2459	2466	rVB3	19822	29276	0.48%	0.044%
55	17.645	2488	2492	2497	rBV7	5242	6913	0.11%	0.010%

56	17.939	2538	2542	2547	rVB	33387	42181	0.70%	0.063%
57	18.163	2574	2580	2588	rBV3	23213	40842	0.68%	0.061%
58	18.234	2589	2592	2595	rVB2	4940	7001	0.12%	0.011%
59	18.592	2649	2653	2657	rVB2	20260	22964	0.38%	0.035%
60	19.116	2738	2742	2745	rVB4	20373	23788	0.39%	0.036%

61	19.222	2756	2760	2768	rBV3	53170	69004	1.14%	0.104%
62	19.292	2768	2772	2777	rBV	51805	71399	1.18%	0.107%
63	19.445	2794	2798	2801	rBV4	4487	6295	0.10%	0.009%
64	19.592	2820	2823	2826	rBV4	7666	8563	0.14%	0.013%
65	19.657	2828	2834	2840	rVV	4559535	6049020	100.00%	9.094%

66	19.698	2840	2841	2850	rVB3	22579	29988	0.50%	0.045%
67	20.169	2918	2921	2922	rBV3	6699	7529	0.12%	0.011%
68	20.251	2931	2935	2938	rBV6	5218	8642	0.14%	0.013%
69	20.657	3000	3004	3007	rBV2	20263	23675	0.39%	0.036%
70	21.151	3084	3088	3095	rBV	133403	180285	2.98%	0.271%

71	21.445	3133	3138	3146	rBV	2425635	2994541	49.50%	4.502%
72	22.063	3240	3243	3248	rVB4	25528	35958	0.59%	0.054%
73	22.551	3321	3326	3333	rBV4	79297	161031	2.66%	0.242%
74	23.110	3417	3421	3428	rVB	77517	119314	1.97%	0.179%
75	23.680	3510	3518	3525	rBV	2355200	4724959	78.11%	7.104%

76	23.839	3537	3545	3558	rVB2	1331730	2686161	44.41%	4.038%
----	--------	------	------	------	------	---------	---------	--------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031522\
Data File : BN018959.D
Acq On : 15 Mar 2022 21:57
Operator : CG/JU
Sample : N1818-06
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBSF2

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN031522.M
Title : SVOA CALIBRATION

77	24.451	3644	3649	3657	rVB	90606	175568	2.90%	0.264%
78	25.280	3786	3790	3801	rVB3	76538	192370	3.18%	0.289%


Sum of corrected areas: 66515860

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031522\
Data File : BN018959.D
Acq On : 15 Mar 2022 21:57
Operator : CG/JU
Sample : N1818-06
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBSF2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN031522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

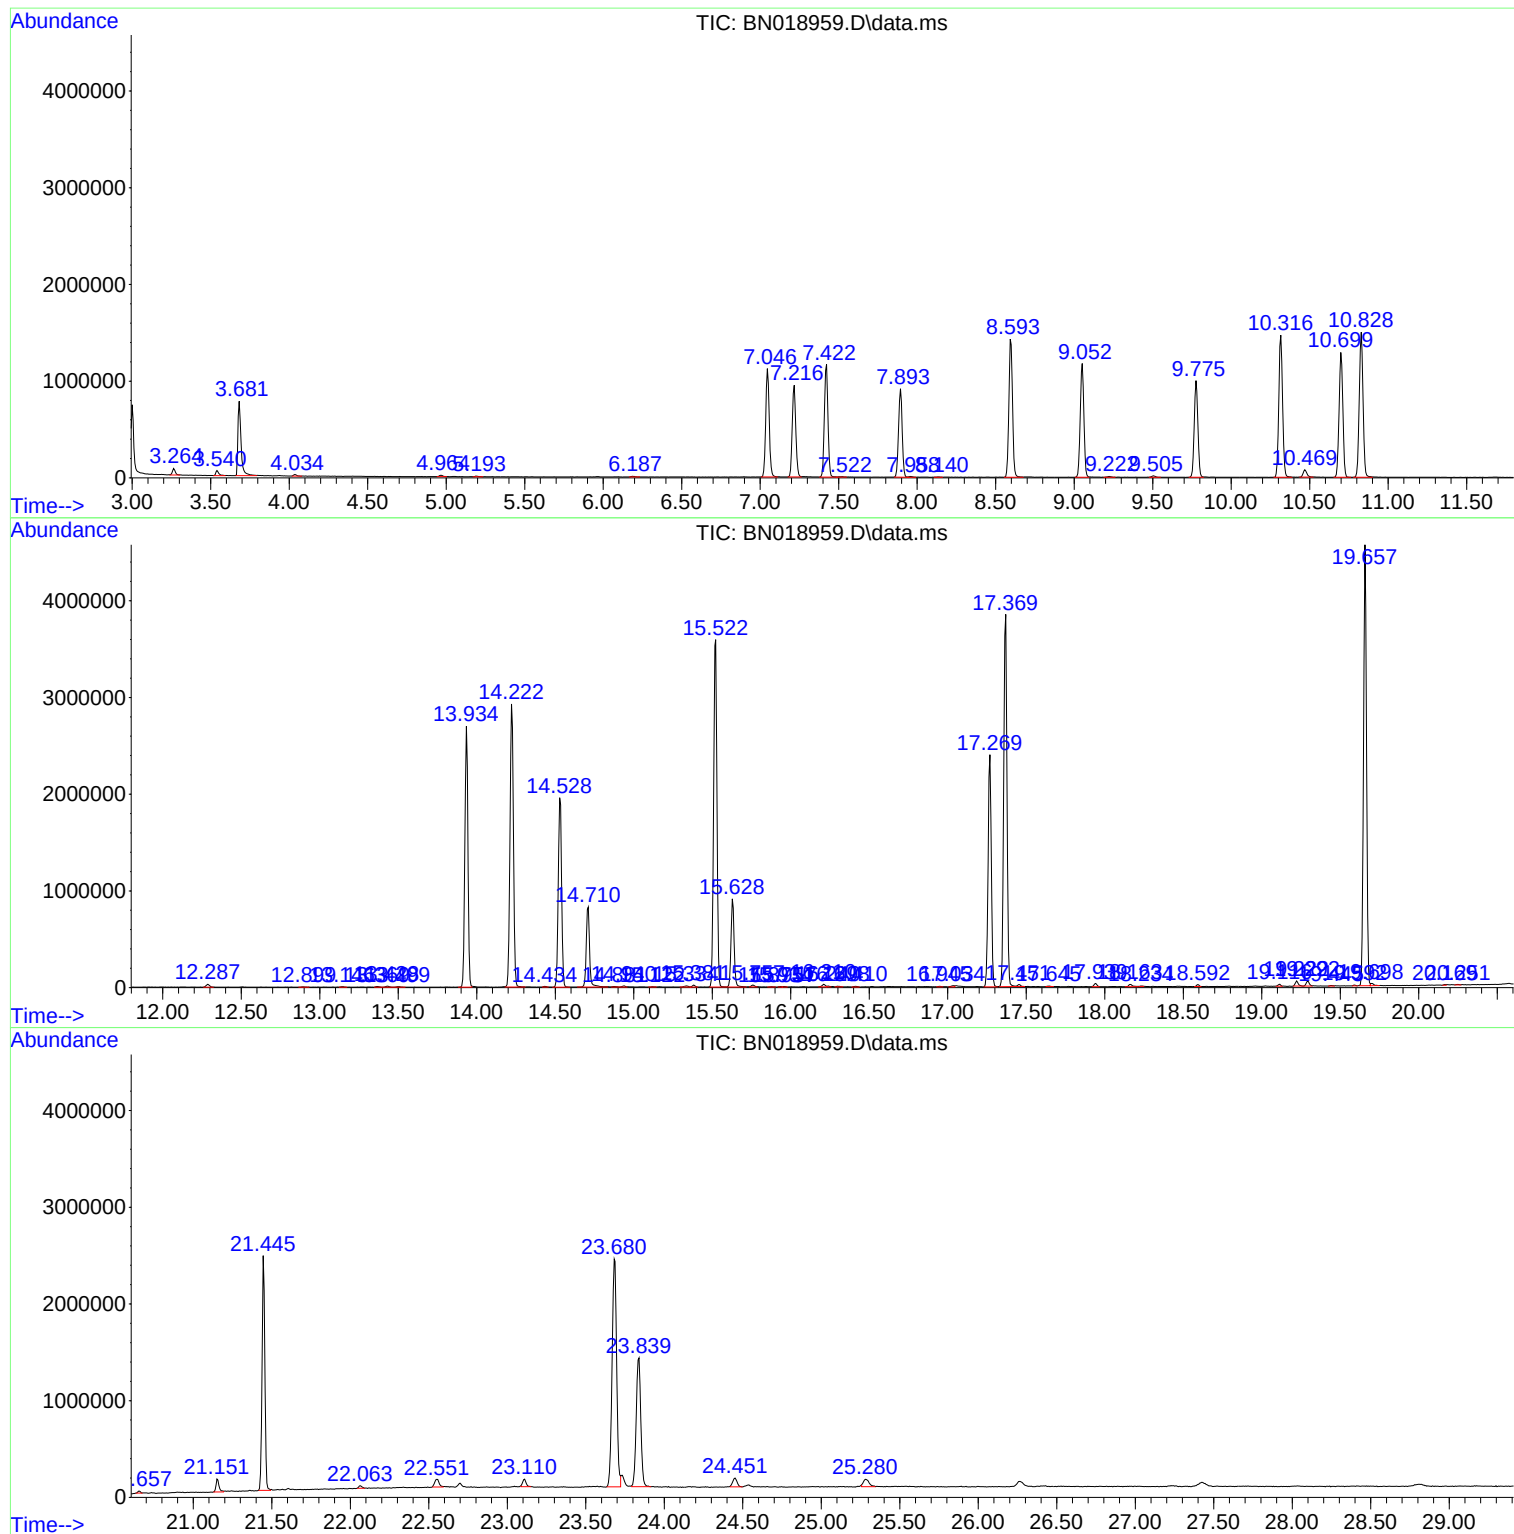

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031522\
Data File : BN018959.D
Acq On : 15 Mar 2022 21:57
Operator : CG/JU
Sample : N1818-06
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBSF2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN031522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031522\
Data File : BN018959.D
Acq On : 15 Mar 2022 21:57
Operator : CG/JU
Sample : N1818-06
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBSF2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN031522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc