

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031522\
 Data File : BN018967.D
 Acq On : 16 Mar 2022 02:45
 Operator : CG/JU
 Sample : N1818-16
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBSG4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN031522.M
 Title : SVOA CALIBRATION

Signal : TIC: BN018967.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.264	43	47	55	rVB	46846	64344	1.40%	0.120%
2	3.540	90	94	101	rBV	32949	47966	1.04%	0.090%
3	3.681	114	118	142	rBV	583430	903207	19.63%	1.688%
4	4.034	174	178	183	rBV	12812	17948	0.39%	0.034%
5	4.964	331	336	342	rVB3	10042	16098	0.35%	0.030%
6	5.193	371	375	380	rVB6	3049	5087	0.11%	0.010%
7	5.958	502	505	513	rVB2	7526	13362	0.29%	0.025%
8	7.046	683	690	703	rBV	797812	1257275	27.33%	2.350%
9	7.211	712	718	727	rBV	618533	977599	21.25%	1.827%
10	7.281	727	730	737	rVB	4842	8069	0.18%	0.015%
11	7.417	745	753	762	rBV	791073	1233506	26.81%	2.305%
12	7.487	762	765	768	rVB4	4390	6136	0.13%	0.011%
13	7.893	827	834	841	rBV	879739	1388179	30.18%	2.594%
14	7.958	841	845	851	rVB3	8943	13775	0.30%	0.026%
15	8.134	871	875	879	rBV4	4872	6842	0.15%	0.013%
16	8.593	946	953	966	rBV	985069	1546461	33.62%	2.890%
17	8.716	969	974	980	rVB4	5671	11323	0.25%	0.021%
18	9.046	1023	1030	1042	rBV	757960	1227574	26.69%	2.294%
19	9.222	1055	1060	1069	rBV7	7179	14677	0.32%	0.027%
20	9.505	1103	1108	1114	rVB2	13371	21554	0.47%	0.040%
21	9.775	1145	1154	1167	rBV	663454	1057976	23.00%	1.977%
22	10.316	1238	1246	1256	rBV	945033	1592789	34.62%	2.977%
23	10.469	1264	1272	1283	rBV	160302	271442	5.90%	0.507%
24	10.699	1303	1311	1320	rVB	1230185	2079783	45.21%	3.887%
25	10.828	1324	1333	1345	rBV	970262	1647883	35.82%	3.080%
26	11.346	1417	1421	1426	rVB7	2587	4770	0.10%	0.009%
27	12.128	1550	1554	1559	rVB2	10306	15852	0.34%	0.030%
28	12.287	1576	1581	1586	rBV2	16231	26624	0.58%	0.050%
29	13.146	1720	1727	1730	rBV6	3586	5711	0.12%	0.011%
30	13.363	1760	1764	1769	rBV2	13848	19727	0.43%	0.037%
31	13.428	1769	1775	1783	rVV4	6531	11268	0.24%	0.021%
32	13.499	1783	1787	1794	rVB4	5263	9042	0.20%	0.017%
33	13.934	1854	1861	1867	rBV	1791991	2461572	53.51%	4.600%
34	14.175	1898	1902	1903	rBV3	4161	4616	0.10%	0.009%
35	14.222	1903	1910	1925	rVB	1964027	2942315	63.96%	5.499%
36	14.434	1939	1946	1955	rBV7	6636	12670	0.28%	0.024%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031522\
 Data File : BN018967.D
 Acq On : 16 Mar 2022 02:45
 Operator : CG/JU
 Sample : N1818-16
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBSG4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN031522.M
 Title : SVOA CALIBRATION

37	14.528	1955	1962	1972	rBV	1938174	2857184	62.11%	5.340%
38	14.704	1984	1992	2015	rBV	724299	1026813	22.32%	1.919%
39	14.940	2027	2032	2037	rBV6	6398	9853	0.21%	0.018%
40	15.051	2045	2051	2058	rVB9	1907	5307	0.12%	0.010%
41	15.116	2058	2062	2066	rBV5	3097	5170	0.11%	0.010%
42	15.328	2094	2098	2103	rBV6	4968	8244	0.18%	0.015%
43	15.381	2103	2107	2112	rVB	8609	10831	0.24%	0.020%
44	15.516	2123	2130	2138	rBV	2583202	3635472	79.03%	6.794%
45	15.628	2141	2149	2158	rBV	715418	929115	20.20%	1.736%
46	15.757	2167	2171	2175	rBV3	11658	16233	0.35%	0.030%
47	15.963	2203	2206	2209	rVB4	5345	6850	0.15%	0.013%
48	16.204	2241	2247	2250	rBV7	5285	8836	0.19%	0.017%
49	16.240	2250	2253	2256	rVV5	5478	7828	0.17%	0.015%
50	16.304	2260	2264	2269	rVB7	6142	9337	0.20%	0.017%
51	16.410	2279	2282	2288	rVB6	5059	8158	0.18%	0.015%
52	16.516	2296	2300	2305	rVB3	5467	7378	0.16%	0.014%
53	17.028	2383	2387	2389	rBV5	6074	7778	0.17%	0.015%
54	17.051	2389	2391	2394	rVV2	10513	14527	0.32%	0.027%
55	17.081	2394	2396	2401	rVB6	4929	6620	0.14%	0.012%
56	17.269	2421	2428	2437	rBV	2365605	3429657	74.55%	6.410%
57	17.363	2437	2444	2456	rVV2	2795180	3943969	85.73%	7.371%
58	17.451	2456	2459	2464	rVB6	19862	26909	0.58%	0.050%
59	17.645	2486	2492	2493	rBV6	4353	6563	0.14%	0.012%
60	17.939	2538	2542	2546	rBV	22104	26759	0.58%	0.050%
61	18.163	2575	2580	2589	rBV3	28739	52706	1.15%	0.099%
62	18.234	2589	2592	2597	rVB4	5174	8096	0.18%	0.015%
63	18.592	2649	2653	2660	rBV3	18042	21421	0.47%	0.040%
64	19.110	2737	2741	2746	rVB6	11637	15980	0.35%	0.030%
65	19.222	2755	2760	2768	rBV2	34395	50071	1.09%	0.094%
66	19.292	2768	2772	2775	rBV	41388	57083	1.24%	0.107%
67	19.434	2793	2796	2800	rBV6	6351	10261	0.22%	0.019%
68	19.586	2820	2822	2827	rVB6	8390	8337	0.18%	0.016%
69	19.657	2827	2834	2839	rBV	3421212	4600224	100.00%	8.597%
70	19.704	2839	2842	2849	rVB3	33029	42216	0.92%	0.079%
71	20.175	2918	2922	2923	rBV4	6323	8573	0.19%	0.016%
72	20.551	2983	2986	2987	rBV3	10100	10436	0.23%	0.020%
73	20.651	3000	3003	3006	rBV2	20972	21556	0.47%	0.040%
74	20.728	3014	3016	3021	rVB5	14170	13506	0.29%	0.025%
75	21.151	3084	3088	3096	rBV2	128715	176467	3.84%	0.330%
76	21.445	3132	3138	3150	rBV	2855888	3714809	80.75%	6.943%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031522\
Data File : BN018967.D
Acq On : 16 Mar 2022 02:45
Operator : CG/JU
Sample : N1818-16
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBSG4

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN031522.M
Title : SVOA CALIBRATION

77	21.598	3162	3164	3168	rBV5	14300	14540	0.32%	0.027%
78	23.104	3416	3420	3424	rVB	74407	108073	2.35%	0.202%
79	23.674	3509	3517	3524	rBV2	2005773	3992161	86.78%	7.461%
80	23.833	3536	3544	3554	rVB2	1626593	3310189	71.96%	6.186%
81	24.439	3643	3647	3656	rVB	85178	159917	3.48%	0.299%
82	25.280	3786	3790	3798	rVB2	69794	150794	3.28%	0.282%




Sum of corrected areas: 53507829

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031522\
Data File : BN018967.D
Acq On : 16 Mar 2022 02:45
Operator : CG/JU
Sample : N1818-16
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBSG4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN031522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

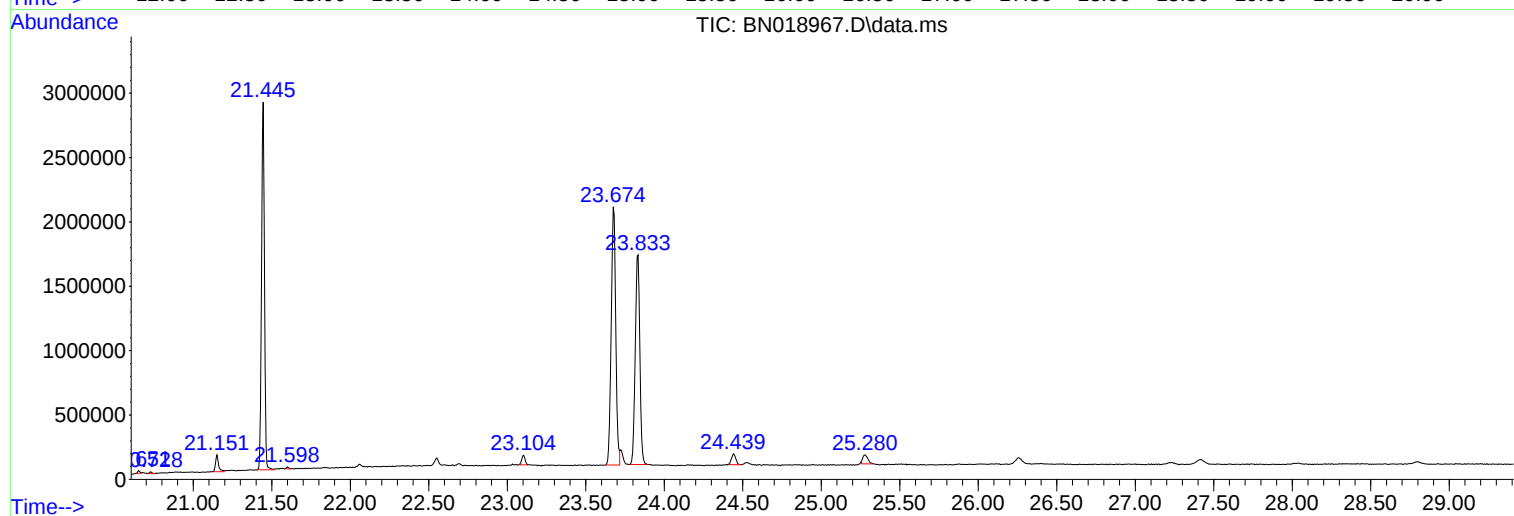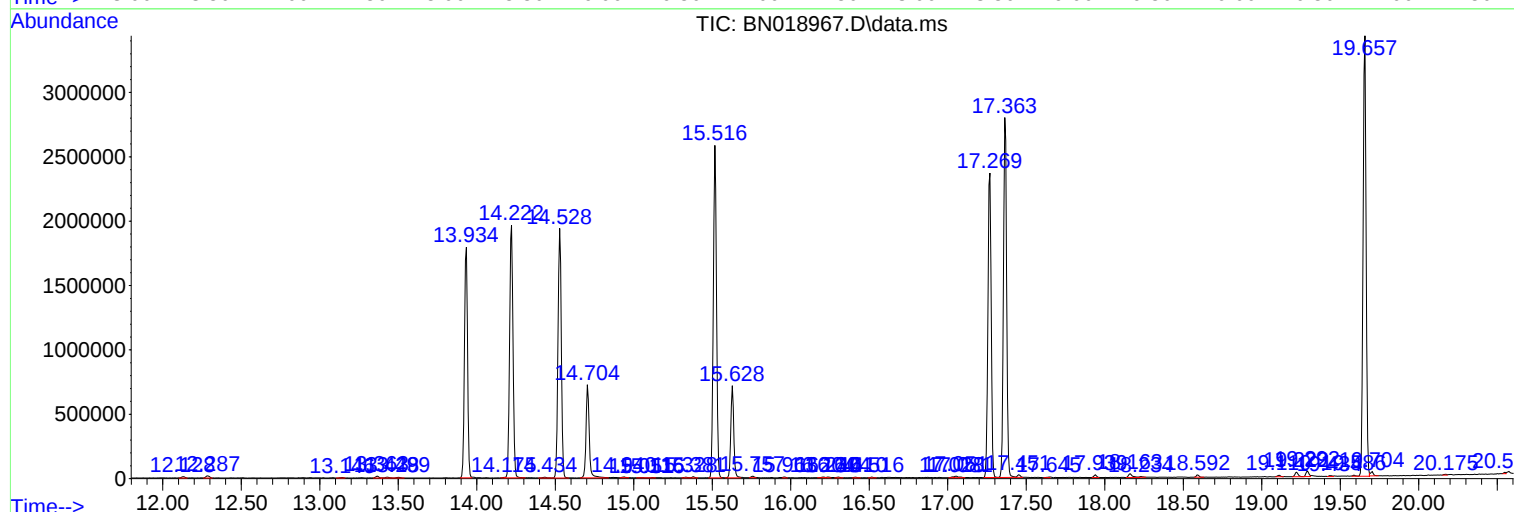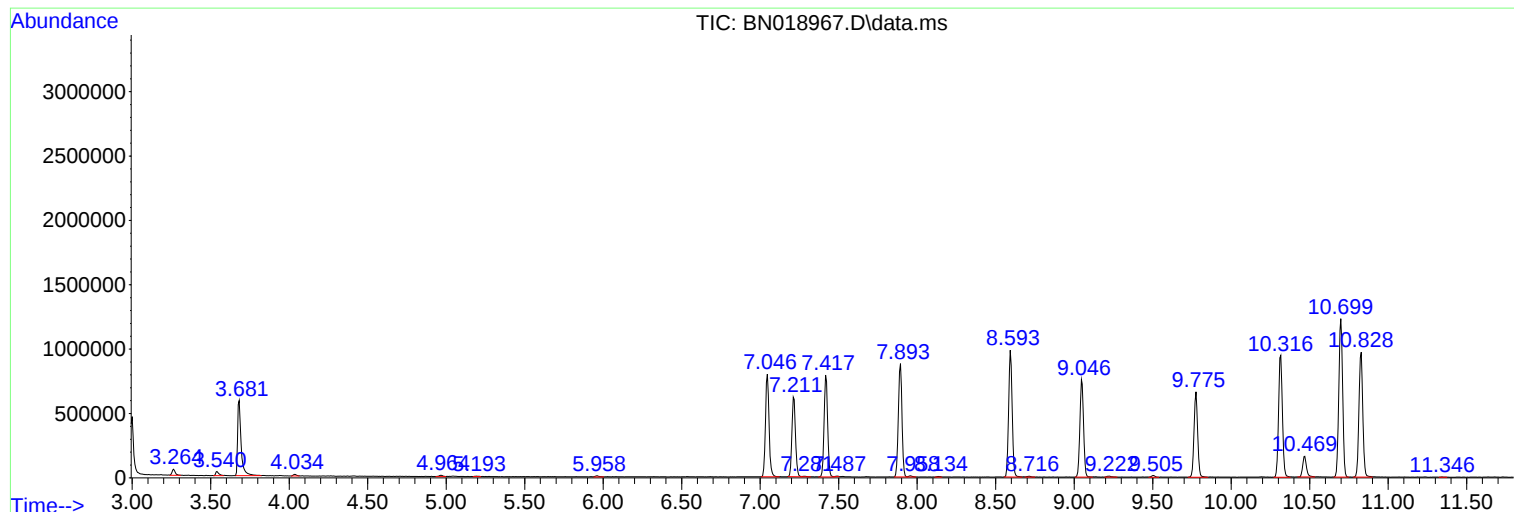

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031522\
Data File : BN018967.D
Acq On : 16 Mar 2022 02:45
Operator : CG/JU
Sample : N1818-16
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBSG4










Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN031522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Ethanol, 2-(2-butoxyethoxy)- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
10.469	2.61 ng/ul	271442	Naphthalene-d8	10.699

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	90
2			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	90
3			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	90
4			Ethanol, 1-(2-butoxyethoxy)-	162	C8H18O3	054446-78-5	83
5			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	72

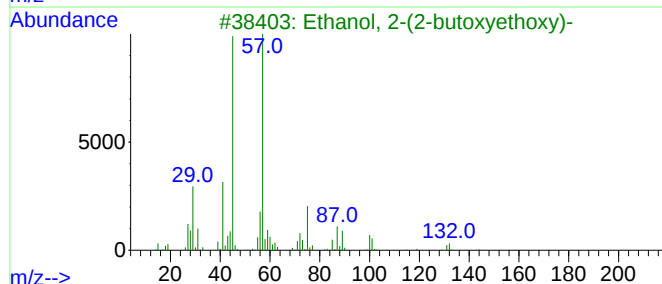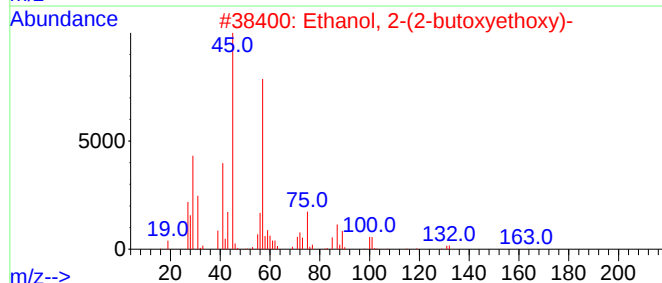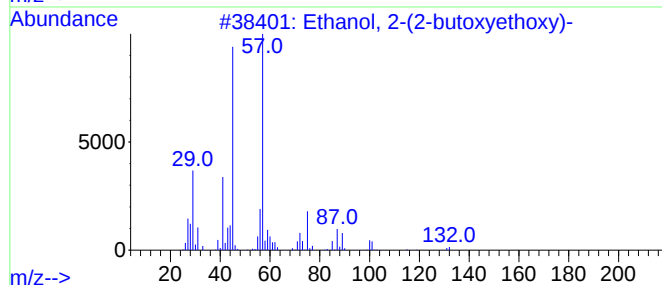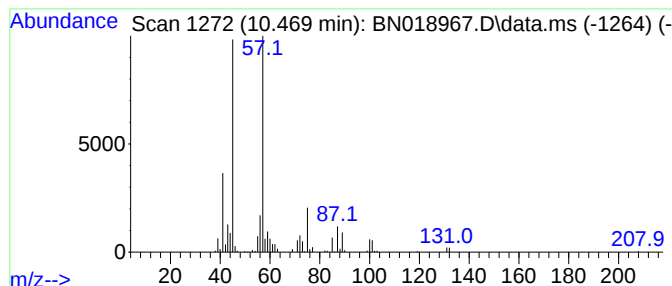

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031522\
Data File : BN018967.D
Acq On : 16 Mar 2022 02:45
Operator : CG/JU
Sample : N1818-16
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBSG4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN031522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Ethanol, 2-(2-b...	10.469	2.6	ng/u1	271442	2	10.699	2079780	20.0