

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031522\
 Data File : BN018969.D
 Acq On : 16 Mar 2022 04:32
 Operator : CG/JU
 Sample : PB143210BL
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK210

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN031522.M
 Title : SVOA CALIBRATION

Signal : TIC: BN018969.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.264	42	47	54	rVB	61276	83174	1.47%	0.138%
2	3.681	114	118	135	rBV	743150	1148906	20.34%	1.909%
3	4.034	175	178	183	rVB	13510	18218	0.32%	0.030%
4	4.264	214	217	221	rVB5	4724	6048	0.11%	0.010%
5	7.046	683	690	704	rBV	989883	1528469	27.07%	2.540%
6	7.211	712	718	730	rVB	761800	1231528	21.81%	2.047%
7	7.416	747	753	761	rBV	959212	1532245	27.13%	2.547%
8	7.893	824	834	843	rBV	741601	1180229	20.90%	1.962%
9	8.593	946	953	964	rBV	1223721	1929724	34.17%	3.207%
10	9.046	1023	1030	1040	rBV	963500	1570308	27.81%	2.610%
11	9.775	1145	1154	1165	rBV	842653	1366334	24.19%	2.271%
12	10.316	1238	1246	1256	rBV	1191009	2018038	35.73%	3.354%
13	10.699	1303	1311	1319	rVB	1095245	1806999	32.00%	3.003%
14	10.828	1325	1333	1354	rBV	1234836	2117556	37.50%	3.519%
15	12.287	1573	1581	1588	rBV2	22722	35941	0.64%	0.060%
16	13.934	1854	1861	1871	rBV	2345480	3180532	56.32%	5.286%
17	14.222	1903	1910	1922	rBV	2557734	3766304	66.69%	6.260%
18	14.528	1955	1962	1971	rBV	1882927	2680608	47.47%	4.455%
19	14.704	1986	1992	2010	rBV	1050532	1490508	26.39%	2.477%
20	15.516	2123	2130	2140	rBV	3234454	4607885	81.59%	7.658%
21	15.628	2143	2149	2163	rVV	1148611	1495589	26.48%	2.486%
22	15.757	2167	2171	2176	rVB3	14835	21937	0.39%	0.036%
23	16.951	2371	2374	2377	rVB4	4718	6032	0.11%	0.010%
24	17.051	2384	2391	2396	rBV2	9456	17709	0.31%	0.029%
25	17.269	2421	2428	2437	rBV	2354918	3271828	57.94%	5.438%
26	17.363	2438	2444	2457	rVV2	3423579	4952902	87.70%	8.232%
27	19.222	2755	2760	2765	rBV	43678	57324	1.02%	0.095%
28	19.292	2767	2772	2778	rBV	45782	60230	1.07%	0.100%
29	19.657	2827	2834	2849	rBV	4150001	5647386	100.00%	9.386%
30	20.651	3000	3003	3008	rVB3	19179	20828	0.37%	0.035%
31	21.445	3132	3138	3147	rBV	2604481	3366864	59.62%	5.596%
32	22.551	3323	3326	3331	rVB	54384	66850	1.18%	0.111%
33	23.104	3416	3420	3426	rVB	95372	150122	2.66%	0.250%
34	23.674	3509	3517	3524	rBV2	2290347	4532405	80.26%	7.533%
35	23.833	3536	3544	3557	rVB2	1355951	2771999	49.08%	4.607%
36	24.439	3642	3647	3655	rVB2	101519	208646	3.69%	0.347%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031522\
Data File : BN018969.D
Acq On : 16 Mar 2022 04:32
Operator : CG/JU
Sample : PB143210BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK210

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN031522.M
Title : SVOA CALIBRATION

37	25.274	3784	3789	3798	rVB	93277	219721	3.89%	0.365%
----	--------	------	------	------	-----	-------	--------	-------	--------




Sum of corrected areas: 60167926

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031522\
Data File : BN018969.D
Acq On : 16 Mar 2022 04:32
Operator : CG/JU
Sample : PB143210BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK210

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN031522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

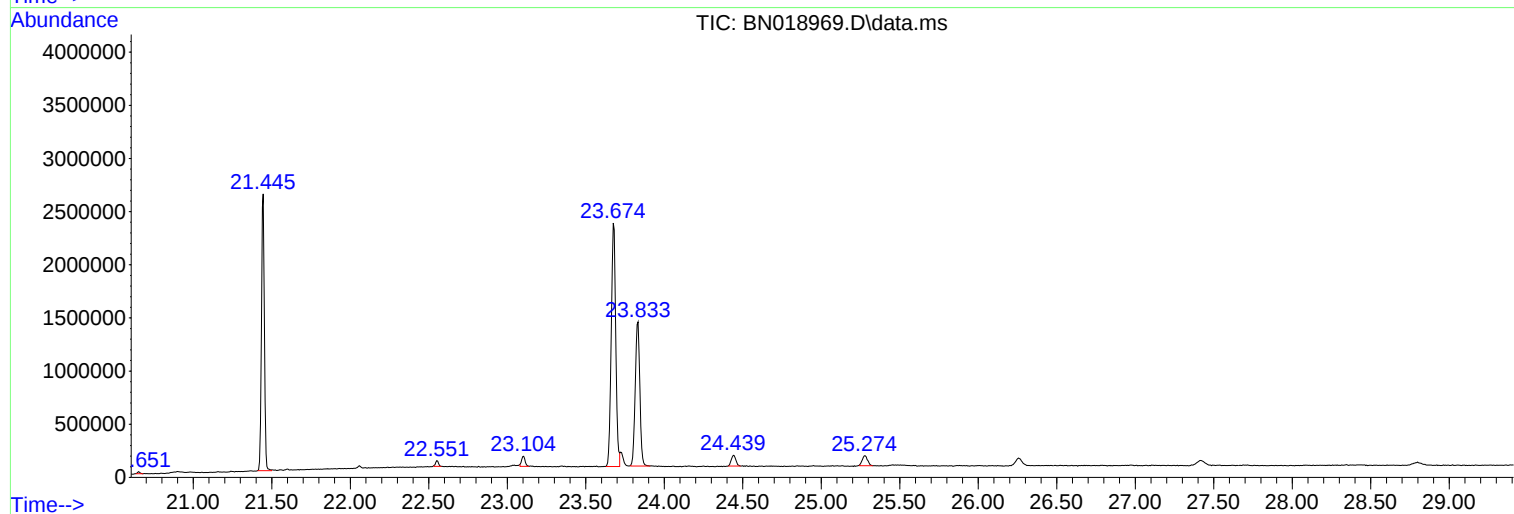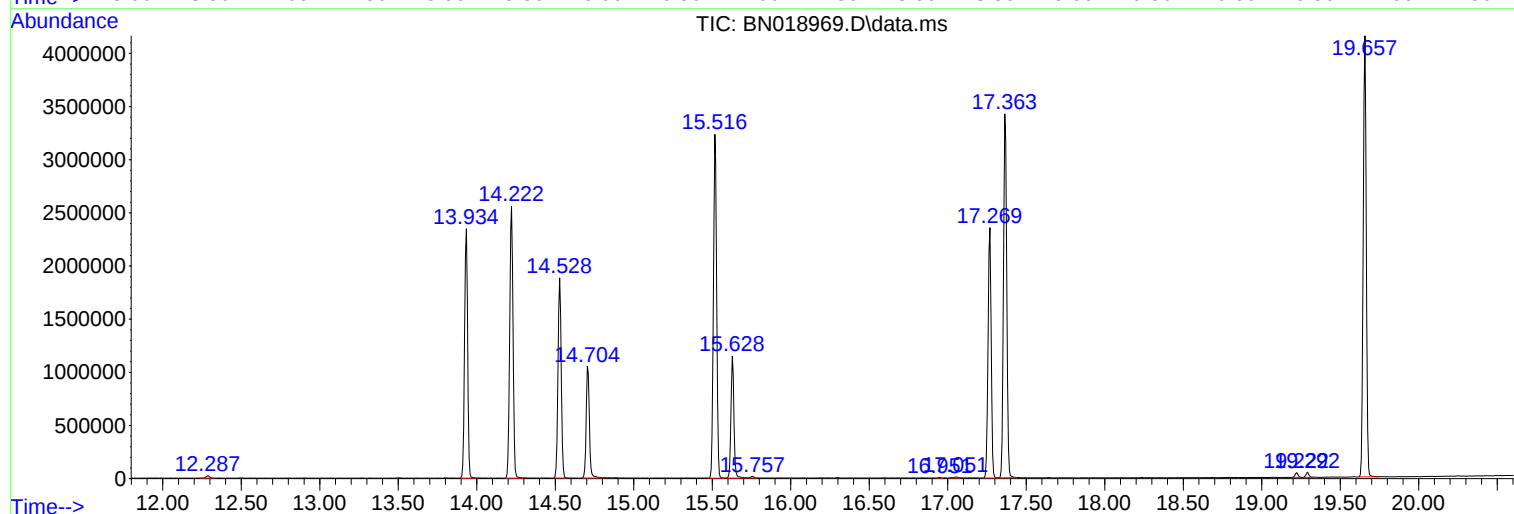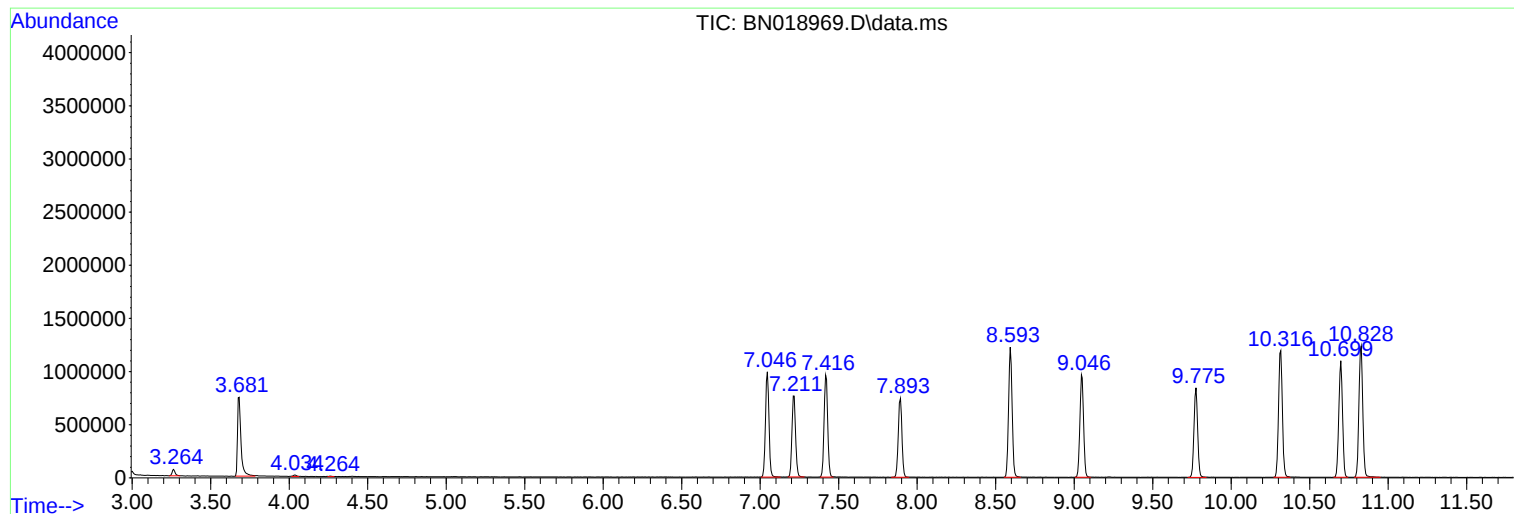

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031522\
Data File : BN018969.D
Acq On : 16 Mar 2022 04:32
Operator : CG/JU
Sample : PB143210BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK210

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN031522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031522\
Data File : BN018969.D
Acq On : 16 Mar 2022 04:32
Operator : CG/JU
Sample : PB143210BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK210

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN031522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------