

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031522\
 Data File : BN018974.D
 Acq On : 16 Mar 2022 07:31
 Operator : CG/JU
 Sample : N1818-15
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBSF9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN031522.M
 Title : SVOA CALIBRATION

Signal : TIC: BN018974.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.264	43	47	54	rVB	66398	83249	1.30%	0.123%
2	3.540	90	94	102	rBV	68323	95494	1.49%	0.141%
3	3.681	114	118	142	rBV	750247	1111331	17.35%	1.641%
4	4.034	174	178	182	rVB	13262	18072	0.28%	0.027%
5	4.970	332	337	341	rBV2	15602	23181	0.36%	0.034%
6	5.958	501	505	513	rVB2	8413	12570	0.20%	0.019%
7	7.046	683	690	701	rBV	1151986	1777161	27.75%	2.624%
8	7.216	711	719	727	rBV	866237	1398982	21.84%	2.065%
9	7.416	746	753	761	rBV	1101623	1712404	26.74%	2.528%
10	7.481	761	764	768	rVV	9164	11251	0.18%	0.017%
11	7.893	826	834	841	rBV	846075	1345342	21.00%	1.986%
12	7.958	841	845	851	rVB3	9534	15390	0.24%	0.023%
13	8.593	946	953	964	rBV	1424593	2241795	35.00%	3.310%
14	8.716	970	974	979	rVB4	7377	11844	0.18%	0.017%
15	9.046	1023	1030	1042	rBV	1073674	1776217	27.73%	2.622%
16	9.222	1054	1060	1067	rVB8	10368	19181	0.30%	0.028%
17	9.505	1103	1108	1114	rVB2	14459	21516	0.34%	0.032%
18	9.775	1146	1154	1165	rBV	967360	1545429	24.13%	2.282%
19	10.316	1238	1246	1259	rBV	1402434	2309166	36.05%	3.409%
20	10.469	1265	1272	1283	rBV	430551	688607	10.75%	1.017%
21	10.699	1302	1311	1323	rVB	1221661	2039165	31.84%	3.010%
22	10.828	1323	1333	1346	rBV	1411662	2410026	37.63%	3.558%
23	11.675	1466	1477	1478	rBV10	3626	7217	0.11%	0.011%
24	12.287	1576	1581	1589	rVB2	26477	43557	0.68%	0.064%
25	12.893	1679	1684	1690	rBV5	3905	6992	0.11%	0.010%
26	13.140	1722	1726	1732	rBV5	6127	9559	0.15%	0.014%
27	13.363	1760	1764	1770	rVV2	8109	10773	0.17%	0.016%
28	13.428	1770	1775	1782	rVV3	10375	16301	0.25%	0.024%
29	13.504	1784	1788	1792	rVB8	5480	9447	0.15%	0.014%
30	13.934	1854	1861	1867	rBV	2643474	3650932	57.00%	5.390%
31	14.175	1897	1902	1903	rBV2	6813	8523	0.13%	0.013%
32	14.222	1903	1910	1921	rVB	2960277	4284754	66.90%	6.326%
33	14.434	1942	1946	1950	rVB	7817	10972	0.17%	0.016%
34	14.528	1955	1962	1972	rVB	1950091	2815426	43.96%	4.157%
35	14.710	1982	1993	2013	rBV	1173137	1758139	27.45%	2.596%
36	14.881	2018	2022	2028	rVV8	4934	9438	0.15%	0.014%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031522\
 Data File : BN018974.D
 Acq On : 16 Mar 2022 07:31
 Operator : CG/JU
 Sample : N1818-15
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBSF9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN031522.M
 Title : SVOA CALIBRATION

37	14.934	2028	2031	2037	rVV4	10159	15426	0.24%	0.023%
38	15.116	2058	2062	2066	rBV5	4482	7544	0.12%	0.011%
39	15.334	2092	2099	2103	rBV5	10482	18529	0.29%	0.027%
40	15.381	2103	2107	2112	rVB	14969	20791	0.32%	0.031%

41	15.516	2121	2130	2141	rBV	3657918	5253830	82.03%	7.756%
42	15.628	2143	2149	2163	rVV	1266664	1643567	25.66%	2.426%
43	15.757	2166	2171	2175	rBV	18190	25544	0.40%	0.038%
44	15.957	2198	2205	2210	rBV7	11560	22584	0.35%	0.033%
45	16.210	2242	2248	2250	rBV8	8113	14964	0.23%	0.022%

46	16.240	2250	2253	2256	rVV3	7423	9353	0.15%	0.014%
47	16.298	2260	2263	2269	rVB7	8093	10825	0.17%	0.016%
48	16.410	2278	2282	2287	rVB7	5982	9115	0.14%	0.013%
49	16.516	2297	2300	2303	rBV3	5232	7407	0.12%	0.011%
50	16.869	2355	2360	2365	rBV3	4469	6901	0.11%	0.010%

51	17.034	2383	2388	2389	rBV5	7566	9832	0.15%	0.015%
52	17.269	2421	2428	2437	rVV	2258945	3349495	52.30%	4.945%
53	17.363	2438	2444	2455	rVV2	3809250	5652362	88.25%	8.345%
54	17.451	2455	2459	2469	rVB4	24213	40718	0.64%	0.060%
55	17.645	2487	2492	2496	rBV6	6428	12716	0.20%	0.019%

56	17.939	2537	2542	2547	rVB	53599	65312	1.02%	0.096%
57	18.163	2575	2580	2589	rBV3	36261	71215	1.11%	0.105%
58	18.592	2649	2653	2657	rBV3	25315	29478	0.46%	0.044%
59	19.016	2721	2725	2729	rBV7	5827	10848	0.17%	0.016%
60	19.110	2737	2741	2745	rVB3	20748	22936	0.36%	0.034%

61	19.222	2755	2760	2767	rBV2	54582	81031	1.27%	0.120%
62	19.292	2767	2772	2784	rVV	59437	90674	1.42%	0.134%
63	19.439	2793	2797	2806	rBV9	11112	20939	0.33%	0.031%
64	19.586	2819	2822	2827	rVB6	8843	10482	0.16%	0.015%
65	19.657	2827	2834	2840	rBV	4685242	6404919	100.00%	9.456%

66	19.704	2840	2842	2848	rVB3	26635	29772	0.46%	0.044%
67	20.169	2918	2921	2924	rBV5	9094	11696	0.18%	0.017%
68	20.651	3001	3003	3006	rVB2	21054	22395	0.35%	0.033%
69	20.728	3014	3016	3021	rVB4	9566	11916	0.19%	0.018%
70	21.151	3084	3088	3094	rBV	200782	260435	4.07%	0.384%

71	21.445	3133	3138	3148	rBV	2475213	3195017	49.88%	4.717%
72	21.604	3163	3165	3169	rBV3	15234	13537	0.21%	0.020%
73	22.545	3320	3325	3333	rBV3	192941	341885	5.34%	0.505%
74	23.110	3416	3421	3425	rVB2	75598	111345	1.74%	0.164%
75	23.680	3510	3518	3534	rBV2	2283348	4700046	73.38%	6.939%

76	23.833	3536	3544	3553	rVV	1254411	2478530	38.70%	3.659%
----	--------	------	------	------	-----	---------	---------	--------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031522\
Data File : BN018974.D
Acq On : 16 Mar 2022 07:31
Operator : CG/JU
Sample : N1818-15
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBSF9

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN031522.M
Title : SVOA CALIBRATION

77	24.445	3644	3648	3657	rVB2	77598	154537	2.41%	0.228%
78	25.280	3786	3790	3801	rVB4	65993	155625	2.43%	0.230%




Sum of corrected areas: 67735476

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031522\
Data File : BN018974.D
Acq On : 16 Mar 2022 07:31
Operator : CG/JU
Sample : N1818-15
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBSF9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN031522.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

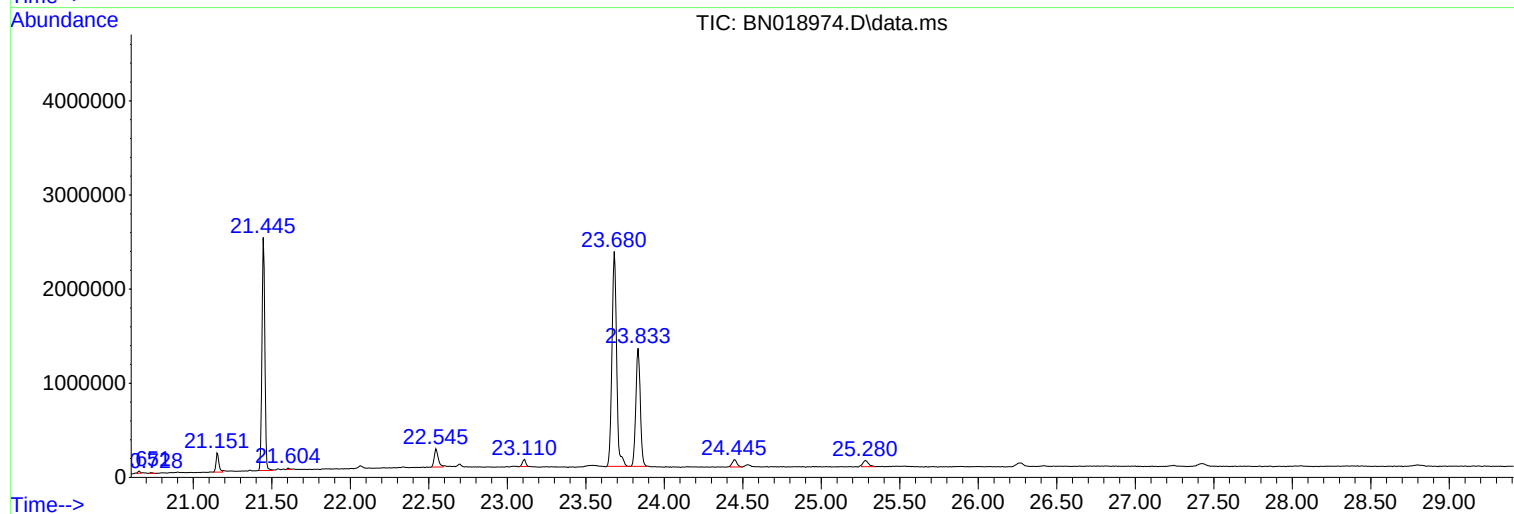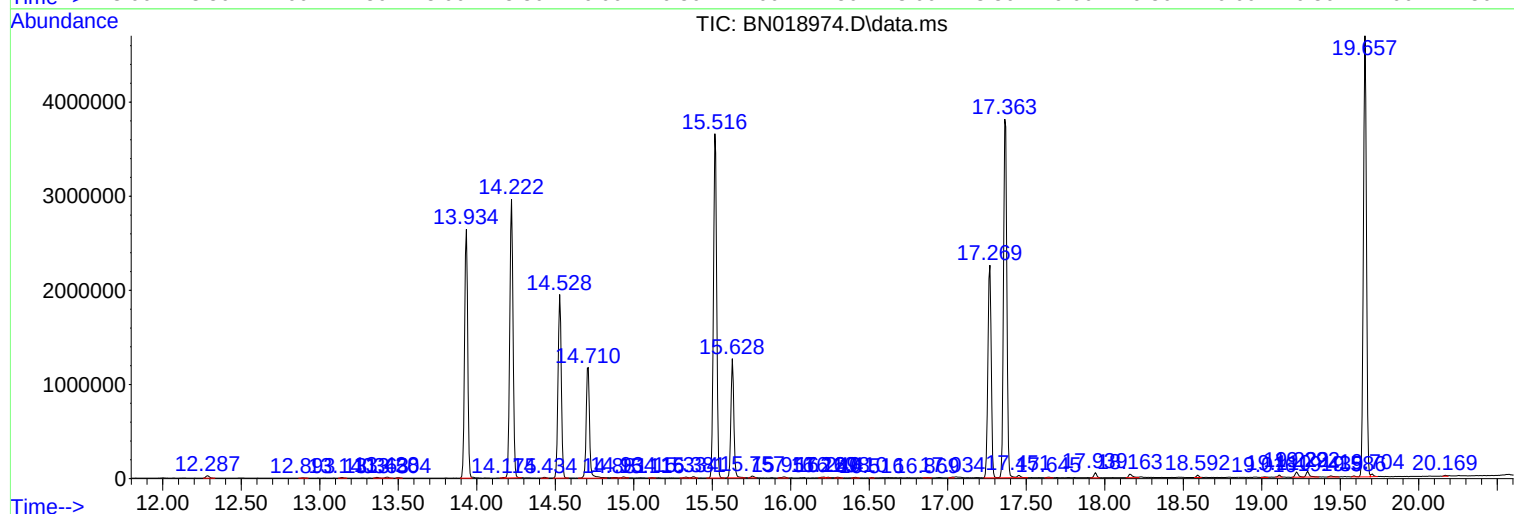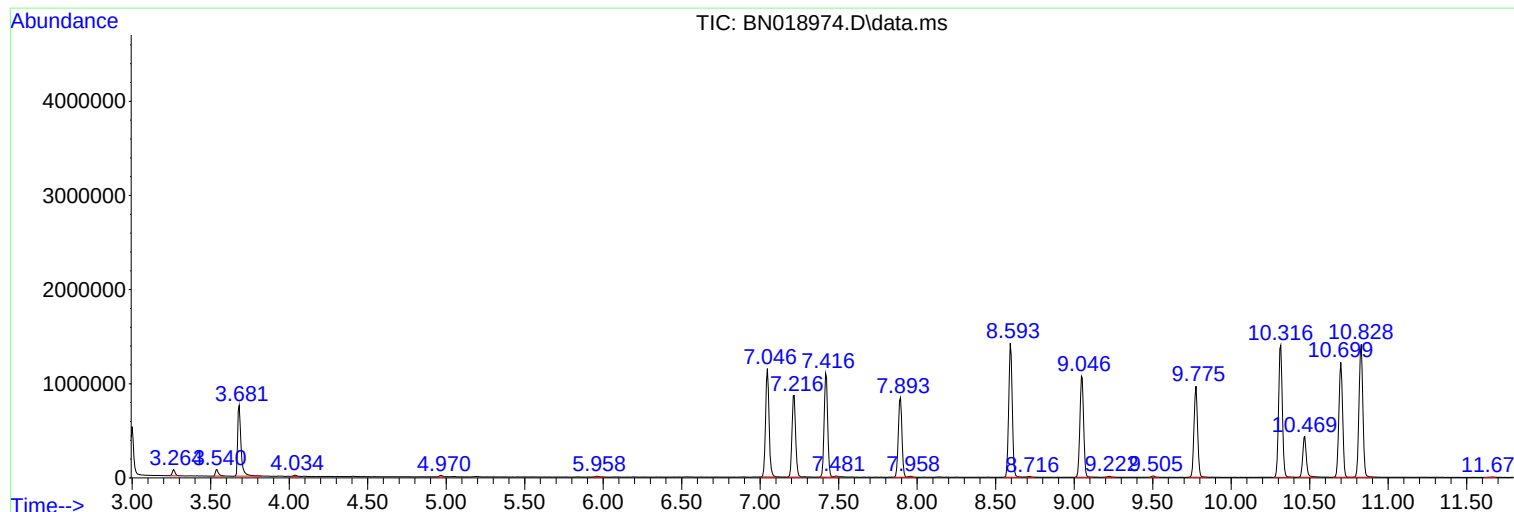

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031522\
Data File : BN018974.D
Acq On : 16 Mar 2022 07:31
Operator : CG/JU
Sample : N1818-15
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBSF9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN031522.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031522\
Data File : BN018974.D
Acq On : 16 Mar 2022 07:31
Operator : CG/JU
Sample : N1818-15
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBSF9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN031522.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc