

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031524\
 Data File : BN030421.D
 Acq On : 15 Mar 2024 20:37
 Operator : MA/JU
 Sample : P1779-03
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AJ6

Quant Time: Mar 15 22:34:58 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN031524.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 15 01:04:41 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.603	152	2107	0.400	ng/ul	0.00
4) Naphthalene-d8	10.376	136	5214	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.252	164	2959	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.007	188	6163	0.400	ng/ul	0.00
17) Chrysene-d12	21.217	240	5150	0.400	ng/ul	# 0.00
23) Perylene-d12	23.423	264	7892	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.147	96	14820	5.769	ng/ul	-0.01
6) 2-Methylnaphthalene-d10	11.981	152	2893	0.402	ng/ul	0.00
18) Fluoranthene-d10	19.045	212	6971	0.440	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.185	88	2934	1.049	ng/ul	94
20) Pyrene	19.412	202	1076	0.049	ng/ul#	1
26) Benzo(a)pyrene	23.280	252	2741	0.098	ng/ul#	46


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031524\
Data File : BN030421.D
Acq On : 15 Mar 2024 20:37
Operator : MA/JU
Sample : P1779-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AJ6

Quant Time: Mar 15 22:34:58 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN031524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 15 01:04:41 2024
Response via : Initial Calibration




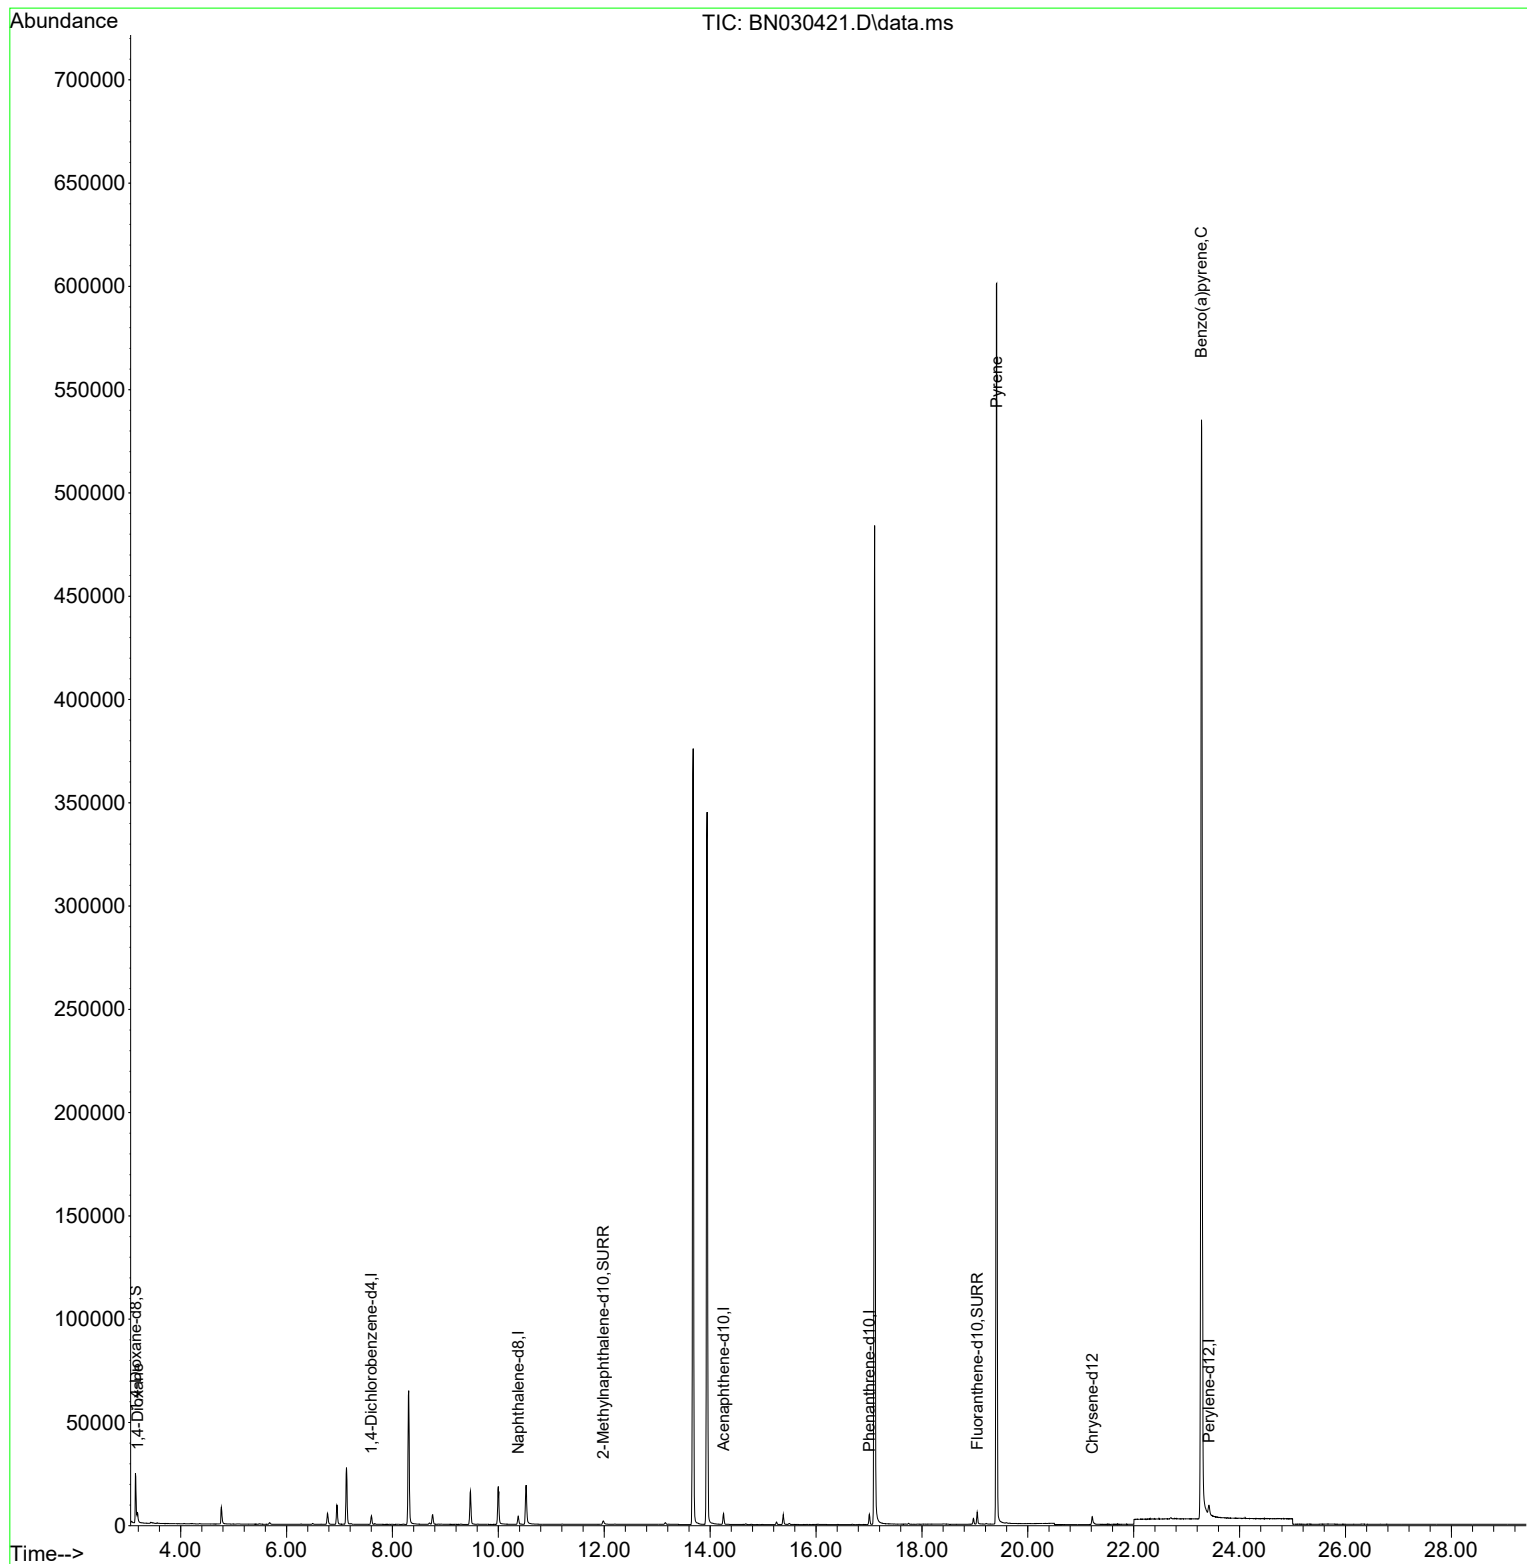


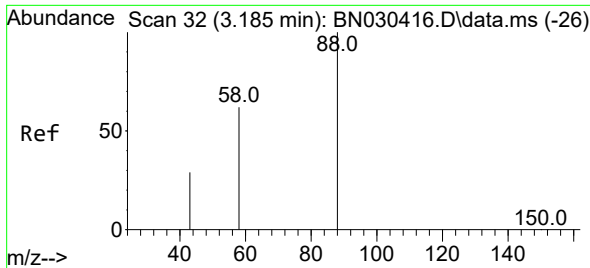

#2
 1,4-Dioxane
 Concen: 1.049 ng/ul
 RT: 3.185 min Scan# 31
 Delta R.T. -0.002 min
 Lab File: BN030421.D
 Acq: 15 Mar 2024 20:37




Instrument :
 BNA_N
 ClientSampleId :
 C0AJ6


Tgt Ion: 88 Resp: 2934
 Ion Ratio Lower Upper
 88 100
 43 30.7 24.7 37.1
 58 52.6 36.6 54.8

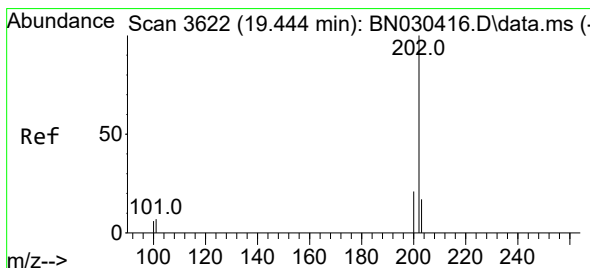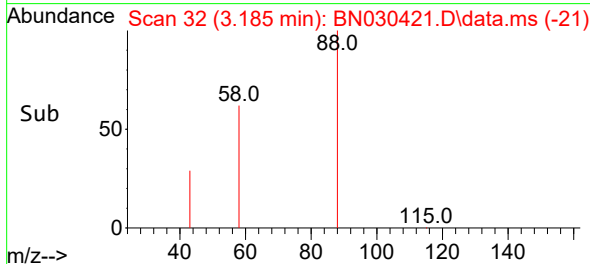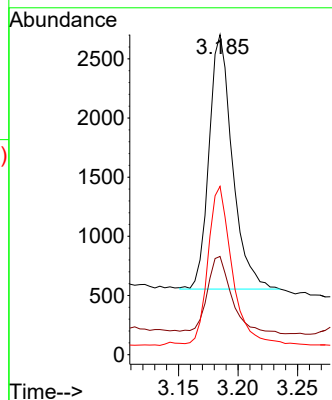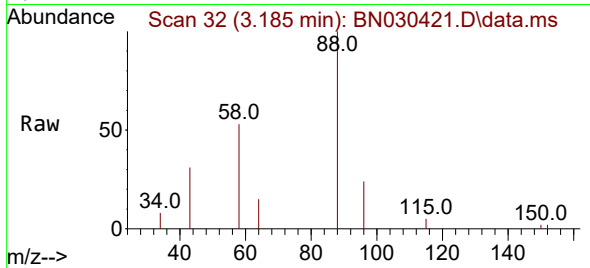

#20
 Pyrene
 Concen: 0.049 ng/ul
 RT: 19.412 min Scan# 3615
 Delta R.T. -0.030 min
 Lab File: BN030421.D
 Acq: 15 Mar 2024 20:37

Tgt Ion: 202 Resp: 1076
 Ion Ratio Lower Upper
 202 100
 101 157.7 7.0 10.6#
 100 1201.3 6.2 9.4#

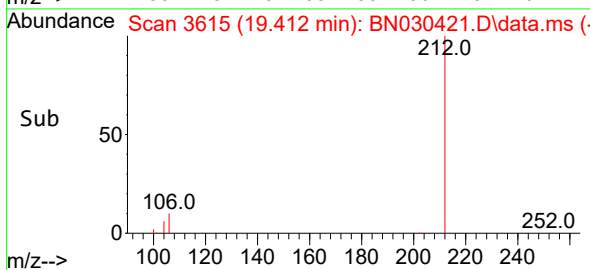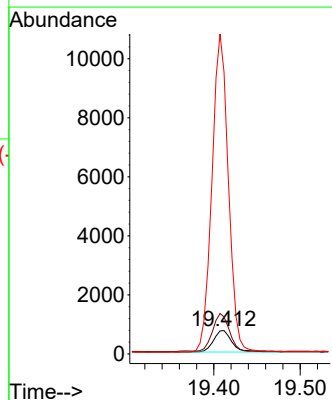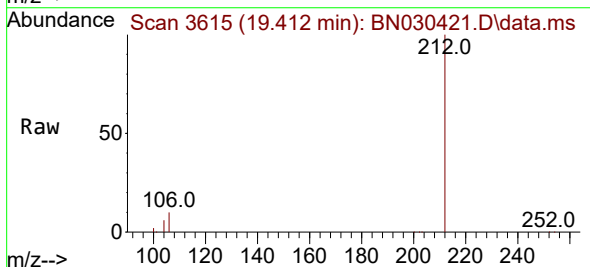

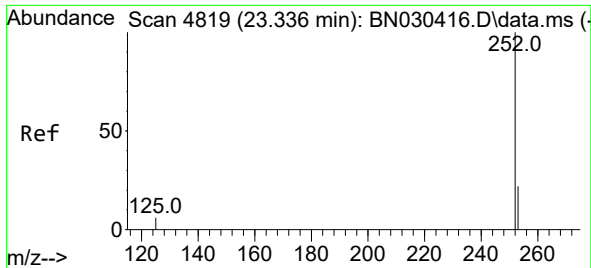

#26

Benzo(a)pyrene

Concen: 0.098 ng/ul

RT: 23.280 min Scan# 4819

Delta R.T. -0.048 min

Lab File: BN030421.D


Acq: 15 Mar 2024 20:37

Instrument :

BNA_N

ClientSampleId :

C0AJ6

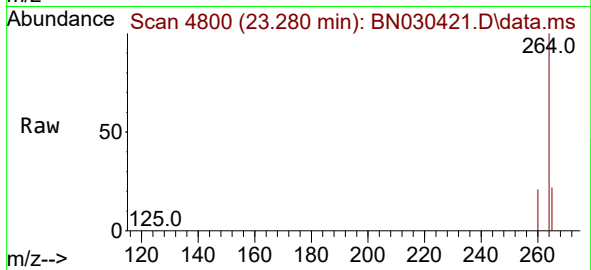

Tgt Ion:252 Resp: 2741

Ion Ratio Lower Upper

252 100

253 75.1 34.4 51.6#

125 37.2 9.0 13.4#

