




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031524\
Data File : BN030415.D
Acq On : 15 Mar 2024 12:11
Operator : MA/JU
Sample : PB159445BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK445

Manual IntegrationsAPPROVED

Quant Time: Mar 15 12:45:30 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN031524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 15 01:04:41 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/15/2024
Supervised By :mohammad ahmed 03/16/2024

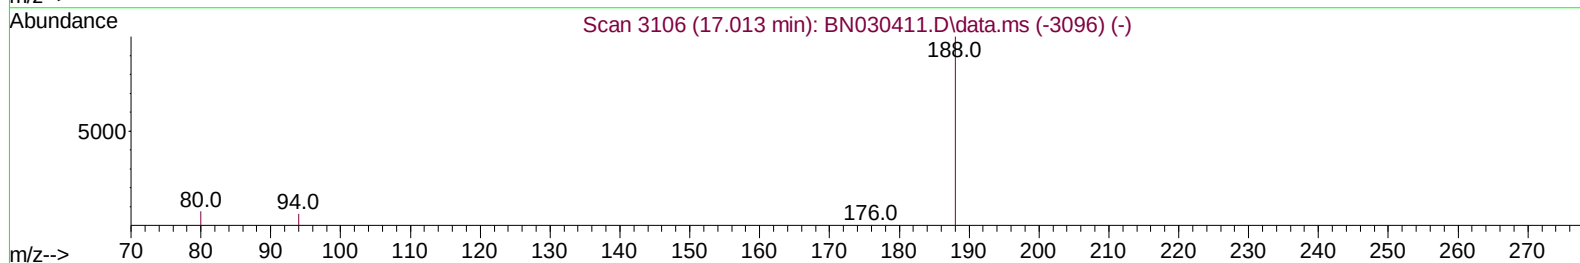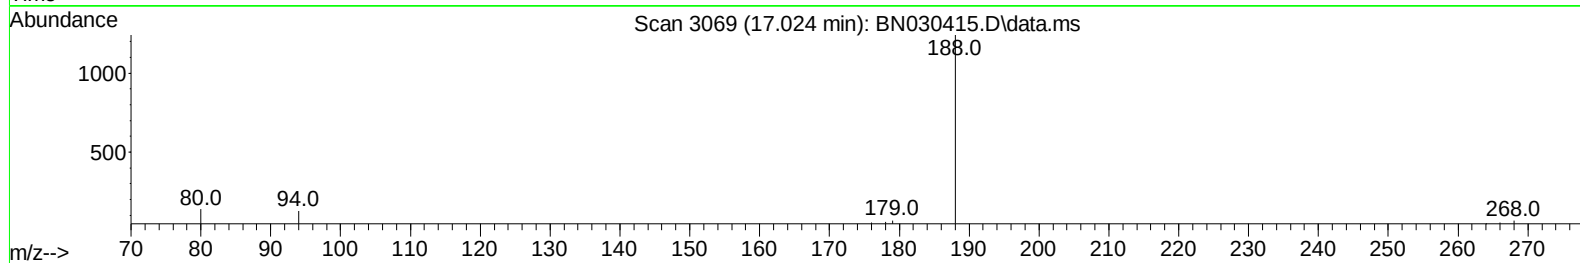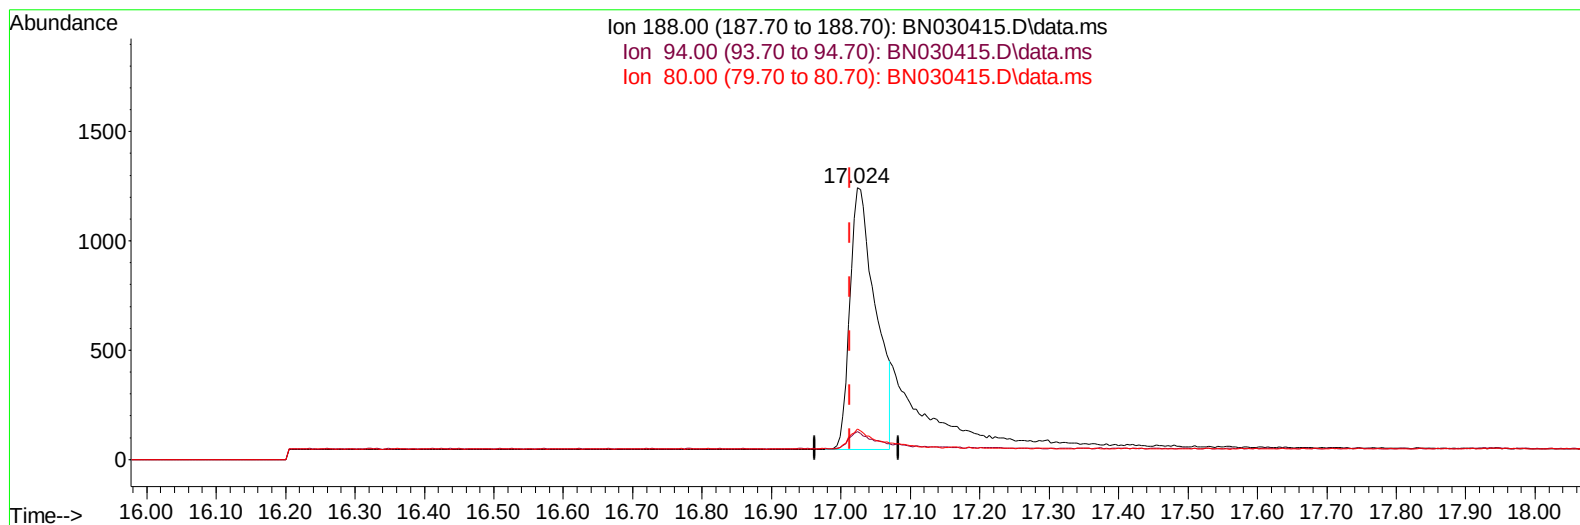

TIC: BN030415.D\data.ms

(13) Phenanthrene-d10 (I)

17.024min (+ 0.011) 0.40 ng/u1

response 3074

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	7.90	10.31#
80.00	8.40	11.19#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031524\
Data File : BN030415.D
Acq On : 15 Mar 2024 12:11
Operator : MA/JU
Sample : PB159445BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK445

Manual IntegrationsAPPROVED

Quant Time: Mar 15 12:45:30 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN031524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 15 01:04:41 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/15/2024
Supervised By :mohammad ahmed 03/16/2024

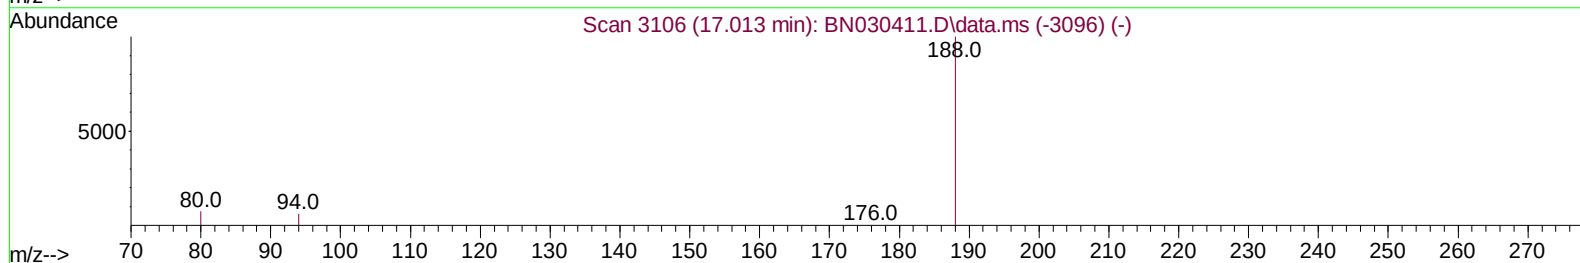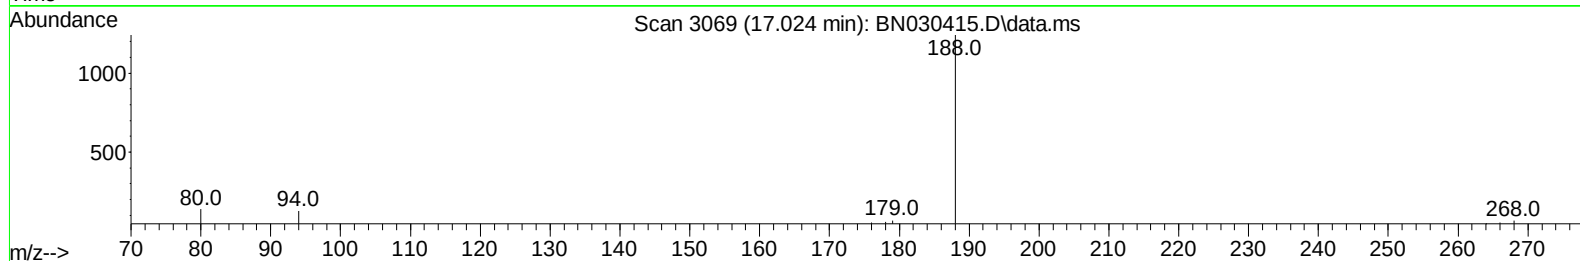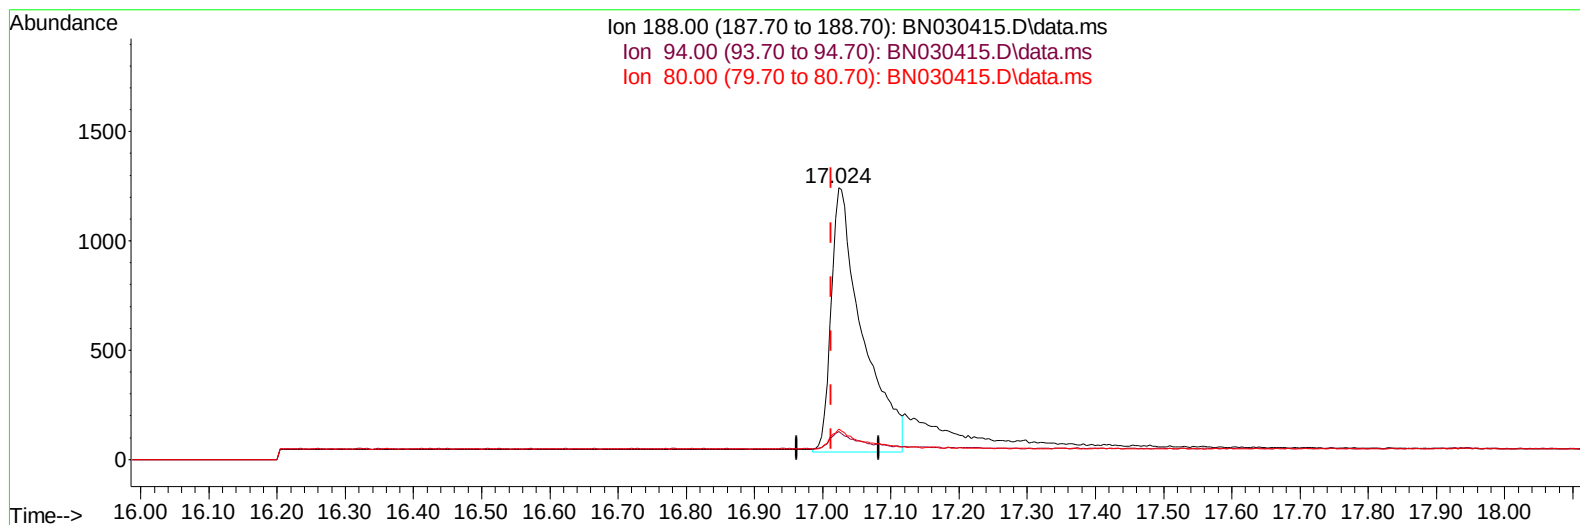

TIC: BN030415.D\data.ms

(13) Phenanthrene-d10 (I)

17.024min (+ 0.011) 0.40 ng/ul m

response 3830

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	7.90	10.31#
80.00	8.40	11.19#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031524\
 Data File : BN030415.D
 Acq On : 15 Mar 2024 12:11
 Operator : MA/JU
 Sample : PB159445BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK445

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 03/15/2024
 Supervised By :mohammad ahmed 03/16/2024

Quant Time: Mar 15 12:45:30 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN031524.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 15 01:04:41 2024
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.607	152		1546	0.400	ng/ul	0.00
4) Naphthalene-d8	10.392	136		3425	0.400	ng/ul #	0.00
9) Acenaphthene-d10	14.257	164		1980	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.024	188		3830m	0.400	ng/ul	0.01
17) Chrysene-d12	21.222	240		3629	0.400	ng/ul	0.00
23) Perylene-d12	23.429	264		4078	0.400	ng/ul	0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.155	96		1410	0.748	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.998	152		1117	0.236	ng/ul	0.01
18) Fluoranthene-d10	19.054	212		3587	0.321	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031524\
Data File : BN030415.D
Acq On : 15 Mar 2024 12:11
Operator : MA/JU
Sample : PB159445BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK445

Manual IntegrationsAPPROVED

Quant Time: Mar 15 12:45:30 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN031524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 15 01:04:41 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/15/2024
Supervised By :mohammad ahmed 03/16/2024

