

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031524\
 Data File : BN030419.D
 Acq On : 15 Mar 2024 19:25
 Operator : MA/JU
 Sample : P1779-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AJ0

Quant Time: Mar 15 22:34:44 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN031524.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 15 01:04:41 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.603	152	1758	0.400	ng/u1	0.00
4) Naphthalene-d8	10.374	136	4133	0.400	ng/u1	0.00
9) Acenaphthene-d10	14.251	164	2432	0.400	ng/u1	0.00
13) Phenanthrene-d10	17.006	188	5315	0.400	ng/u1	0.00
17) Chrysene-d12	21.217	240	4533	0.400	ng/u1	0.00
23) Perylene-d12	23.421	264	7477	0.400	ng/u1	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.151	96	13681	6.383	ng/u1	0.00
6) 2-Methylnaphthalene-d10	11.980	152	2487	0.435	ng/u1	0.00
18) Fluoranthene-d10	19.043	212	6251	0.448	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.185	88	3345	1.433	ng/u1	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031524\
Data File : BN030419.D
Acq On : 15 Mar 2024 19:25
Operator : MA/JU
Sample : P1779-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AJ0


Quant Time: Mar 15 22:34:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN031524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 15 01:04:41 2024
Response via : Initial Calibration

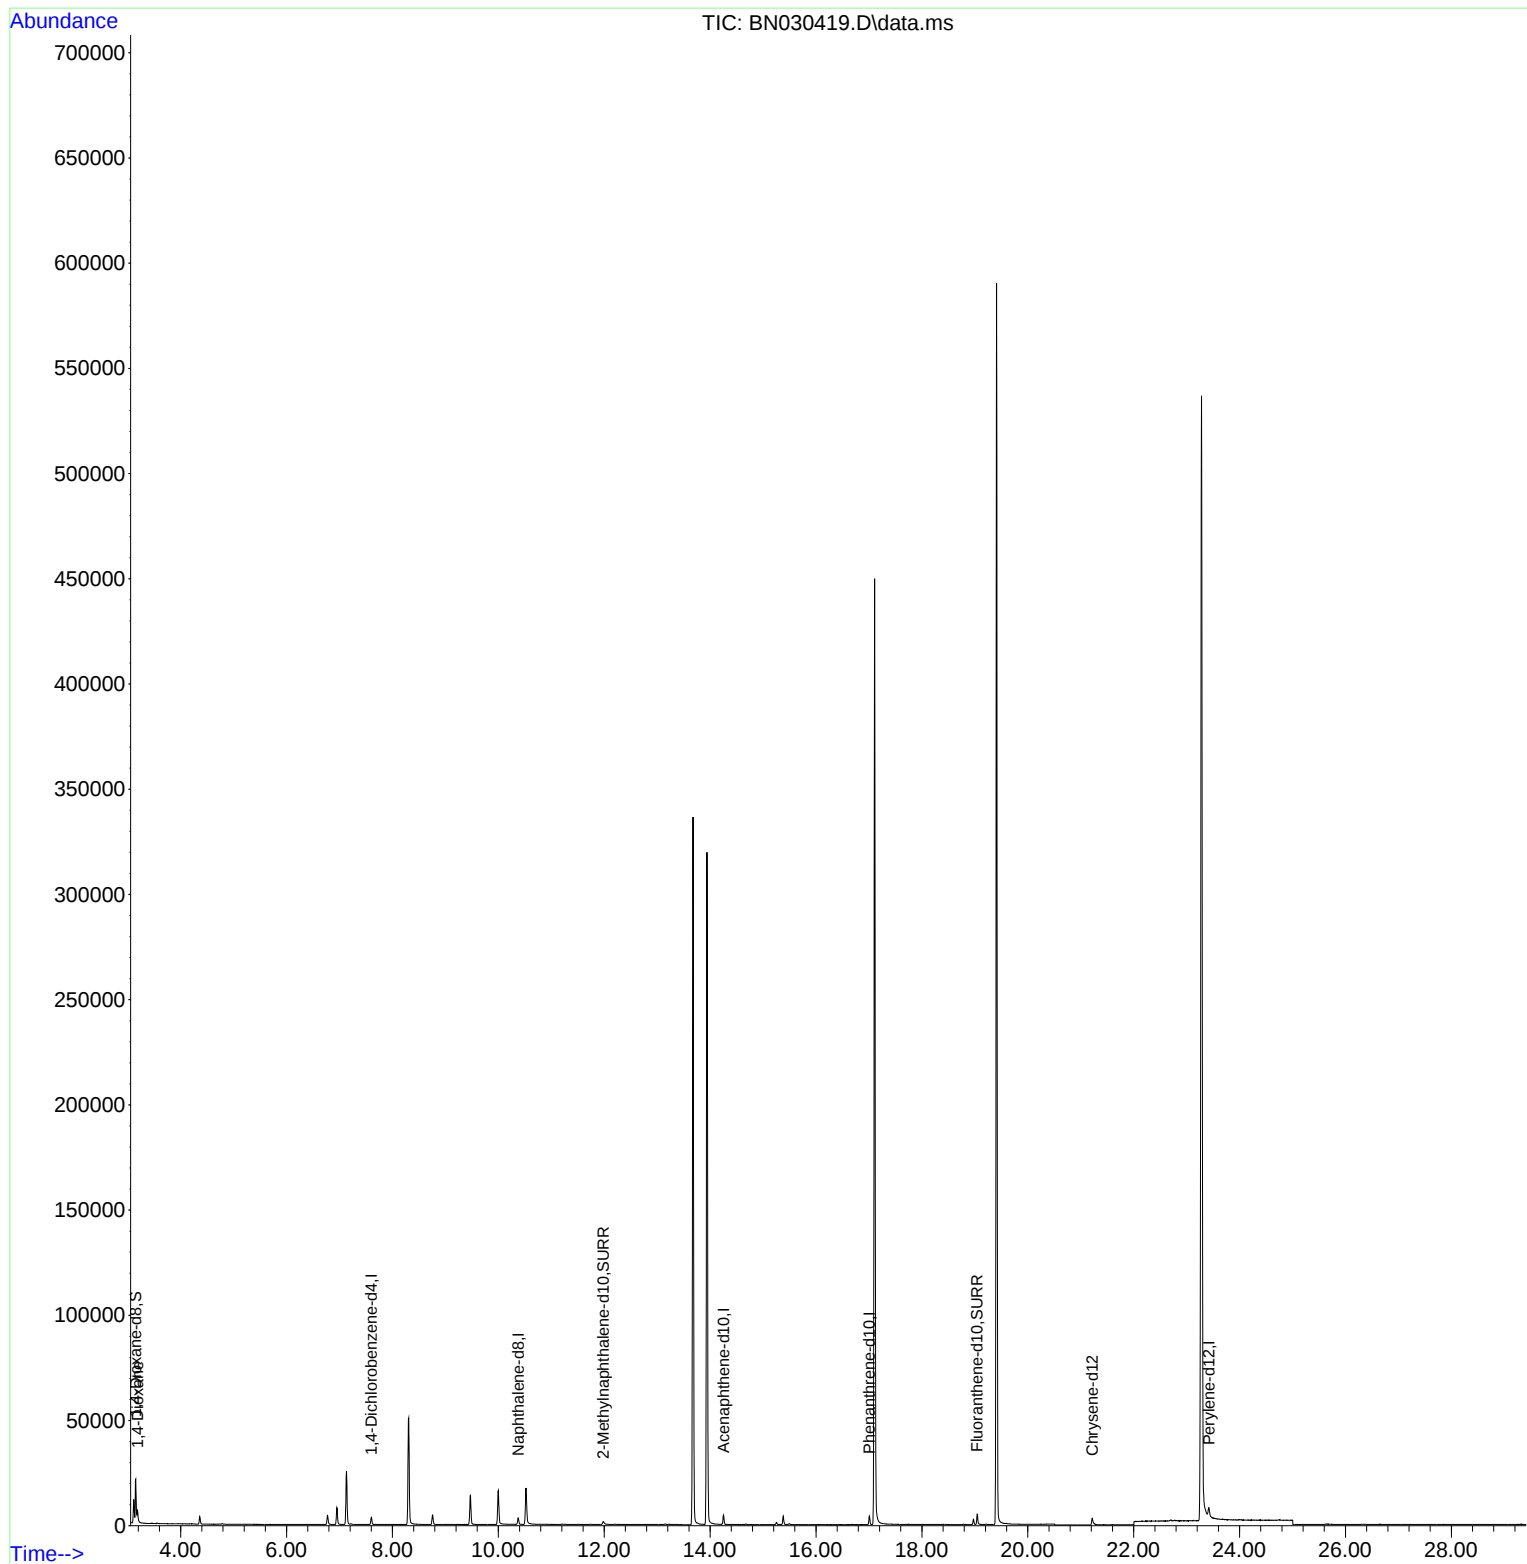

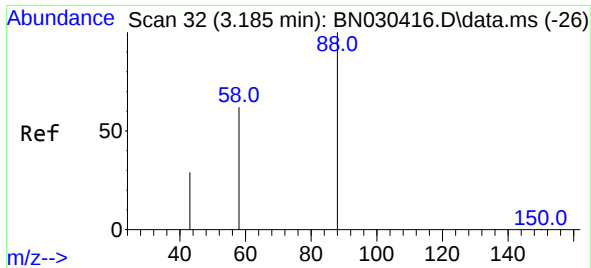

#2
1,4-Dioxane
Concen: 1.433 ng/ul
RT: 3.185 min Scan# 31
Delta R.T. -0.002 min
Lab File: BN030419.D
Acq: 15 Mar 2024 19:25

Instrument :
BNA_N
ClientSampleId :
C0AJ0

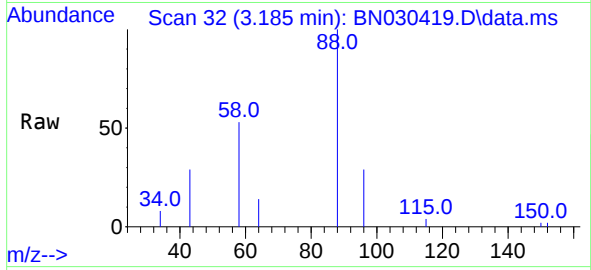

Tgt Ion: 88 Resp: 3345
Ion Ratio Lower Upper
88 100
43 28.8 24.7 37.1
58 53.1 36.6 54.8

