

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031524\
Data File : BN030421.D
Acq On : 15 Mar 2024 20:37
Operator : MA/JU
Sample : P1779-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AJ6

Quant Time: Mar 15 22:34:58 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN031524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 15 01:04:41 2024
Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.603	152	2107	0.400	ng/u1	0.00
4) Naphthalene-d8	10.376	136	5214	0.400	ng/u1	0.00
9) Acenaphthene-d10	14.252	164	2959	0.400	ng/u1	0.00
13) Phenanthrene-d10	17.007	188	6163	0.400	ng/u1	0.00
17) Chrysene-d12	21.217	240	5150	0.400	ng/u1	# 0.00
23) Perylene-d12	23.423	264	7892	0.400	ng/u1	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.147	96	14820	5.769	ng/u1	-0.01
6) 2-Methylnaphthalene-d10	11.981	152	2893	0.402	ng/u1	0.00
18) Fluoranthene-d10	19.045	212	6971	0.440	ng/u1	0.00
Target Compounds					Qvalue	
2) 1,4-Dioxane	3.185	88	2934	1.049	ng/u1	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031524\
Data File : BN030421.D
Acq On : 15 Mar 2024 20:37
Operator : MA/JU
Sample : P1779-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AJ6


Quant Time: Mar 15 22:34:58 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN031524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 15 01:04:41 2024
Response via : Initial Calibration

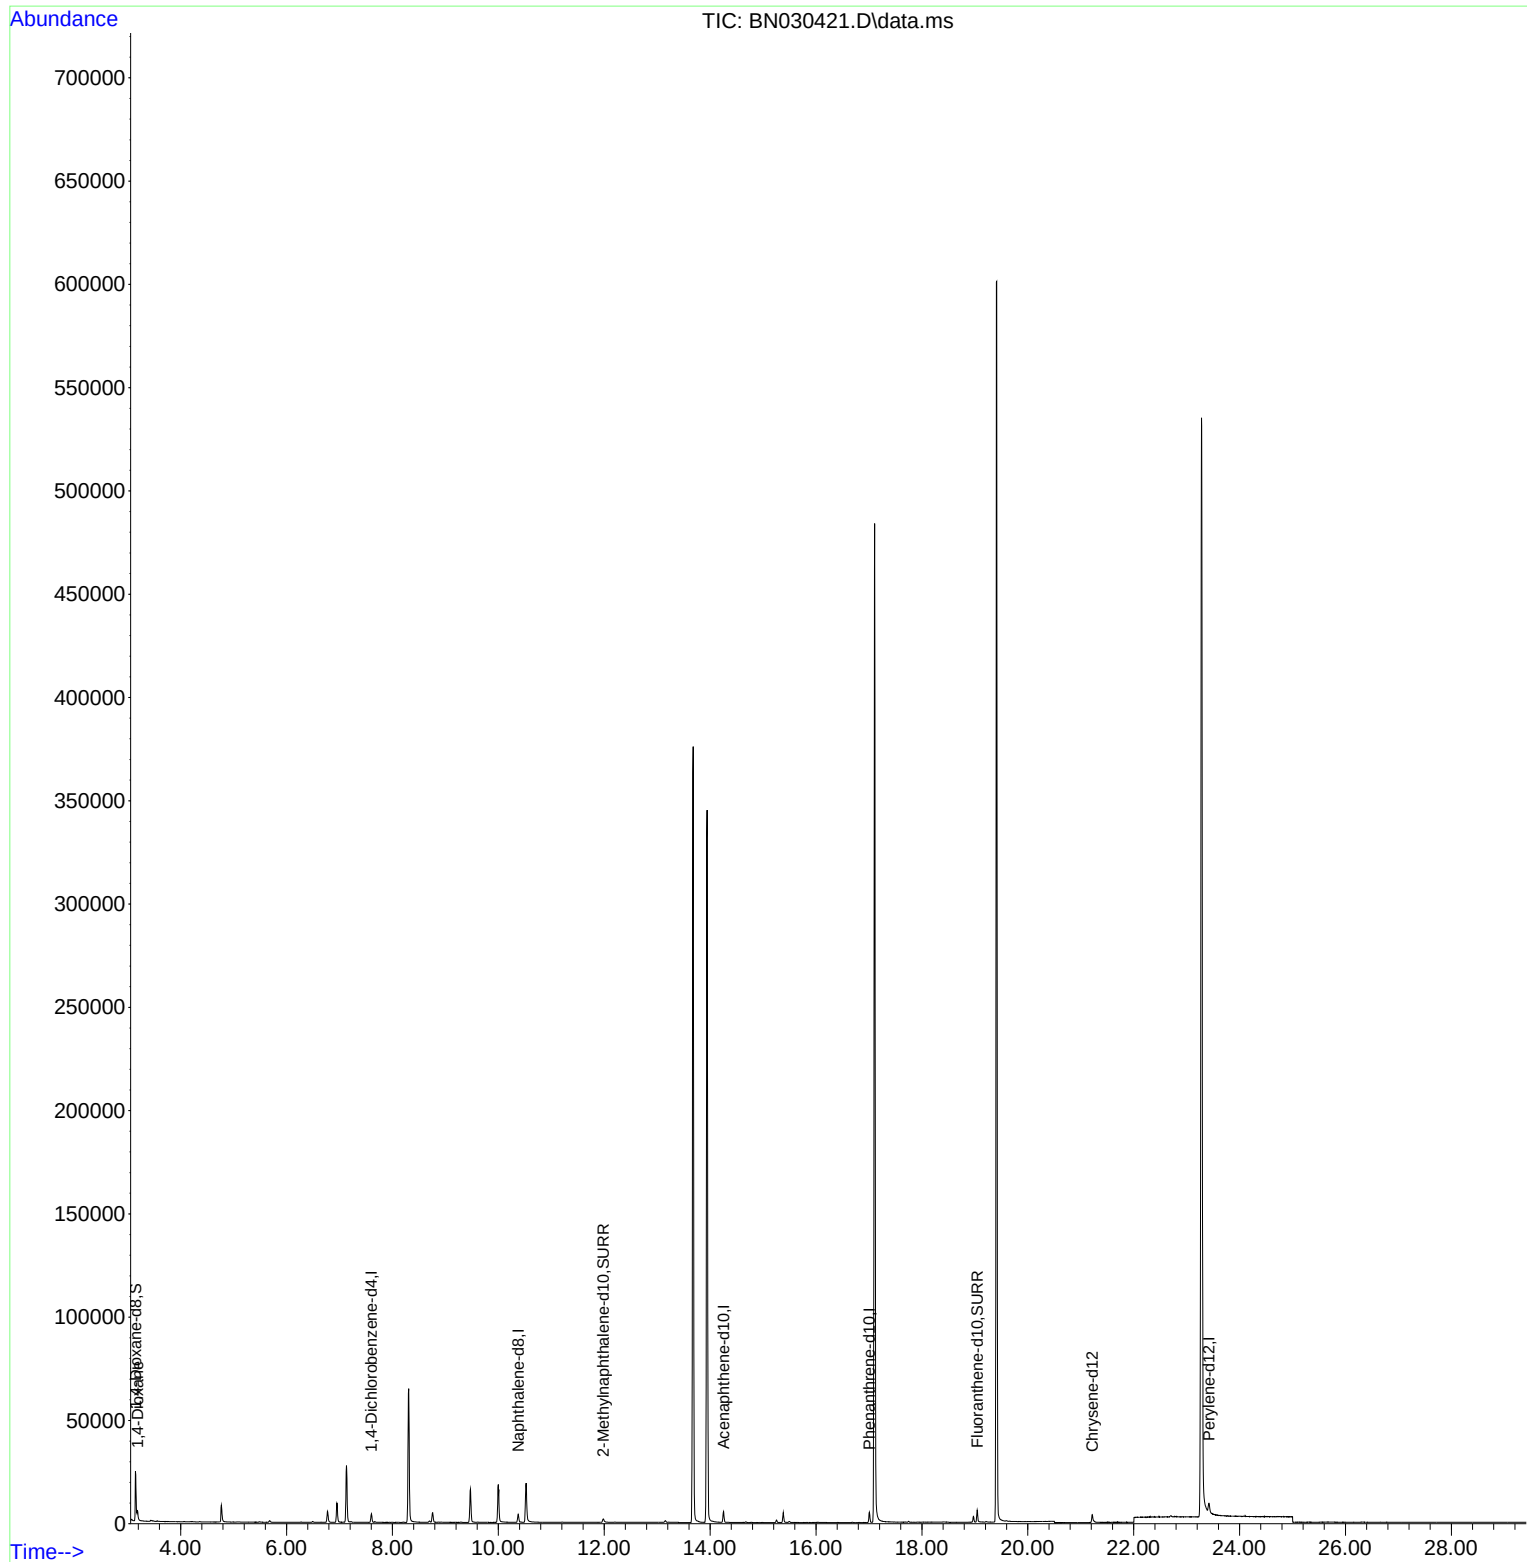

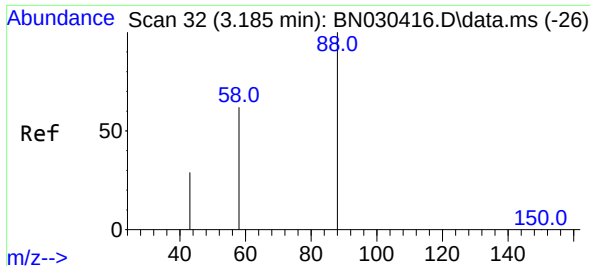

#2
1,4-Dioxane
Concen: 1.049 ng/ul
RT: 3.185 min Scan# 31
Delta R.T. -0.002 min
Lab File: BN030421.D
Acq: 15 Mar 2024 20:37

Instrument :
BNA_N
ClientSampleId :
C0AJ6

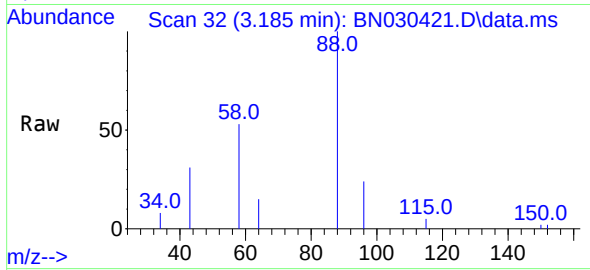

Tgt Ion: 88 Resp: 2934

Ion	Ratio	Lower	Upper
88	100		
43	30.7	24.7	37.1
58	52.6	36.6	54.8

