

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031623\
 Data File : BN024320.D
 Acq On : 16 Mar 2023 20:35
 Operator : CG/JU
 Sample : PB151396BS
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 PB151396BS

Quant Time: Mar 17 04:43:43 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN031323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 17 04:37:08 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.040	152	9539	0.400	ng	0.00
7) Naphthalene-d8	10.855	136	26953	0.400	ng	# 0.00
13) Acenaphthene-d10	14.675	164	12171	0.400	ng	0.00
19) Phenanthrene-d10	17.413	188	24357	0.400	ng	# 0.00
29) Chrysene-d12	21.610	240	17573	0.400	ng	0.00
35) Perylene-d12	24.120	264	13298	0.400	ng	# 0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.584	112	9504	0.450	ng	0.00
5) Phenol-d6	7.188	99	12318	0.454	ng	0.00
8) Nitrobenzene-d5	9.201	82	7635	0.424	ng	0.00
11) 2-Methylnaphthalene-d10	12.441	152	11570	0.349	ng	0.00
14) 2,4,6-Tribromophenol	16.159	330	2174	0.349	ng	0.00
15) 2-Fluorobiphenyl	13.307	172	18581	0.404	ng	0.00
27) Fluoranthene-d10	19.446	212	18251	0.353	ng	0.00
31) Terphenyl-d14	20.034	244	10870	0.367	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.439	88	4353	0.419	ng	92
3) n-Nitrosodimethylamine	3.764	42	7429	0.488	ng	# 88
6) bis(2-Chloroethyl)ether	7.455	93	11143	0.414	ng	94
9) Naphthalene	10.909	128	26517	0.387	ng	99
10) Hexachlorobutadiene	11.197	225	5060	0.389	ng	# 99
12) 2-Methylnaphthalene	12.512	142	16360	0.354	ng	99
16) Acenaphthylene	14.397	152	21271	0.369	ng	100
17) Acenaphthene	14.739	154	13989	0.381	ng	96
18) Fluorene	15.712	166	15806	0.360	ng	100
20) 4,6-Dinitro-2-methylph...	15.787	198	946	0.386	ng	96
21) 4-Bromophenyl-phenylether	16.606	248	4909	0.339	ng	# 81
22) Hexachlorobenzene	16.730	284	6636	0.373	ng	95
23) Atrazine	16.867	200	3536	0.385	ng	# 91
24) Pentachlorophenol	17.065	266	2218	0.334	ng	98
25) Phenanthrene	17.462	178	27712	0.384	ng	99
26) Anthracene	17.549	178	23659	0.355	ng	100
28) Fluoranthene	19.476	202	28783	0.364	ng	99
30) Pyrene	19.838	202	28689	0.403	ng	100
32) Benzo(a)anthracene	21.592	228	21207	0.361	ng	99
33) Chrysene	21.646	228	25001	0.399	ng	99
34) Bis(2-ethylhexyl)phtha...	21.511	149	11060	0.400	ng	96
36) Indeno(1,2,3-cd)pyrene	26.743	276	18999	0.382	ng	96
37) Benzo(b)fluoranthene	23.398	252	21708	0.420	ng	97
38) Benzo(k)fluoranthene	23.398	252	20338	0.381	ng	97
39) Benzo(a)pyrene	24.006	252	17714	0.373	ng	# 94
40) Dibenzo(a,h)anthracene	26.766	278	14335	0.372	ng	96
41) Benzo(g,h,i)perylene	27.558	276	17761	0.394	ng	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031623\
 Data File : BN024320.D
 Acq On : 16 Mar 2023 20:35
 Operator : CG/JU
 Sample : PB151396BS
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 PB151396BS

Quant Time: Mar 17 04:43:43 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN031323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 17 04:37:08 2023
 Response via : Initial Calibration



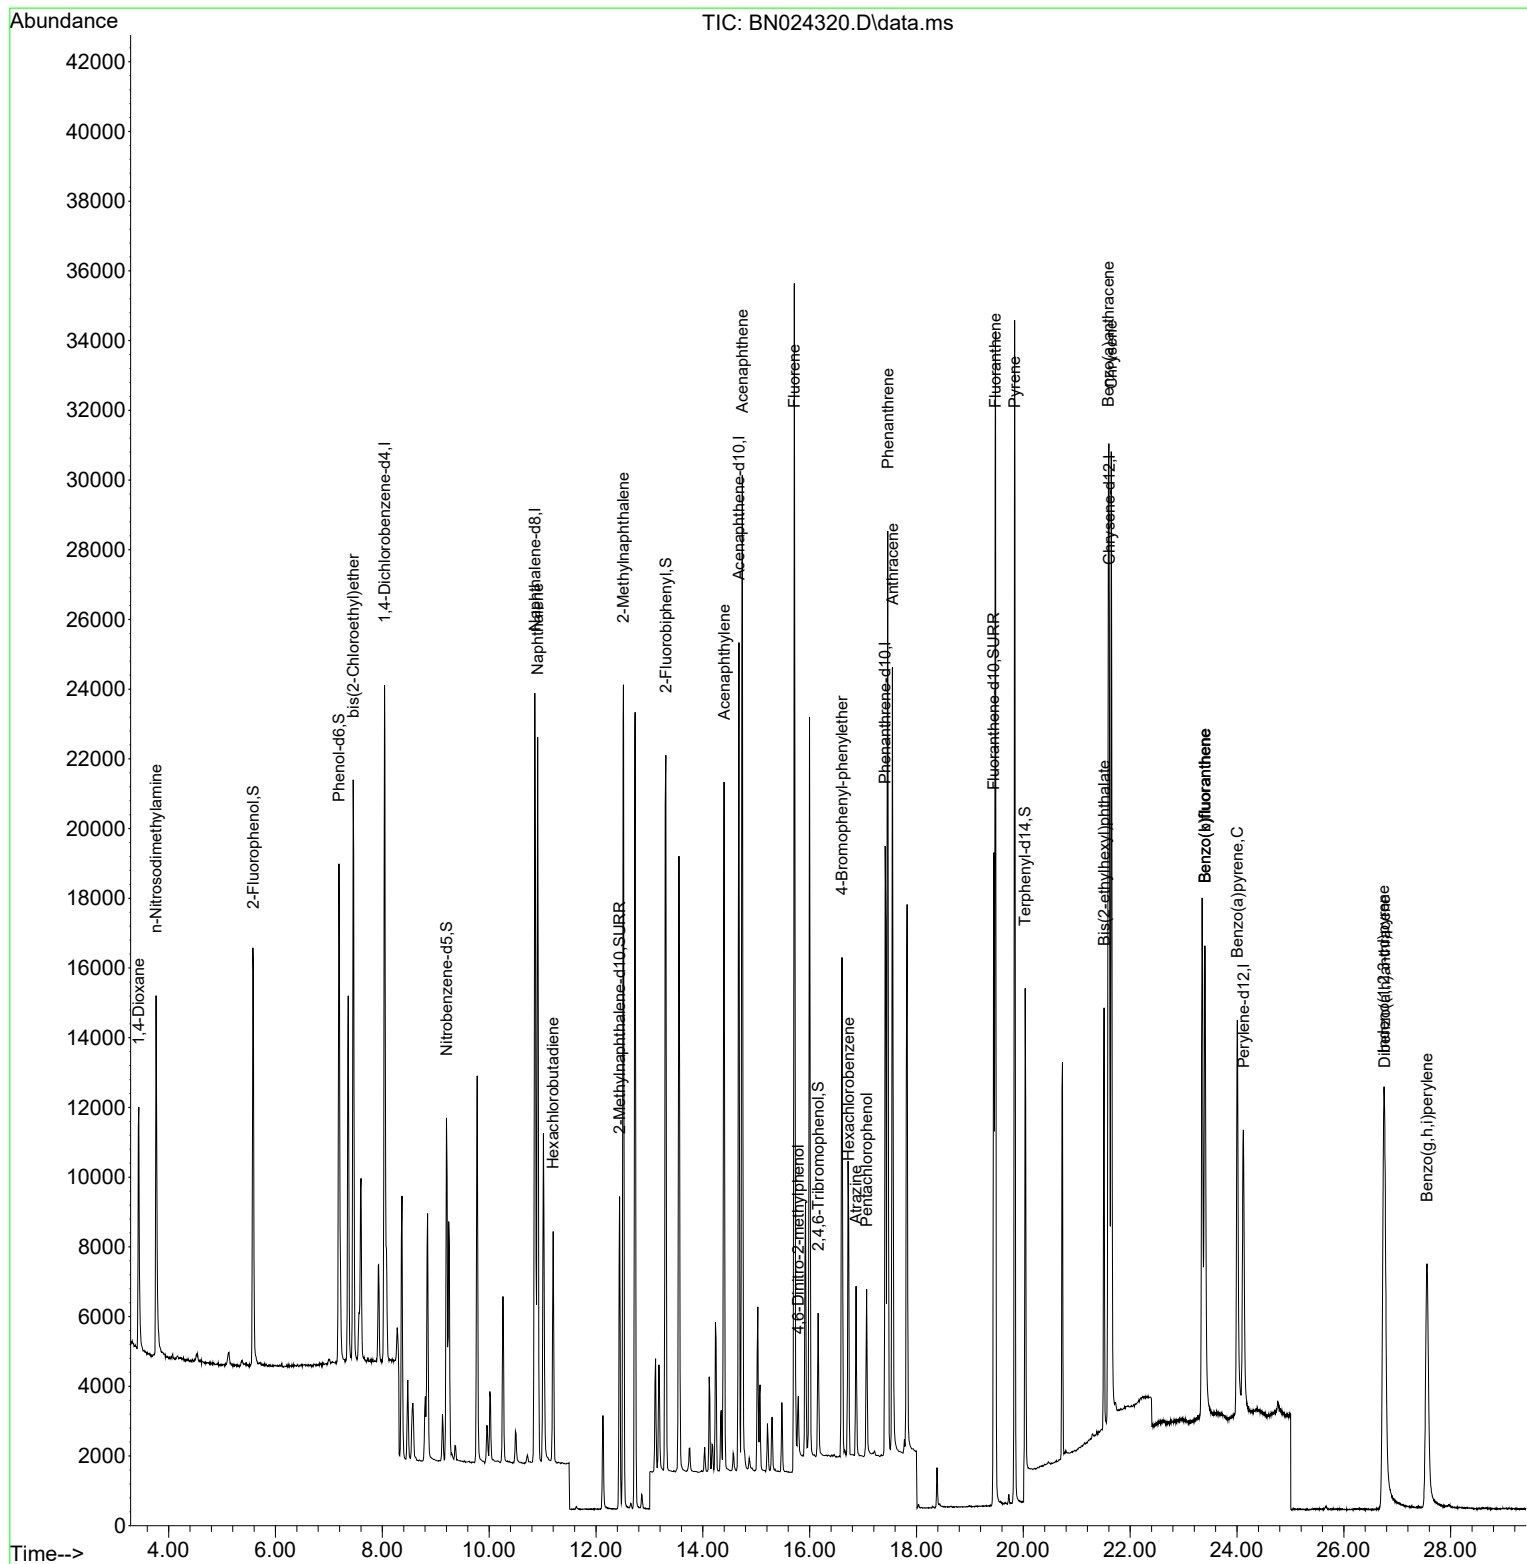




#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 8.040 min Scan# 61
 Delta R.T. -0.000 min
 Lab File: BN024320.D
 Acq: 16 Mar 2023 20:35




Instrument :
 BNA_N
 ClientSampleId :
 PB151396BS


Tgt Ion:152 Resp: 9539
 Ion Ratio Lower Upper
 152 100
 150 157.9 124.7 187.1
 115 64.2 49.1 73.7

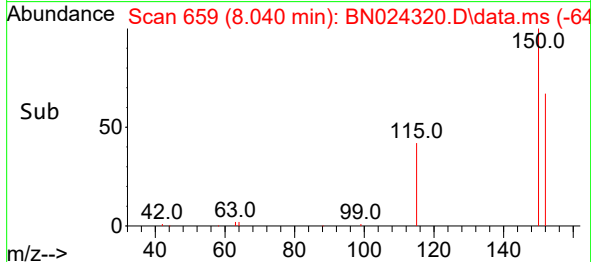

#2
 1,4-Dioxane
 Concen: 0.419 ng
 RT: 3.439 min Scan# 22
 Delta R.T. 0.000 min
 Lab File: BN024320.D
 Acq: 16 Mar 2023 20:35

Tgt Ion: 88 Resp: 4353
 Ion Ratio Lower Upper
 88 100
 43 41.2 29.0 43.4
 58 91.4 67.3 100.9




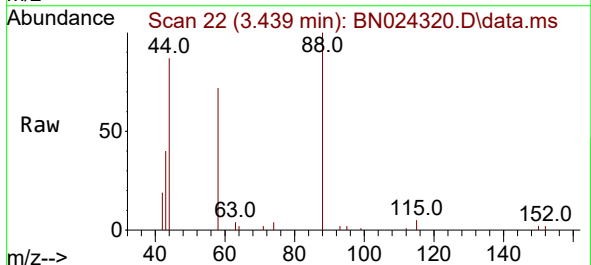




#3
 n-Nitrosodimethylamine
 Concen: 0.488 ng
 RT: 3.764 min Scan# 61
 Delta R.T. 0.000 min
 Lab File: BN024320.D
 Acq: 16 Mar 2023 20:35




Instrument :
 BNA_N
 ClientSampleId :
 PB151396BS

Tgt Ion: 42 Resp: 7429
 Ion Ratio Lower Upper
 42 100
 74 88.9 81.6 122.4
 44 7.3 7.3 10.9#

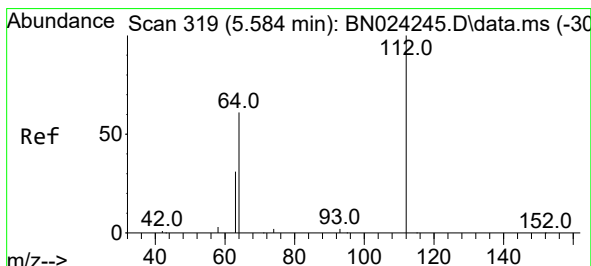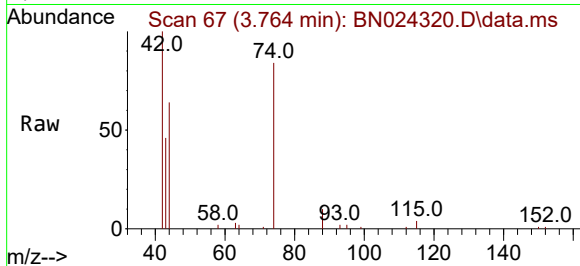

#4
 2-Fluorophenol
 Concen: 0.450 ng
 RT: 5.584 min Scan# 319
 Delta R.T. 0.007 min
 Lab File: BN024320.D
 Acq: 16 Mar 2023 20:35

Tgt Ion: 112 Resp: 9504
 Ion Ratio Lower Upper
 112 100
 64 67.9 49.0 73.6
 63 36.7 25.7 38.5



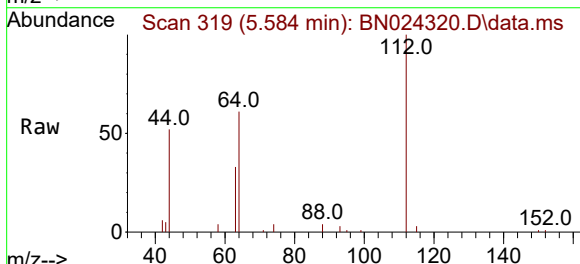




#5
Phenol-d6
Concen: 0.454 ng
RT: 7.188 min Scan# 541
Delta R.T. 0.000 min
Lab File: BN024320.D
Acq: 16 Mar 2023 20:35




Instrument :
BNA_N
ClientSampleId :
PB151396BS

Tgt Ion: 99 Resp: 12318
Ion Ratio Lower Upper
99 100
42 29.7 20.1 30.1
71 34.1 25.8 38.8

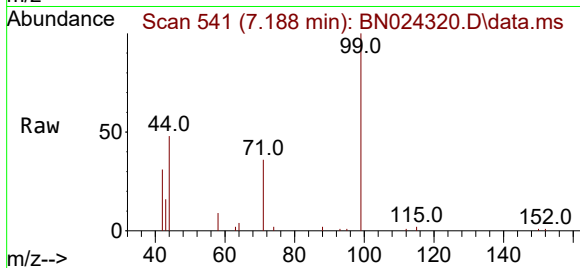

#6
bis(2-Chloroethyl)ether
Concen: 0.414 ng
RT: 7.455 min Scan# 578
Delta R.T. 0.000 min
Lab File: BN024320.D
Acq: 16 Mar 2023 20:35

Tgt Ion: 93 Resp: 11143
Ion Ratio Lower Upper
93 100
63 88.9 65.4 98.2
95 32.1 25.8 38.8




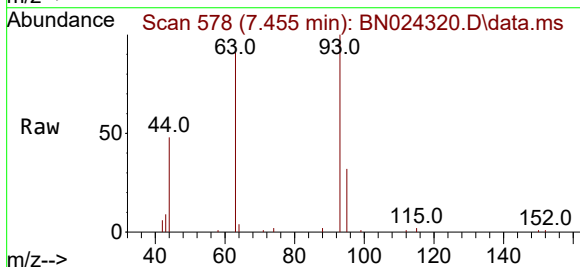




#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.855 min Scan# 91
Delta R.T. 0.000 min
Lab File: BN024320.D
Acq: 16 Mar 2023 20:35




Instrument :
BNA_N
ClientSampleId :
PB151396BS


Tgt Ion:	136	Resp:	26953
Ion Ratio	Lower	Upper	
136	100		
137	11.1	8.9	13.3
54	13.3	7.1	10.7#
68	9.0	5.3	7.9#

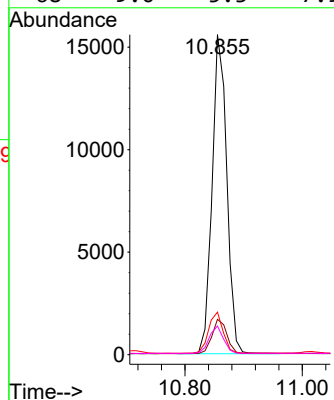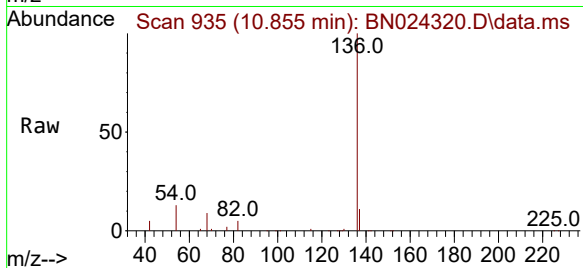

#8
Nitrobenzene-d5
Concen: 0.424 ng
RT: 9.201 min Scan# 780
Delta R.T. 0.000 min
Lab File: BN024320.D
Acq: 16 Mar 2023 20:35

Tgt Ion:	82	Resp:	7635
Ion Ratio	Lower	Upper	
82	100		
128	31.9	32.4	48.6#
54	67.8	45.2	67.8

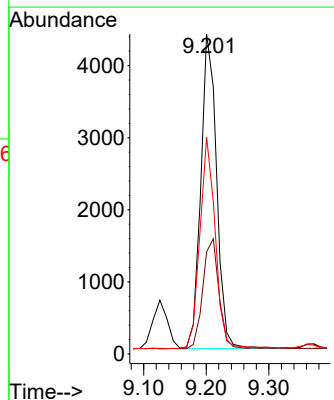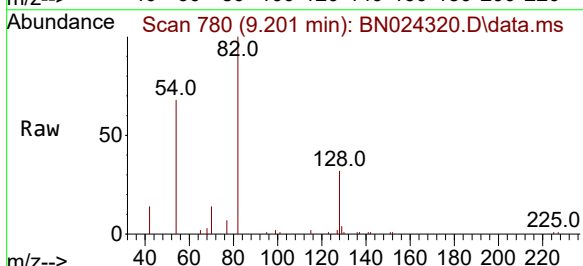



#9

Naphthalene

Concen: 0.387 ng

RT: 10.909 min Scan# 941

Delta R.T. 0.000 min

Lab File: BN024320.D

Acq: 16 Mar 2023 20:35

Instrument :

BNA_N

ClientSampleId :

PB151396BS





Tgt Ion:128 Resp: 26517

Ion Ratio Lower Upper

128 100

129 11.2 9.0 13.6

127 13.5 10.2 15.4

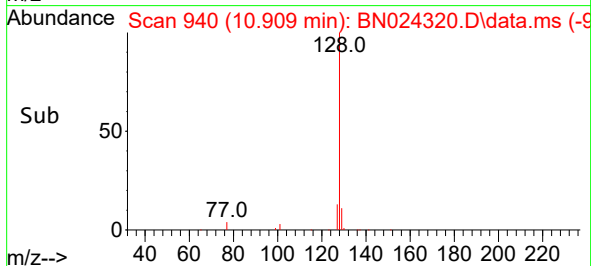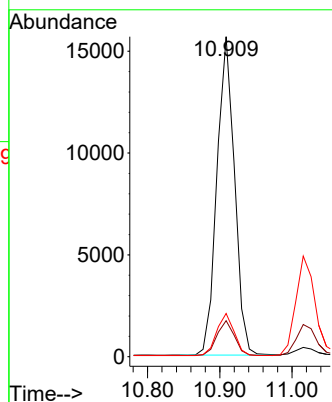

#10

Hexachlorobutadiene

Concen: 0.389 ng

RT: 11.197 min Scan# 967

Delta R.T. 0.000 min

Lab File: BN024320.D

Acq: 16 Mar 2023 20:35




Tgt Ion:225 Resp: 5060

Ion Ratio Lower Upper

225 100

223 0.0 0.0 0.0

227 63.2 51.0 76.4

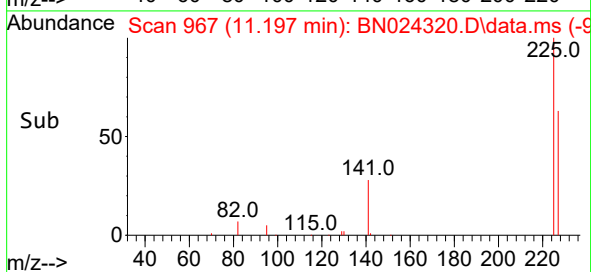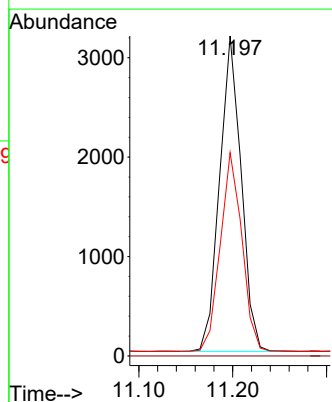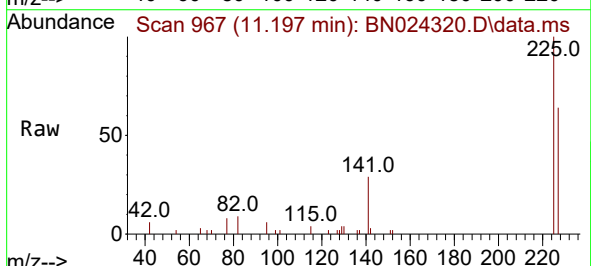



#11

2-Methylnaphthalene-d10

Concen: 0.349 ng

RT: 12.441 min Scan# 11

Delta R.T. 0.000 min

Lab File: BN024320.D

Acq: 16 Mar 2023 20:35

Instrument :

BNA_N

ClientSampleId :





PB151396BS

Tgt Ion:152 Resp: 11570

Ion Ratio Lower Upper

152 100

151 21.6 16.8 25.2



#12

2-Methylnaphthalene

Concen: 0.354 ng

RT: 12.512 min Scan# 1262

Delta R.T. 0.000 min

Lab File: BN024320.D

Acq: 16 Mar 2023 20:35




Tgt Ion:142 Resp: 16360

Ion Ratio Lower Upper

142 100

141 89.9 71.8 107.6

115 38.9 30.0 45.0



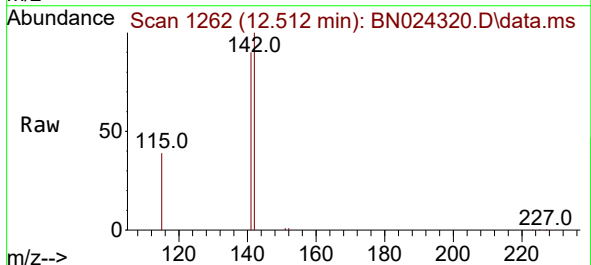




#13
 Acenaphthene-d10
 Concen: 0.400 ng
 RT: 14.675 min Scan# 1549
 Delta R.T. 0.000 min
 Lab File: BN024320.D
 Acq: 16 Mar 2023 20:35




Instrument :
 BNA_N
 ClientSampleId :
 PB151396BS

Tgt Ion:164 Resp: 12171
 Ion Ratio Lower Upper
 164 100
 162 106.7 84.7 127.1
 160 56.9 44.6 66.8

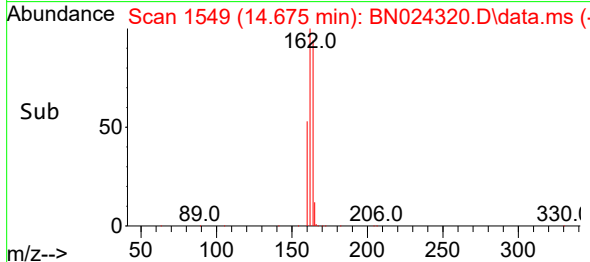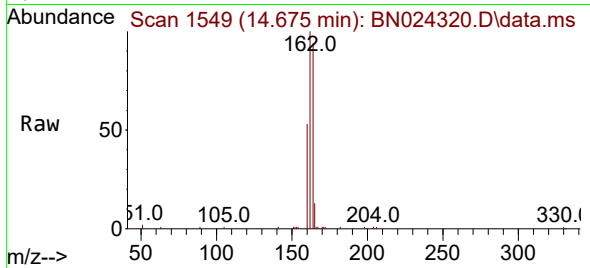

#14
 2,4,6-Tribromophenol
 Concen: 0.349 ng
 RT: 16.159 min Scan# 1682
 Delta R.T. 0.000 min
 Lab File: BN024320.D
 Acq: 16 Mar 2023 20:35

Tgt Ion:330 Resp: 2174
 Ion Ratio Lower Upper
 330 100
 332 96.7 78.0 117.0
 141 45.3 30.8 46.2


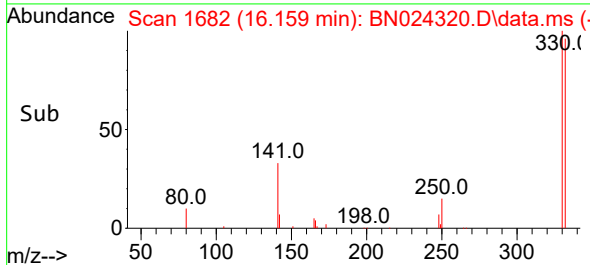

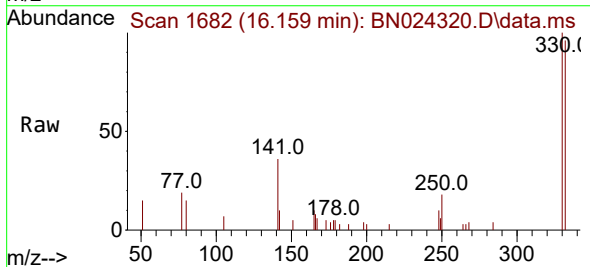




#15
2-Fluorobiphenyl
Concen: 0.404 ng
RT: 13.307 min Scan# 1421
Delta R.T. 0.000 min
Lab File: BN024320.D
Acq: 16 Mar 2023 20:35




Instrument :
BNA_N
ClientSampleId :
PB151396BS


Tgt Ion:172 Resp: 18581
Ion Ratio Lower Upper
172 100
171 34.0 27.8 41.8
170 23.5 19.0 28.6

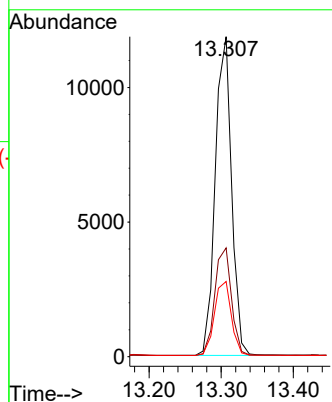

#16
Acenaphthylene
Concen: 0.369 ng
RT: 14.397 min Scan# 1523
Delta R.T. 0.000 min
Lab File: BN024320.D
Acq: 16 Mar 2023 20:35

Tgt Ion:152 Resp: 21271
Ion Ratio Lower Upper
152 100
151 19.5 15.4 23.0
153 13.0 10.4 15.6

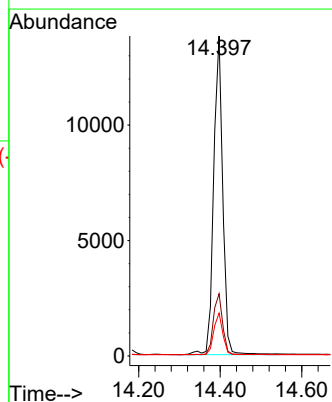



#17

Acenaphthene

Concen: 0.381 ng

RT: 14.739 min Scan# 1555

Delta R.T. 0.000 min

Lab File: BN024320.D

Acq: 16 Mar 2023 20:35

Instrument :

BNA_N

ClientSampleId :

PB151396BS





Tgt Ion:154 Resp: 13989

Ion Ratio Lower Upper

154 100

153 114.3 88.4 132.6

152 64.9 48.7 73.1



#18

Fluorene

Concen: 0.360 ng

RT: 15.712 min Scan# 1646

Delta R.T. 0.000 min

Lab File: BN024320.D

Acq: 16 Mar 2023 20:35




Tgt Ion:166 Resp: 15806

Ion Ratio Lower Upper

166 100

165 100.4 80.2 120.2

167 13.1 10.8 16.2

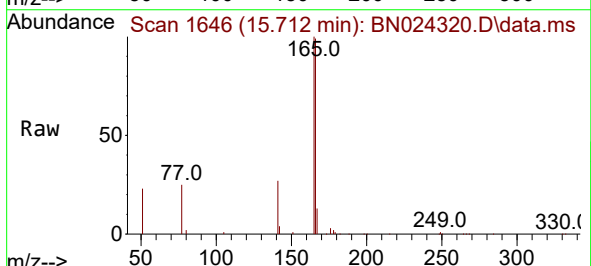



#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 17.413 min Scan# 11

Delta R.T. 0.000 min

Lab File: BN024320.D

Acq: 16 Mar 2023 20:35

Instrument :

BNA_N

ClientSampleId :

PB151396BS





Tgt Ion:188 Resp: 24357

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0

80 21.4 8.9 13.3#

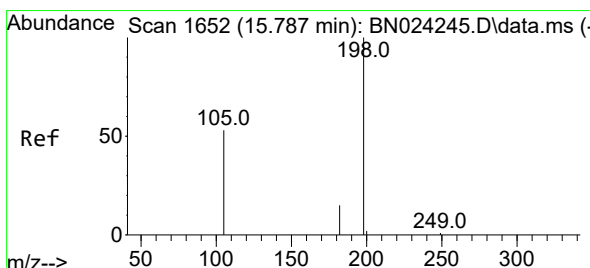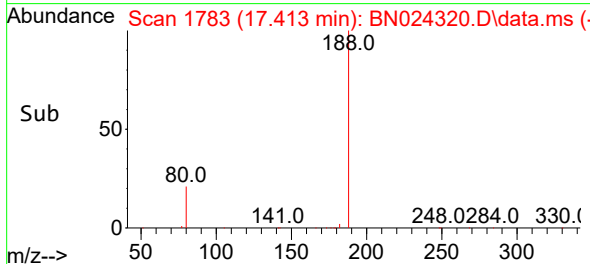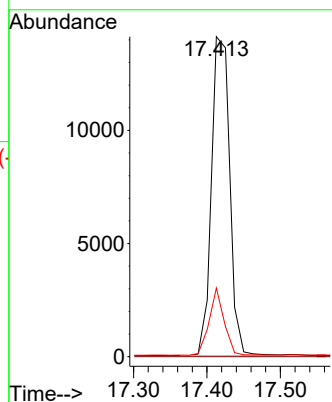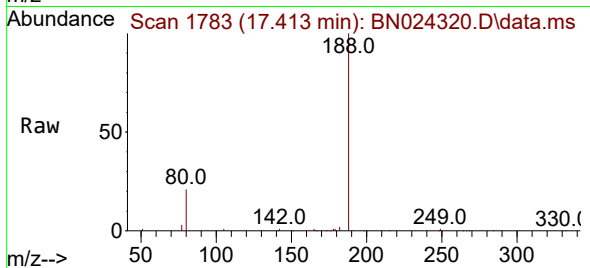

#20

4,6-Dinitro-2-methylphenol

Concen: 0.386 ng

RT: 15.787 min Scan# 1652

Delta R.T. 0.000 min

Lab File: BN024320.D

Acq: 16 Mar 2023 20:35




Tgt Ion:198 Resp: 946


Ion Ratio Lower Upper

198 100

51 91.8 68.2 102.2

105 63.8 51.6 77.4


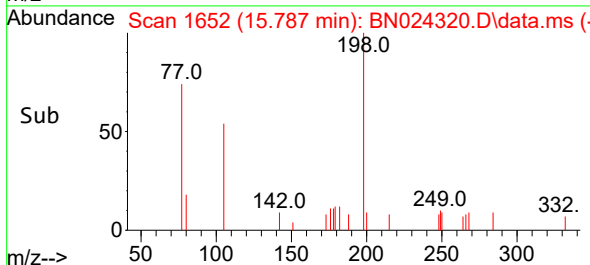

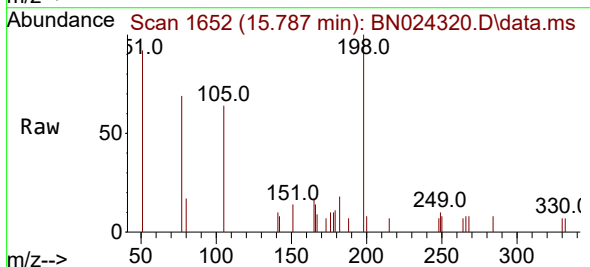




#21
4-Bromophenyl-phenylether
Concen: 0.339 ng
RT: 16.606 min Scan# 1718
Delta R.T. 0.000 min
Lab File: BN024320.D
Acq: 16 Mar 2023 20:35




Instrument :
BNA_N
ClientSampleId :
PB151396BS

Tgt Ion:248 Resp: 4909
Ion Ratio Lower Upper
248 100
250 95.9 81.9 122.9
141 66.5 28.2 42.2#



#22
Hexachlorobenzene
Concen: 0.373 ng
RT: 16.730 min Scan# 1728
Delta R.T. 0.000 min
Lab File: BN024320.D
Acq: 16 Mar 2023 20:35

Tgt Ion:284 Resp: 6636
Ion Ratio Lower Upper
284 100
142 42.1 30.2 45.4
249 31.4 24.5 36.7





#23

Atrazine

Concen: 0.385 ng

RT: 16.867 min Scan# 1739

Delta R.T. 0.000 min

Lab File: BN024320.D

Acq: 16 Mar 2023 20:35

Instrument :

BNA_N

ClientSampleId :

PB151396BS





Tgt Ion:200 Resp: 3536

Ion Ratio Lower Upper

200 100

173 31.5 18.9 28.3#

215 42.3 36.7 55.1

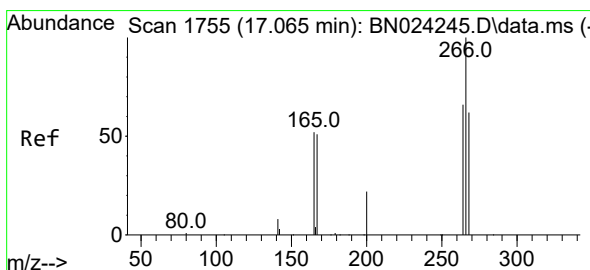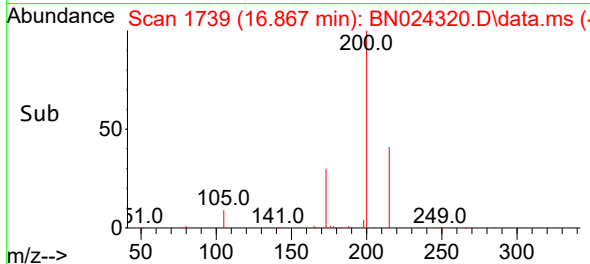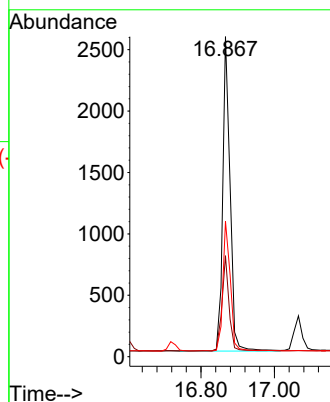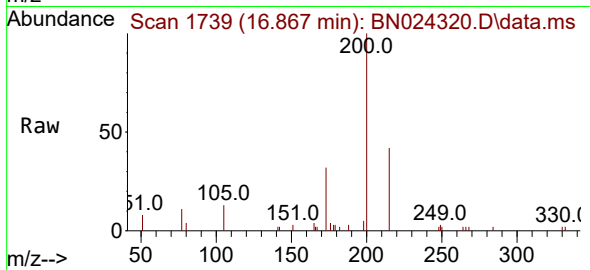

#24

Pentachlorophenol

Concen: 0.334 ng

RT: 17.065 min Scan# 1755

Delta R.T. 0.000 min

Lab File: BN024320.D

Acq: 16 Mar 2023 20:35




Tgt Ion:266 Resp: 2218


Ion Ratio Lower Upper

266 100

264 63.4 51.1 76.7

268 62.8 52.2 78.4


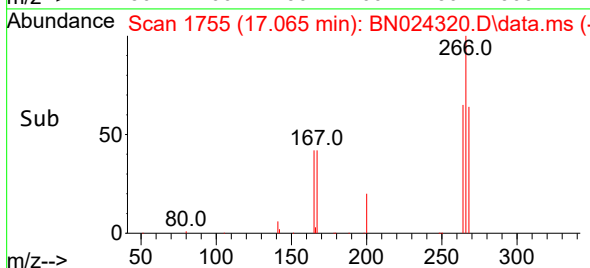

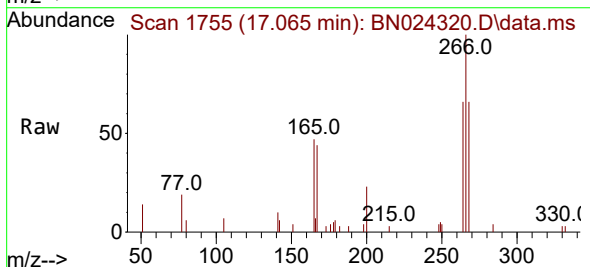


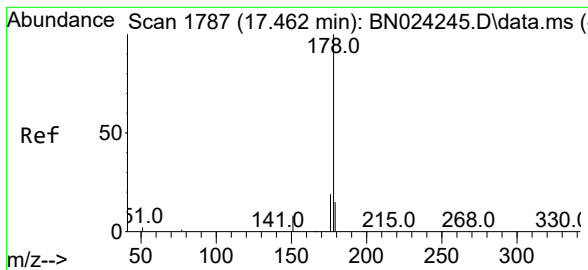

#25
 Phenanthrene
 Concen: 0.384 ng
 RT: 17.462 min Scan# 1787
 Delta R.T. 0.000 min
 Lab File: BN024320.D
 Acq: 16 Mar 2023 20:35




Instrument :
 BNA_N
 ClientSampleId :
 PB151396BS


Tgt Ion:	178	Resp:	27712
Ion Ratio	Lower	Upper	
178	100		
176	19.6	15.4	23.0
179	15.3	12.2	18.2

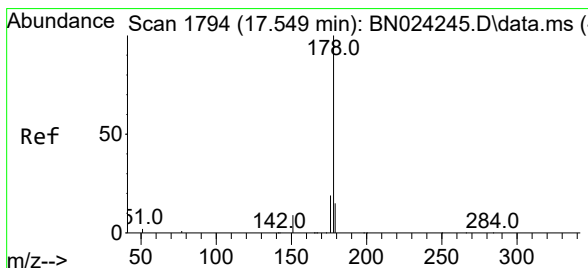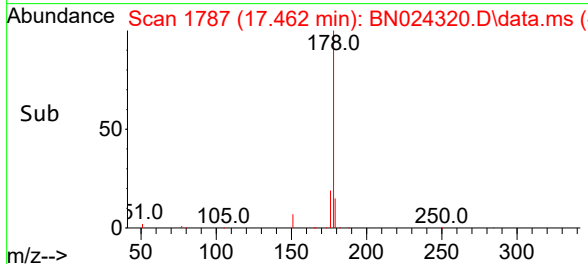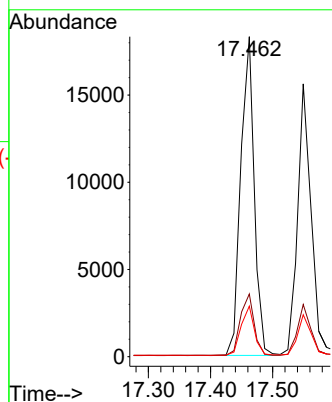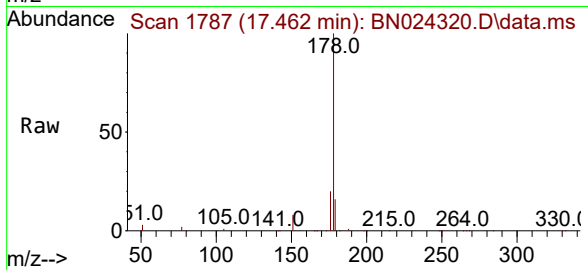

#26
 Anthracene
 Concen: 0.355 ng
 RT: 17.549 min Scan# 1794
 Delta R.T. 0.000 min
 Lab File: BN024320.D
 Acq: 16 Mar 2023 20:35

Tgt Ion:	178	Resp:	23659
Ion Ratio	Lower	Upper	
178	100		
176	18.9	15.1	22.7
179	14.8	12.1	18.1

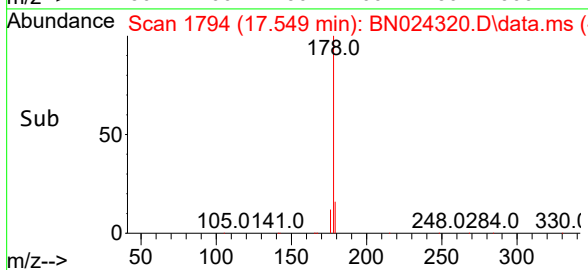

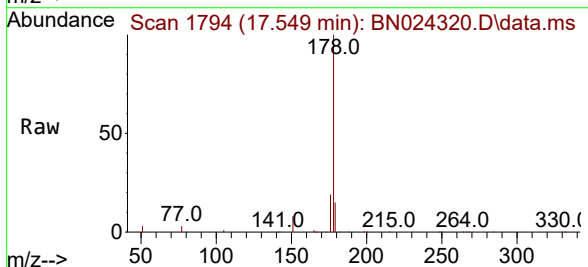




#27
Fluoranthene-d10
Concen: 0.353 ng
RT: 19.446 min Scan# 2172
Delta R.T. 0.000 min
Lab File: BN024320.D
Acq: 16 Mar 2023 20:35




Instrument :
BNA_N
ClientSampleId :
PB151396BS

Tgt Ion:212 Resp: 18251
Ion Ratio Lower Upper
212 100
106 21.2 15.4 23.2
104 12.4 8.6 13.0



#28
Fluoranthene
Concen: 0.364 ng
RT: 19.476 min Scan# 2179
Delta R.T. 0.000 min
Lab File: BN024320.D
Acq: 16 Mar 2023 20:35

Tgt Ion:202 Resp: 28783
Ion Ratio Lower Upper
202 100
101 15.3 11.3 16.9
203 17.0 13.6 20.4





#29

Chrysene-d12

Concen: 0.400 ng

RT: 21.610 min Scan# 2484

Delta R.T. 0.009 min

Lab File: BN024320.D

Acq: 16 Mar 2023 20:35

Instrument :

BNA_N

ClientSampleId :

PB151396BS





Tgt Ion:240 Resp: 17573

Ion Ratio Lower Upper

240 100

120 17.4 12.8 19.2

236 28.5 22.5 33.7

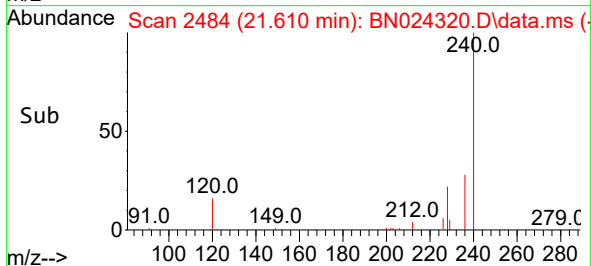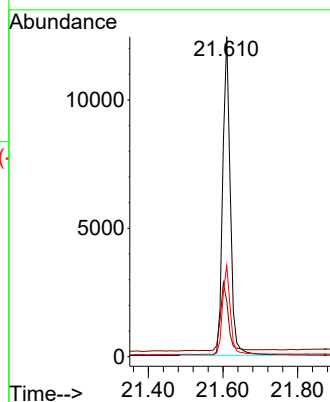

#30

Pyrene

Concen: 0.403 ng

RT: 19.838 min Scan# 2265

Delta R.T. 0.000 min

Lab File: BN024320.D

Acq: 16 Mar 2023 20:35




Tgt Ion:202 Resp: 28689

Ion Ratio Lower Upper

202 100

200 21.2 17.0 25.4

203 17.8 14.2 21.2

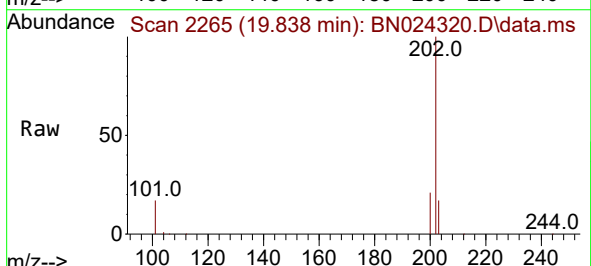



#31

Terphenyl-d14

Concen: 0.367 ng

RT: 20.034 min Scan# 21

Delta R.T. 0.000 min

Lab File: BN024320.D

Acq: 16 Mar 2023 20:35

Instrument :

BNA_N

ClientSampleId :

PB151396BS




Tgt Ion:244 Resp: 10870

Ion Ratio Lower Upper

244 100

212 11.4 7.6 11.4#

122 26.5 15.1 22.7#

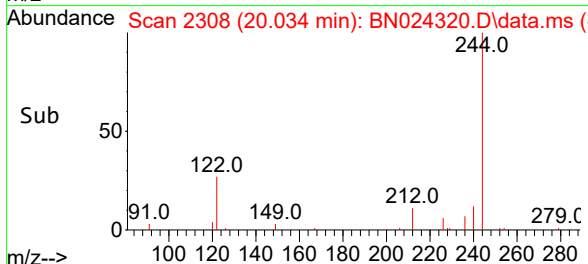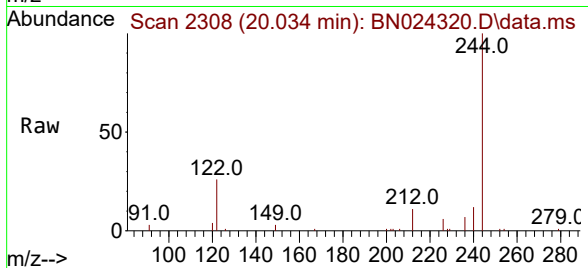

#32

Benzo(a)anthracene

Concen: 0.361 ng

RT: 21.592 min Scan# 2482

Delta R.T. 0.009 min

Lab File: BN024320.D

Acq: 16 Mar 2023 20:35




Tgt Ion:228 Resp: 21207

Ion Ratio Lower Upper

228 100

226 28.2 22.2 33.2

229 19.9 15.9 23.9

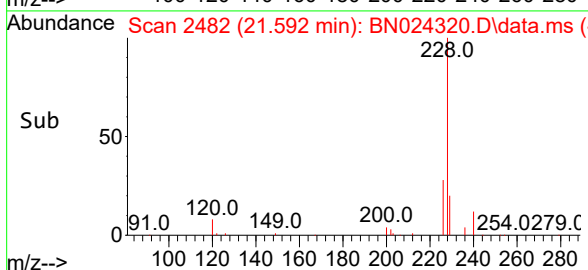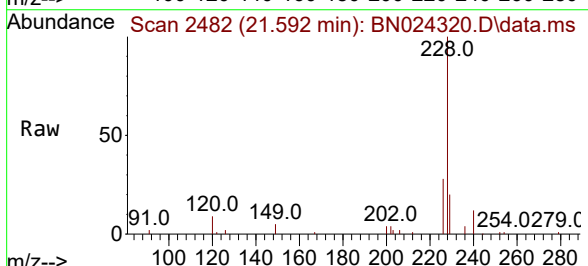



#33

Chrysene

Concen: 0.399 ng

RT: 21.646 min Scan# 2488

Delta R.T. 0.000 min

Lab File: BN024320.D

Acq: 16 Mar 2023 20:35

Instrument :

BNA_N

ClientSampleId :

PB151396BS





Tgt Ion:228 Resp: 25001

Ion Ratio Lower Upper

228 100

226 31.3 24.5 36.7

229 19.3 15.5 23.3

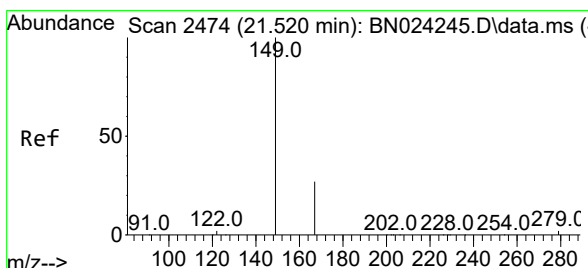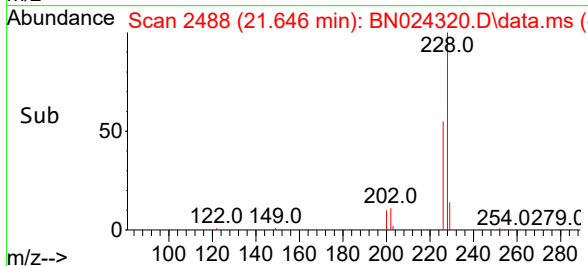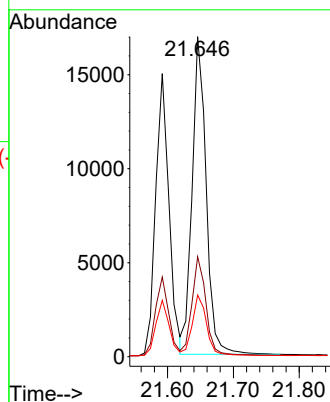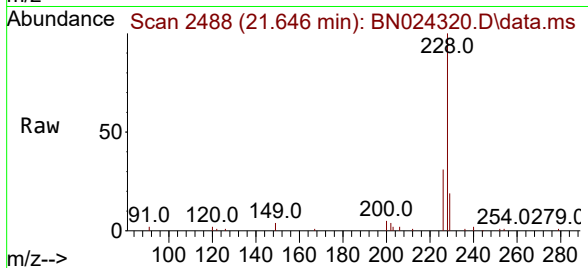

#34

Bis(2-ethylhexyl)phthalate

Concen: 0.400 ng

RT: 21.511 min Scan# 2473

Delta R.T. 0.009 min

Lab File: BN024320.D

Acq: 16 Mar 2023 20:35




Tgt Ion:149 Resp: 11060


Ion Ratio Lower Upper

149 100

167 24.5 21.2 31.8

279 2.4 1.8 2.8

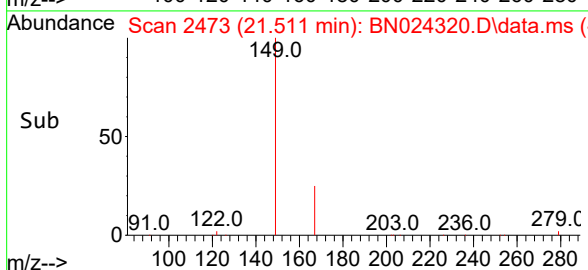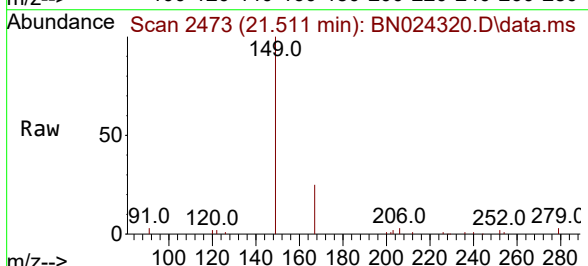




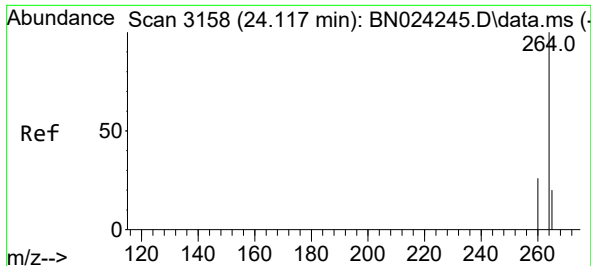


#35
Perylene-d12

Concen: 0.400 ng
RT: 24.120 min Scan# 3159
Delta R.T. 0.006 min
Lab File: BN024320.D
Acq: 16 Mar 2023 20:35




Instrument :
BNA_N
ClientSampleId :
PB151396BS


Tgt Ion:264 Resp: 13298
Ion Ratio Lower Upper
264 100
260 27.5 21.4 32.2
265 54.5 35.7 53.5#

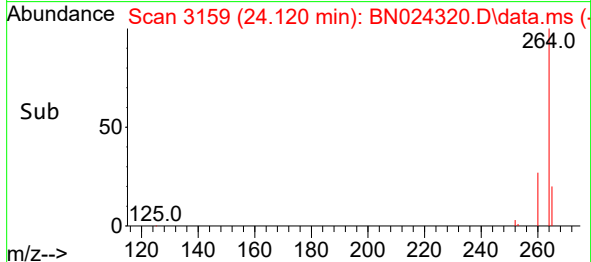

#36
Indeno(1,2,3-cd)pyrene
Concen: 0.382 ng
RT: 26.743 min Scan# 4056
Delta R.T. 0.003 min
Lab File: BN024320.D
Acq: 16 Mar 2023 20:35

Tgt Ion:276 Resp: 18999
Ion Ratio Lower Upper
276 100
138 38.0 27.4 41.2
277 25.0 19.8 29.6

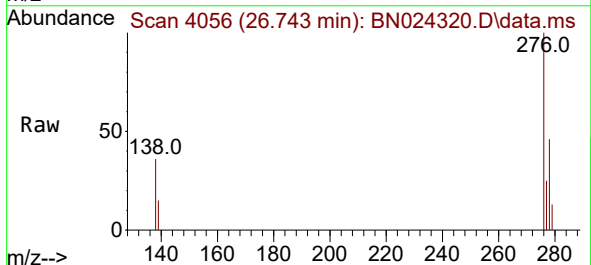



#37

Benzo(b)fluoranthene

Concen: 0.420 ng

RT: 23.398 min Scan# 2912

Delta R.T. 0.056 min

Lab File: BN024320.D

Acq: 16 Mar 2023 20:35

Instrument :

BNA_N

ClientSampleId :

PB151396BS





Tgt Ion:252 Resp: 21708

Ion Ratio Lower Upper

252 100

253 23.9 18.9 28.3

125 20.2 13.8 20.6



#38

Benzo(k)fluoranthene

Concen: 0.381 ng

RT: 23.398 min Scan# 2912

Delta R.T. 0.003 min

Lab File: BN024320.D

Acq: 16 Mar 2023 20:35




Tgt Ion:252 Resp: 20338

Ion Ratio Lower Upper

252 100

253 23.9 19.0 28.6

125 20.2 13.5 20.3









#39
Benzo(a)pyrene
Concen: 0.373 ng
RT: 24.006 min Scan# 3119
Delta R.T. 0.009 min
Lab File: BN024320.D
Acq: 16 Mar 2023 20:35




Instrument :
BNA_N
ClientSampleId :
PB151396BS

Tgt Ion:252 Resp: 17714
Ion Ratio Lower Upper
252 100
253 25.5 19.5 29.3
125 25.4 16.2 24.4#



#40
Dibenzo(a,h)anthracene
Concen: 0.372 ng
RT: 26.766 min Scan# 4064
Delta R.T. 0.006 min
Lab File: BN024320.D
Acq: 16 Mar 2023 20:35


Tgt Ion:278 Resp: 14335
Ion Ratio Lower Upper
278 100
139 26.8 19.4 29.0
279 27.0 20.7 31.1





#41
 Benzo(g,h,i)perylene
 Concen: 0.394 ng
 RT: 27.558 min Scan# 41
 Delta R.T. 0.003 min
 Lab File: BN024320.D
 Acq: 16 Mar 2023 20:35

Instrument :
 BNA_N
 ClientSampleId :
 PB151396BS

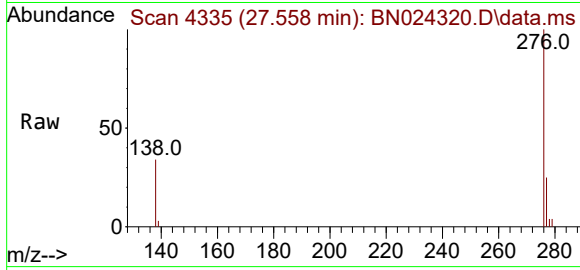

Tgt Ion:	276	Resp:	17761
Ion	Ratio	Lower	Upper
276	100		
277	24.7	19.9	29.9
138	34.2	24.5	36.7

