
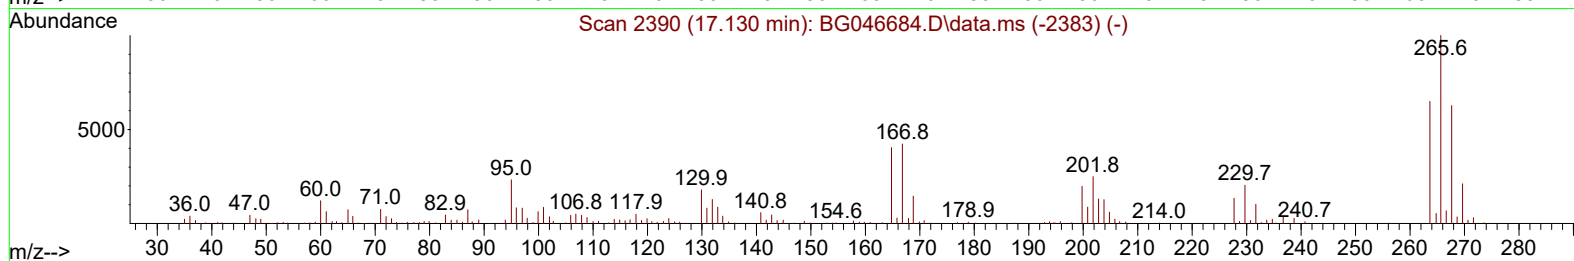
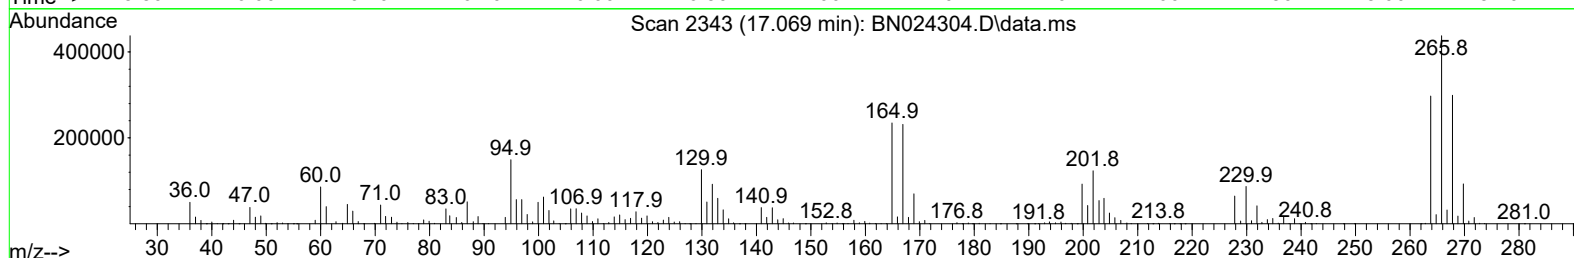


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031623\
Data File : BN024304.D
Acq On : 16 Mar 2023 09:23
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 17 07:35:56 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 17 07:35:50 2023
Response via : Initial Calibration

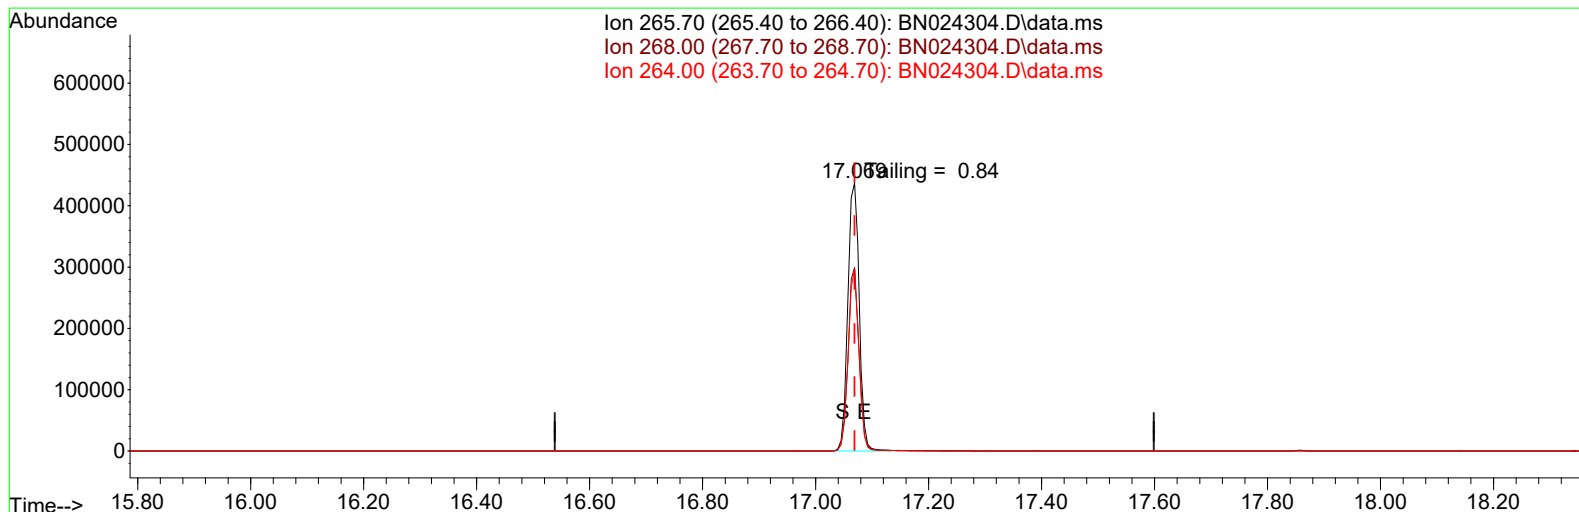

TIC: BN024304.D\data.ms

(70) Pentachlorophenol (C)




17.069min (0.000) 23753.83 ng

response 613116

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	68.36
264.00	61.60	67.89
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031623\
Data File : BN024304.D
Acq On : 16 Mar 2023 09:23
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 17 07:35:56 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 17 07:35:50 2023
Response via : Initial Calibration

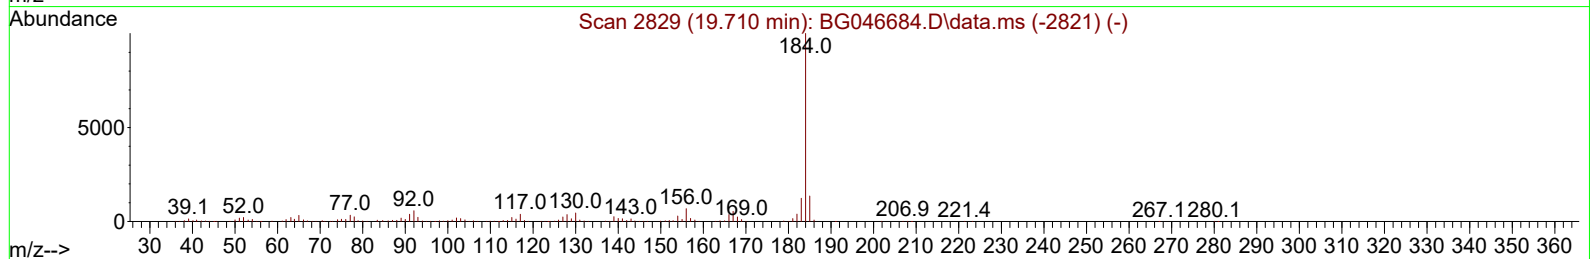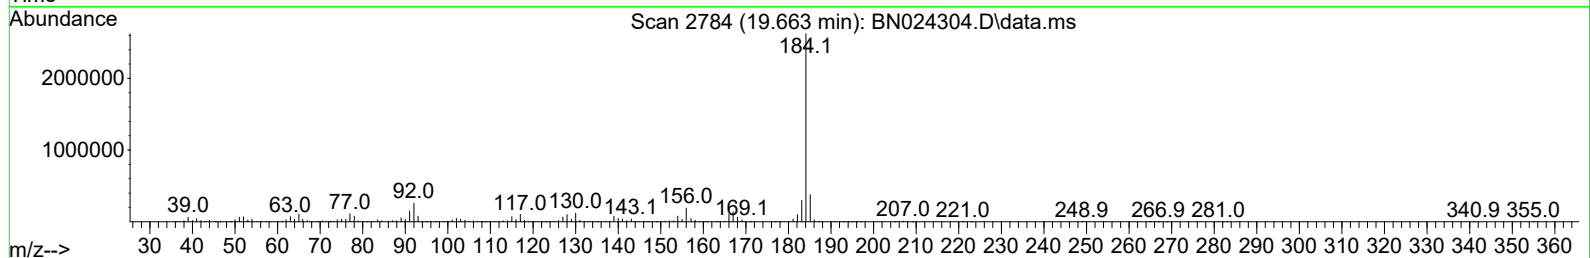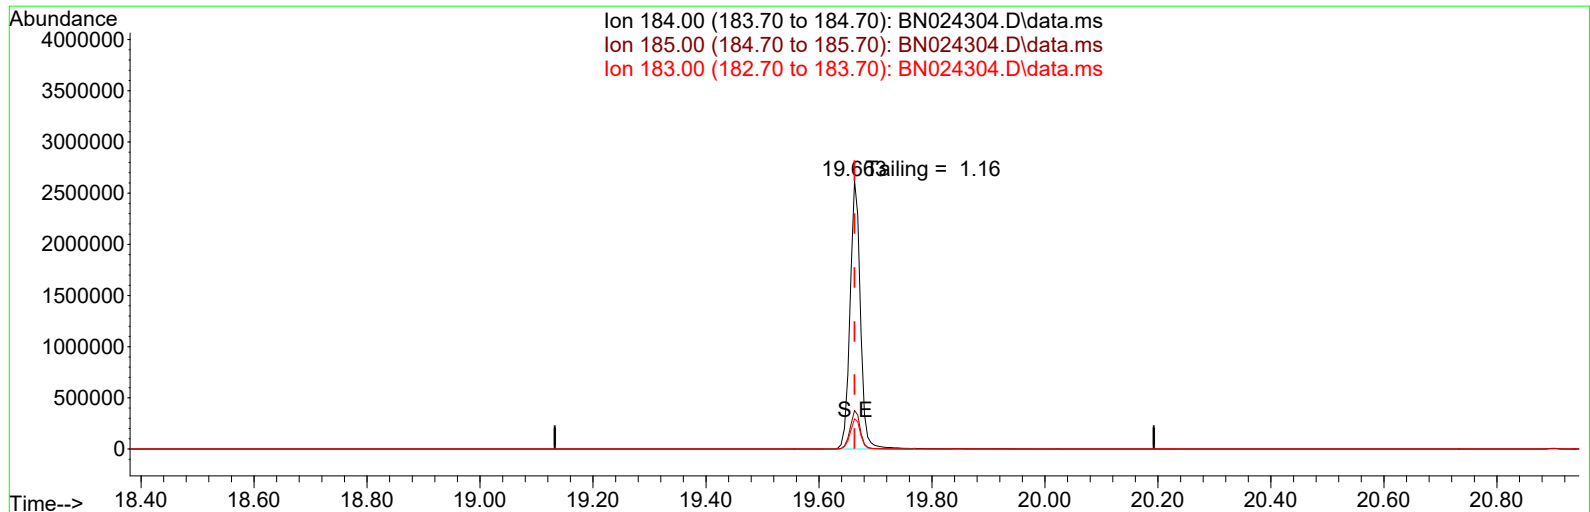

TIC: BN024304.D\data.ms

(77) Benzidine**19.663min (0.000) 933545.25 ng****response 3338118**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.42
183.00	13.20	11.29
0.00	0.00	0.00