
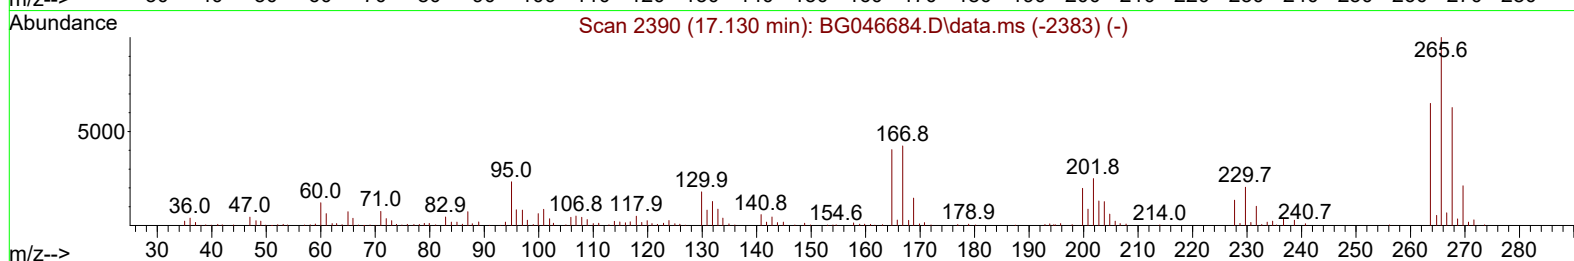
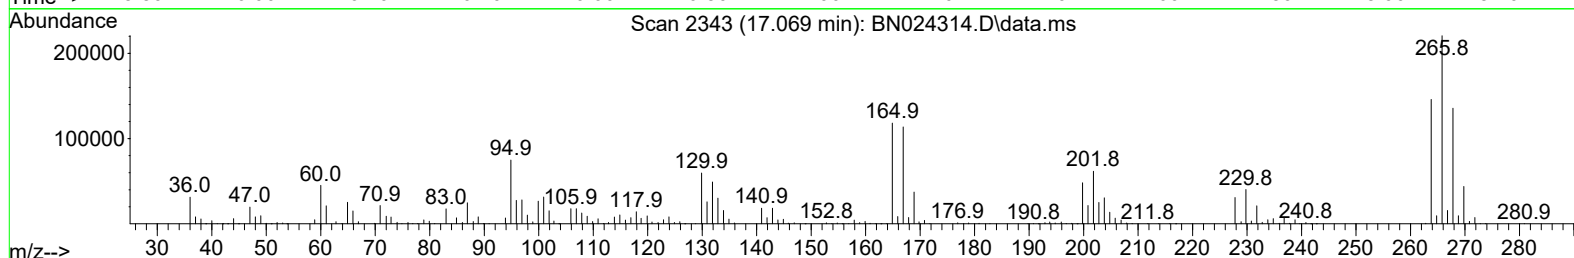


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031623\
 Data File : BN024314.D
 Acq On : 16 Mar 2023 16:54
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 17 07:37:07 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 17 07:35:50 2023
 Response via : Initial Calibration

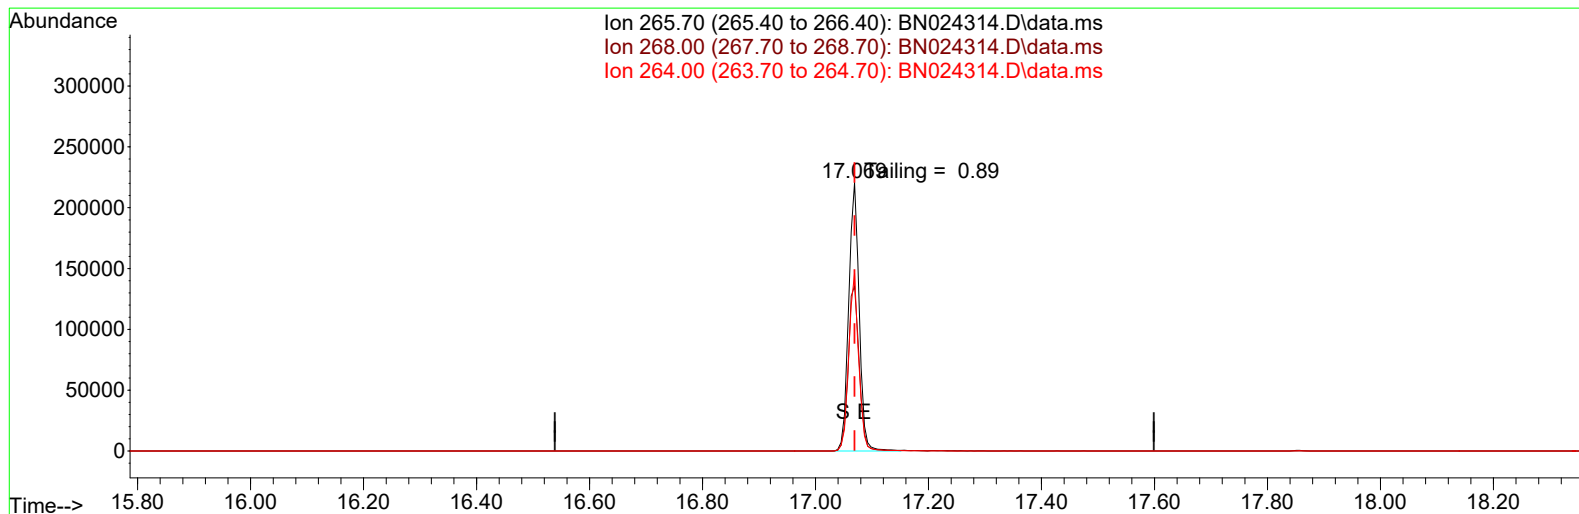

TIC: BN024314.D\data.ms

(70) Pentachlorophenol (C)




17.069min (+ 0.000) 25419.35 ng

response 286061

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.47
264.00	61.60	66.17
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031623\
 Data File : BN024314.D
 Acq On : 16 Mar 2023 16:54
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 17 07:37:07 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 17 07:35:50 2023
 Response via : Initial Calibration

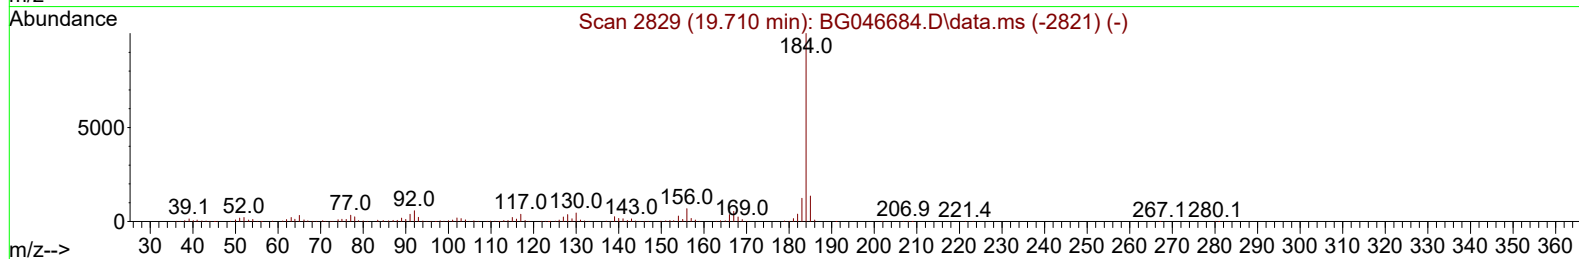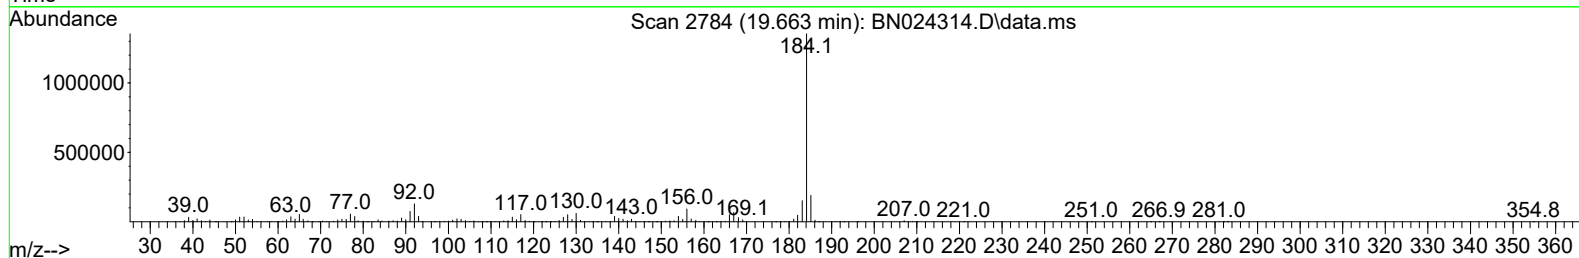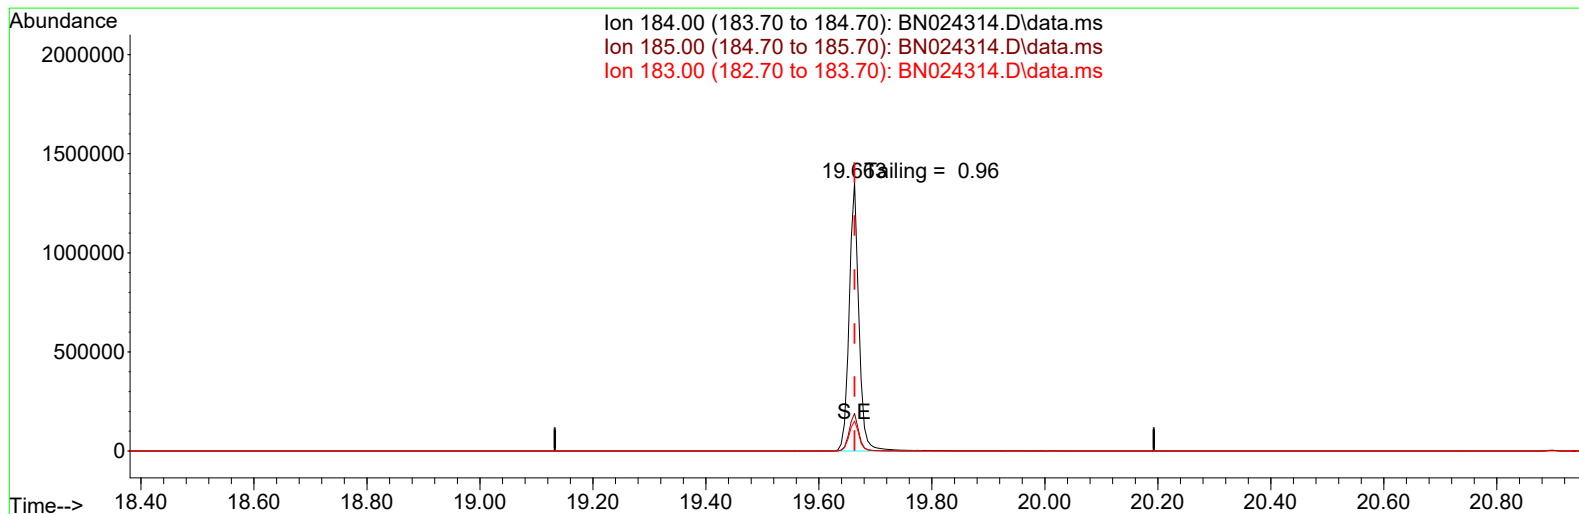

TIC: BN024314.D\data.ms

(77) Benzidine**19.663min (+ 0.000) 0.00 ng****response 1634680**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.03
183.00	13.20	11.25
0.00	0.00	0.00