
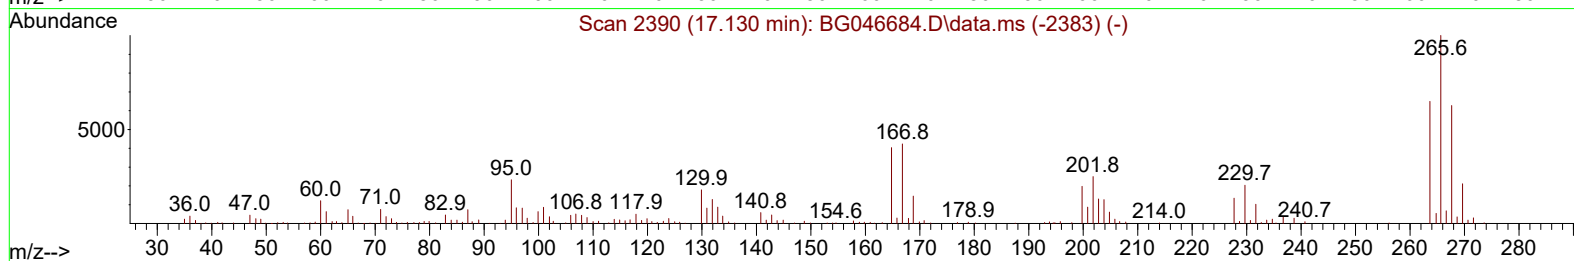
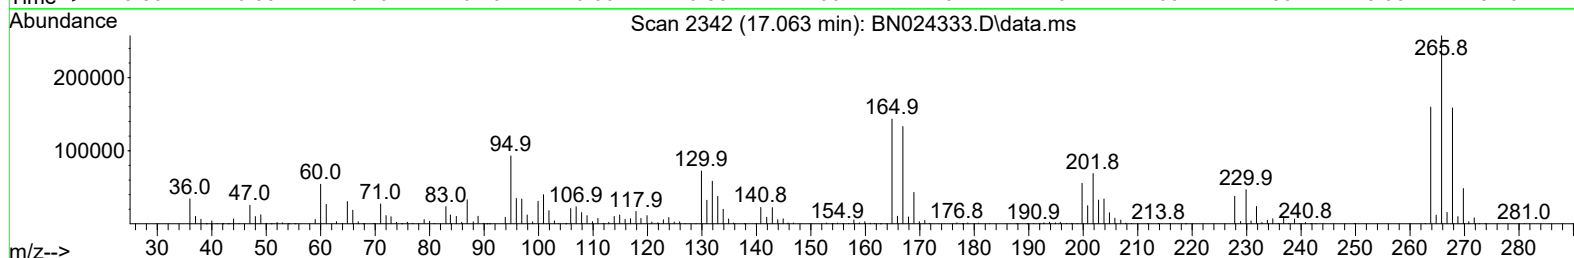


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031623\
Data File : BN024333.D
Acq On : 17 Mar 2023 05:47
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 17 07:38:11 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 17 07:35:50 2023
Response via : Initial Calibration

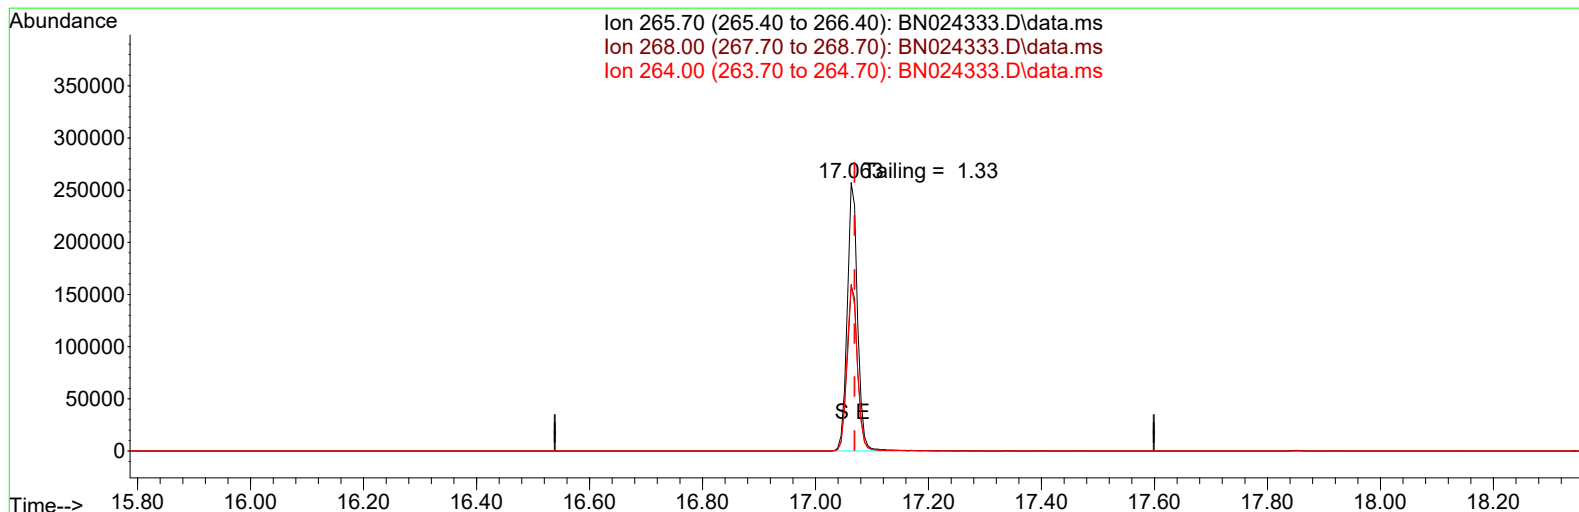

TIC: BN024333.D\data.ms

(70) Pentachlorophenol (C)




17.063min (-0.006) 22393.06 ng

response 327043

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.61
264.00	61.60	62.08
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031623\  
Data File : BN024333.D  
Acq On    : 17 Mar 2023   05:47  
Operator  : CG/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Quant Time: Mar 17 07:38:11 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 17 07:35:50 2023
Response via : Initial Calibration

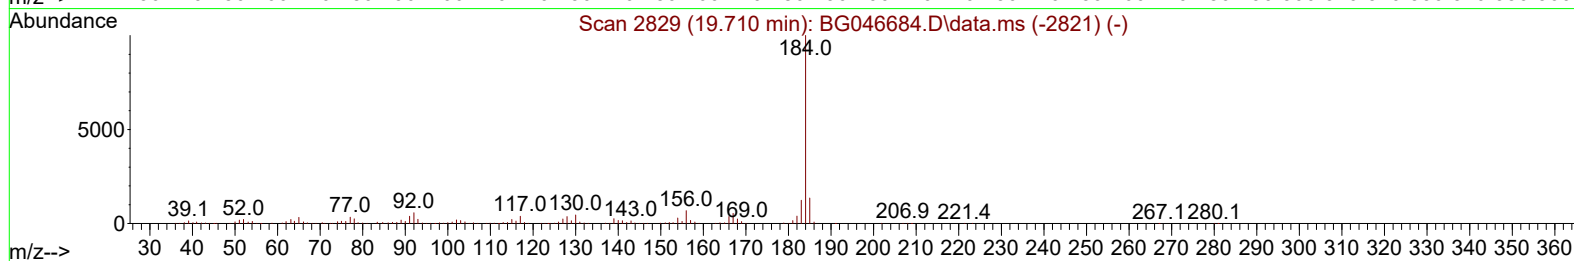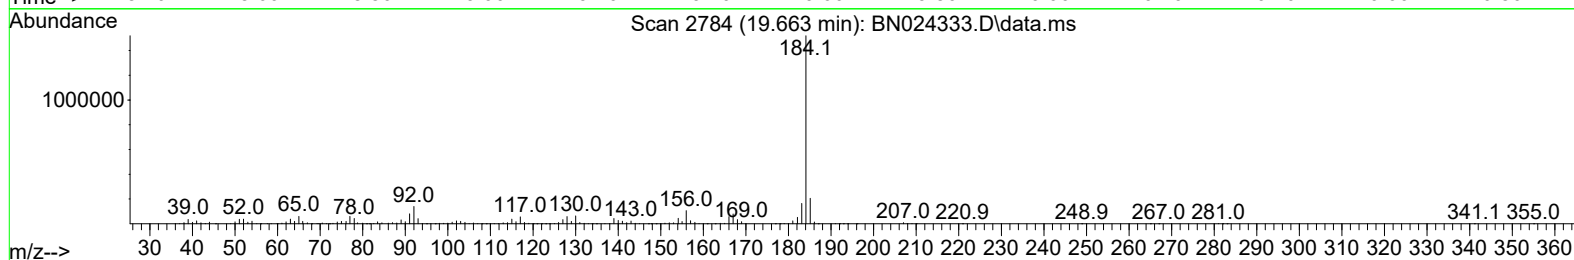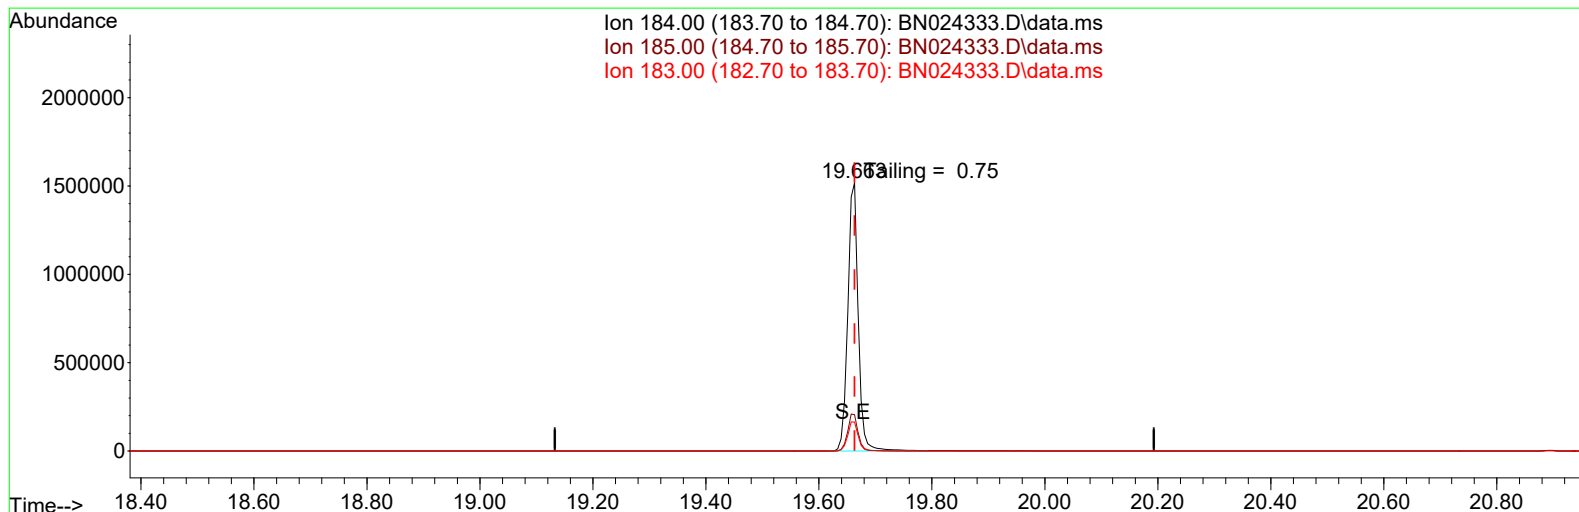

TIC: BN024333.D\data.ms

(77) Benzidine

19.663min (+ 0.000) 0.00 ng

response **1949034**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.56
183.00	13.20	10.80
0.00	0.00	0.00