


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031623\
 Data File : BN024304.D
 Acq On : 16 Mar 2023 09:23
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN031323.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Mar 17 04:37:08 2023

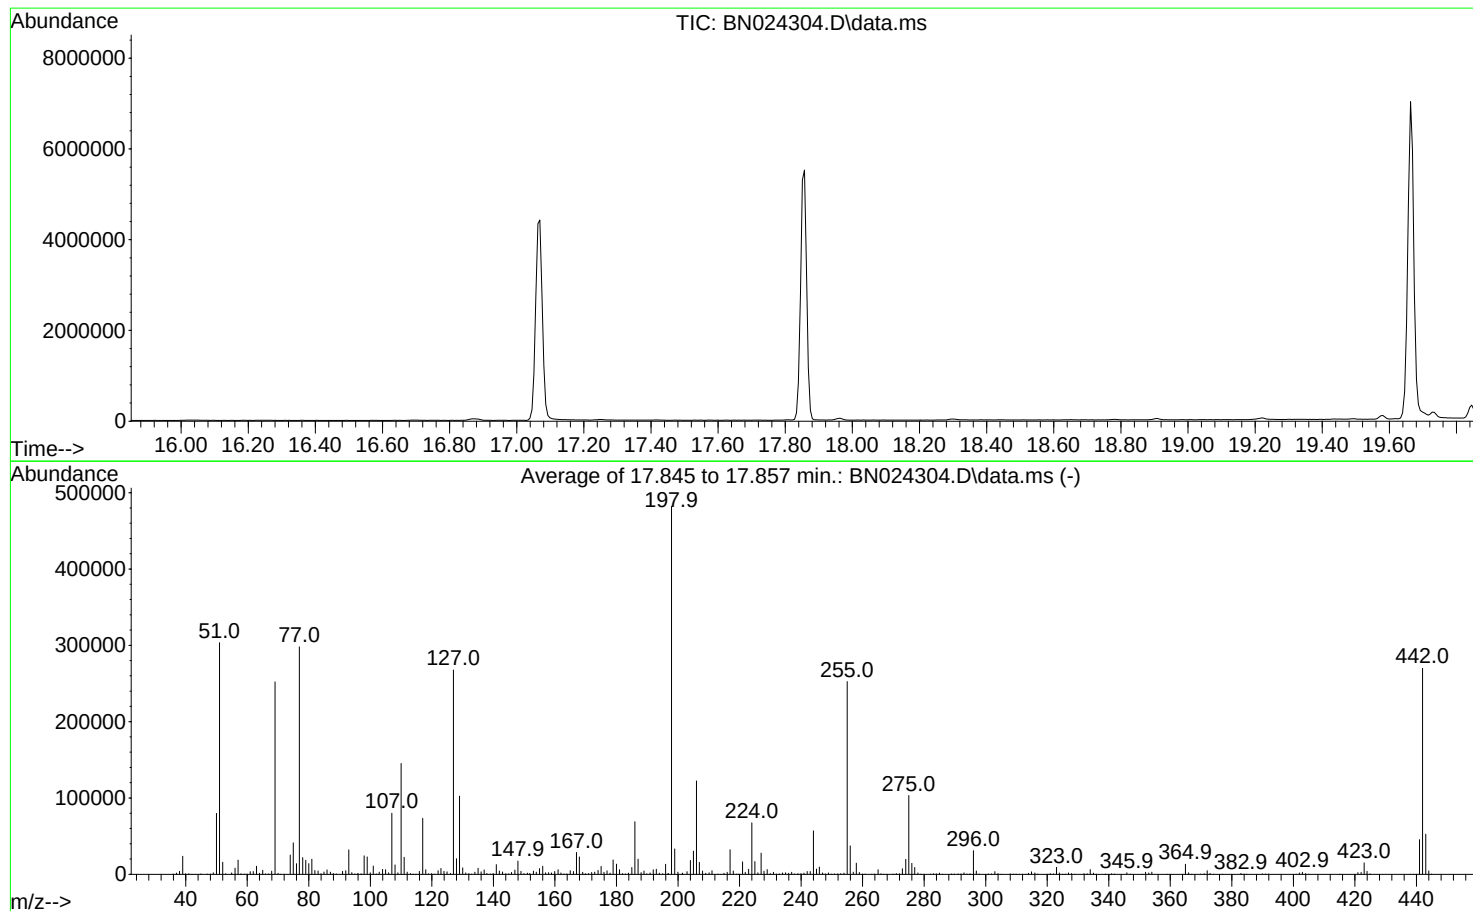




AutoFind: Scans 2475, 2476, 2477; Background Corrected with Scan 2469

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	63.0	303572	PASS
68	69	0.00	2	1.6	4133	PASS
69	198	0.00	100	52.3	252139	PASS
70	69	0.00	2	0.5	1339	PASS
127	198	10	80	55.5	267605	PASS
197	198	0.00	2	0.2	1040	PASS
198	198	100	100	100.0	481984	PASS
199	198	5	9	6.9	33216	PASS
275	198	10	60	21.4	103227	PASS
365	198	1	100	2.7	13106	PASS
441	198	0.01	100	9.4	45373	PASS
442	442	50	100	100.0	269851	PASS
443	442	15	24	19.5	52491	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031623\
 Data File : BN024304.D
 Acq On : 16 Mar 2023 09:23
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Mar 17 07:35:56 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 17 07:35:50 2023
 Response via : Initial Calibration

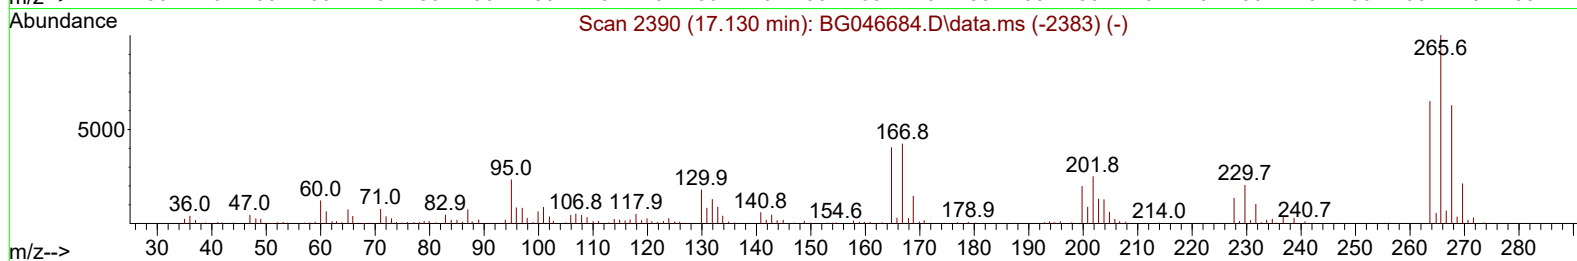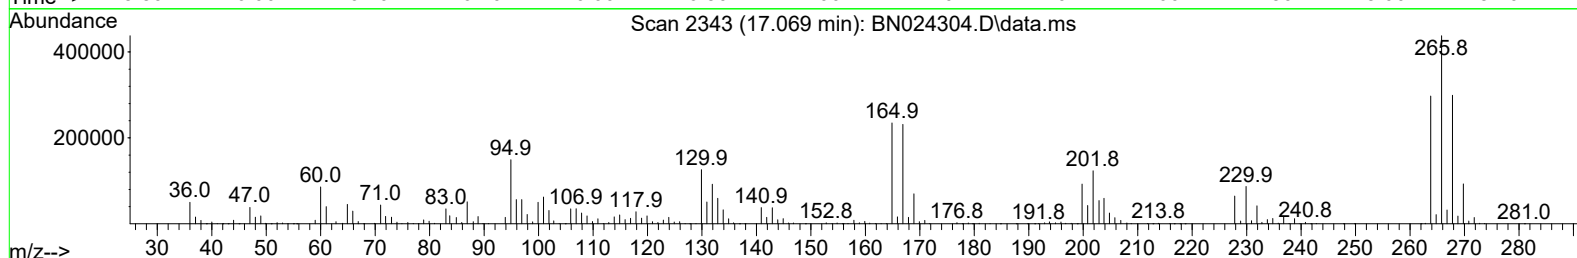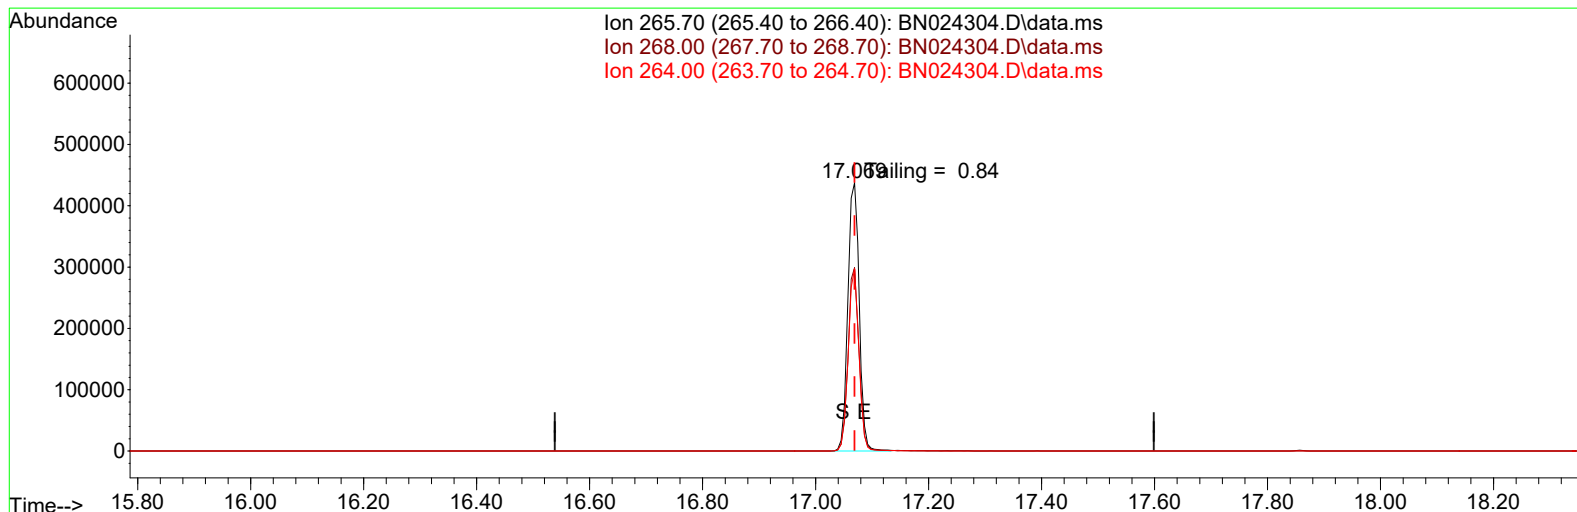

TIC: BN024304.D\data.ms

(70) Pentachlorophenol (C)

17.069min (0.000) 23753.83 ng




response 613116

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	68.36
264.00	61.60	67.89
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031623\
Data File : BN024304.D
Acq On : 16 Mar 2023 09:23
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 17 07:35:56 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 17 07:35:50 2023
Response via : Initial Calibration

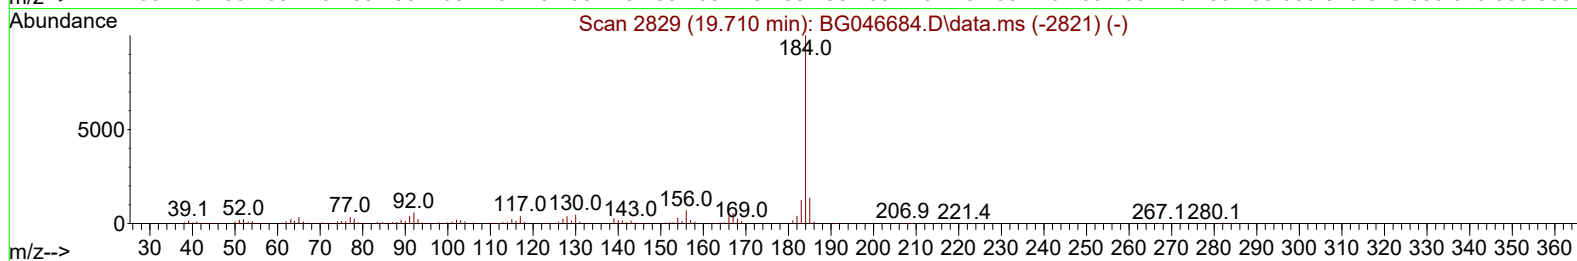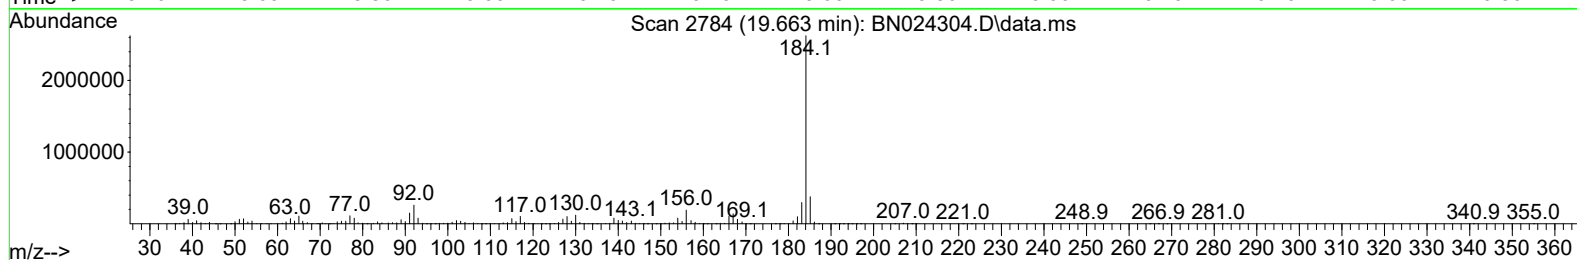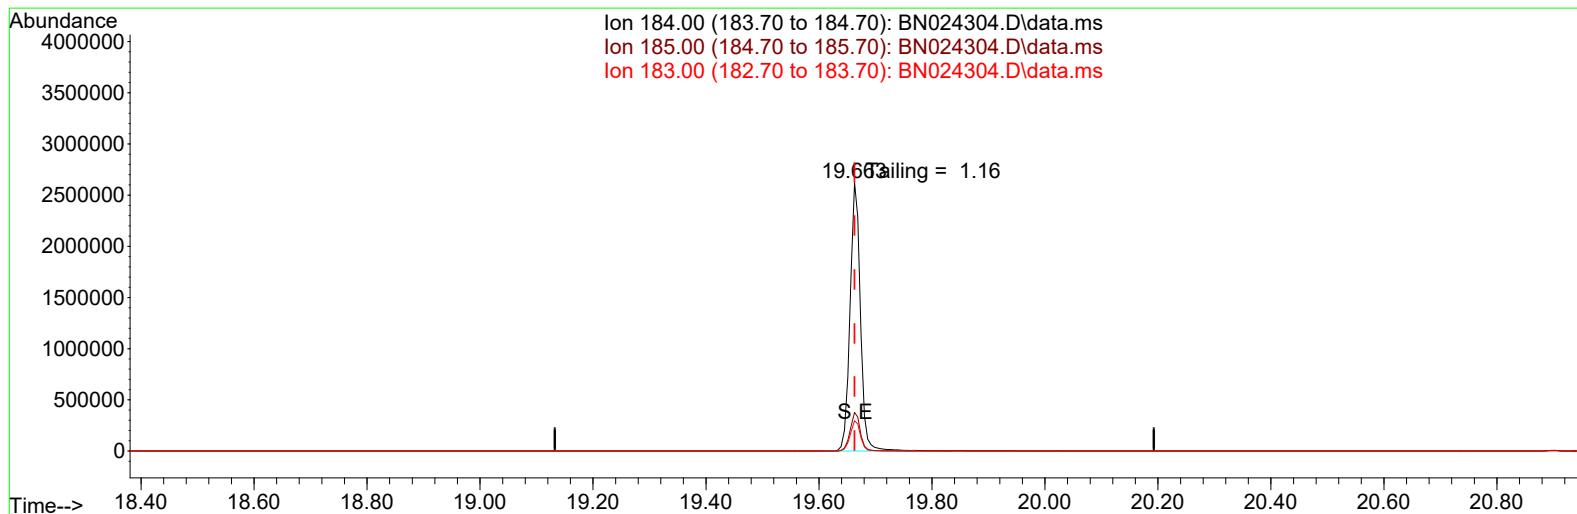

TIC: BN024304.D\data.ms

(77) Benzidine

19.663min (0.000) 933545.25 ng

response 3338118

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.42
183.00	13.20	11.29
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/16/2023	BNA_N	<u>BN024304.D</u>
Compound Name	Response	Retention Time
DDT	1625666	20.904
DDD	34368	20.457
DDE	1818	19.945
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
36186	1661852	2.18

Instrument :
BNA_N
ClientSampleId :
DFTPP