
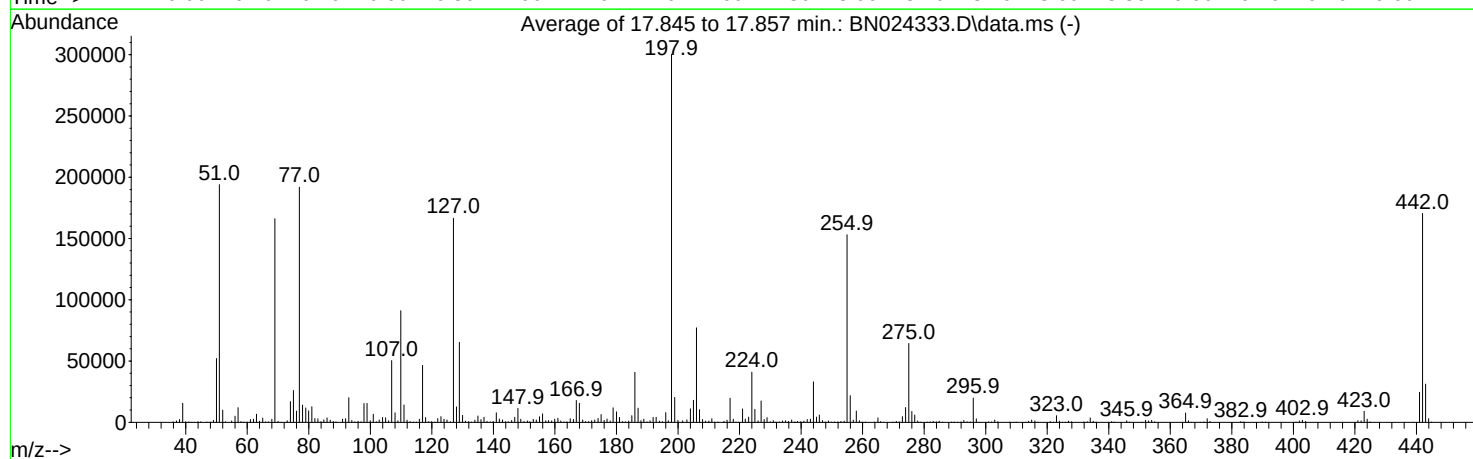


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031623\
 Data File : BN024333.D
 Acq On : 17 Mar 2023 05:47
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN031323.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Mar 17 04:37:08 2023

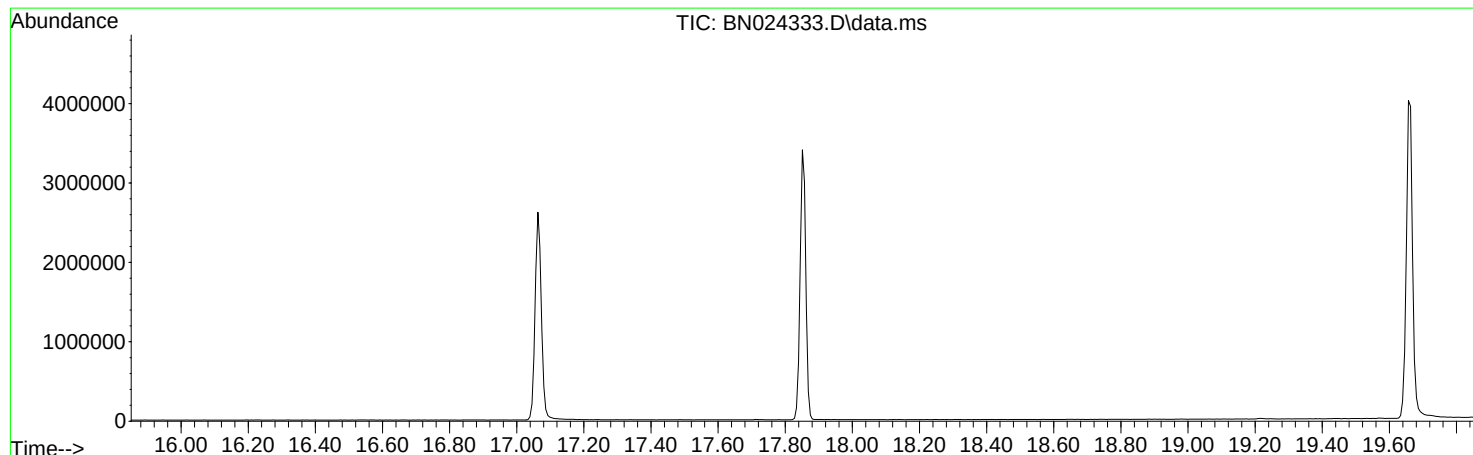




AutoFind: Scans 2475, 2476, 2477; Background Corrected with Scan 2469

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	64.6	193971	PASS
68	69	0.00	2	1.5	2551	PASS
69	198	0.00	100	55.3	166144	PASS
70	69	0.00	2	0.5	859	PASS
127	198	10	80	55.5	166637	PASS
197	198	0.00	2	0.4	1303	PASS
198	198	100	100	100.0	300245	PASS
199	198	5	9	6.8	20276	PASS
275	198	10	60	21.4	64315	PASS
365	198	1	100	2.6	7691	PASS
441	198	0.01	100	8.1	24438	PASS
442	442	50	100	100.0	170520	PASS
443	442	15	24	18.3	31157	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031623\
 Data File : BN024333.D
 Acq On : 17 Mar 2023 05:47
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Mar 17 07:38:11 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 17 07:35:50 2023
 Response via : Initial Calibration

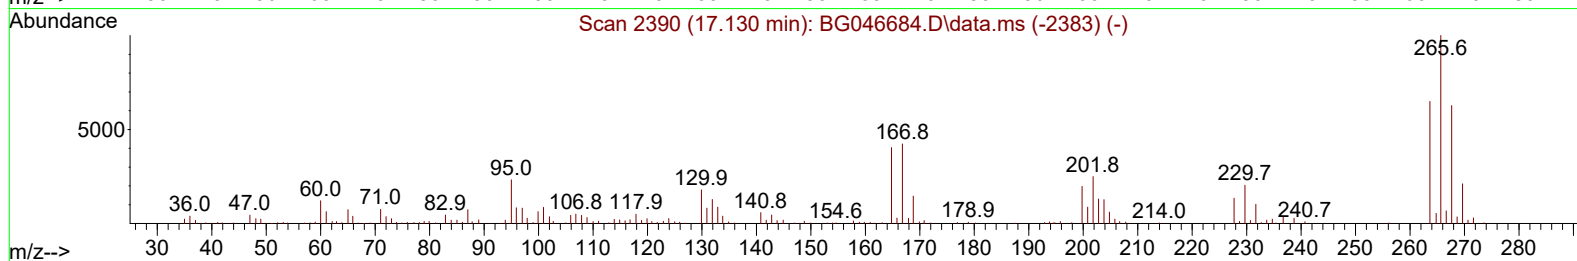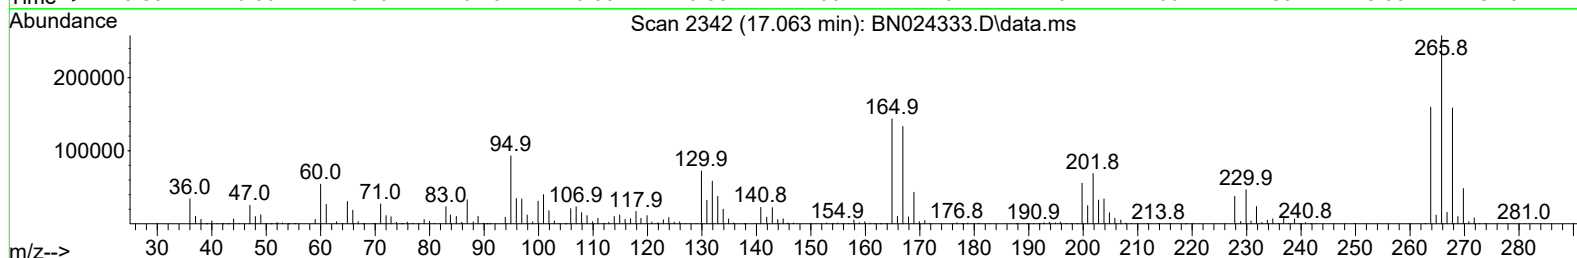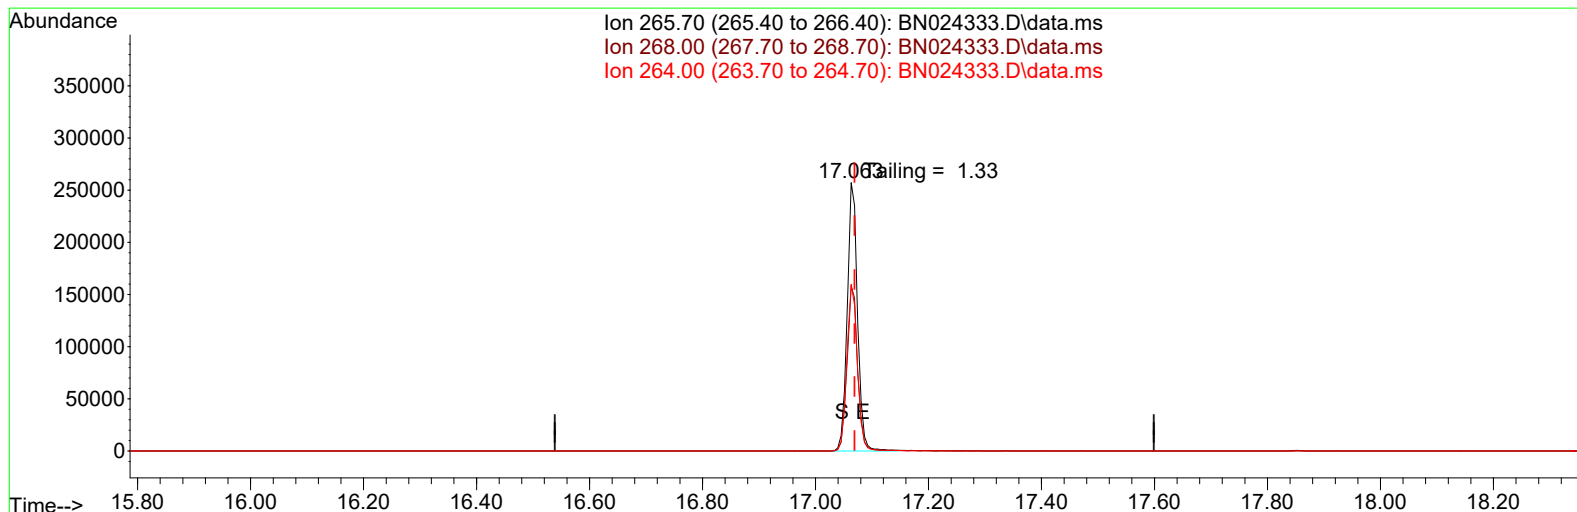

TIC: BN024333.D\data.ms

(70) Pentachlorophenol (C)

17.063min (-0.006) 22393.06 ng




response 327043

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.61
264.00	61.60	62.08
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031623\  
Data File : BN024333.D  
Acq On    : 17 Mar 2023   05:47  
Operator  : CG/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 17 07:38:11 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Qlast Update : Fri Mar 17 07:35:50 2023
Response via : Initial Calibration

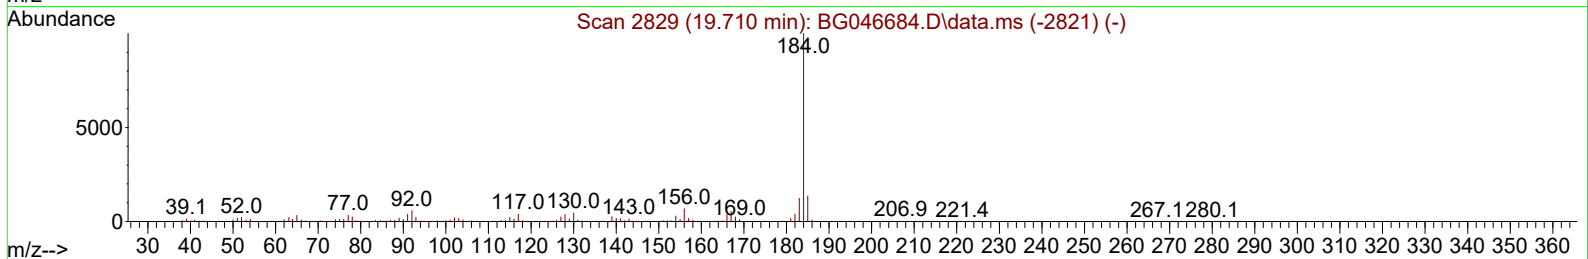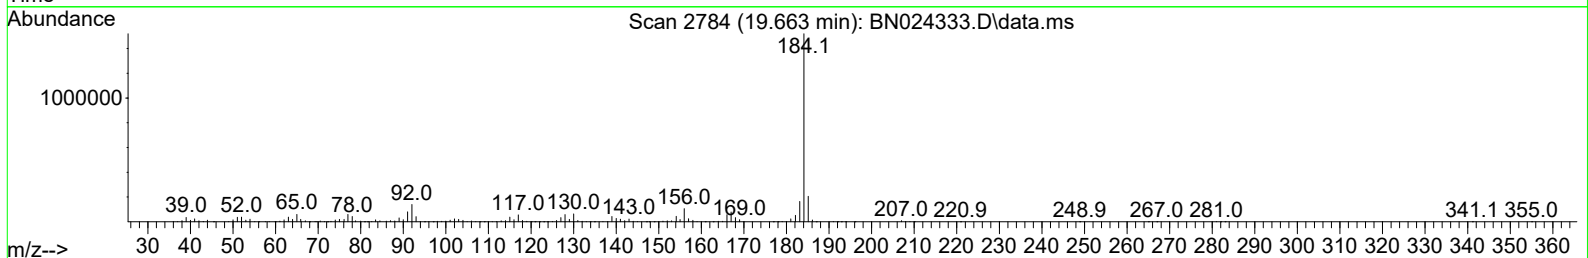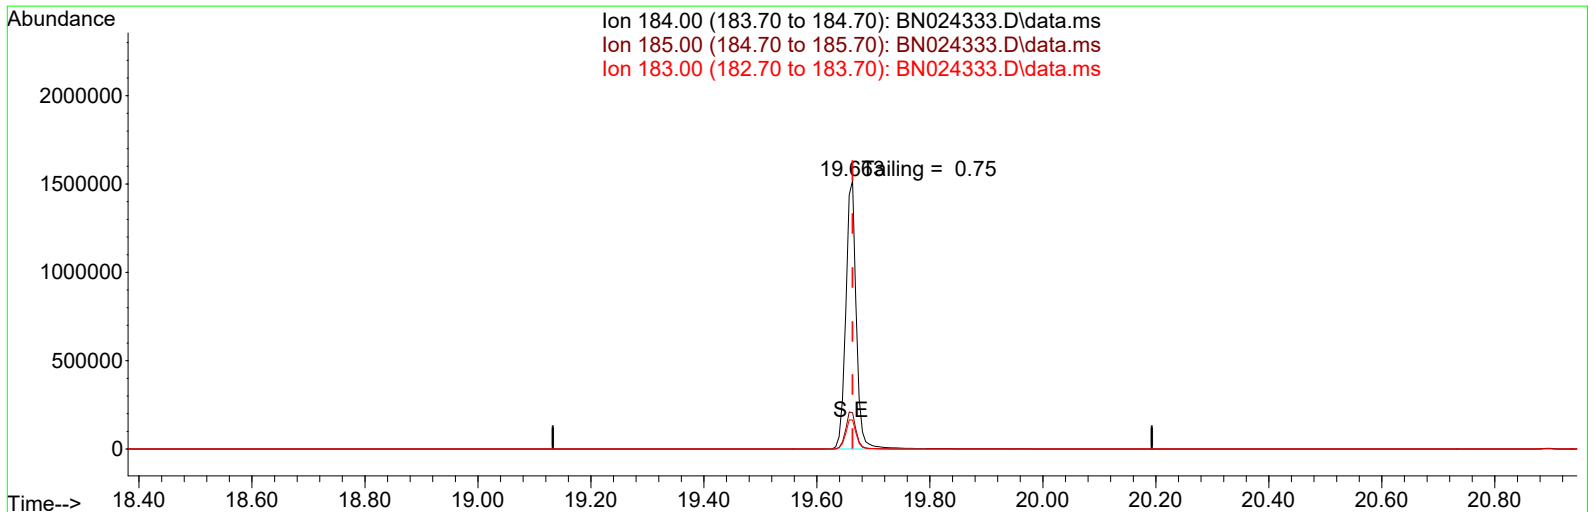

TIC: BN024333.D\data.ms

(77) Benzidine

19.663min (+ 0.000) 0.00 ng

response **1949034**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.56
183.00	13.20	10.80
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/16/2023	BNA_N	<u>BN024333.D</u>
Compound Name	Response	Retention Time
DDT	885395	20.892
DDD	21241	20.451
DDE	1026	19.945
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
22267	907662	2.45

Instrument :
BNA_N
ClientSampleId :
DFTPP