

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN031720\
 Data File : BN010241.D
 Acq On : 17 Mar 2020 15:59
 Operator : CG/JU
 Sample : L1903-05
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 MW201D1-20200307

Quant Time: Mar 17 17:25:53 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN031320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 16 02:17:23 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.63	152	3445	0.40	ng	0.00
7) Naphthalene-d8	10.39	136	11647	0.40	ng	0.00
13) Acenaphthene-d10	14.25	164	6917	0.40	ng	-0.01
19) Phenanthrene-d10	17.00	188	16474	0.40	ng	0.00
27) Chrysene-d12	21.19	240	17450	0.40	ng	-0.01
34) Perylene-d12	23.36	264	21437	0.40	ng	-0.01
System Monitoring Compounds						
4) 2-Fluorophenol	5.26	112	1265	0.16	ng	0.00
5) Phenol-d6	6.81	99	1002	0.10	ng	0.00
8) Nitrobenzene-d5	8.76	82	2744	0.39	ng	-0.01
11) 2-Methylnaphthalene-d10	11.98	152	6644	0.35	ng	0.00
14) 2,4,6-Tribromophenol	15.74	330	897	0.36	ng	-0.01
15) 2-Fluorobiphenyl	12.88	172	11370	0.46	ng	0.00
25) Fluoranthene-d10	19.03	212	18357	0.36	ng	0.00
29) Terphenyl-d14	19.64	244	18142	0.46	ng	-0.01
Target Compounds						
2) 1,4-Dioxane	3.26	88	216	0.064	ng	# 60
32) Bis(2-ethylhexyl)phthalate	21.14	149	586	0.023	ng	# 96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN031720\
Data File : BN010241.D
Acq On : 17 Mar 2020 15:59
Operator : CG/JU
Sample : L1903-05
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
MW201D1-20200307

Quant Time: Mar 17 17:25:53 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN031320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 16 02:17:23 2020
Response via : Initial Calibration

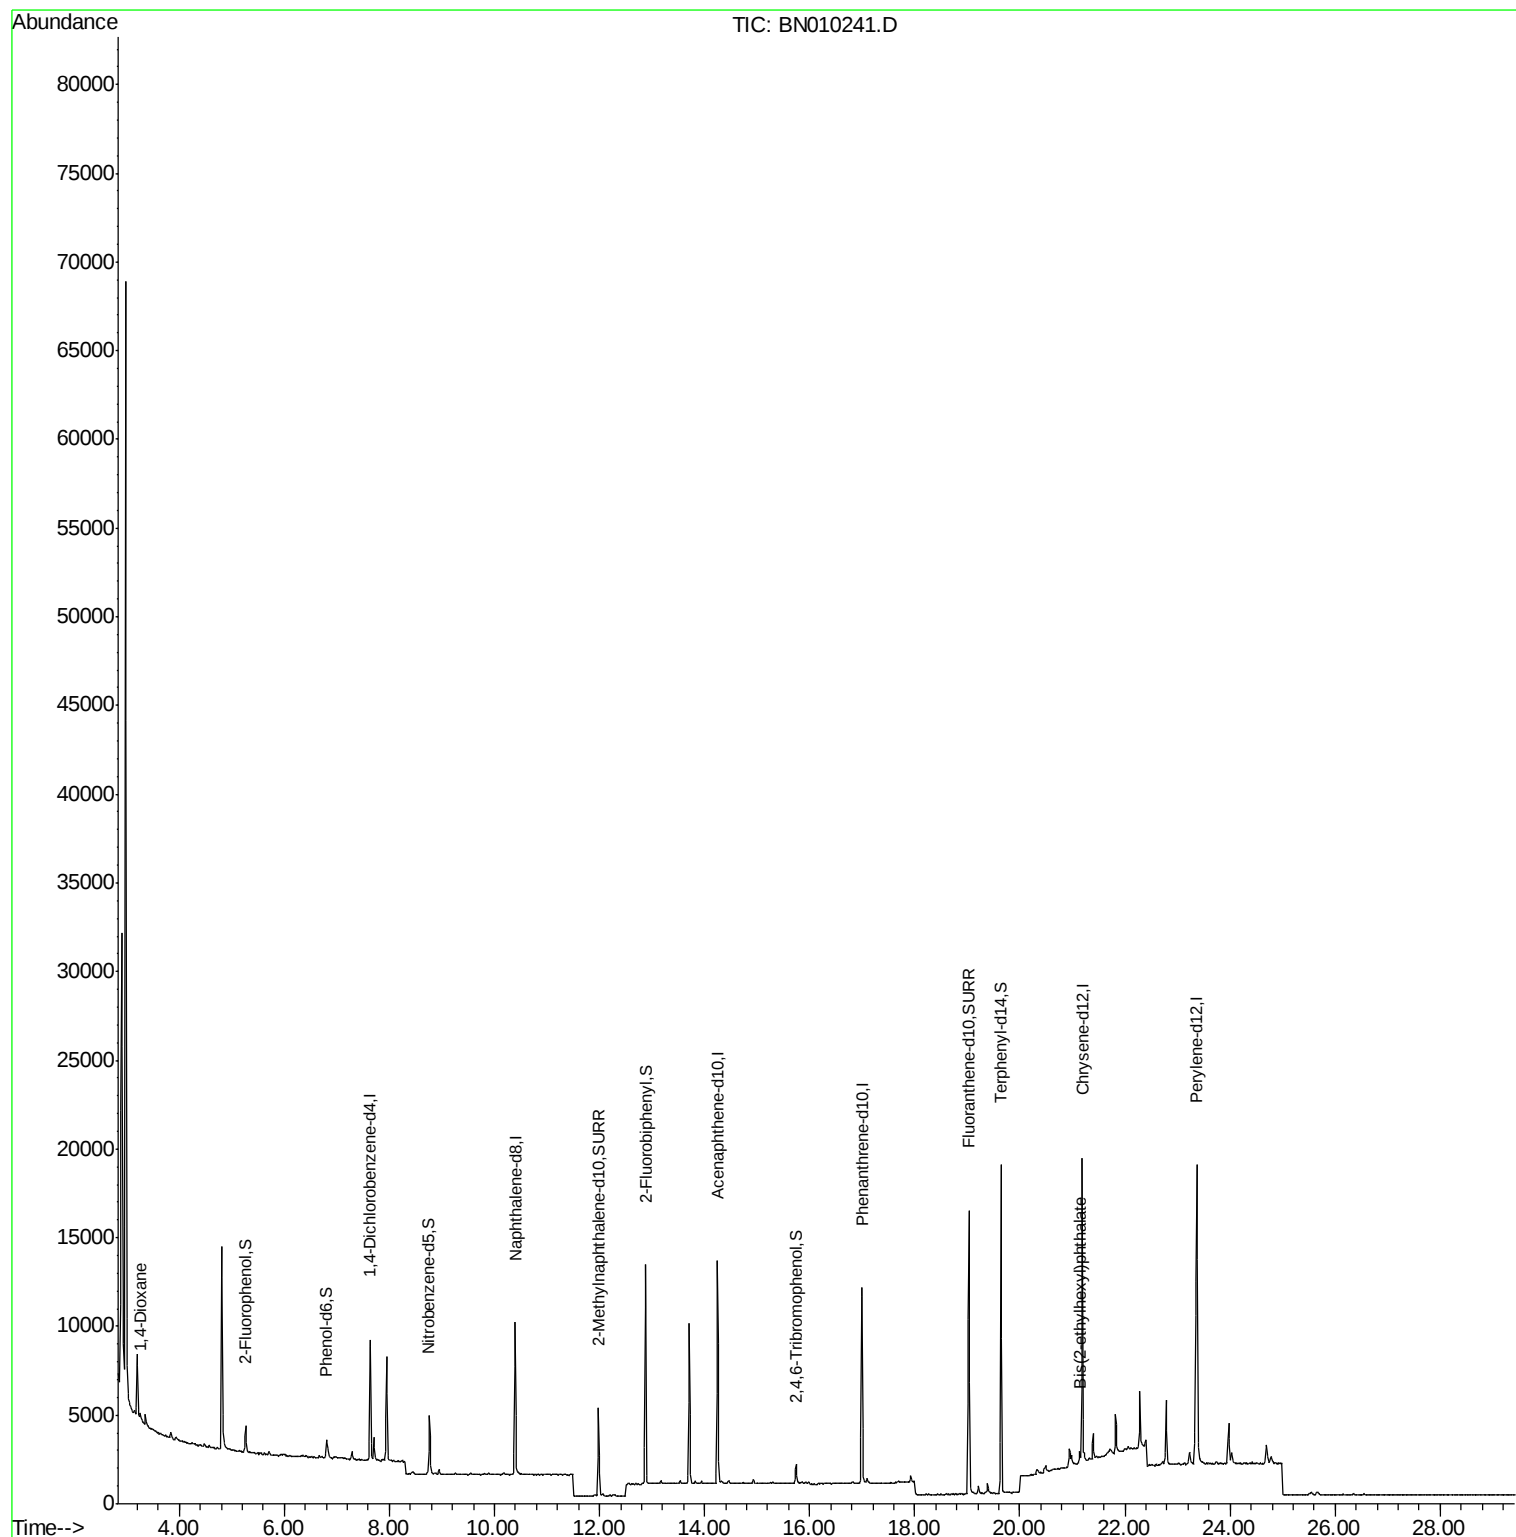




#1




1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.63 min Scan# 596
Delta R.T. -0.01 min
Lab File: BN010241.D
Acq: 17 Mar 2020 15:59

Instrument :
BNA_N
ClientSampleId :
MW201D1-20200307

Tot Ion:152 Resp: 3445
Ion Ratio Lower Upper
152 100
150 156.4 119.5 179.3
115 59.3 50.9 76.3

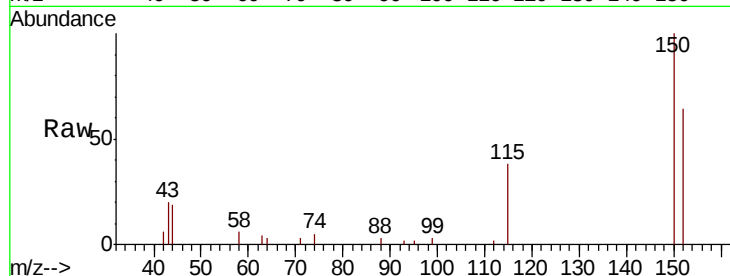


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

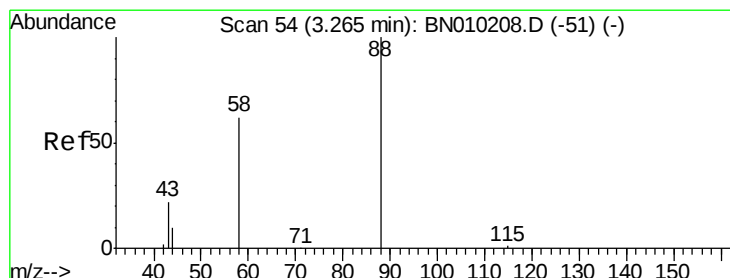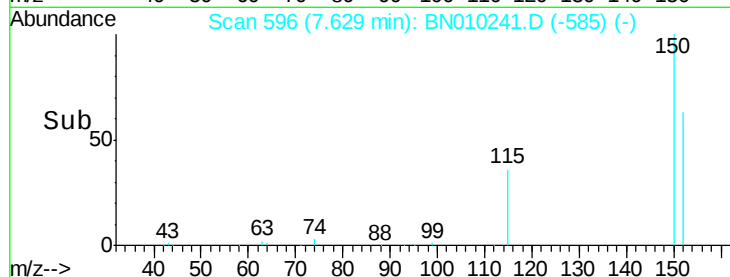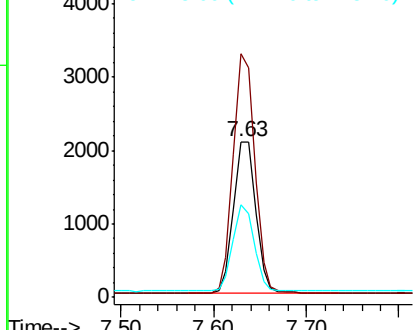



#2


1,4-Dioxane
Concen: 0.064 ng
RT: 3.26 min Scan# 54
Delta R.T. 0.00 min
Lab File: BN010241.D
Acq: 17 Mar 2020 15:59

Tgt Ion: 88 Resp: 216
Ion Ratio Lower Upper
88 100
58 97.2 97.8 146.8#
43 0.0 45.1 67.7#

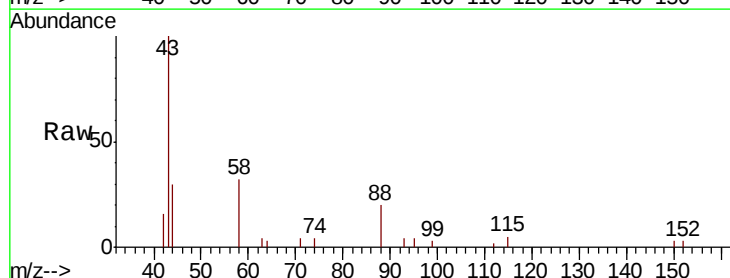

Abundance Ion 88.00 (87.70 to 88.70): BN0
Ion 58.00 (57.70 to 58.70): BN0
Ion 43.00 (42.70 to 43.70): BN0

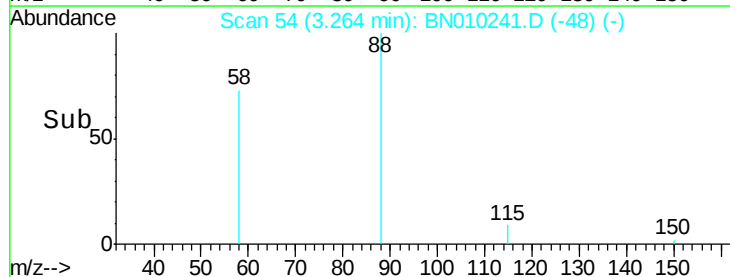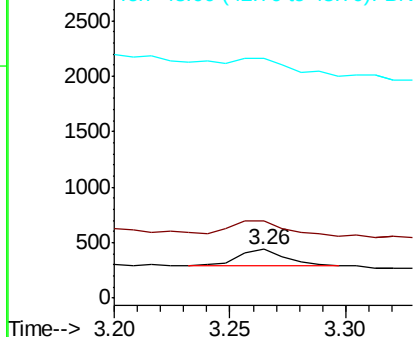

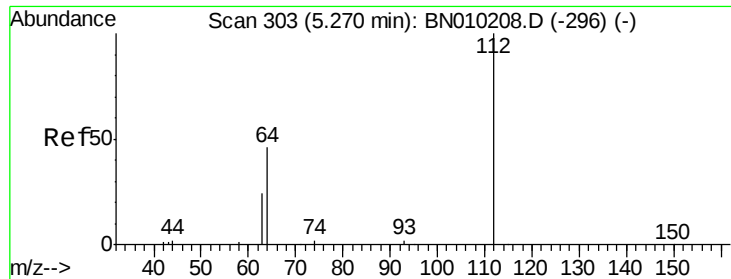

#4

2-Fluorophenol

Concen: 0.157 ng

RT: 5.26 min Scan# 302

Delta R.T. -0.01 min

Lab File: BN010241.D

Acq: 17 Mar 2020 15:59

Instrument :

BNA_N

ClientSampleId :

MW201D1-20200307


Tot Ion:112 Resp: 1265

Ion Ratio Lower Upper

112 100

64 53.8 42.6 63.8




63 29.6 23.6 35.4

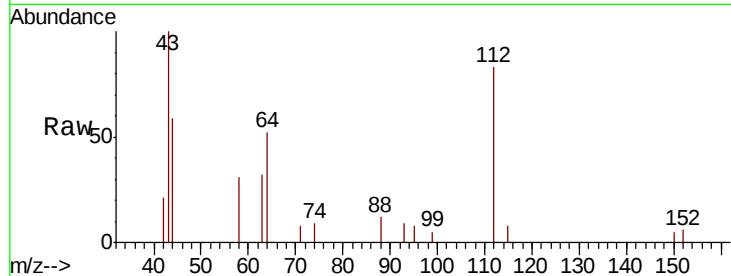

Abundance Ion 112.00 (111.70 to 112.70): B

Ion 64.00 (63.70 to 64.70): BNO

Ion 63.00 (62.70 to 63.70): BNO

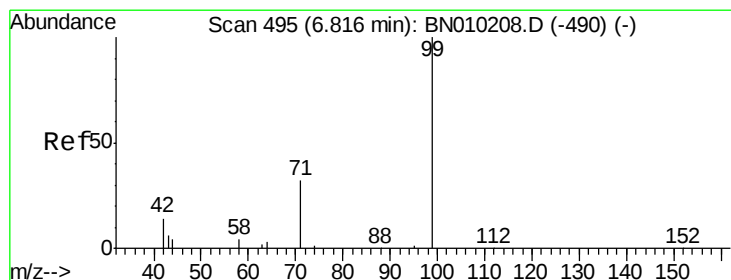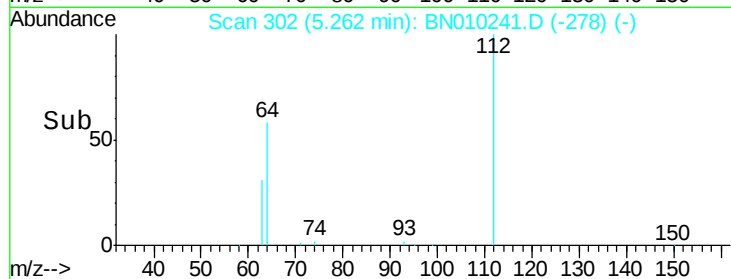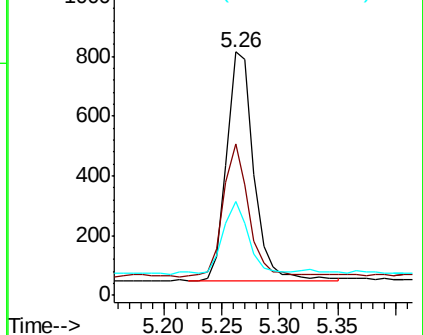

#5

Phenol-d6

Concen: 0.099 ng

RT: 6.81 min Scan# 494

Delta R.T. -0.01 min

Lab File: BN010241.D

Acq: 17 Mar 2020 15:59


Tgt Ion: 99 Resp: 1002

Ion Ratio Lower Upper

99 100

42 25.8 12.0 18.0#



71 38.7 22.6 33.8#




Abundance Ion 99.00 (98.70 to 99.70): BNO

Ion 42.00 (41.70 to 42.70): BNO

Ion 71.00 (70.70 to 71.70): BNO

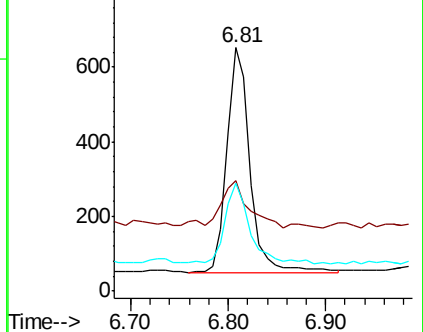



#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.39 min Scan# 845

Delta R.T. -0.00 min

Lab File: BN010241.D

Acq: 17 Mar 2020 15:59

Instrument :

BNA_N

ClientSampleId :

MW201D1-20200307

Tot Ion:136 Resp: 11647


Ion Ratio Lower Upper

136 100

137 11.7 10.6 15.8

54 5.6 9.5 14.3#

68 5.1 9.7 14.5#

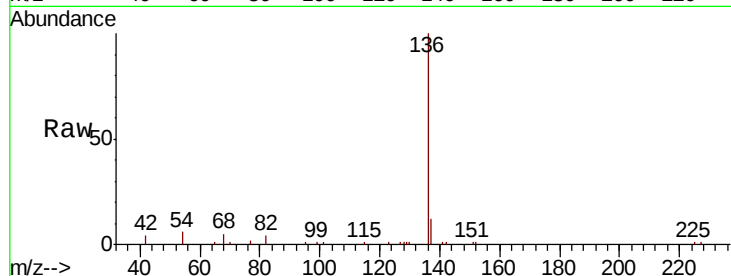


Abundance Ion 136.00 (135.70 to 136.70): E


Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BNC

Ion 68.00 (67.70 to 68.70): BNC



Time-->



#8

Nitrobenzene-d5

Concen: 0.393 ng

RT: 8.76 min Scan# 716

Delta R.T. -0.01 min

Lab File: BN010241.D

Acq: 17 Mar 2020 15:59


Tgt Ion: 82 Resp: 2744

Ion Ratio Lower Upper

82 100

128 38.2 35.0 52.6


54 52.9 37.0 55.4




Abundance Ion 82.00 (81.70 to 82.70): BNC

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BNC







Time-->



#11
 2-Methylnaphthalene-d10
 Concen: 0.345 ng
 RT: 11.98 min Scan# 1040
 Delta R.T. -0.01 min
 Lab File: BN010241.D
 Acq: 17 Mar 2020 15:59




Instrument :
 BNA_N
 ClientSampleId :
 MW201D1-20200307


Tot Ion:152 Resp: 6644
 Ion Ratio Lower Upper
 152 100
 151 19.7 15.0 22.6

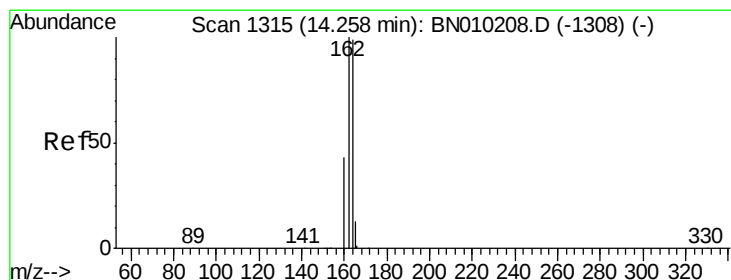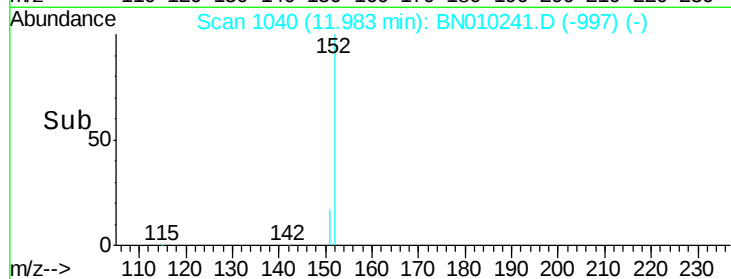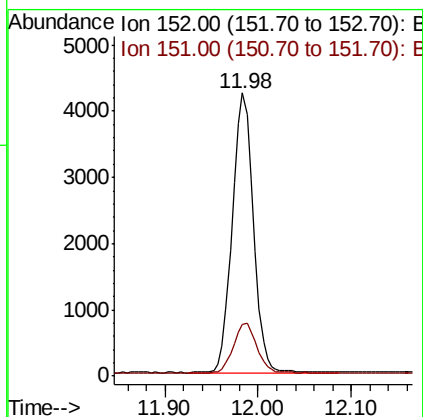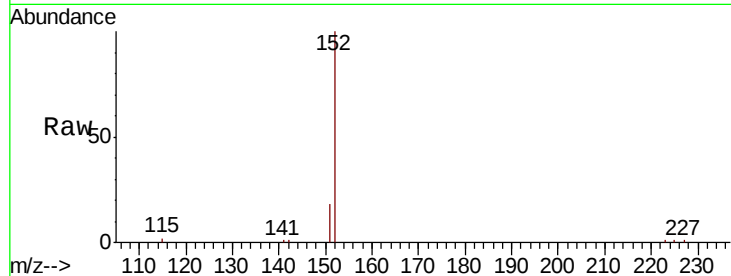

#13
 Acenaphthene-d10
 Concen: 0.400 ng
 RT: 14.25 min Scan# 1314
 Delta R.T. -0.01 min
 Lab File: BN010241.D
 Acq: 17 Mar 2020 15:59

Tgt Ion:164 Resp: 6917
 Ion Ratio Lower Upper
 164 100
 162 101.7 81.0 121.4
 160 50.4 35.6 53.4

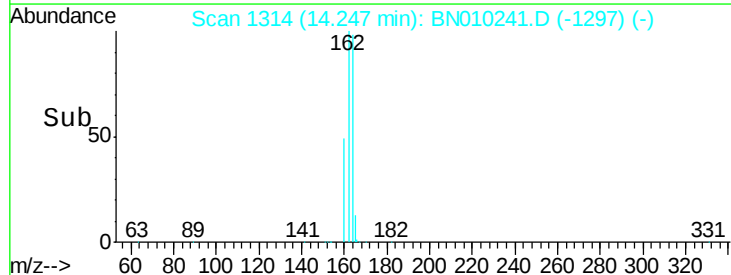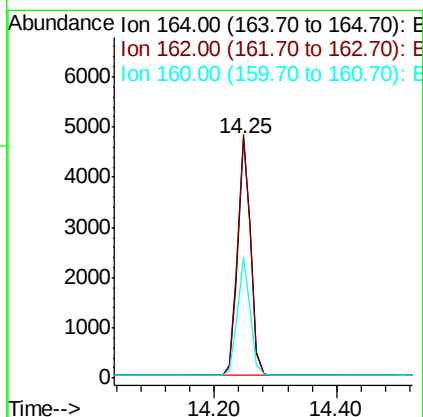


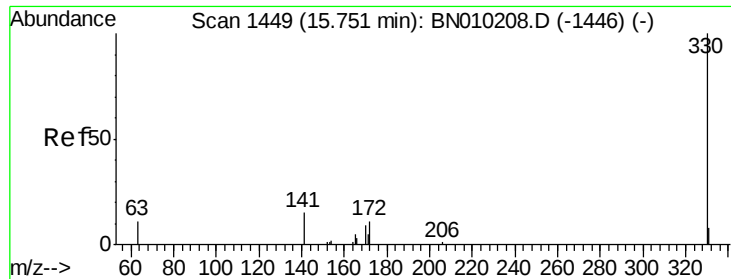

#14
 2,4,6-Tribromophenol
 Concen: 0.362 ng
 RT: 15.74 min Scan# 1448
 Delta R.T. -0.01 min
 Lab File: BN010241.D
 Acq: 17 Mar 2020 15:59




Instrument :
 BNA_N
 ClientSampleId :
 MW201D1-20200307

Tot Ion:330 Resp: 897
 Ion Ratio Lower Upper
 330 100
 332 0.0 0.0 0.0
 141 34.3 25.1 37.7

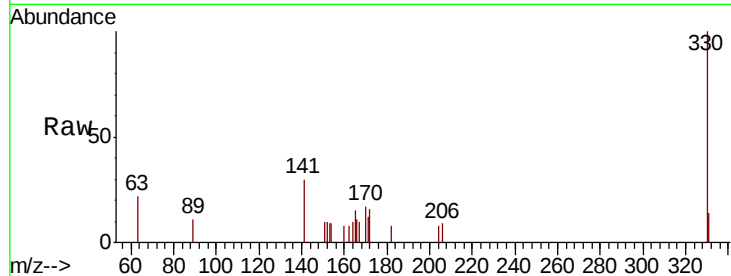


Abundance Ion 330.00 (329.70 to 330.70): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

15.74

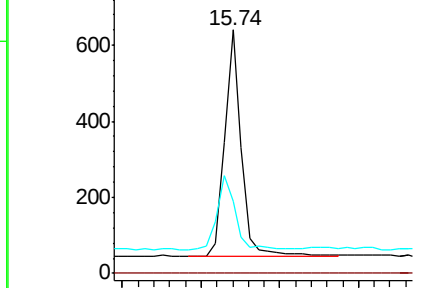



#15
 2-Fluorobiphenyl
 Concen: 0.462 ng
 RT: 12.88 min Scan# 1191
 Delta R.T. -0.00 min
 Lab File: BN010241.D
 Acq: 17 Mar 2020 15:59


Tgt Ion:172 Resp: 11370
 Ion Ratio Lower Upper
 172 100
 171 33.5 29.4 44.2
 170 22.3 20.2 30.4



Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

12.88

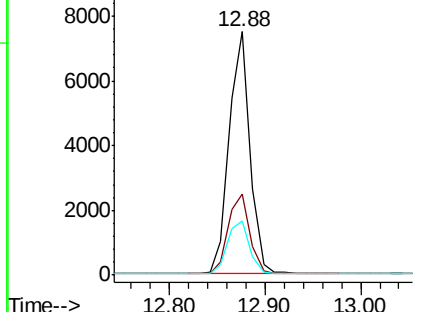

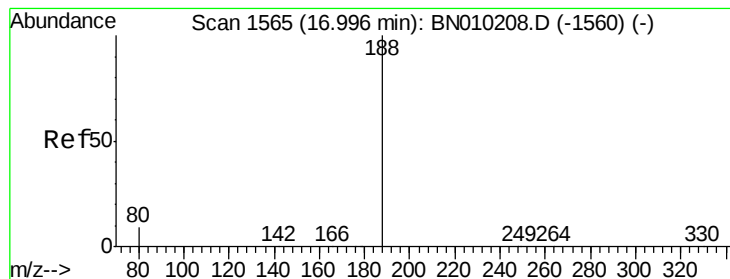

#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 17.00 min Scan# 1565

Delta R.T. -0.00 min

Lab File: BN010241.D

Acq: 17 Mar 2020 15:59

Instrument :

BNA_N

ClientSampleId :

MW201D1-20200307


Tot Ion:188 Resp: 16474

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0




80 5.9 8.6 12.8#

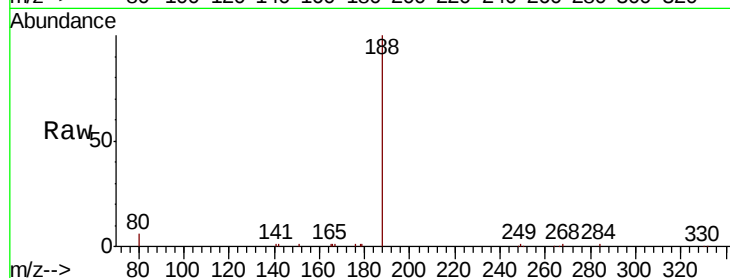

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BNC

Ion 80.00 (79.70 to 80.70): BNC

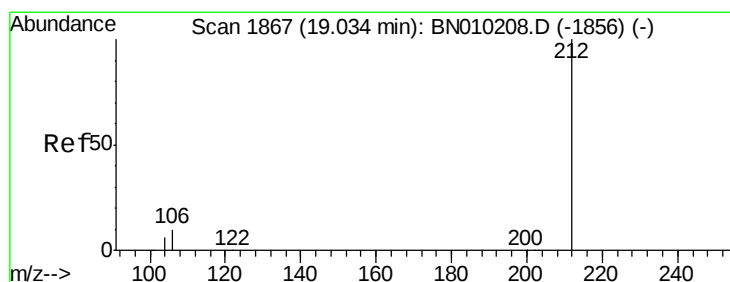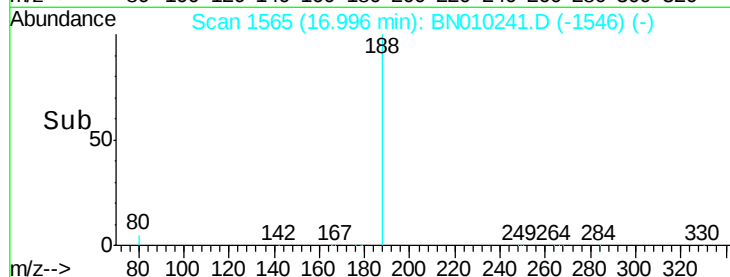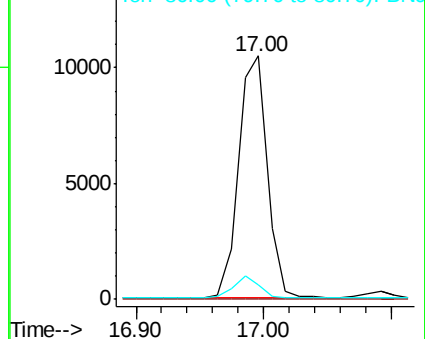

#25

Fluoranthene-d10

Concen: 0.361 ng

RT: 19.03 min Scan# 1866

Delta R.T. -0.01 min

Lab File: BN010241.D

Acq: 17 Mar 2020 15:59


Tgt Ion:212 Resp: 18357

Ion Ratio Lower Upper

212 100

106 9.4 8.1 12.1



104 5.4 4.7 7.1

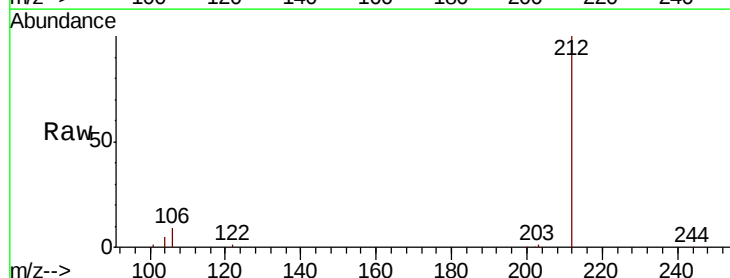


Abundance Ion 212.00 (211.70 to 212.70): E

Ion 106.00 (105.70 to 106.70): E

Ion 104.00 (103.70 to 104.70): E

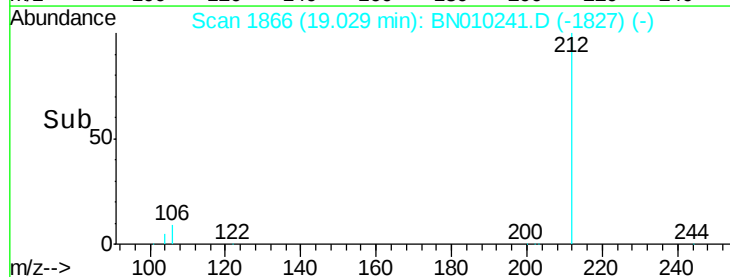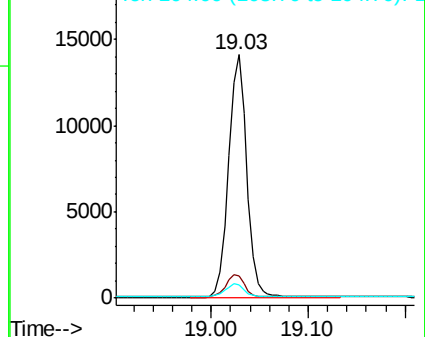



#27

Chrysene-d12

Concen: 0.400 ng

RT: 21.19 min Scan# 2174

Delta R.T. -0.01 min

Lab File: BN010241.D

Acq: 17 Mar 2020 15:59

Instrument :

BNA_N

ClientSampleId :

MW201D1-20200307


Tot Ion:240 Resp: 17450

Ion Ratio Lower Upper

240 100

120 11.0 7.7 11.5




236 28.1 21.8 32.6



Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

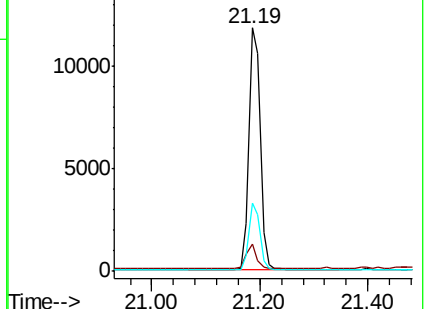

#29

Terphenyl-d14

Concen: 0.456 ng

RT: 19.64 min Scan# 1989

Delta R.T. -0.01 min

Lab File: BN010241.D

Acq: 17 Mar 2020 15:59


Tgt Ion:244 Resp: 18142

Ion Ratio Lower Upper

244 100

212 8.1 6.4 9.6



122 9.0 8.1 12.1




Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

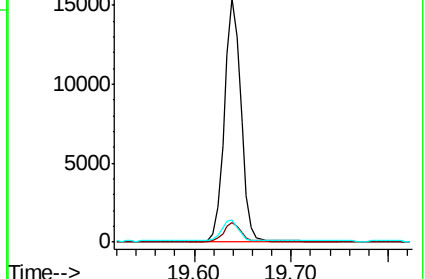



#32

Bis(2-ethylhexyl)phthalate

Concen: 0.023 ng

RT: 21.14 min Scan# 2170

Delta R.T. -0.01 min

Lab File: BN010241.D

Acq: 17 Mar 2020 15:59

Instrument :

BNA_N

ClientSampleId :

MW201D1-20200307


Tot Ion:149 Resp: 586

Ion Ratio Lower Upper

149 100

167 27.5 21.0 31.4




279 8.0 3.1 4.7#



Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

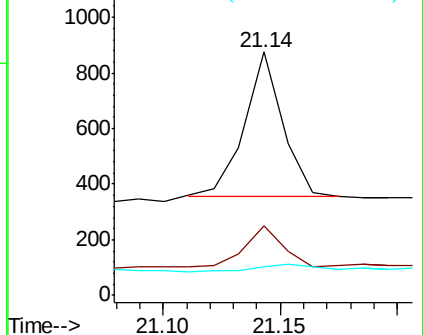

#34

Perylene-d12

Concen: 0.400 ng

RT: 23.36 min Scan# 2569

Delta R.T. -0.01 min

Lab File: BN010241.D

Acq: 17 Mar 2020 15:59


Tgt Ion:264 Resp: 21437

Ion Ratio Lower Upper

264 100

260 24.4 19.7 29.5

265 32.6 25.8 38.6



Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

