

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN031720\
 Data File : BN010243.D
 Acq On : 17 Mar 2020 17:12
 Operator : CG/JU
 Sample : L1903-07
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DUP03-20200307

Quant Time: Mar 17 17:58:45 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN031320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 16 02:17:23 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.63	152	3391	0.40	ng	0.00
7) Naphthalene-d8	10.39	136	12030	0.40	ng	0.00
13) Acenaphthene-d10	14.25	164	7485	0.40	ng	-0.01
19) Phenanthrene-d10	17.00	188	17880	0.40	ng	0.00
27) Chrysene-d12	21.19	240	19409	0.40	ng	-0.01
34) Perylene-d12	23.37	264	23409	0.40	ng	-0.01
System Monitoring Compounds						
4) 2-Fluorophenol	5.26	112	1122	0.14	ng	0.00
5) Phenol-d6	6.81	99	913	0.09	ng	0.00
8) Nitrobenzene-d5	8.76	82	4457	0.62	ng	-0.01
11) 2-Methylnaphthalene-d10	11.98	152	6111	0.31	ng	0.00
14) 2,4,6-Tribromophenol	15.74	330	899	0.34	ng	-0.01
15) 2-Fluorobiphenyl	12.88	172	22370	0.84	ng	0.00
25) Fluoranthene-d10	19.03	212	17942	0.33	ng	0.00
29) Terphenyl-d14	19.64	244	27390	0.62	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.26	88	1432	0.433	ng	# 55
32) Bis(2-ethylhexyl)phthalate	21.14	149	3178	0.113	ng	# 99
36) Benzo(k)fluoranthene	22.78	252	1465	0.020	ng	# 1

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN031720\
Data File : BN010243.D
Acq On : 17 Mar 2020 17:12
Operator : CG/JU
Sample : L1903-07
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DUP03-20200307

Quant Time: Mar 17 17:58:45 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN031320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 16 02:17:23 2020
Response via : Initial Calibration

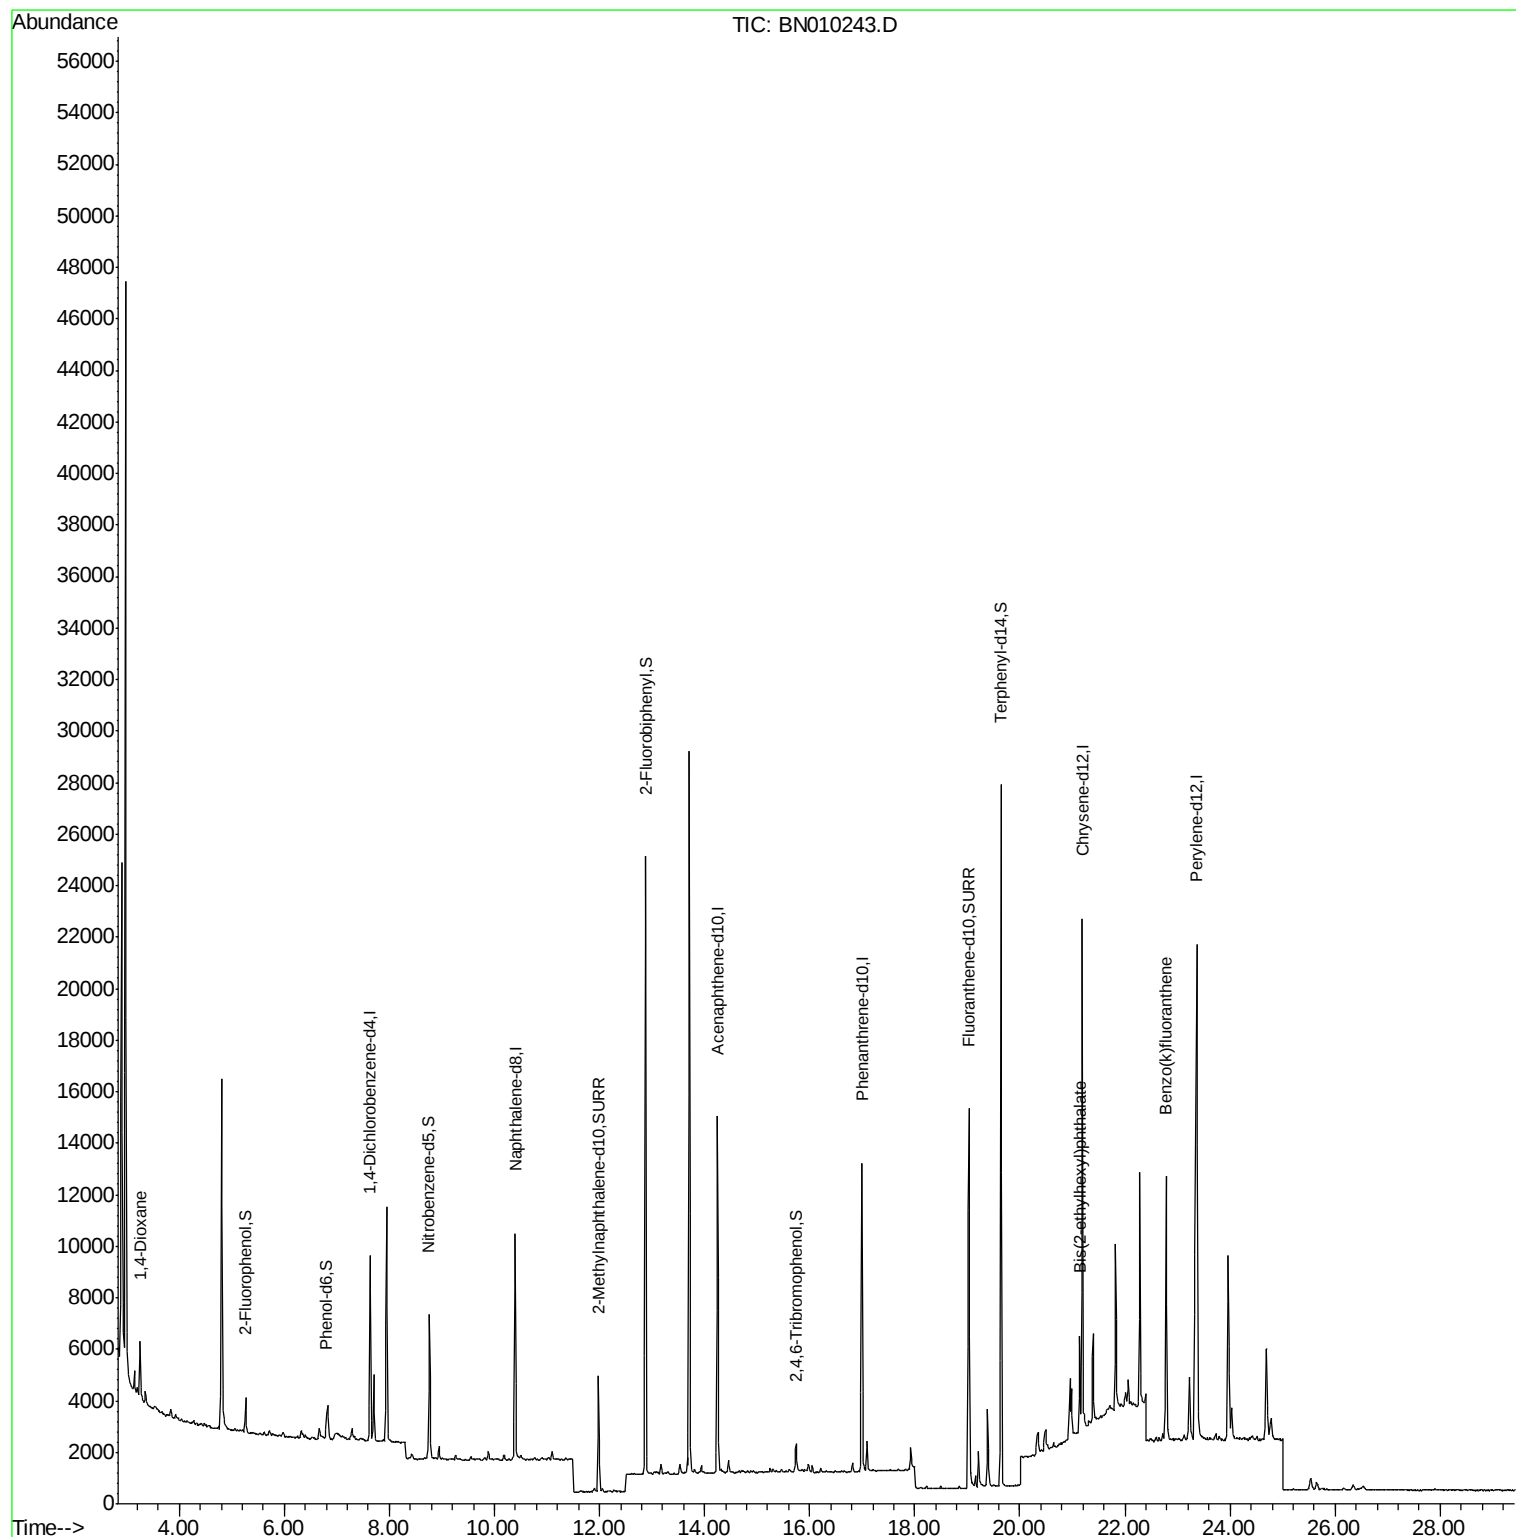



#1

1,4-Dichlorobenzene-d4

Concen: 0.400 ng

RT: 7.63 min Scan# 596

Delta R.T. -0.01 min

Lab File: BN010243.D

Acq: 17 Mar 2020 17:12

Instrument :

BNA_N

ClientSampleId :

DUP03-20200307


Tot Ion:152 Resp: 3391

Ion Ratio Lower Upper

152 100

150 154.7 119.5 179.3




115 59.6 50.9 76.3

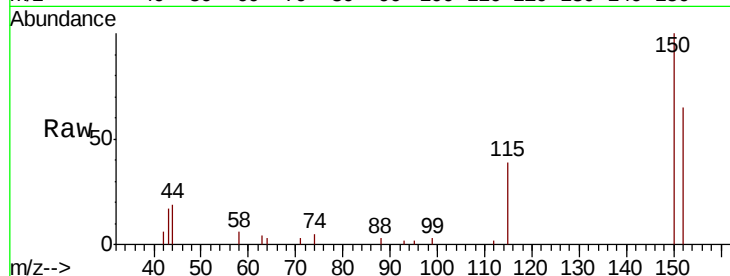

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

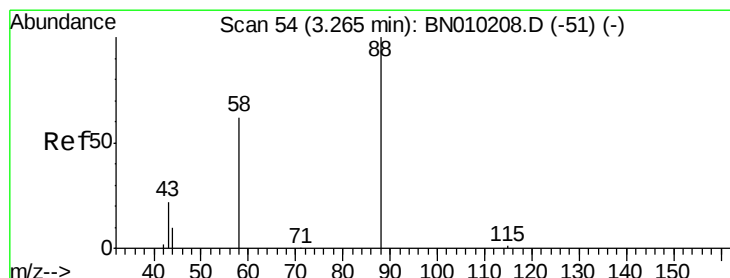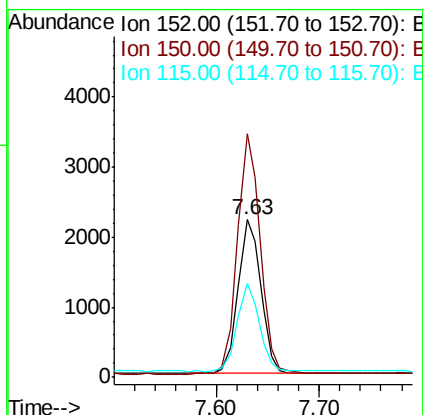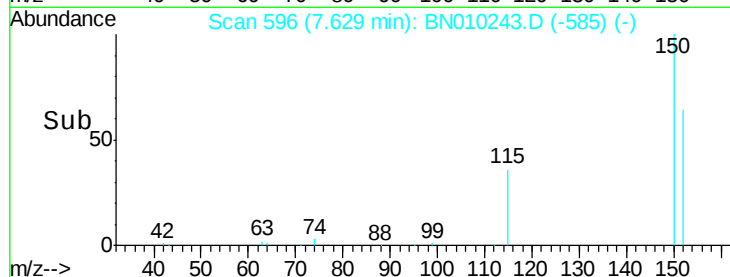

#2

1,4-Dioxane

Concen: 0.433 ng

RT: 3.26 min Scan# 53

Delta R.T. -0.01 min

Lab File: BN010243.D

Acq: 17 Mar 2020 17:12


Tgt Ion: 88 Resp: 1432

Ion Ratio Lower Upper

88 100

58 63.0 97.8 146.8#



43 35.2 45.1 67.7#

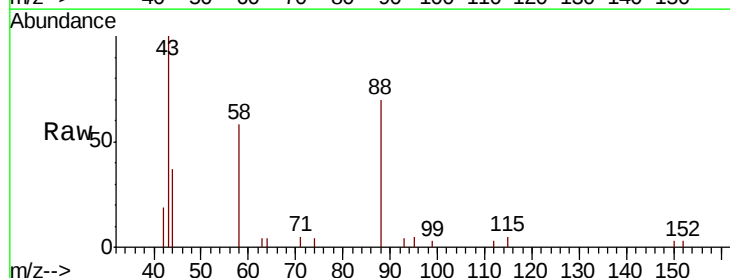


Abundance Ion 88.00 (87.70 to 88.70): BN0

Ion 58.00 (57.70 to 58.70): BN0

Ion 43.00 (42.70 to 43.70): BN0

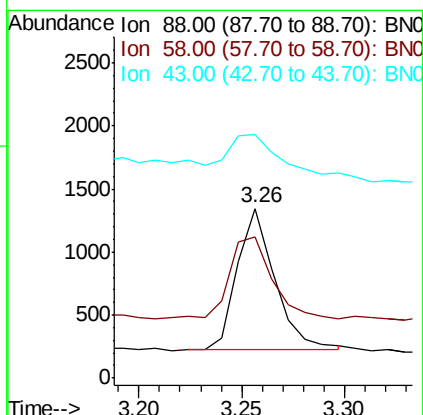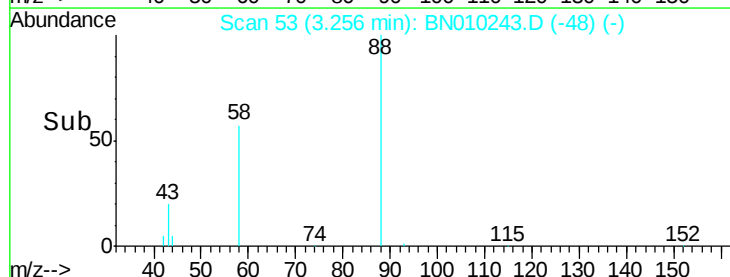

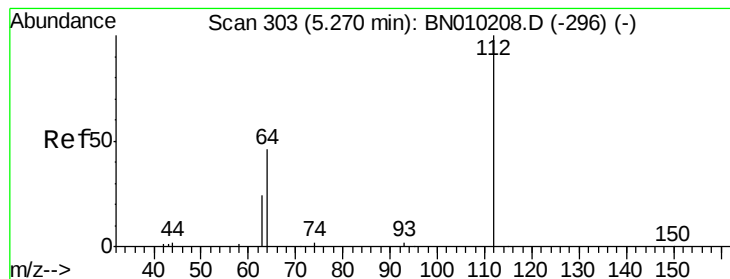

#4

2-Fluorophenol

Concen: 0.141 ng

RT: 5.26 min Scan# 302

Delta R.T. -0.01 min

Lab File: BN010243.D

Acq: 17 Mar 2020 17:12

Instrument :

BNA_N

ClientSampleId :

DUP03-20200307


Tot Ion: 112 Resp: 1122

Ion Ratio Lower Upper

112 100

64 53.3 42.6 63.8




63 27.9 23.6 35.4

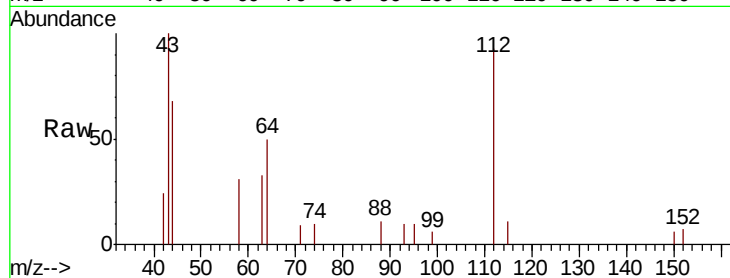

Abundance Ion 112.00 (111.70 to 112.70): B

Ion 64.00 (63.70 to 64.70): BNO

Ion 63.00 (62.70 to 63.70): BNO

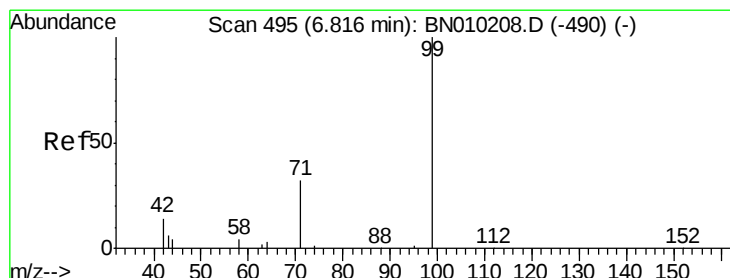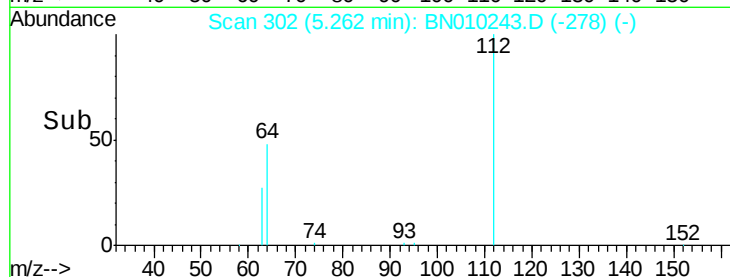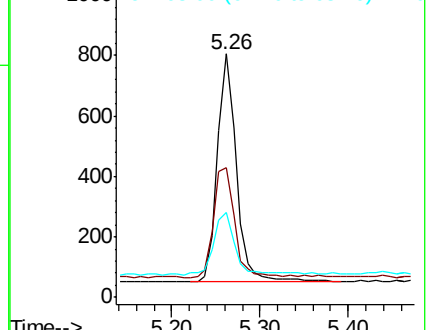

#5

Phenol-d6

Concen: 0.092 ng

RT: 6.81 min Scan# 494

Delta R.T. -0.01 min

Lab File: BN010243.D

Acq: 17 Mar 2020 17:12


Tgt Ion: 99 Resp: 913

Ion Ratio Lower Upper

99 100

42 35.3 12.0 18.0#



71 37.3 22.6 33.8#

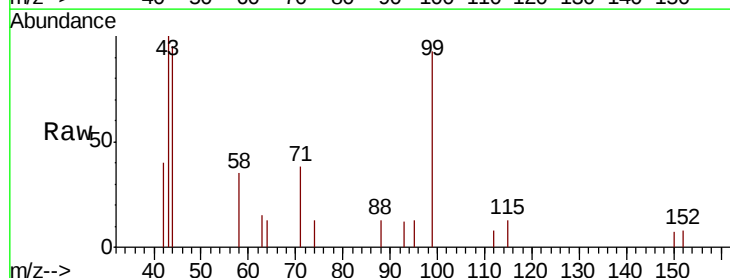


Abundance Ion 99.00 (98.70 to 99.70): BNO

Ion 42.00 (41.70 to 42.70): BNO

Ion 71.00 (70.70 to 71.70): BNO

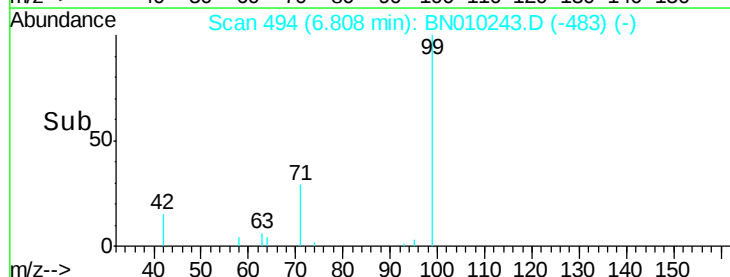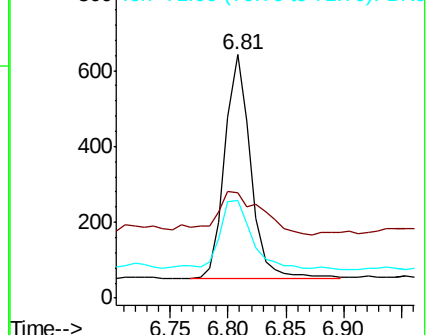

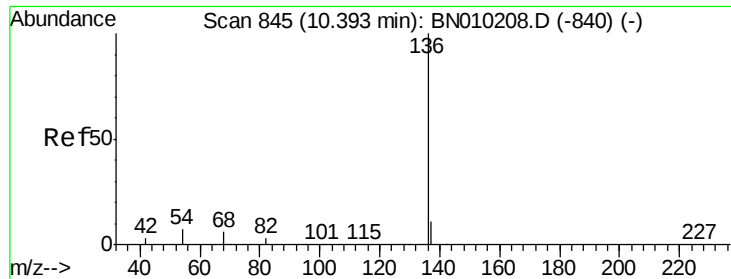

#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.39 min Scan# 845

Delta R.T. -0.00 min

Lab File: BN010243.D

Acq: 17 Mar 2020 17:12

Instrument :

BNA_N

ClientSampleId :

DUP03-20200307

Tot Ion:136 Resp: 12030


Ion Ratio Lower Upper

136 100

137 11.5 10.6 15.8

54 5.3 9.5 14.3#

68 4.7 9.7 14.5#






Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BNC

Ion 68.00 (67.70 to 68.70): BNC

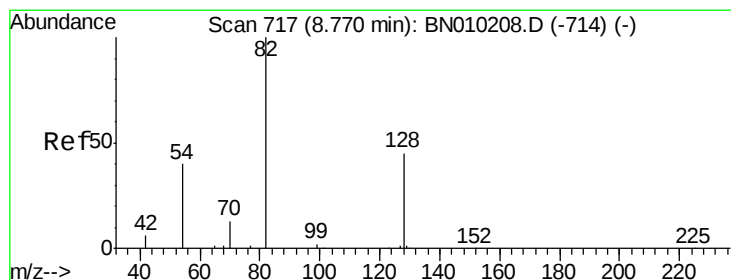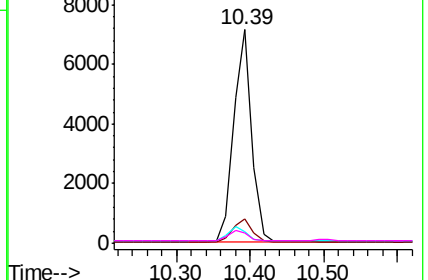

#8

Nitrobenzene-d5

Concen: 0.618 ng

RT: 8.76 min Scan# 716

Delta R.T. -0.01 min

Lab File: BN010243.D

Acq: 17 Mar 2020 17:12


Tgt Ion: 82 Resp: 4457

Ion Ratio Lower Upper

82 100

128 39.2 35.0 52.6



54 48.1 37.0 55.4




Abundance Ion 82.00 (81.70 to 82.70): BNC

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BNC



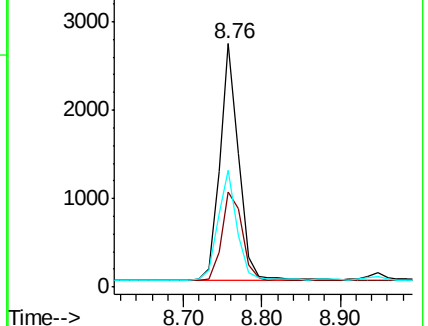
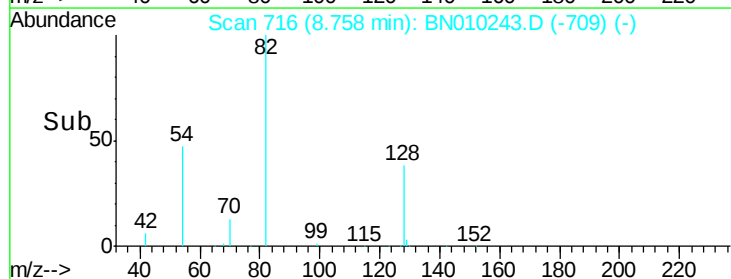




#11
2-Methylnaphthalene-d10
Concen: 0.308 ng
RT: 11.98 min Scan# 1040
Delta R.T. -0.01 min
Lab File: BN010243.D
Acq: 17 Mar 2020 17:12




Instrument :
BNA_N
ClientSampleId :
DUP03-20200307


Tot Ion:152 Resp: 6111
Ion Ratio Lower Upper
152 100
151 19.6 15.0 22.6

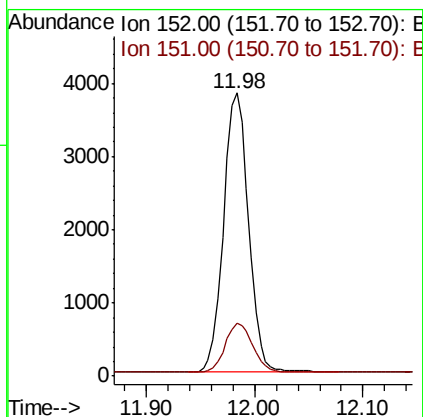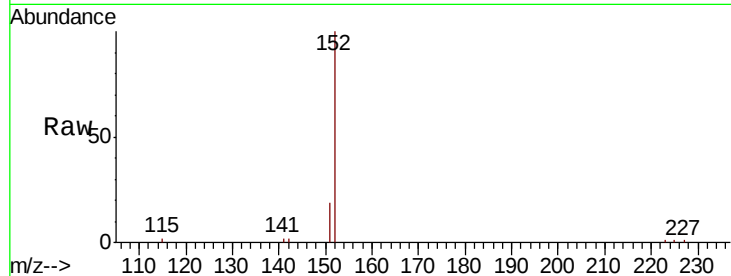

#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.25 min Scan# 1314
Delta R.T. -0.01 min
Lab File: BN010243.D
Acq: 17 Mar 2020 17:12

Tgt Ion:164 Resp: 7485
Ion Ratio Lower Upper
164 100
162 102.0 81.0 121.4
160 48.7 35.6 53.4



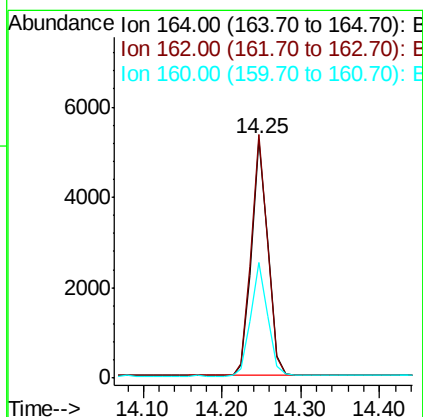



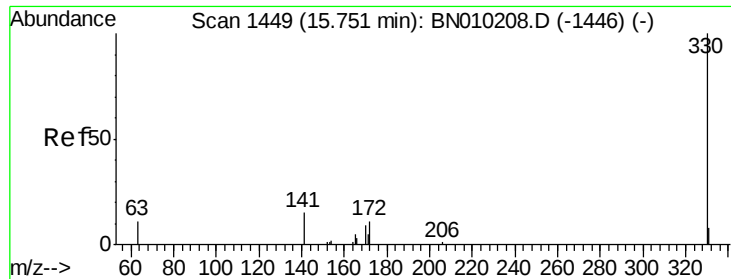

#14
 2,4,6-Tribromophenol
 Concen: 0.336 ng
 RT: 15.74 min Scan# 1448
 Delta R.T. -0.01 min
 Lab File: BN010243.D
 Acq: 17 Mar 2020 17:12




Instrument :
 BNA_N
 ClientSampleId :
 DUP03-20200307


Tot Ion:330 Resp: 899
 Ion Ratio Lower Upper
 330 100
 332 0.0 0.0 0.0
 141 38.5 25.1 37.7#

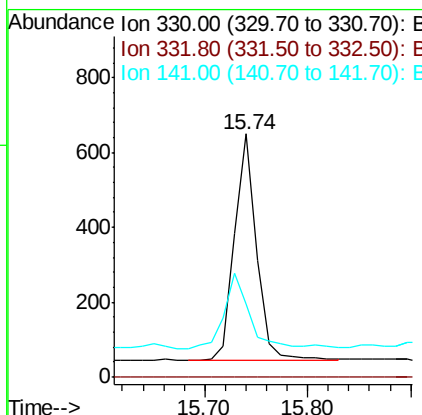

#15
 2-Fluorobiphenyl
 Concen: 0.839 ng
 RT: 12.88 min Scan# 1191
 Delta R.T. -0.00 min
 Lab File: BN010243.D
 Acq: 17 Mar 2020 17:12

Tgt Ion:172 Resp: 22370
 Ion Ratio Lower Upper
 172 100
 171 34.3 29.4 44.2
 170 22.0 20.2 30.4

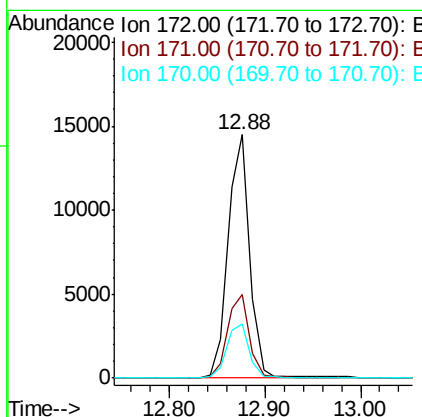



#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 17.00 min Scan# 1565

Delta R.T. -0.00 min

Lab File: BN010243.D

Acq: 17 Mar 2020 17:12

Instrument :

BNA_N

ClientSampleId :

DUP03-20200307


Tot Ion:188 Resp: 17880

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0


80 6.0 8.6 12.8#

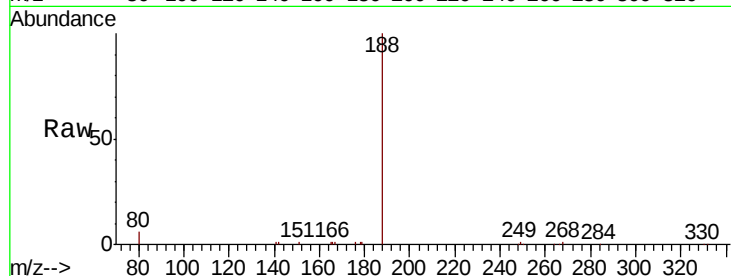



Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BNC

Ion 80.00 (79.70 to 80.70): BNC

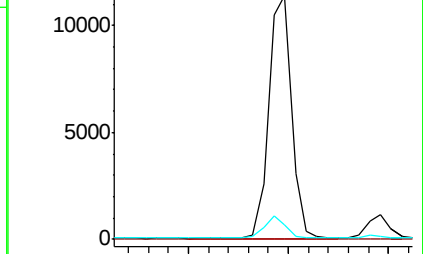

Time-->



#25

Fluoranthene-d10

Concen: 0.325 ng

RT: 19.03 min Scan# 1866

Delta R.T. -0.01 min

Lab File: BN010243.D

Acq: 17 Mar 2020 17:12


Tgt Ion:212 Resp: 17942

Ion Ratio Lower Upper

212 100

106 9.5 8.1 12.1


104 5.5 4.7 7.1




Abundance Ion 212.00 (211.70 to 212.70): E


Ion 106.00 (105.70 to 106.70): E

Ion 104.00 (103.70 to 104.70): E

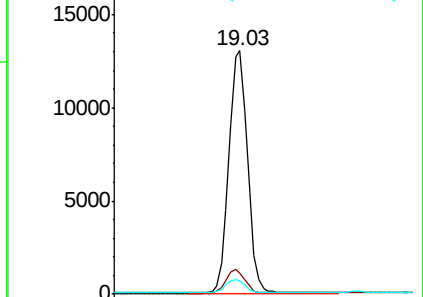

Time-->









#27
Chrysene-d12
Concen: 0.400 ng
RT: 21.19 min Scan# 2174
Delta R.T. -0.01 min
Lab File: BN010243.D
Acq: 17 Mar 2020 17:12




Instrument :
BNA_N
ClientSampleId :
DUP03-20200307


Tot Ion:240 Resp: 19409
Ion Ratio Lower Upper
240 100
120 10.1 7.7 11.5
236 27.5 21.8 32.6

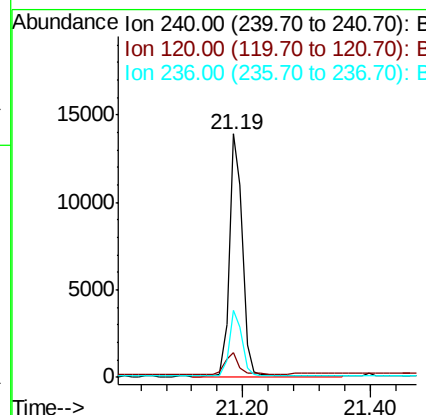

#29
Terphenyl-d14
Concen: 0.619 ng
RT: 19.64 min Scan# 1989
Delta R.T. -0.01 min
Lab File: BN010243.D
Acq: 17 Mar 2020 17:12

Tgt Ion:244 Resp: 27390
Ion Ratio Lower Upper
244 100
212 7.6 6.4 9.6
122 8.9 8.1 12.1

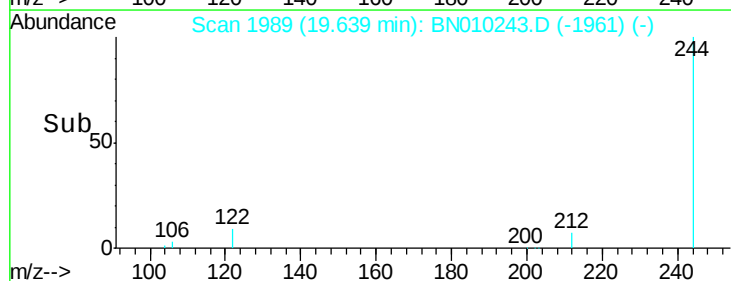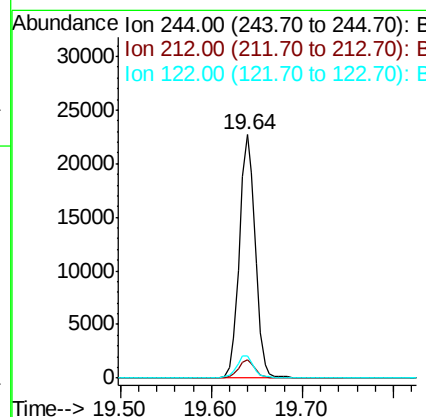



#32

Bis(2-ethylhexyl)phthalate

Concen: 0.113 ng

RT: 21.14 min Scan# 2170

Delta R.T. -0.01 min

Lab File: BN010243.D

Acq: 17 Mar 2020 17:12

Instrument :

BNA_N

ClientSampleId :

DUP03-20200307


Tot Ion:149 Resp: 3178

Ion Ratio Lower Upper

149 100

167 26.7 21.0 31.4




279 5.0 3.1 4.7#



Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

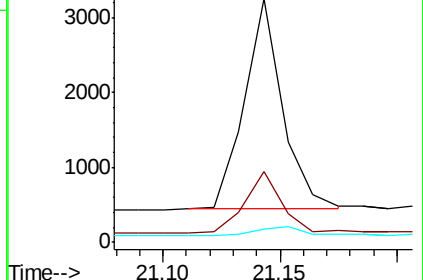

#34

Perylene-d12

Concen: 0.400 ng

RT: 23.37 min Scan# 2569

Delta R.T. -0.01 min

Lab File: BN010243.D

Acq: 17 Mar 2020 17:12


Tgt Ion:264 Resp: 23409

Ion Ratio Lower Upper

264 100

260 24.3 19.7 29.5



265 32.5 25.8 38.6




Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

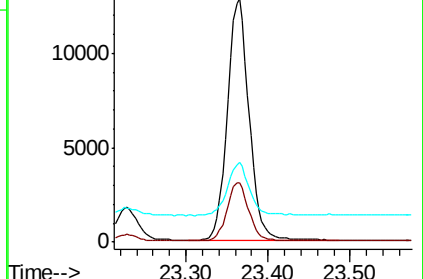

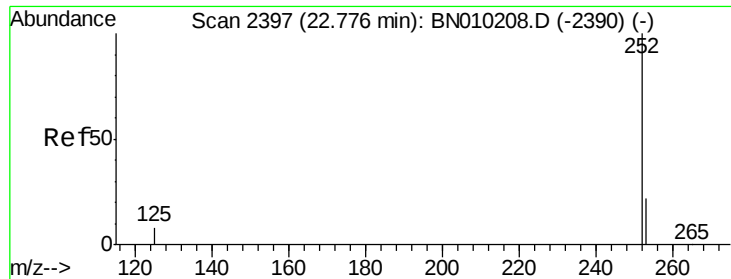

#36

Benzo(k)fluoranthene

Concen: 0.020 ng

RT: 22.78 min Scan# 2399

Delta R.T. 0.01 min

Lab File: BN010243.D

Acq: 17 Mar 2020 17:12

Instrument :

BNA_N

ClientSampleId :

DUP03-20200307


Tot Ion: 252 Resp: 1465

Ion Ratio Lower Upper

252 100

253 172.2 18.8 28.2#

125 697.0 8.2 12.4#



Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

