

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN031720\
 Data File : BN010254.D
 Acq On : 18 Mar 2020 07:35
 Operator : CG/JU
 Sample : L1903-17
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 TT101D1-20200310

Quant Time: Mar 18 09:07:07 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN031320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 16 02:17:23 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.63	152	3691	0.40	ng	0.00
7) Naphthalene-d8	10.38	136	13021	0.40	ng	-0.01
13) Acenaphthene-d10	14.24	164	7797	0.40	ng	-0.02
19) Phenanthrene-d10	16.99	188	18615	0.40	ng	0.00
27) Chrysene-d12	21.19	240	19669	0.40	ng	0.00
34) Perylene-d12	23.36	264	21152	0.40	ng	-0.02
System Monitoring Compounds						
4) 2-Fluorophenol	5.26	112	1011	0.12	ng	0.00
5) Phenol-d6	6.81	99	772	0.07	ng	0.00
8) Nitrobenzene-d5	8.76	82	4378	0.56	ng	-0.01
11) 2-Methylnaphthalene-d10	11.98	152	5976	0.28	ng	-0.01
14) 2,4,6-Tribromophenol	15.74	330	896	0.32	ng	-0.02
15) 2-Fluorobiphenyl	12.87	172	17360	0.63	ng	0.00
25) Fluoranthene-d10	19.02	212	17232	0.30	ng	-0.01
29) Terphenyl-d14	19.64	244	23674	0.53	ng	-0.01
Target Compounds						
2) 1,4-Dioxane	3.25	88	18274	5.075	ng	Qvalue # 53
6) bis(2-Chloroethyl)ether	7.07	93	600	0.066	ng	96
32) Bis(2-ethylhexyl)phthalate	21.13	149	4077	0.143	ng	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN031720\
Data File : BN010254.D
Acq On : 18 Mar 2020 07:35
Operator : CG/JU
Sample : L1903-17
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
TT101D1-20200310

Quant Time: Mar 18 09:07:07 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN031320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 16 02:17:23 2020
Response via : Initial Calibration

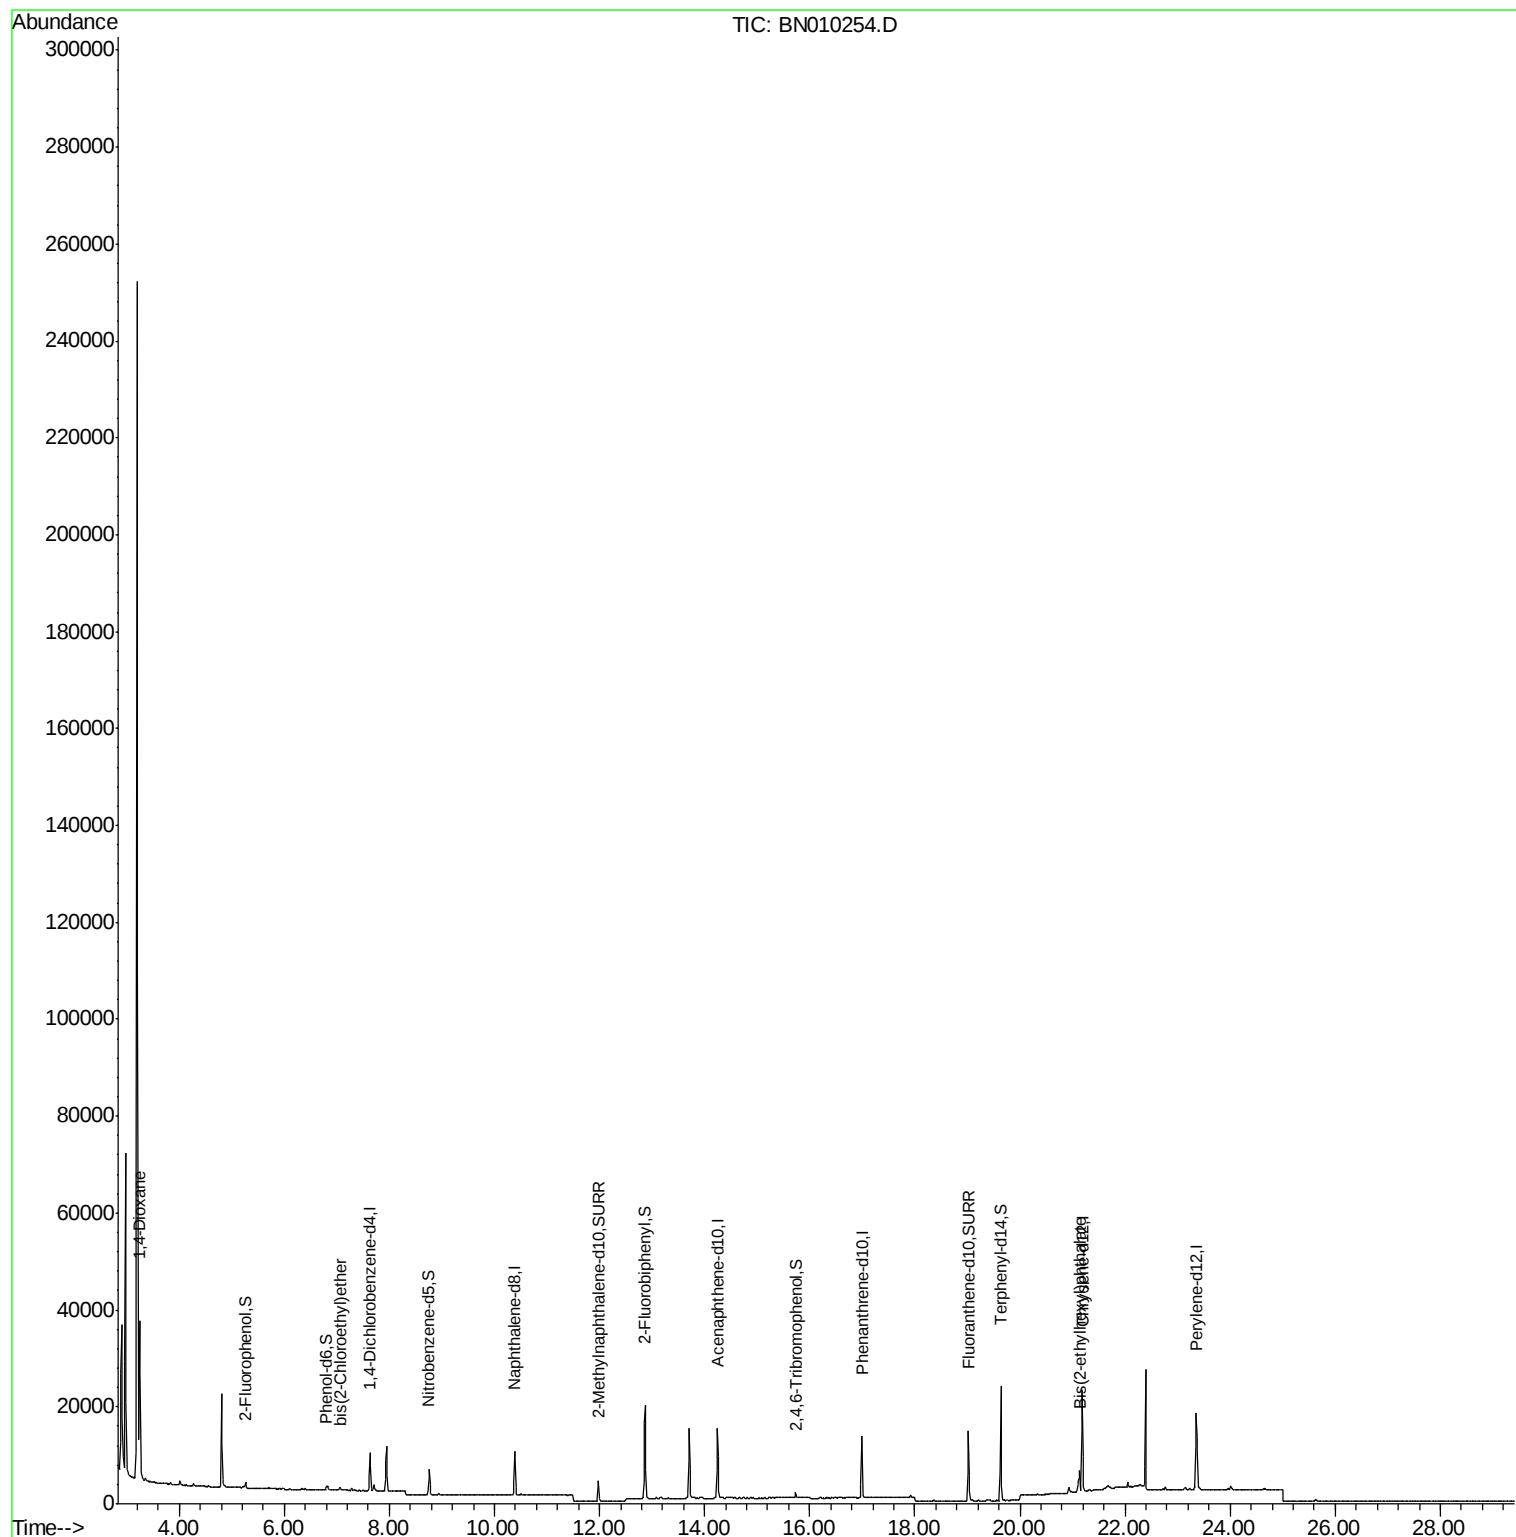

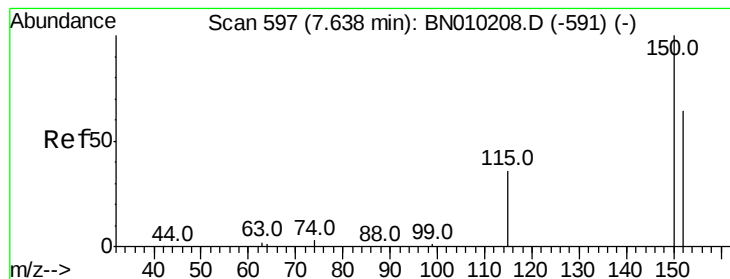


#1




1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.63 min Scan# 596
Delta R.T. -0.01 min
Lab File: BN010254.D
Acq: 18 Mar 2020 07:35

Instrument :
BNA_N
ClientSampleId :
TT101D1-20200310

Tot Ion:152 Resp: 3691
Ion Ratio Lower Upper
152 100
150 153.6 119.5 179.3
115 55.3 50.9 76.3

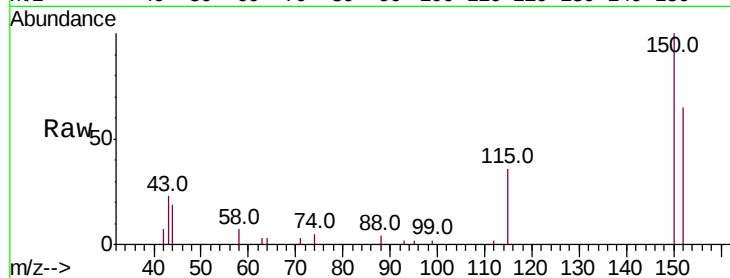


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

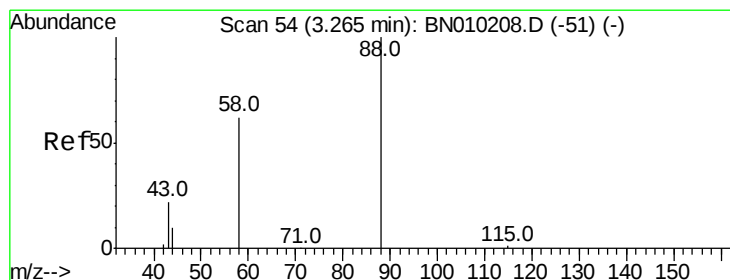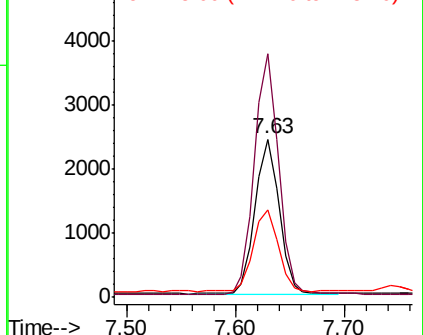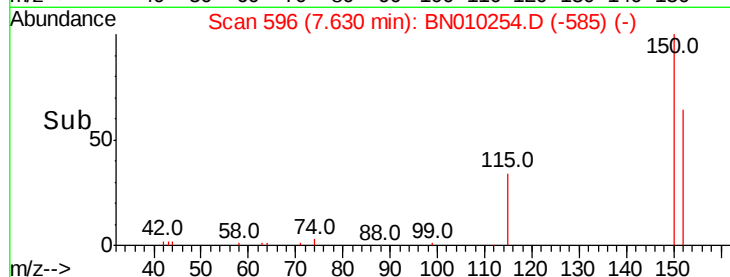



#2


1,4-Dioxane
Concen: 5.075 ng
RT: 3.25 min Scan# 52
Delta R.T. -0.02 min
Lab File: BN010254.D
Acq: 18 Mar 2020 07:35

Tgt Ion: 88 Resp: 18274
Ion Ratio Lower Upper
88 100
58 64.7 97.8 146.8#
43 27.9 45.1 67.7#

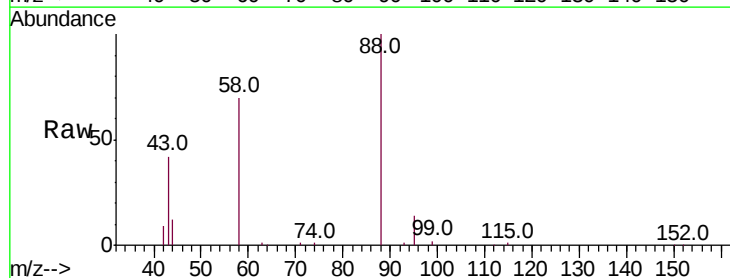

Abundance Ion 88.00 (87.70 to 88.70): BNC
Ion 58.00 (57.70 to 58.70): BNC
Ion 43.00 (42.70 to 43.70): BNC

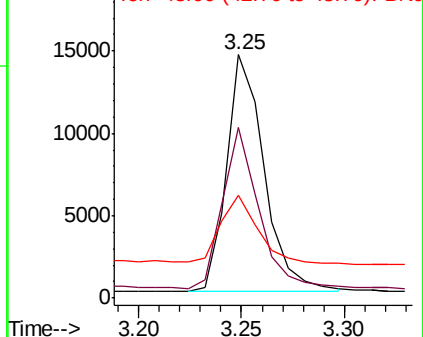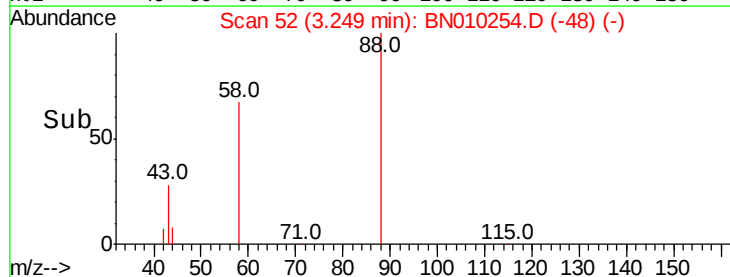

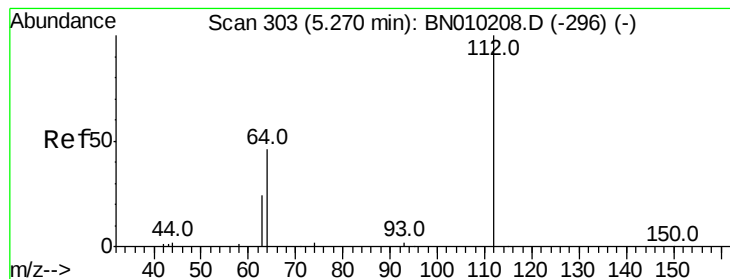

#4

2-Fluorophenol

Concen: 0.117 ng

RT: 5.26 min Scan# 302

Delta R.T. -0.01 min

Lab File: BN010254.D

Acq: 18 Mar 2020 07:35

Instrument :

BNA_N

ClientSampleId :

TT101D1-20200310


Tot Ion:112 Resp: 1011

Ion Ratio Lower Upper

112 100

64 51.4 42.6 63.8




63 27.4 23.6 35.4

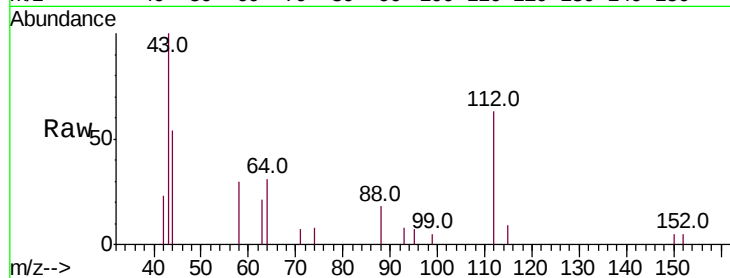

Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BN0

Ion 63.00 (62.70 to 63.70): BN0

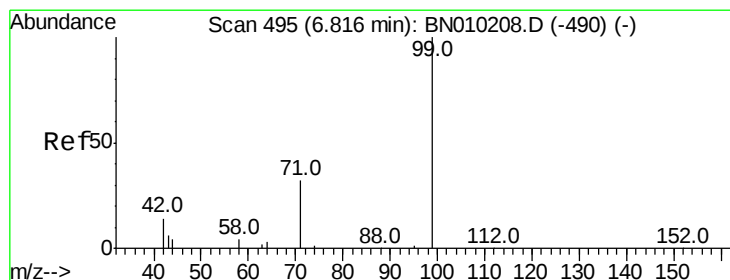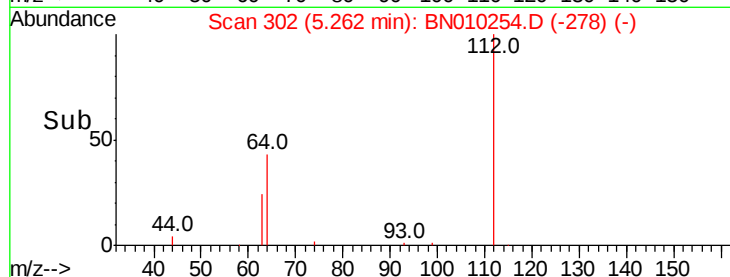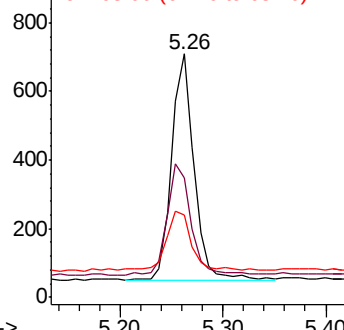

#5

Phenol-d6

Concen: 0.071 ng

RT: 6.81 min Scan# 494

Delta R.T. -0.01 min

Lab File: BN010254.D

Acq: 18 Mar 2020 07:35


Tgt Ion: 99 Resp: 772

Ion Ratio Lower Upper

99 100

42 37.8 12.0 18.0#



71 39.1 22.6 33.8#

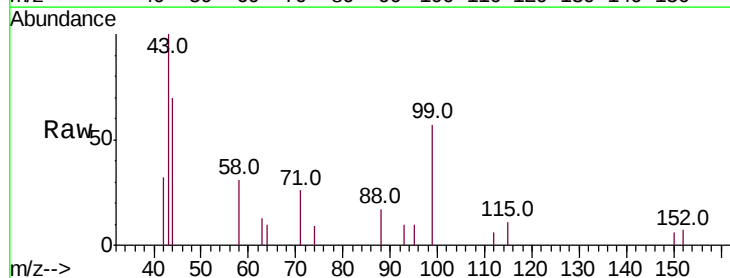


Abundance Ion 99.00 (98.70 to 99.70): BN0

Ion 42.00 (41.70 to 42.70): BN0

Ion 71.00 (70.70 to 71.70): BN0

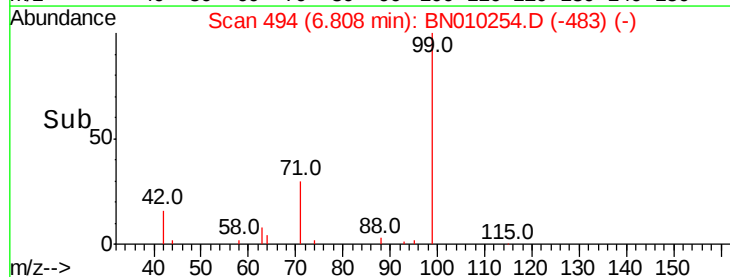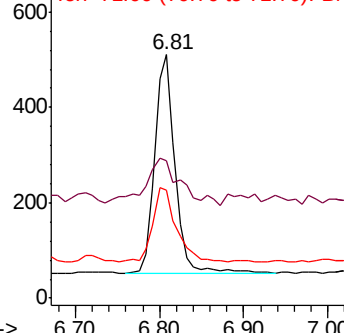

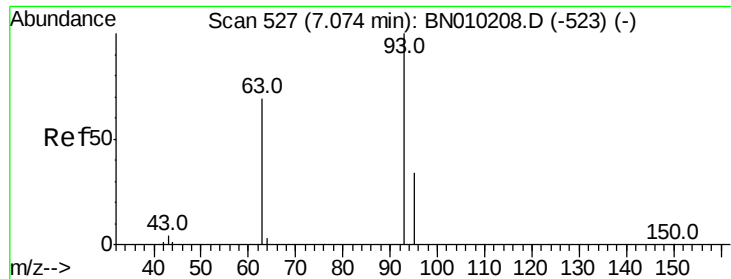

#6

bis(2-Chloroethyl)ether

Concen: 0.066 ng

RT: 7.07 min Scan# 526

Delta R.T. -0.01 min

Lab File: BN010254.D

Acq: 18 Mar 2020 07:35

Instrument :

BNA_N

ClientSampleId :

TT101D1-20200310


Tot Ion: 93 Resp: 600

Ion Ratio Lower Upper

93 100

63 68.3 53.4 80.0

95 30.7 28.6 42.8



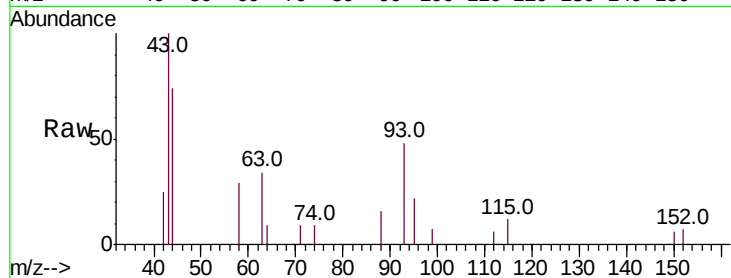


Abundance Ion 93.00 (92.70 to 93.70): BN010208.D (-523) (-)

Ion 63.00 (62.70 to 63.70): BN010208.D (-523) (-)

Ion 95.00 (94.70 to 95.70): BN010208.D (-523) (-)

Time-->

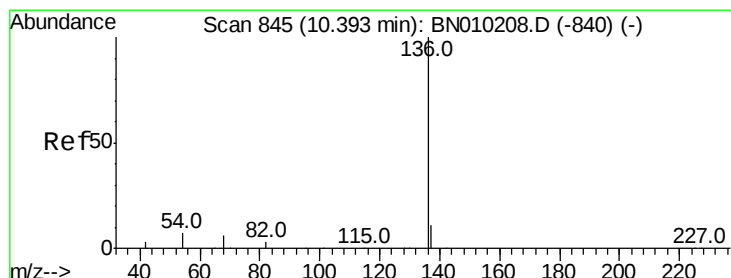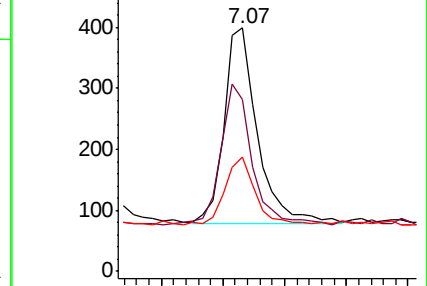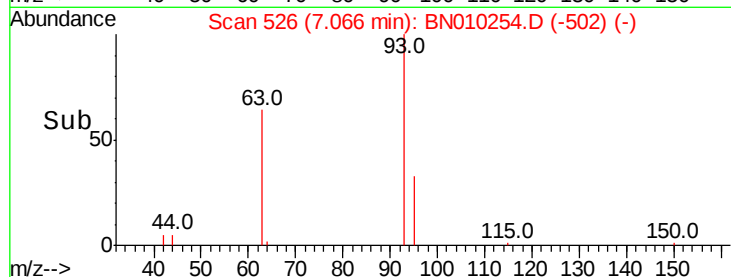

#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.38 min Scan# 844

Delta R.T. -0.01 min

Lab File: BN010254.D

Acq: 18 Mar 2020 07:35

Tgt Ion: 136 Resp: 13021


Ion Ratio Lower Upper

136 100

137 11.7 10.6 15.8

54 8.3 9.5 14.3#

68 7.2 9.7 14.5#

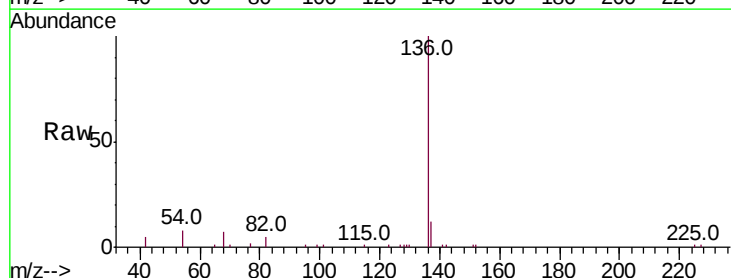



Abundance Ion 136.00 (135.70 to 136.70): BN010208.D (-840) (-)


Ion 137.00 (136.70 to 137.70): BN010208.D (-840) (-)

Ion 54.00 (53.70 to 54.70): BN010208.D (-840) (-)

Ion 68.00 (67.70 to 68.70): BN010208.D (-840) (-)

Time-->

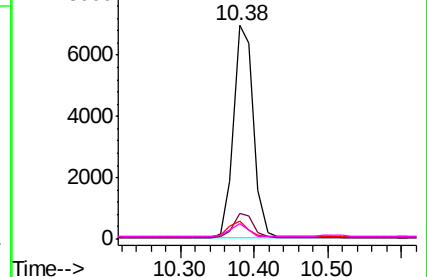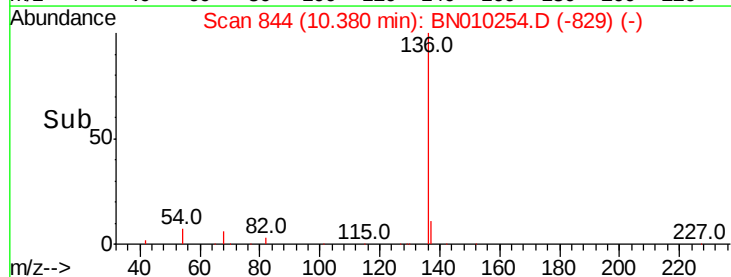

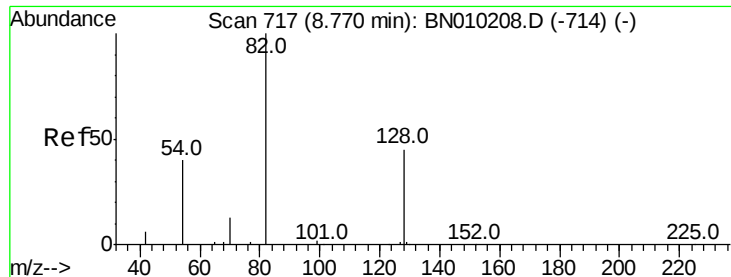

#8

Nitrobenzene-d5

Concen: 0.561 ng

RT: 8.76 min Scan# 716

Delta R.T. -0.01 min

Lab File: BN010254.D

Acq: 18 Mar 2020 07:35

Instrument :

BNA_N

ClientSampleId :

TT101D1-20200310


Tot Ion: 82 Resp: 4378

Ion Ratio Lower Upper

82 100

128 45.0 35.0 52.6




54 45.4 37.0 55.4

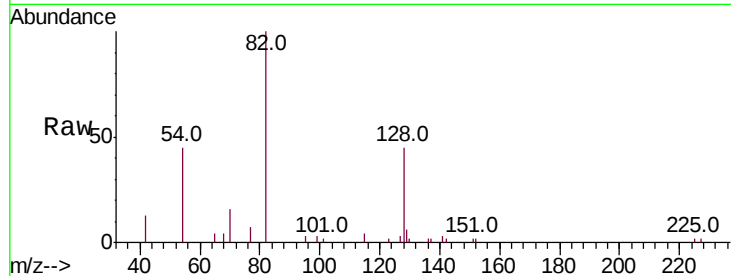

Abundance Ion 82.00 (81.70 to 82.70): BN010208.D (-714) (-)

Ion 128.00 (127.70 to 128.70): BN010208.D (-714) (-)

Ion 54.00 (53.70 to 54.70): BN010208.D (-714) (-)

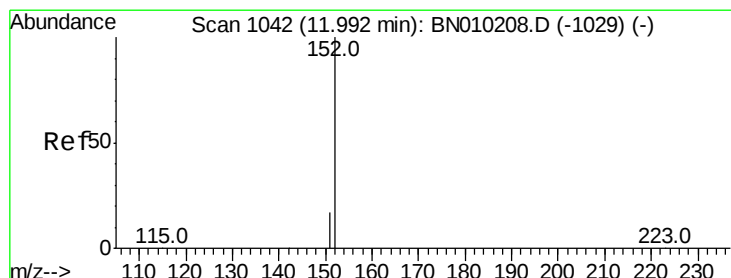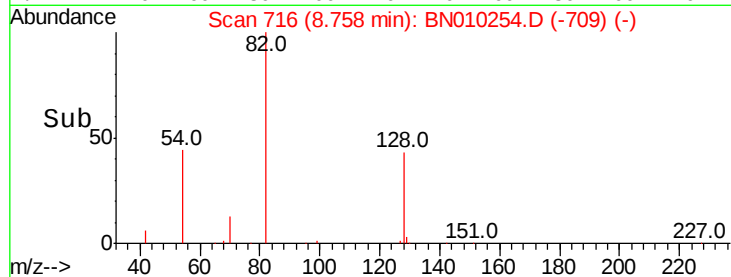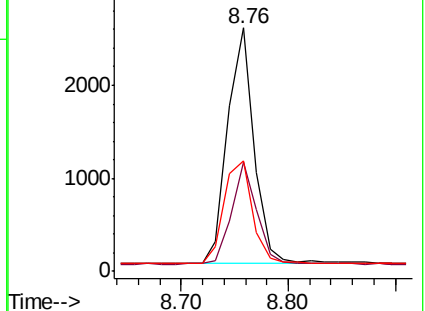

#11

2-Methylnaphthalene-d10

Concen: 0.278 ng

RT: 11.98 min Scan# 1039

Delta R.T. -0.01 min

Lab File: BN010254.D


Acq: 18 Mar 2020 07:35

Tgt Ion: 152 Resp: 5976

Ion Ratio Lower Upper



152 100


151 19.3 15.0 22.6

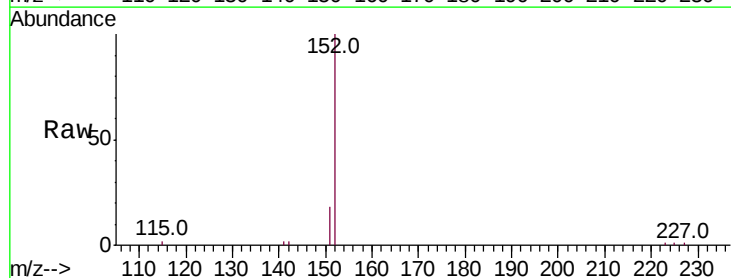

Abundance Ion 152.00 (151.70 to 152.70): BN010208.D (-1029) (-)

Ion 151.00 (150.70 to 151.70): BN010208.D (-1029) (-)

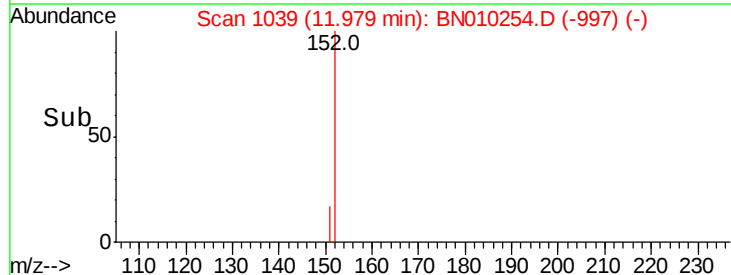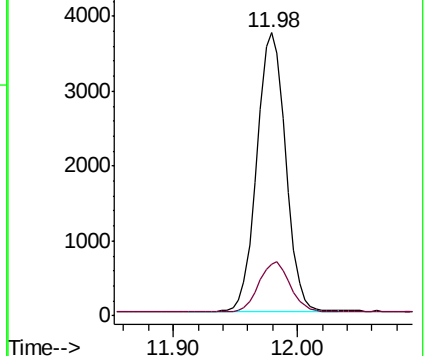

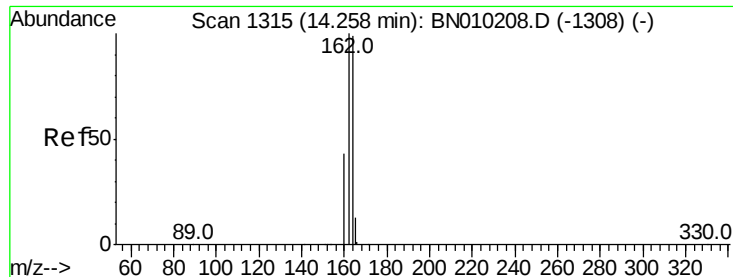

#13

Acenaphthene-d10

Concen: 0.400 ng

RT: 14.24 min Scan# 1313

Delta R.T. -0.02 min

Lab File: BN010254.D

Acq: 18 Mar 2020 07:35

Instrument :

BNA_N

ClientSampleId :

TT101D1-20200310


Tot Ion:164 Resp: 7797

Ion Ratio Lower Upper

164 100

162 103.1 81.0 121.4




160 48.4 35.6 53.4

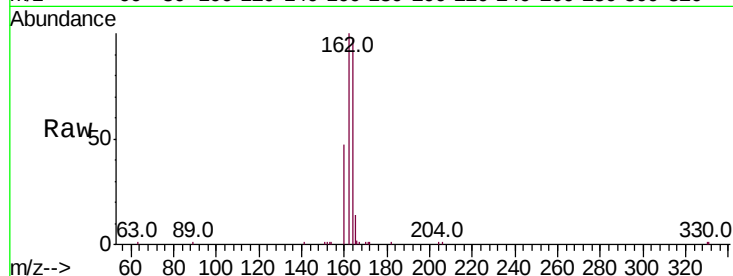

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

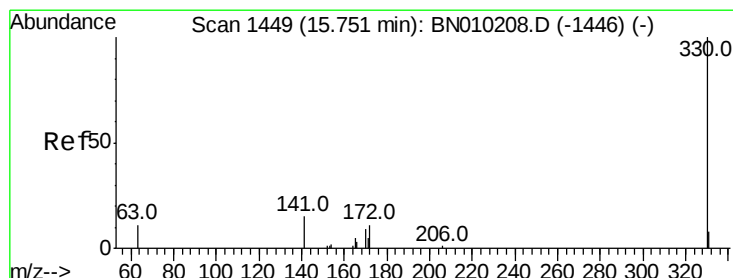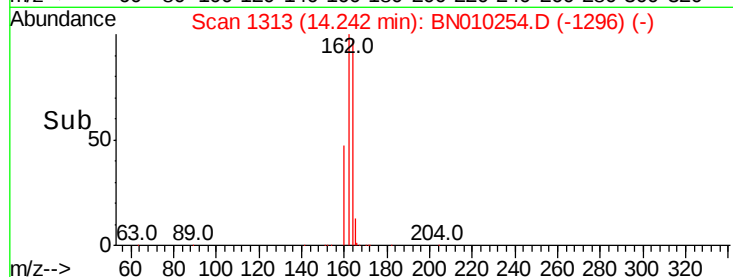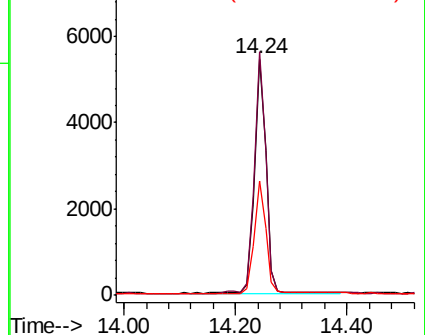

#14

2,4,6-Tribromophenol

Concen: 0.321 ng

RT: 15.74 min Scan# 1447

Delta R.T. -0.02 min

Lab File: BN010254.D

Acq: 18 Mar 2020 07:35


Tgt Ion:330 Resp: 896

Ion Ratio Lower Upper

330 100

332 0.0 0.0 0.0



141 37.1 25.1 37.7

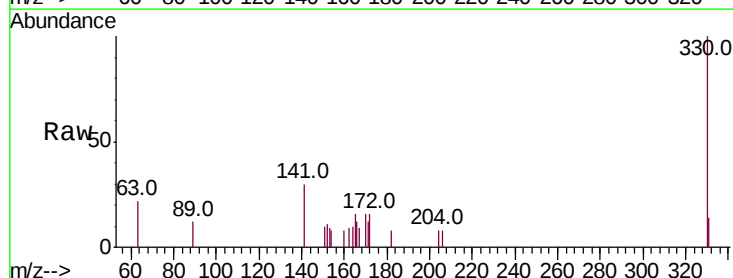


Abundance Ion 330.00 (329.70 to 330.70): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E



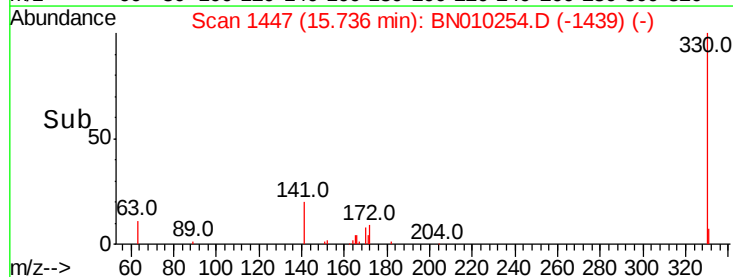
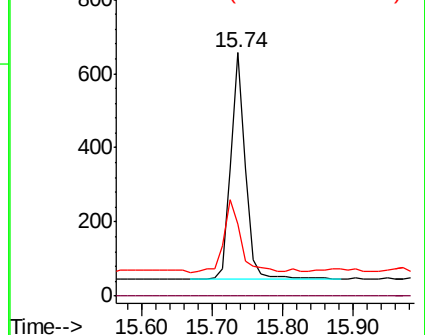


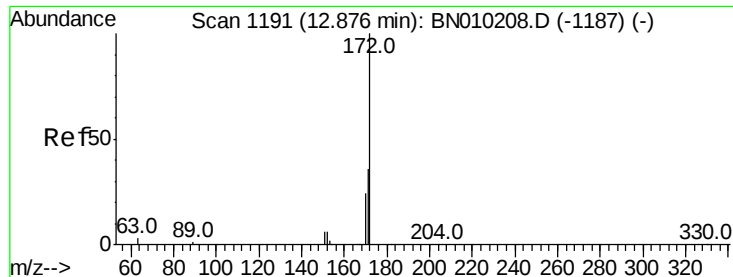

#15
2-Fluorobiphenyl
Concen: 0.625 ng
RT: 12.87 min Scan# 1190
Delta R.T. -0.00 min
Lab File: BN010254.D
Acq: 18 Mar 2020 07:35




Instrument :
BNA_N
ClientSampleId :
TT101D1-20200310


Tot Ion:172 Resp: 17360
Ion Ratio Lower Upper
172 100
171 34.3 29.4 44.2
170 22.3 20.2 30.4

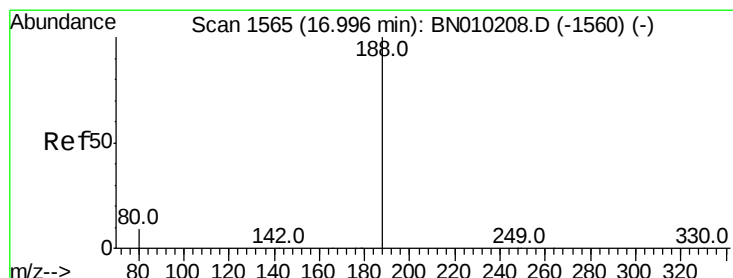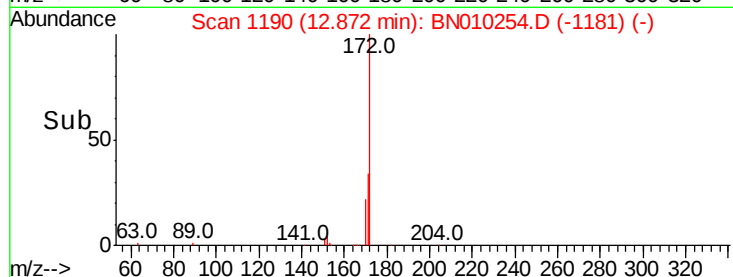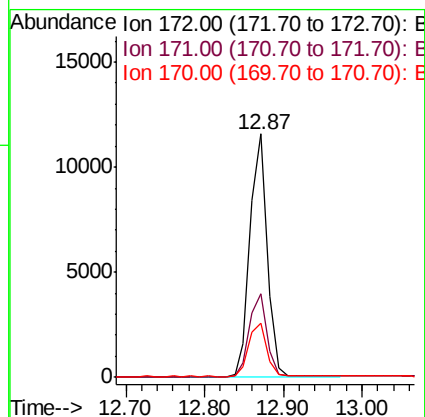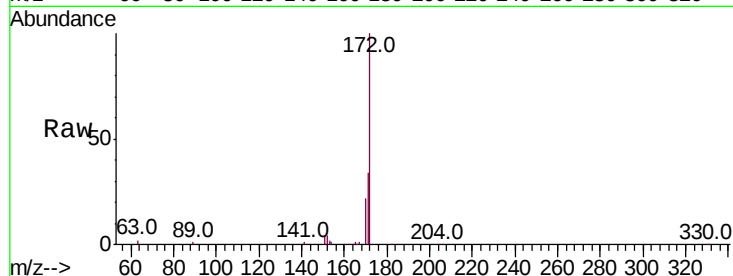

#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 16.99 min Scan# 1564
Delta R.T. -0.00 min
Lab File: BN010254.D
Acq: 18 Mar 2020 07:35

Tgt Ion:188 Resp: 18615
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 5.9 8.6 12.8#

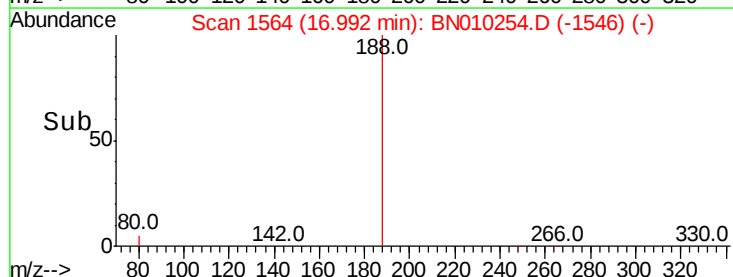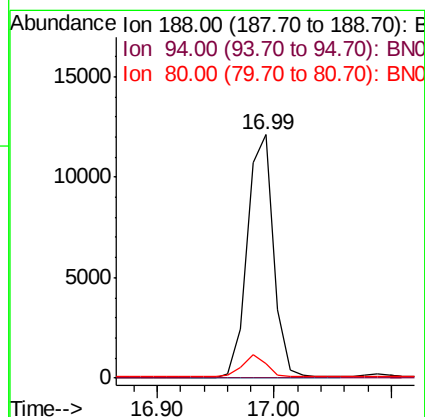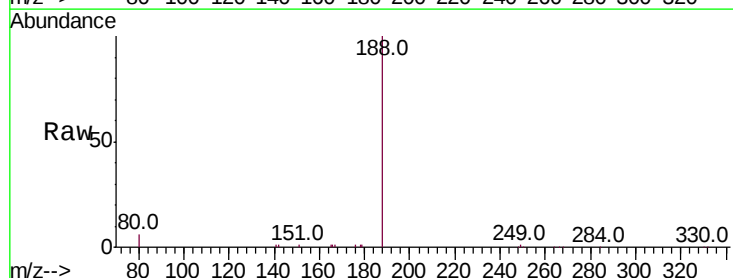

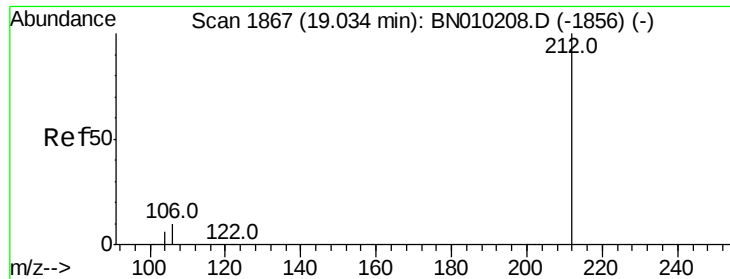

#25

Fluoranthene-d10

Concen: 0.300 ng

RT: 19.02 min Scan# 1863

Delta R.T. -0.01 min

Lab File: BN010254.D

Acq: 18 Mar 2020 07:35

Instrument :

BNA_N

ClientSampleId :

TT101D1-20200310


Tot Ion:212 Resp: 17232

Ion Ratio Lower Upper

212 100

106 9.5 8.1 12.1




104 5.4 4.7 7.1

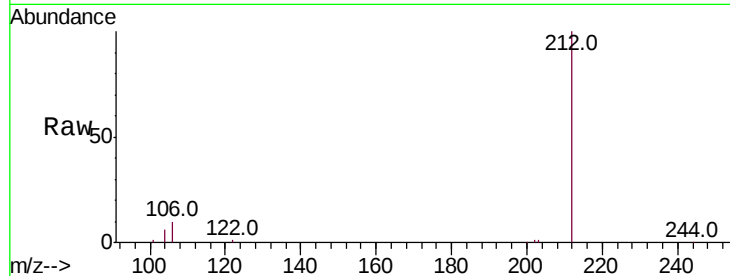

Abundance Ion 212.00 (211.70 to 212.70): E

Ion 106.00 (105.70 to 106.70): E

Ion 104.00 (103.70 to 104.70): E

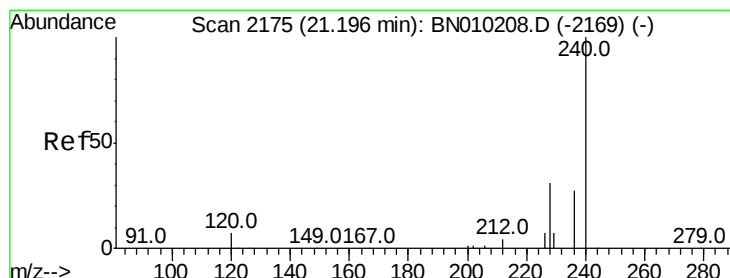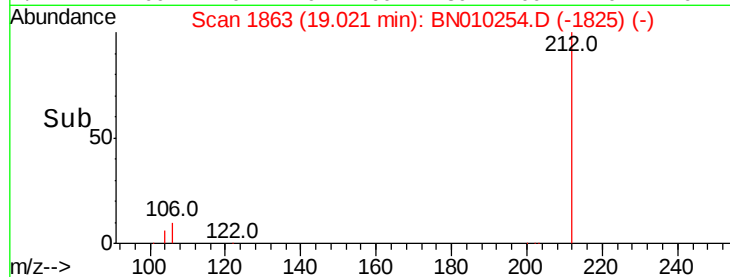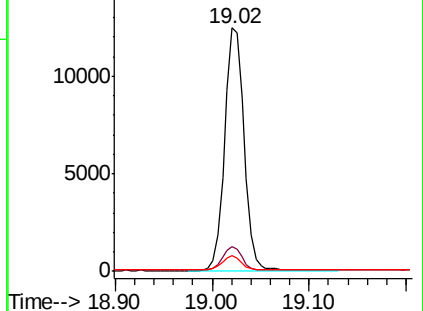

#27

Chrysene-d12

Concen: 0.400 ng

RT: 21.19 min Scan# 2173

Delta R.T. -0.01 min

Lab File: BN010254.D

Acq: 18 Mar 2020 07:35


Tgt Ion:240 Resp: 19669

Ion Ratio Lower Upper

240 100

120 6.0 7.7 11.5#



236 26.7 21.8 32.6

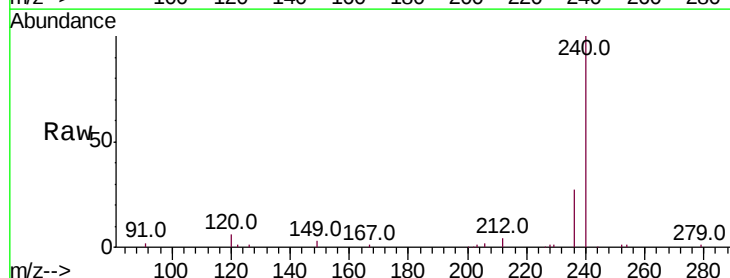


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

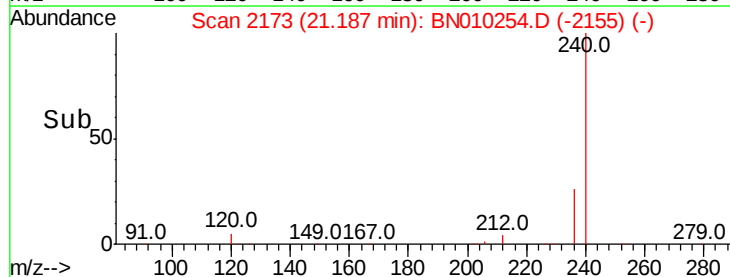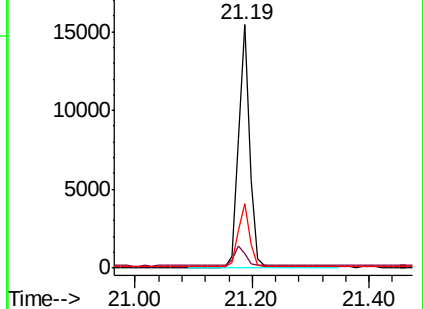

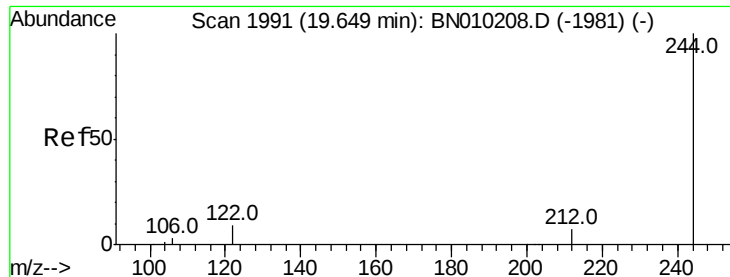

#29

Terphenyl-d14

Concen: 0.528 ng

RT: 19.64 min Scan# 1987

Delta R.T. -0.01 min

Lab File: BN010254.D

Acq: 18 Mar 2020 07:35

Instrument :

BNA_N

ClientSampleId :

TT101D1-20200310


Tot Ion:244 Resp: 23674

Ion Ratio Lower Upper

244 100

212 7.5 6.4 9.6




122 8.6 8.1 12.1

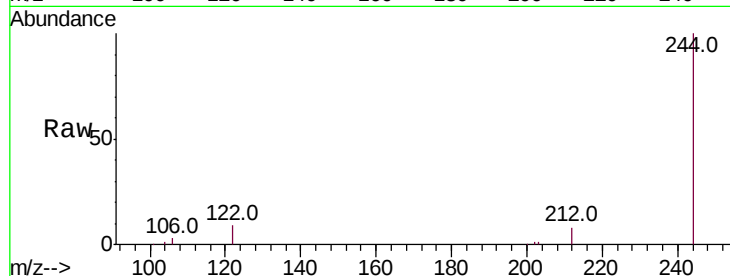

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

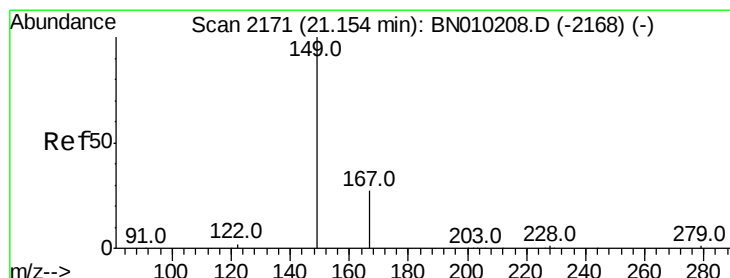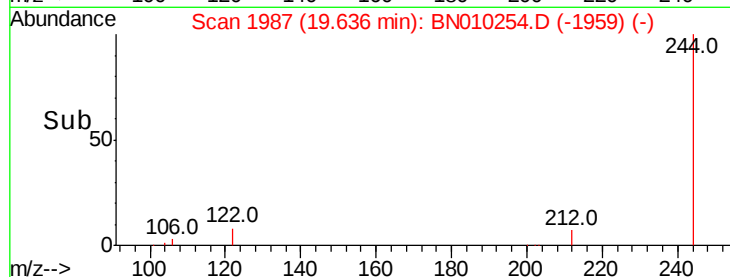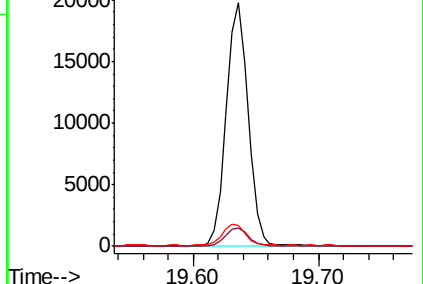

#32

Bis(2-ethylhexyl)phthalate

Concen: 0.143 ng

RT: 21.13 min Scan# 2168

Delta R.T. -0.02 min

Lab File: BN010254.D

Acq: 18 Mar 2020 07:35


Tgt Ion:149 Resp: 4077

Ion Ratio Lower Upper

149 100

167 29.8 21.0 31.4



279 4.3 3.1 4.7

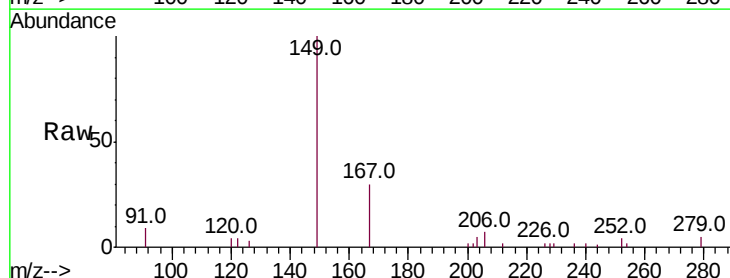


Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

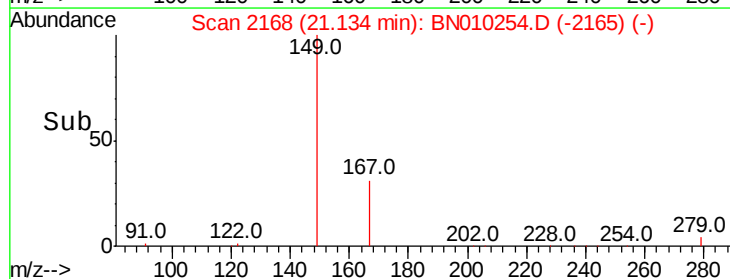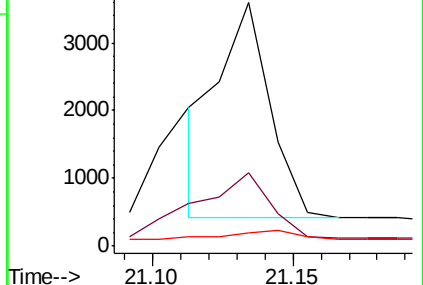

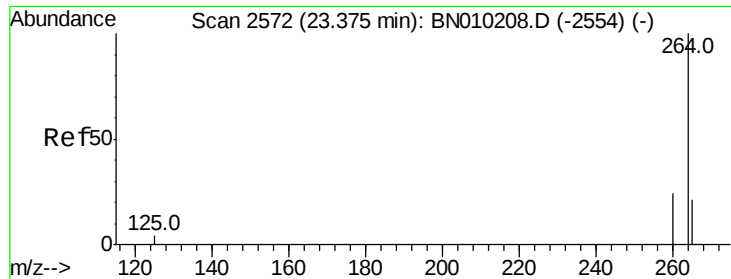

#34

Pervlene-d12

Concen: 0.400 ng

RT: 23.36 min Scan# 2566

Delta R.T. -0.02 min

Lab File: BN010254.D

Acq: 18 Mar 2020 07:35

Instrument :

BNA_N

ClientSampleId :

TT101D1-20200310


Tot Ion:264 Resp: 21152

Ion Ratio Lower Upper

264 100

260 24.8 19.7 29.5

265 37.0 25.8 38.6

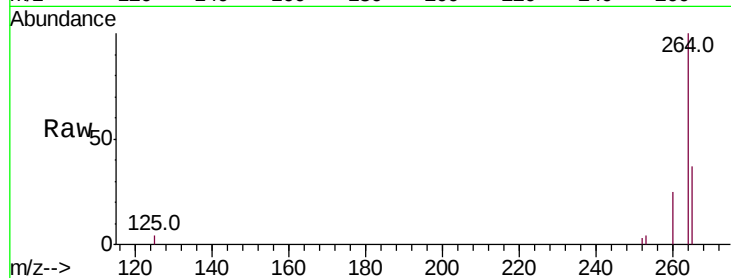

Abundance Ion 264.00 (263.70 to 264.70): E

15000 Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

