
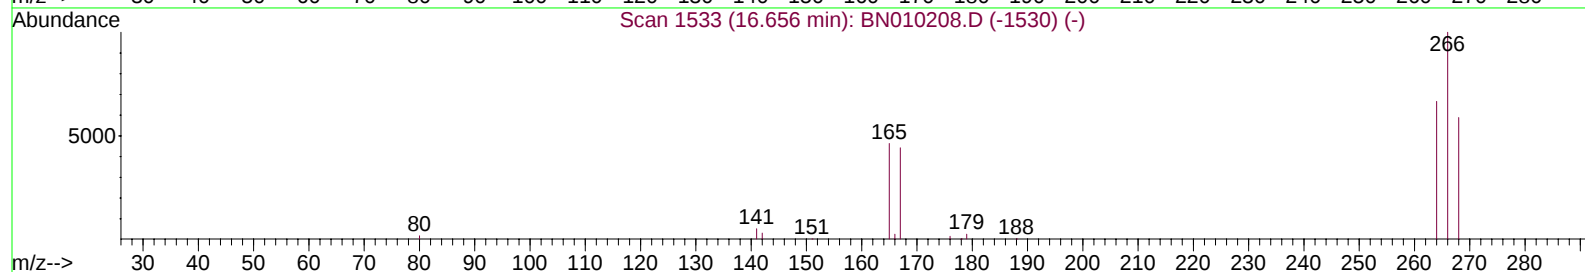
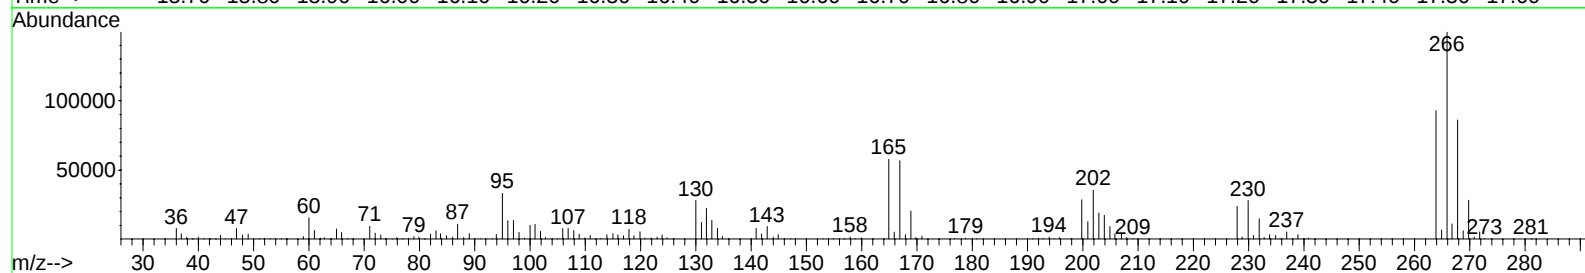


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN031720\
 Data File : BN010230.D
 Acq On : 17 Mar 2020 09:04
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 17 17:49:38 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN031320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 16 02:17:23 2020
 Response via : Initial Calibration

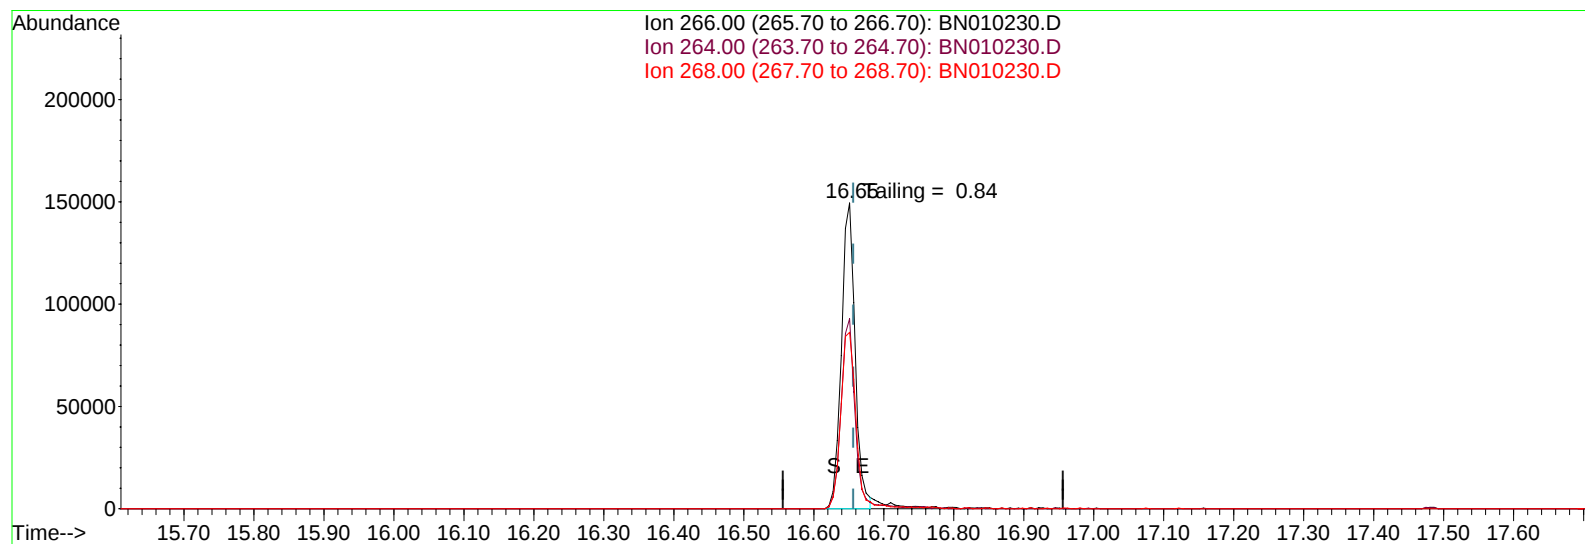

TIC: BN010230.D

(22) Pentachlorophenol

16.651min (-0.005) 0.00ng

response 206947

Ion	Exp%	Act%
266.00	100	100
264.00	70.20	62.16
268.00	76.80	57.71#
0.00	0.00	0.00