
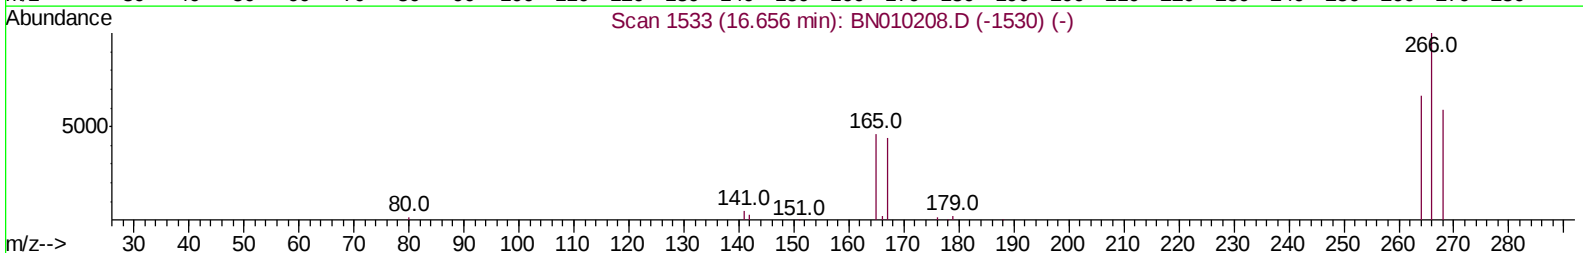
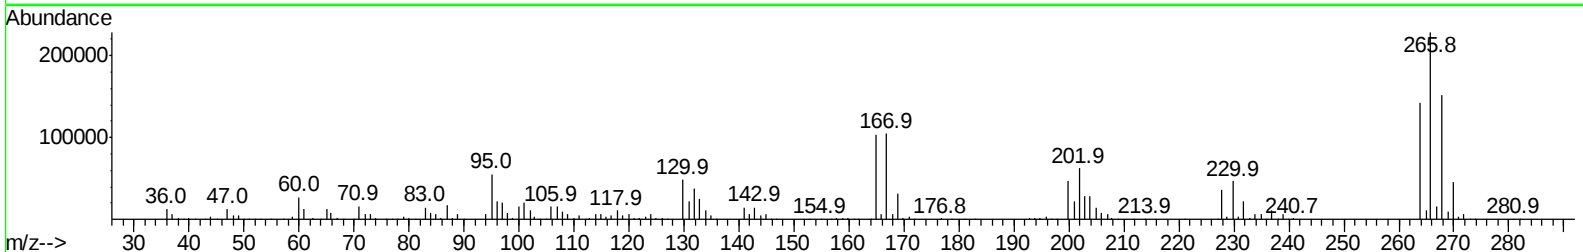


```
Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN031720\  
Data File : BN010246.D  
Acq On    : 18 Mar 2020 01:37  
Operator  : CG/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1      Sample Multiplier: 1
```

Quant Time: Mar 19 01:06:43 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN031320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 16 02:17:23 2020
Response via : Initial Calibration

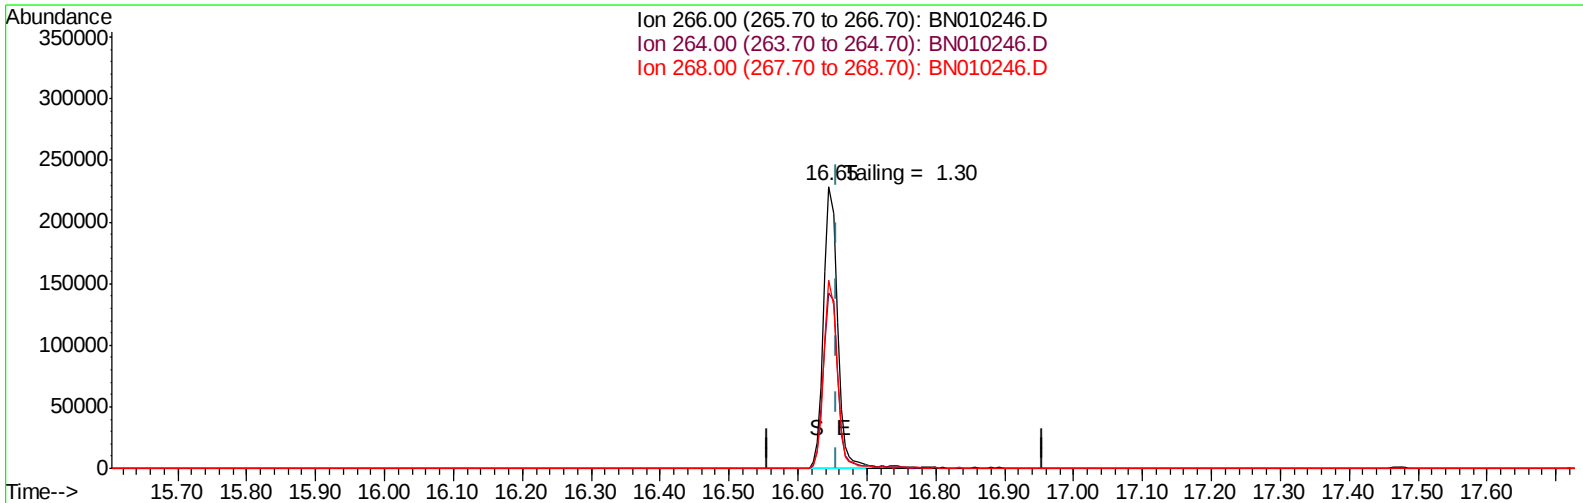

TIC: BN010246.D

(22) Pentachlorophenol		
16.645min (-0.011) 0.00ng		
response 320288		
Ion	Exp%	Act%
266.00	100	100
264.00	70.20	62.28
268.00	76.80	66.62
0.00	0.00	0.00