


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN031720\
 Data File : BN010230.D
 Acq On : 17 Mar 2020 09:04
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN031320.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Mar 16 02:17:23 2020

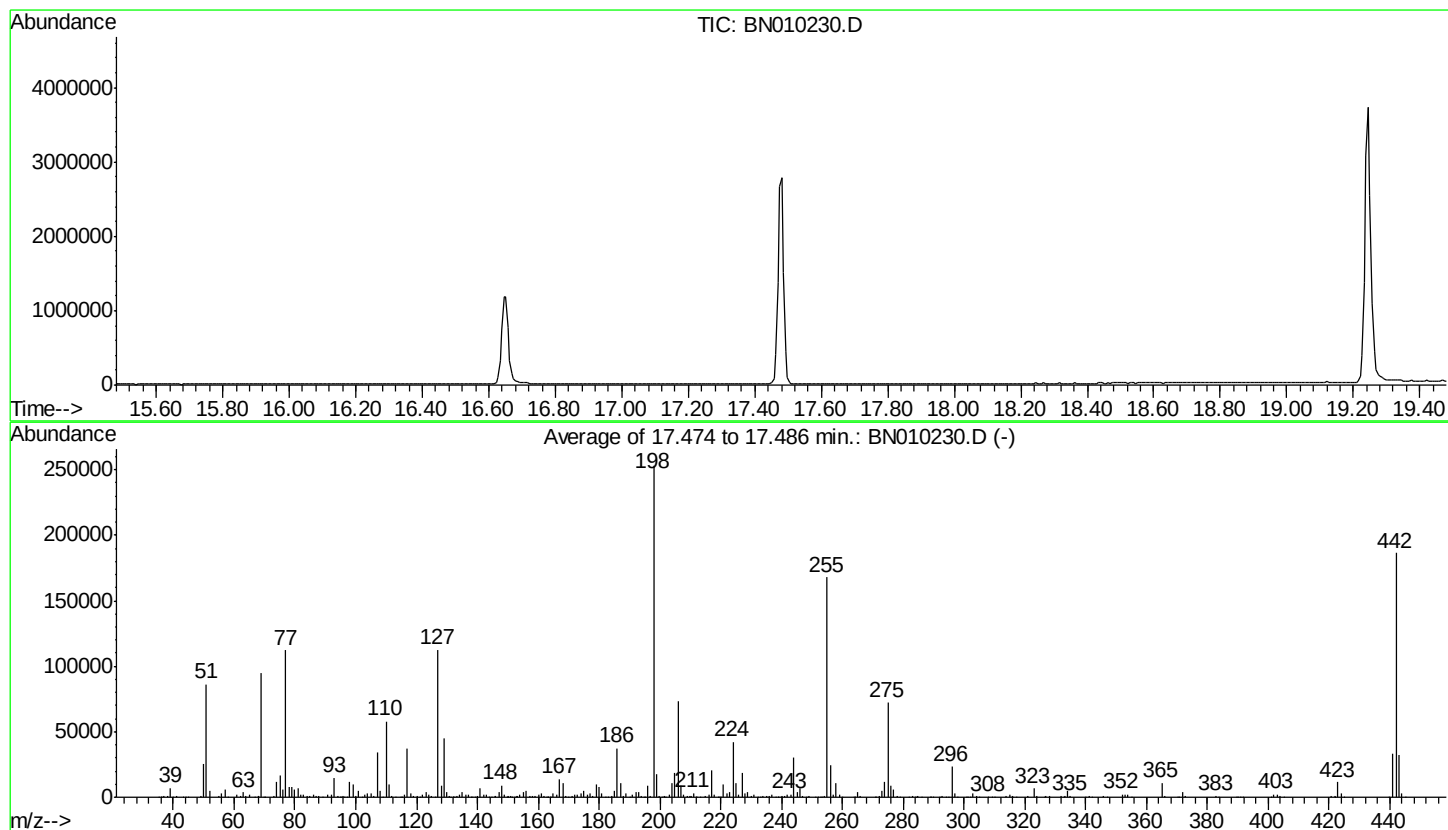

AutoFind: Scans 2497, 2498, 2499; Background Corrected with Scan 2490

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.1	86410	PASS
68	69	0.00	2	1.2	1103	PASS
69	198	0.00	100	37.3	94501	PASS
70	69	0.00	2	0.5	492	PASS
127	198	10	80	44.6	112866	PASS
197	198	0.00	2	0.3	663	PASS
198	198	100	100	100.0	253226	PASS
199	198	5	9	6.8	17275	PASS
275	198	10	60	28.4	71946	PASS
365	198	1	100	4.4	11228	PASS
441	198	0.01	100	13.0	33008	PASS
442	198	50	100	73.7	186688	PASS
443	442	15	24	17.5	32664	PASS