


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN031720\
 Data File : BN010246.D
 Acq On : 18 Mar 2020 01:37
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN031320.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Mar 16 02:17:23 2020

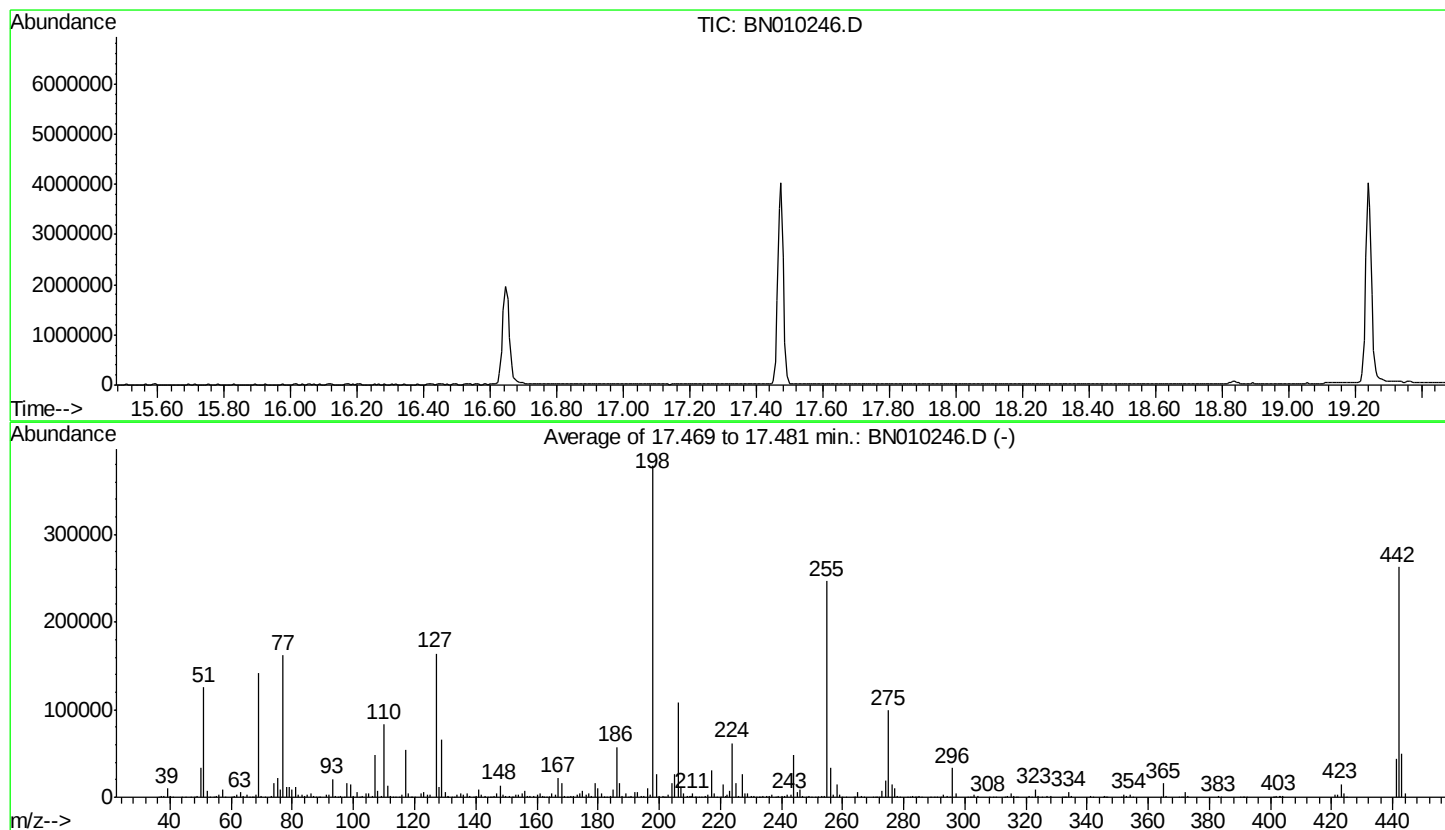

AutoFind: Scans 2496, 2497, 2498; Background Corrected with Scan 2488

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.1	125136	PASS
68	69	0.00	2	1.9	2677	PASS
69	198	0.00	100	37.3	141221	PASS
70	69	0.00	2	0.7	1027	PASS
127	198	10	80	43.3	164010	PASS
197	198	0.00	2	0.6	2303	PASS
198	198	100	100	100.0	378432	PASS
199	198	5	9	7.1	26880	PASS
275	198	10	60	26.1	98917	PASS
365	198	1	100	4.1	15664	PASS
441	198	0.01	100	11.4	43242	PASS
442	198	50	100	69.4	262549	PASS
443	442	15	24	18.8	49352	PASS