
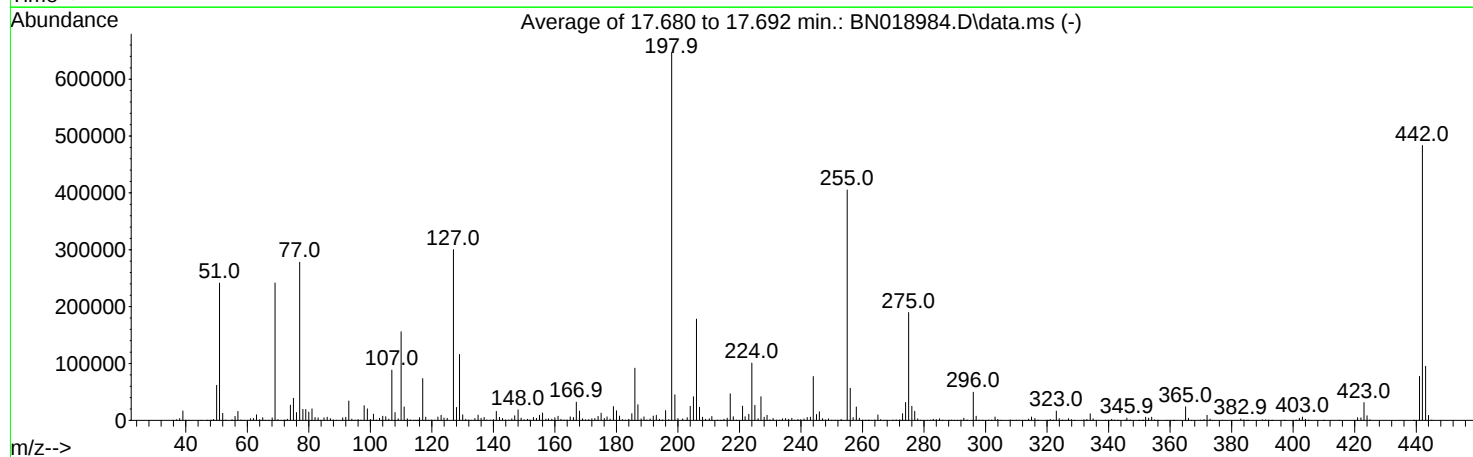


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031722\
 Data File : BN018984.D
 Acq On : 17 Mar 2022 08:23
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN031722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Mar 17 13:18:23 2022

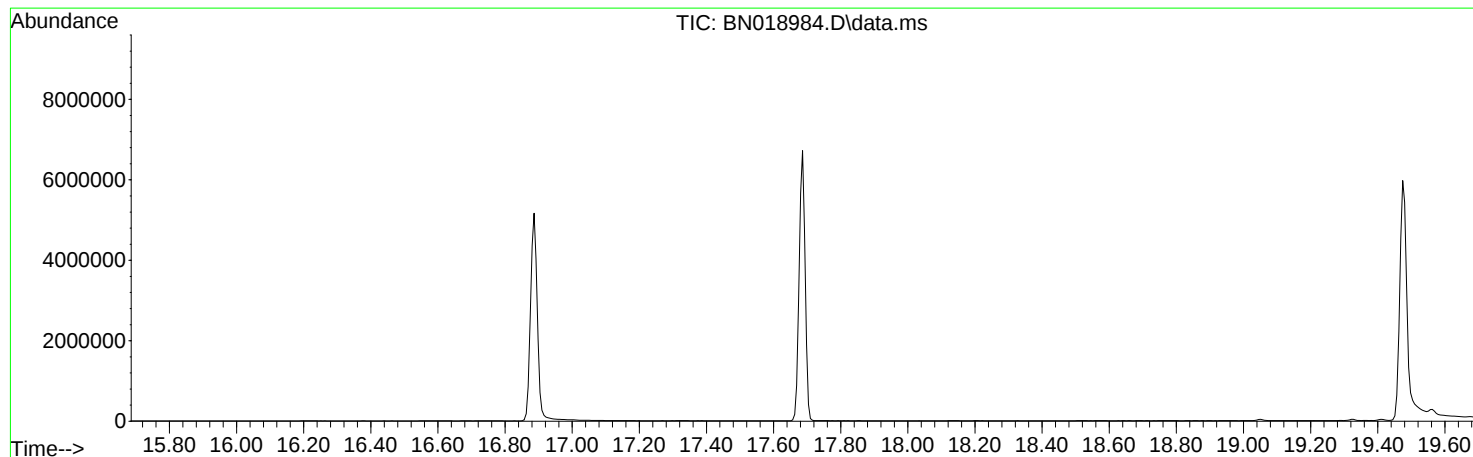




AutoFind: Scans 2498, 2499, 2500; Background Corrected with Scan 2490

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.3	241355	PASS
68	69	0.00	2	1.9	4516	PASS
69	198	0.00	100	37.4	241676	PASS
70	69	0.00	2	0.6	1387	PASS
127	198	10	80	46.4	300309	PASS
197	198	0.00	2	0.2	1507	PASS
198	198	100	100	100.0	646912	PASS
199	198	5	9	6.9	44904	PASS
275	198	10	60	29.3	189632	PASS
365	198	1	100	3.7	23843	PASS
441	198	0.01	100	12.0	77307	PASS
442	442	50	100	100.0	483392	PASS
443	442	15	24	19.7	95011	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031722\
Data File : BN018984.D
Acq On : 17 Mar 2022 08:23
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 17 12:37:10 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 14 15:11:57 2022
Response via : Initial Calibration

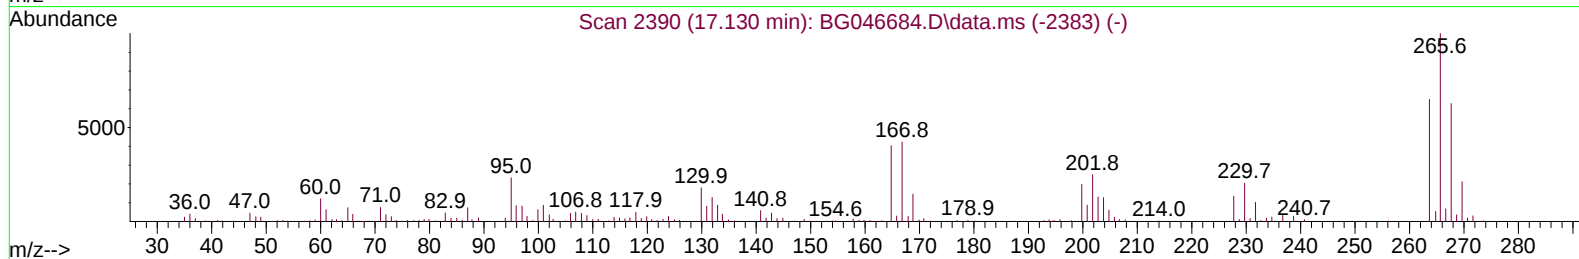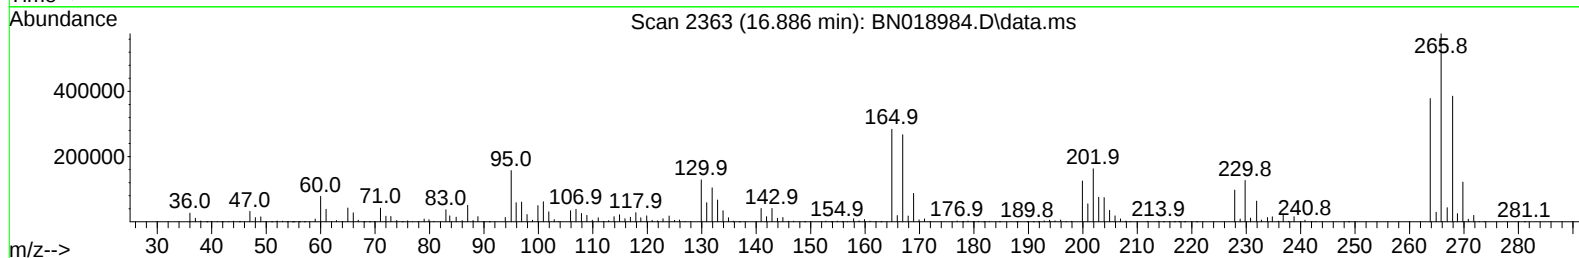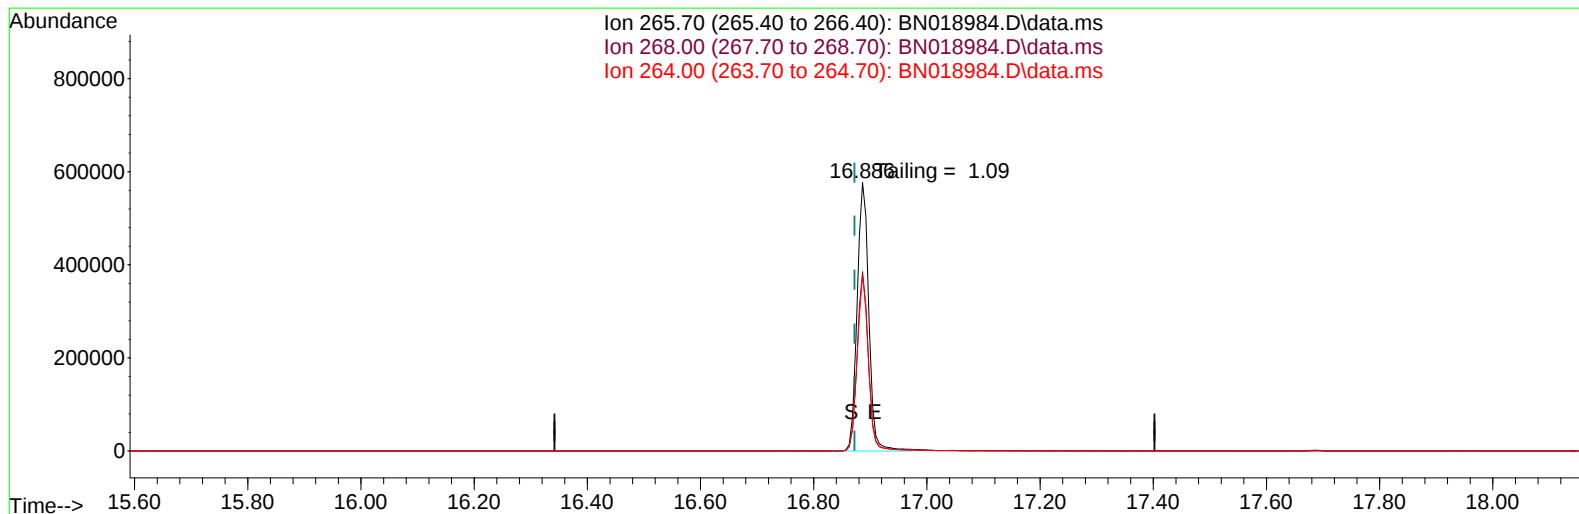

TIC: BN018984.D\data.ms

(70) Pentachlorophenol (C)

16.886min (+ 0.014) 24094.00 ng




response 836317

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	66.81
264.00	61.60	65.58
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031722\
Data File : BN018984.D
Acq On : 17 Mar 2022 08:23
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 17 12:37:10 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 14 15:11:57 2022
Response via : Initial Calibration

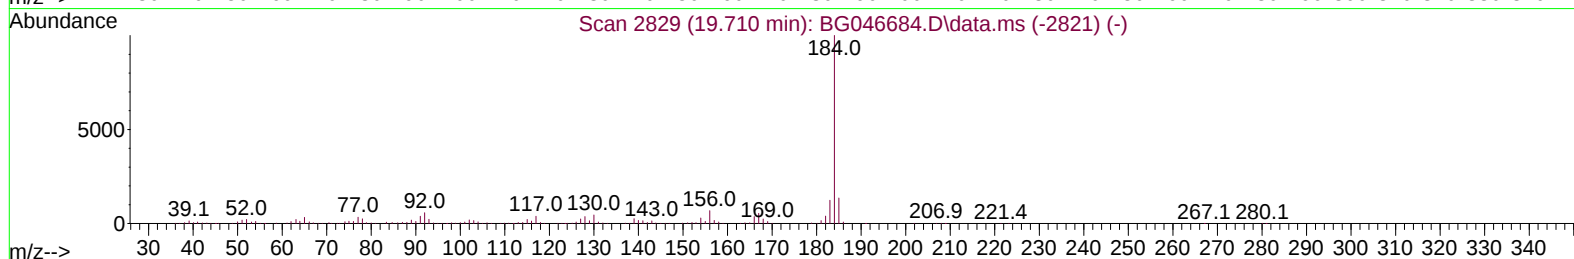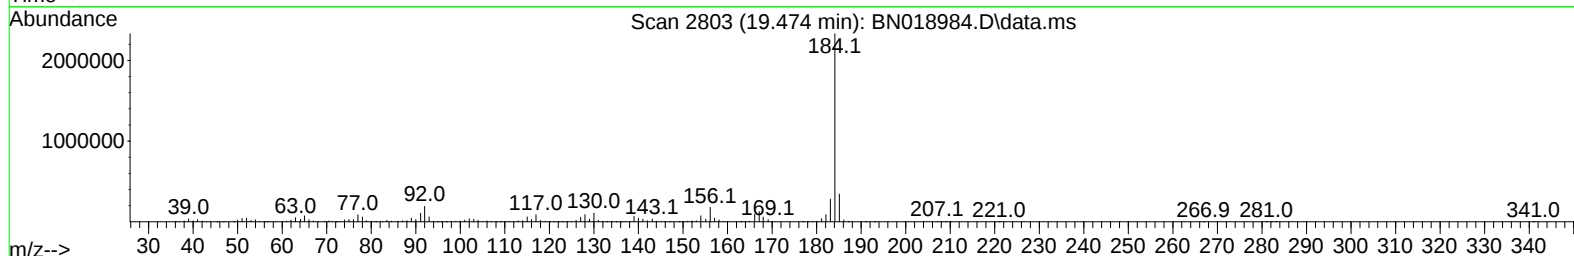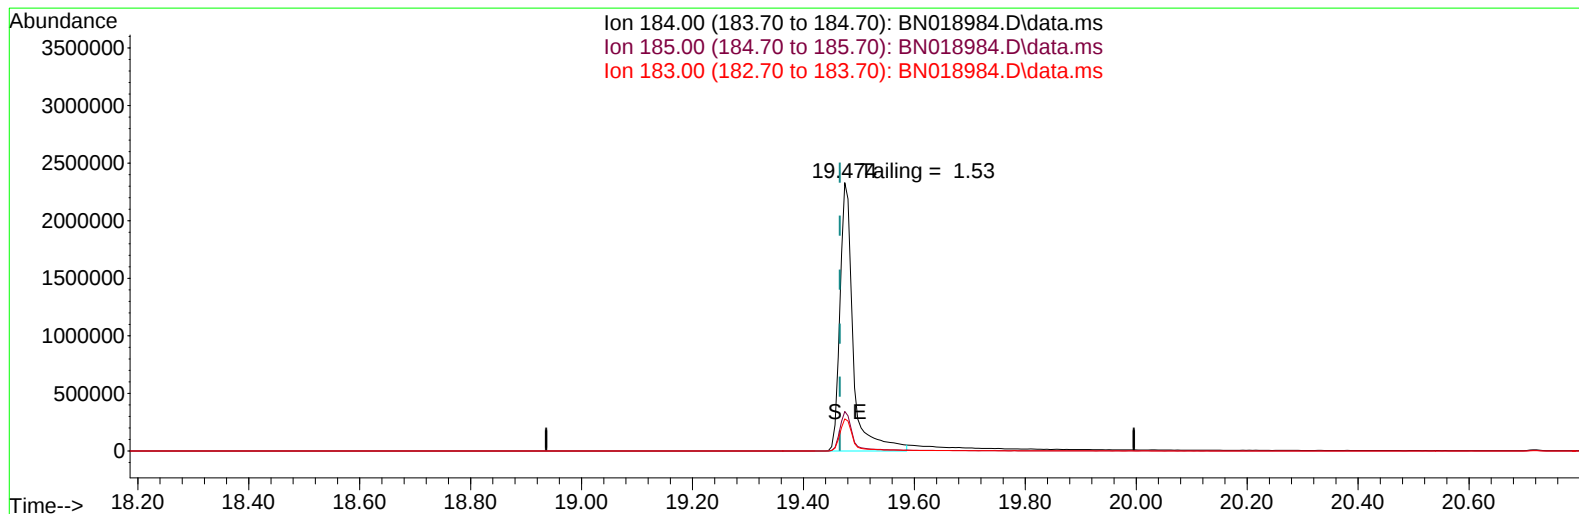

TIC: BN018984.D\data.ms

(77) Benzidine

19.474min (+ 0.009) 0.00 ng

response 4233026

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.76
183.00	13.20	11.98
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/17/2022	BNA_N	<u>BN018984.D</u>
Compound Name	Response	Retention Time
DDT	2286642	20.72
DDD	27079	20.27
DDE	766	19.76
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
27845	2314487	1.20

Instrument :
BNA_N
ClientSampleId :
DFTPP