
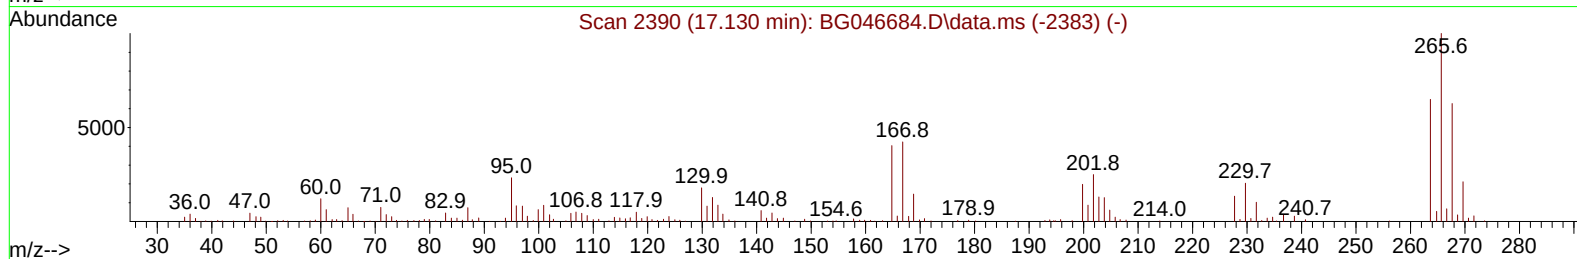
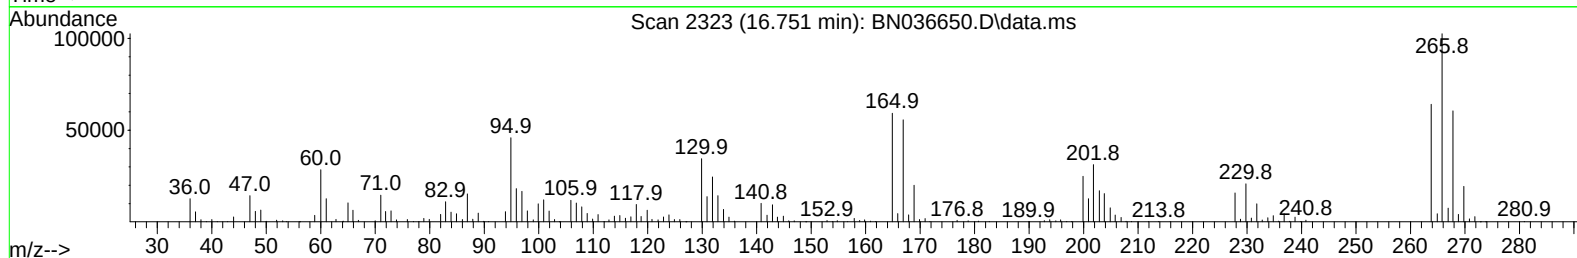


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031725\
Data File : BN036650.D
Acq On : 17 Mar 2025 09:10
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 17 18:55:39 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 17 01:20:13 2025
Response via : Initial Calibration

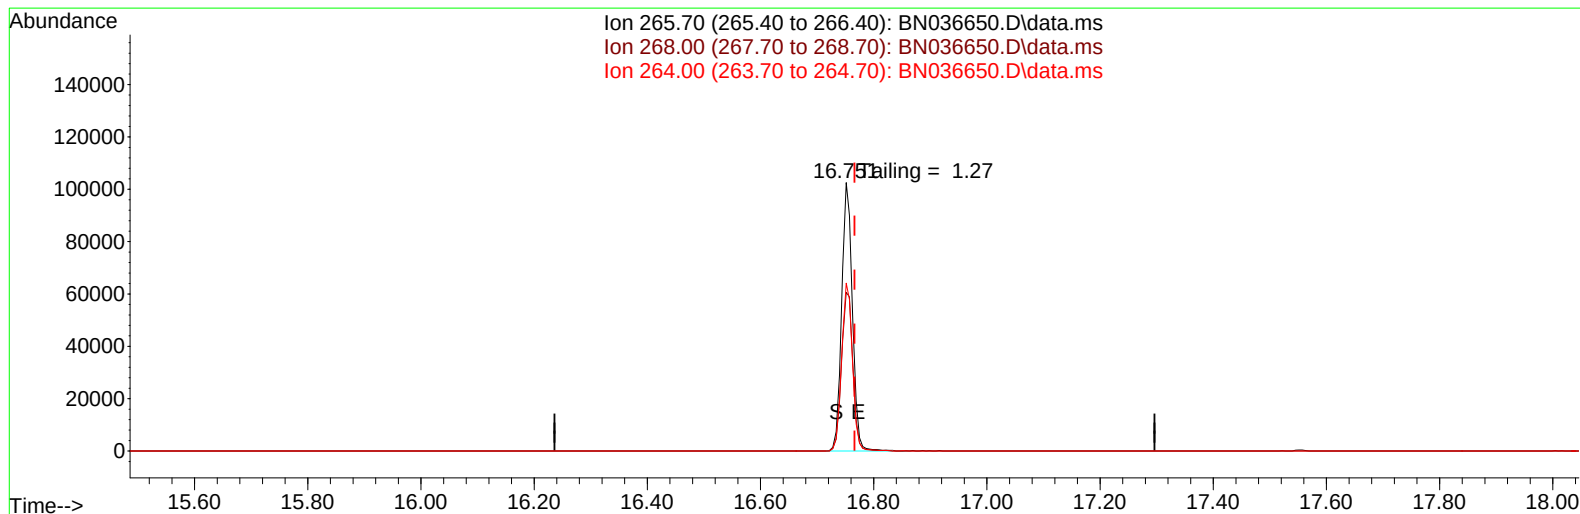

TIC: BN036650.D\data.ms

(70) Pentachlorophenol (C)




16.751min (-0.015) 17170.72 ng

response 134482

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	59.07
264.00	61.60	62.53
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031725\
Data File : BN036650.D
Acq On : 17 Mar 2025 09:10
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 17 18:55:39 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 17 01:20:13 2025
Response via : Initial Calibration

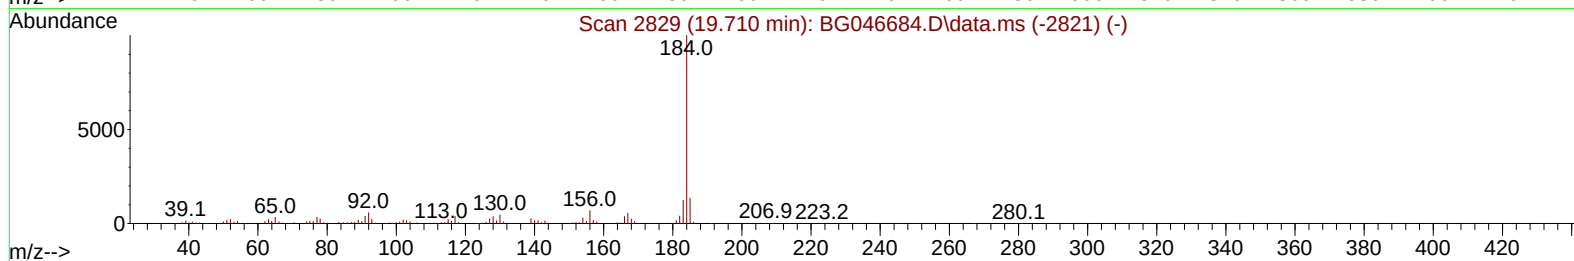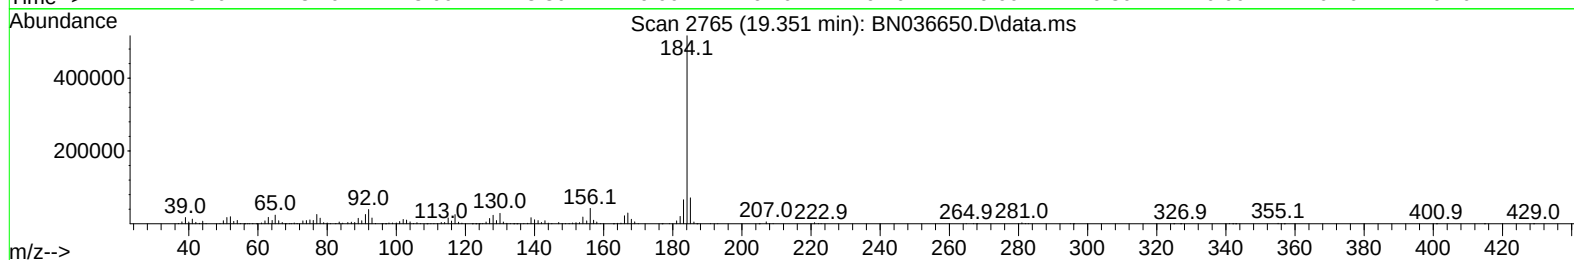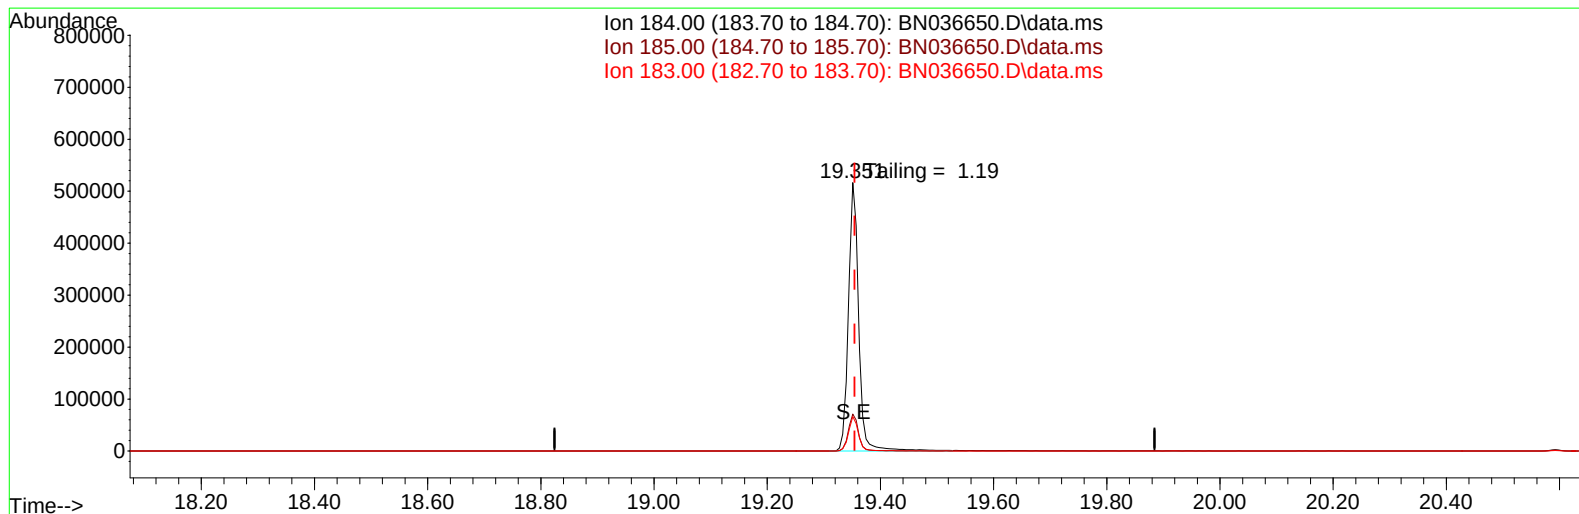

TIC: BN036650.D\data.ms

(77) Benzidine

19.351min (-0.003) 0.00 ng

response 648586

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.79
183.00	13.20	12.82
0.00	0.00	0.00