
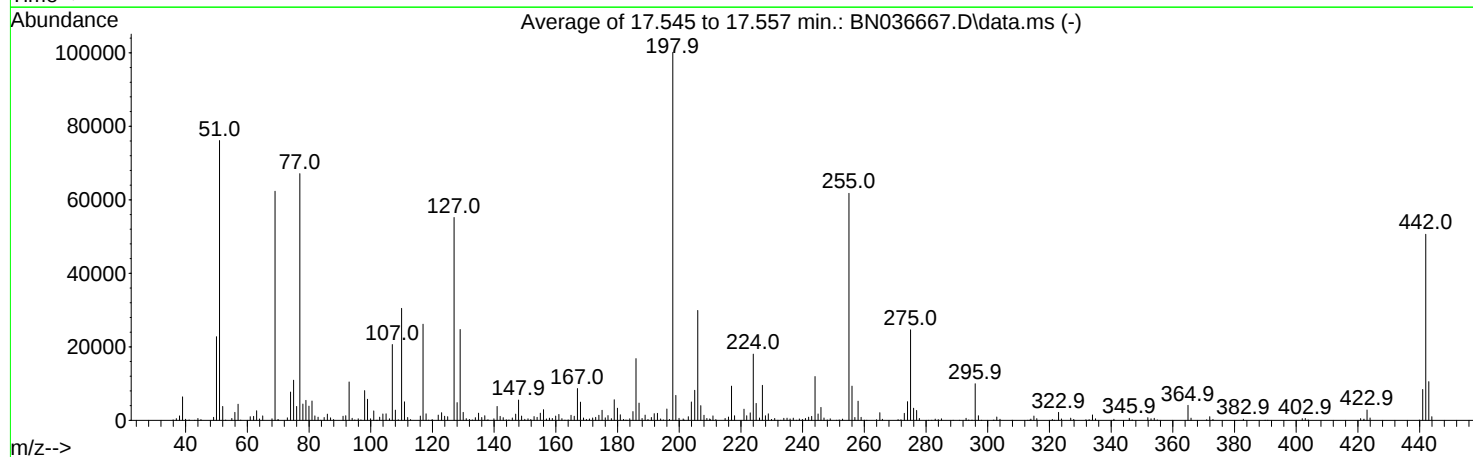


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031725\
Data File : BN036667.D
Acq On : 17 Mar 2025 20:23
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN031025.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Mar 10 16:06:28 2025

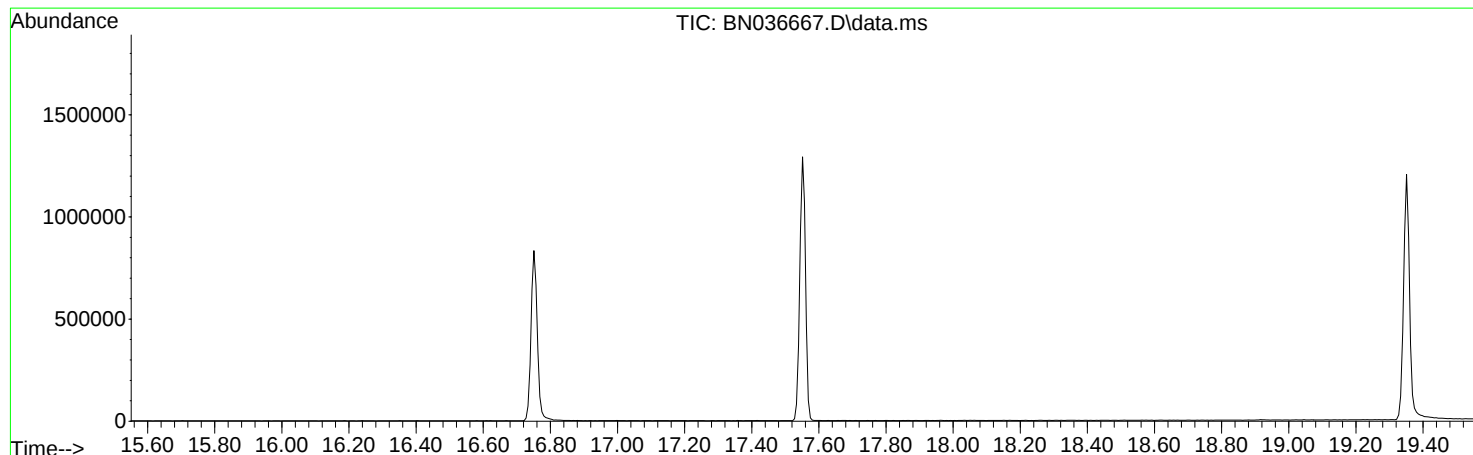




AutoFind: Scans 2458, 2459, 2460; Background Corrected with Scan 2452

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	76.1	76120	PASS
68	69	0.00	2	0.7	429	PASS
69	198	0.00	100	62.3	62344	PASS
70	69	0.00	2	0.3	205	PASS
127	198	10	80	55.2	55208	PASS
197	198	0.00	2	0.2	248	PASS
198	198	100	100	100.0	100083	PASS
199	198	5	9	6.8	6805	PASS
275	198	10	60	24.6	24659	PASS
365	198	1	100	4.1	4079	PASS
441	198	0.01	100	8.4	8421	PASS
442	442	50	100	100.0	50624	PASS
443	442	15	24	20.8	10520	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031725\
Data File : BN036667.D
Acq On : 17 Mar 2025 20:23
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 18 01:27:33 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 18 01:27:23 2025
Response via : Initial Calibration

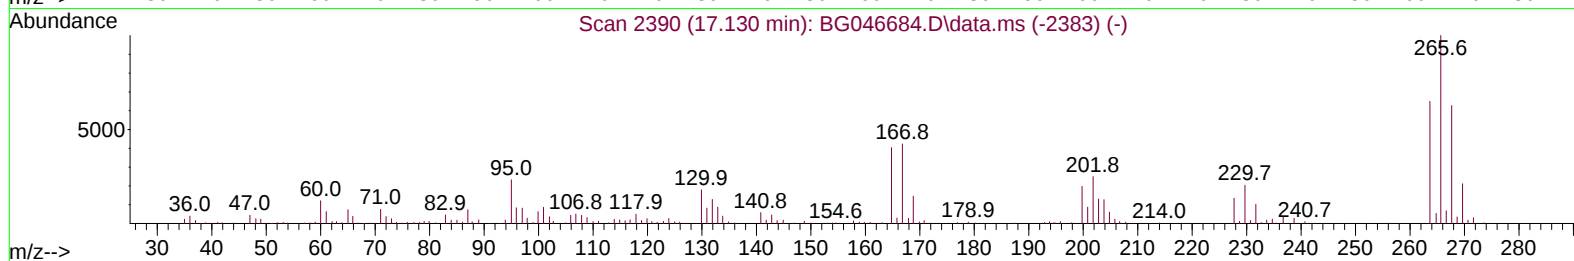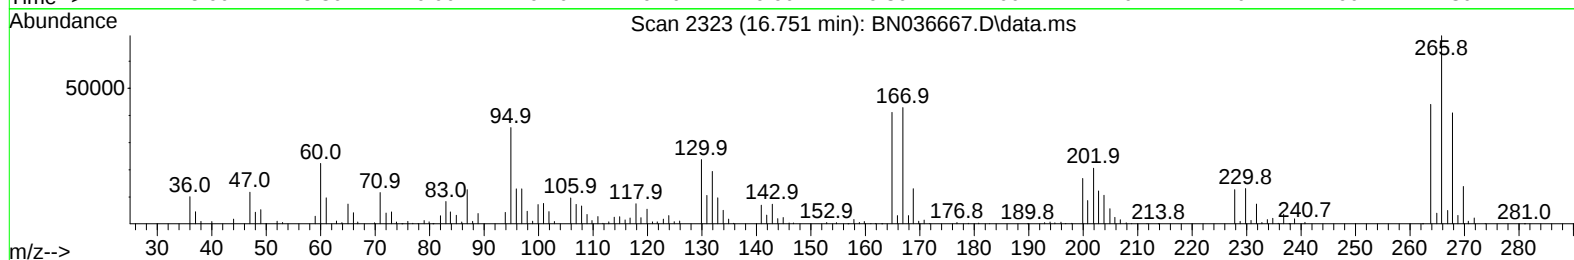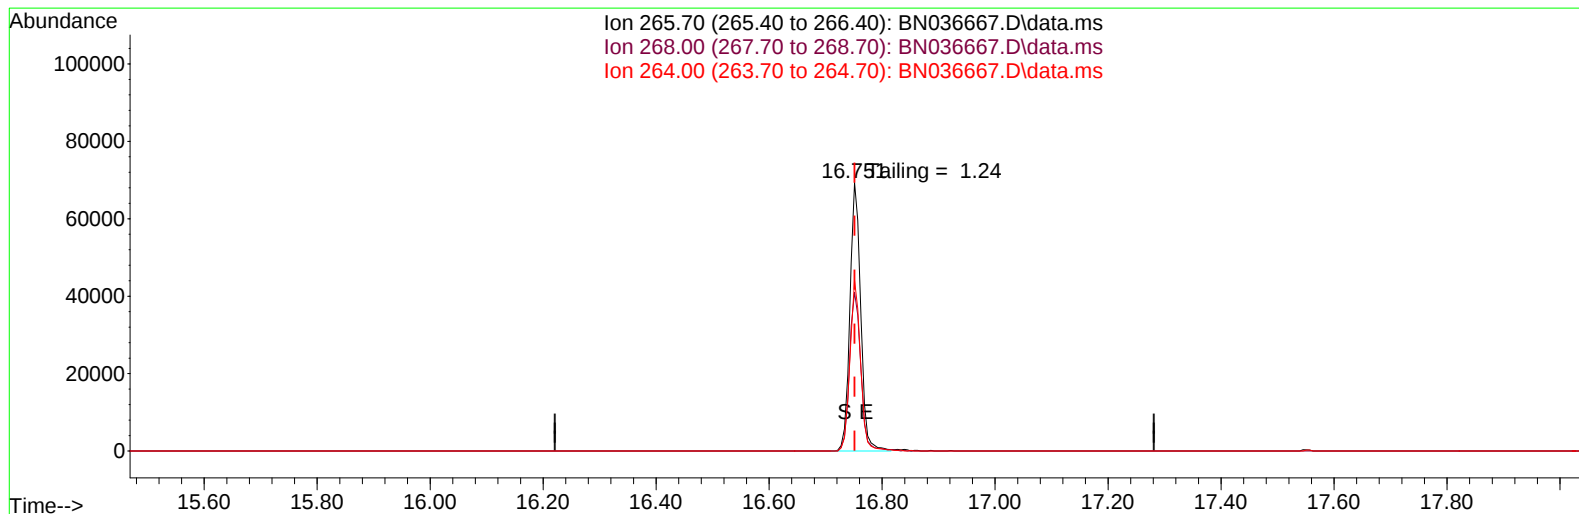

TIC: BN036667.D\data.ms

(70) Pentachlorophenol (C)

16.751min (0.000) 16844.36 ng




response 92401

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	59.06
264.00	61.60	63.56
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031725\
Data File : BN036667.D
Acq On : 17 Mar 2025 20:23
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 18 01:27:33 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 18 01:27:23 2025
Response via : Initial Calibration

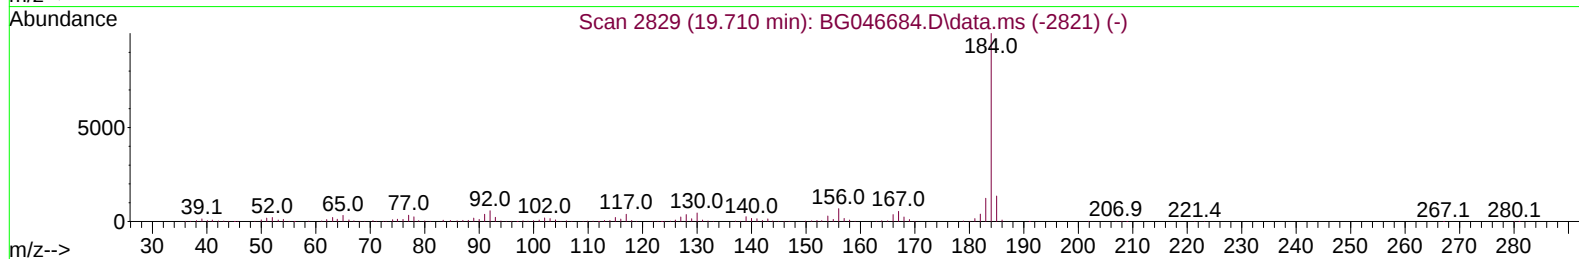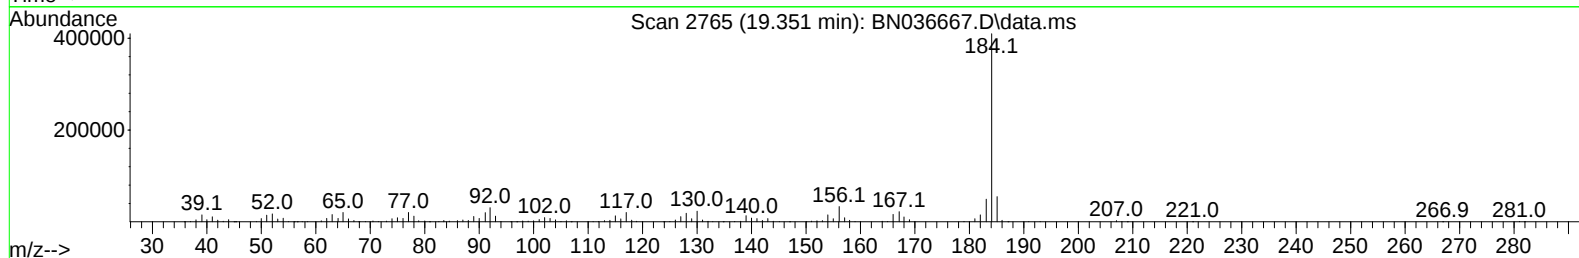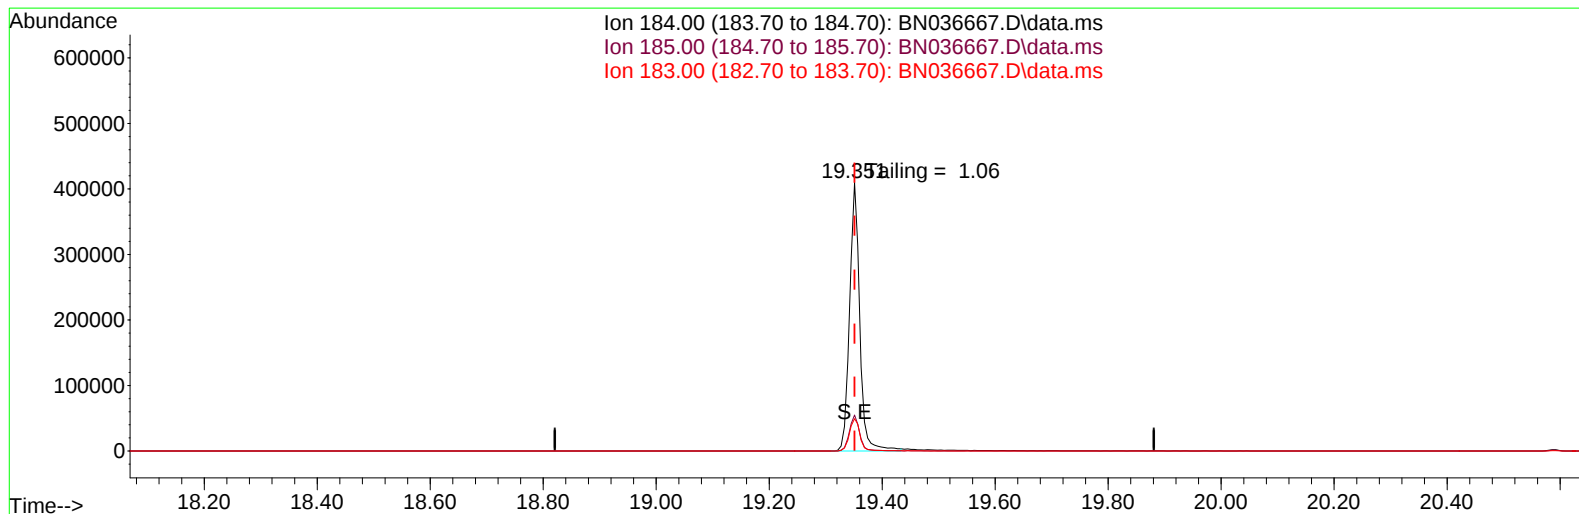

TIC: BN036667.D\data.ms

(77) Benzidine

19.351min (0.000) 0.00 ng

response 518588

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.44
183.00	13.20	12.05
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/17/2025	BNA_N	<u>BN036667.D</u>
Compound Name	Response	Retention Time
DDT	323246	20.592
DDD	4464	20.151
DDE	248	19.645
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4712	327958	1.44

Instrument :
BNA_N
ClientSampleId :
DFTPP