


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN031820\
 Data File : BN010264.D
 Acq On : 18 Mar 2020 15:32
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN031320.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Mar 16 02:17:23 2020

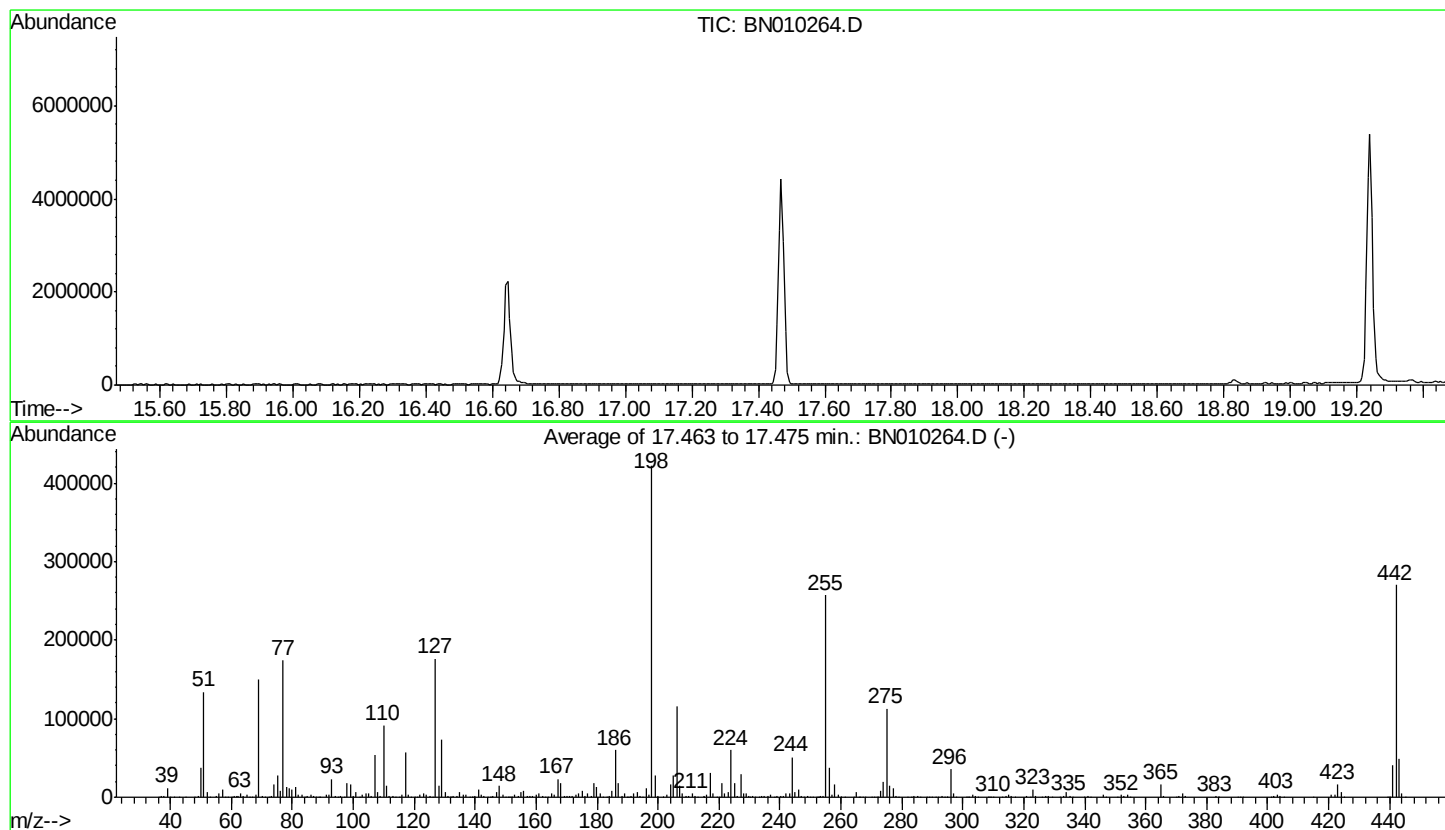

AutoFind: Scans 2495, 2496, 2497; Background Corrected with Scan 2489

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.8	134197	PASS
68	69	0.00	2	2.0	2914	PASS
69	198	0.00	100	35.3	149173	PASS
70	69	0.00	2	0.6	898	PASS
127	198	10	80	41.8	176426	PASS
197	198	0.00	2	0.7	3109	PASS
198	198	100	100	100.0	422165	PASS
199	198	5	9	6.5	27293	PASS
275	198	10	60	26.7	112688	PASS
365	198	1	100	3.8	15842	PASS
441	198	0.01	100	9.5	40013	PASS
442	198	50	100	64.0	270037	PASS
443	442	15	24	18.2	49280	PASS