
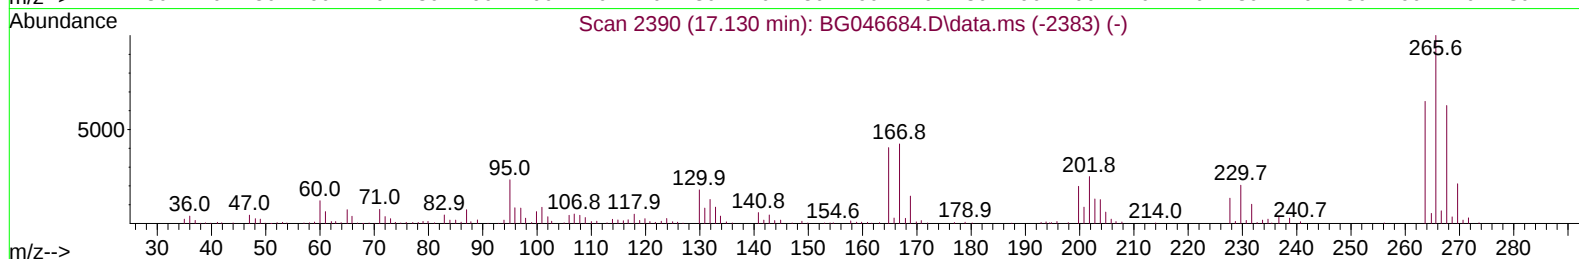
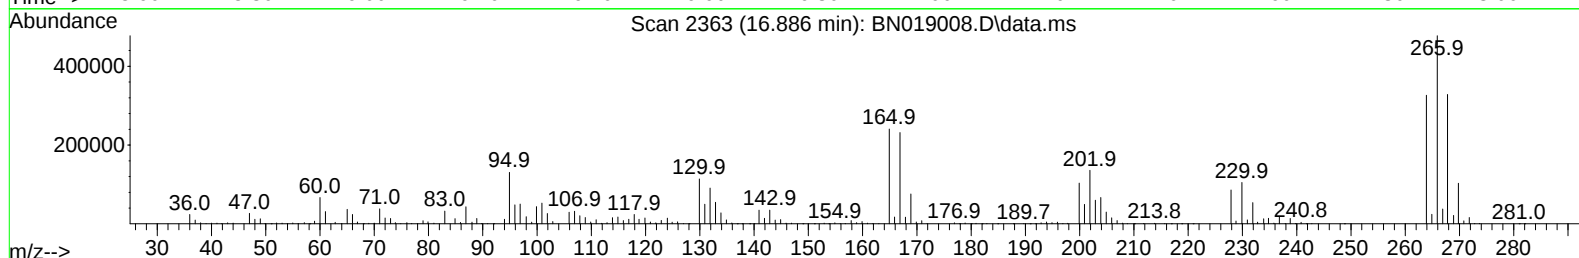


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031822\
Data File : BN019008.D
Acq On : 18 Mar 2022 08:51
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 18 15:17:30 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 14 15:11:57 2022
Response via : Initial Calibration

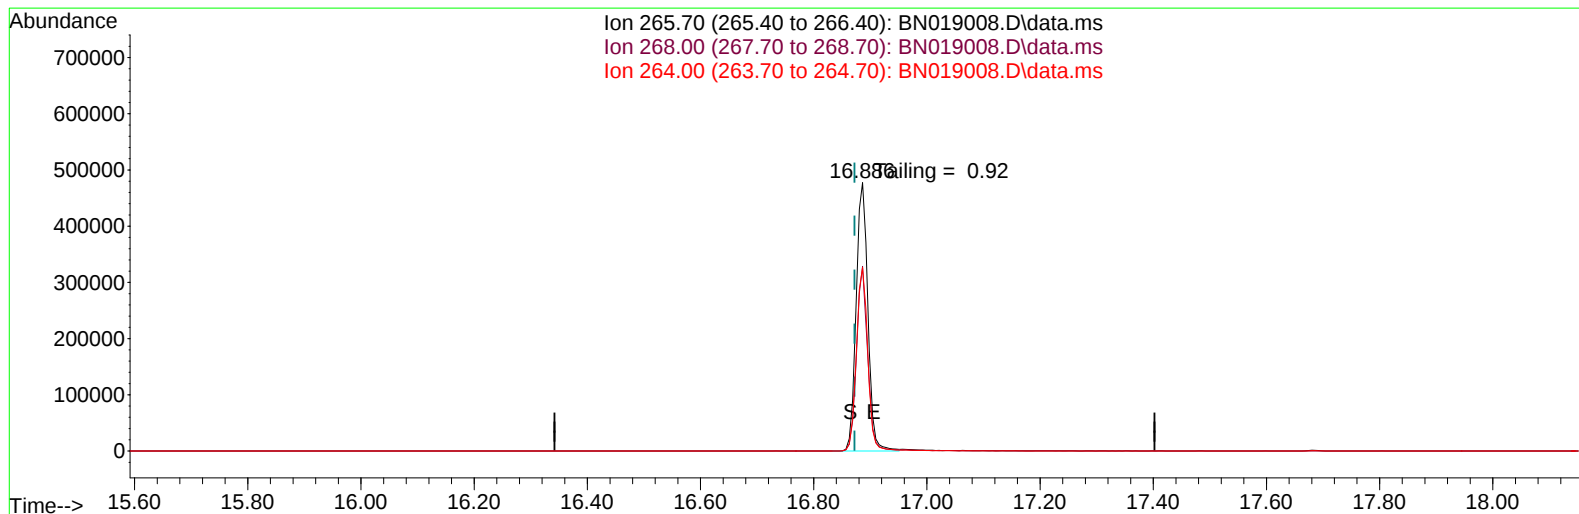

TIC: BN019008.D\data.ms

(70) Pentachlorophenol (C)




16.886min (+ 0.014) 22341.54 ng

response 694836

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	68.78
264.00	61.60	68.34
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031822\
Data File : BN019008.D
Acq On : 18 Mar 2022 08:51
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 18 15:17:30 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 14 15:11:57 2022
Response via : Initial Calibration

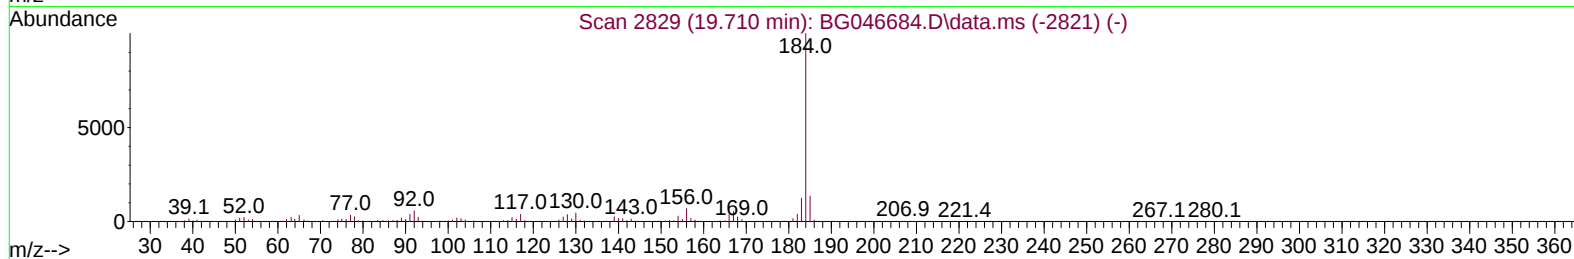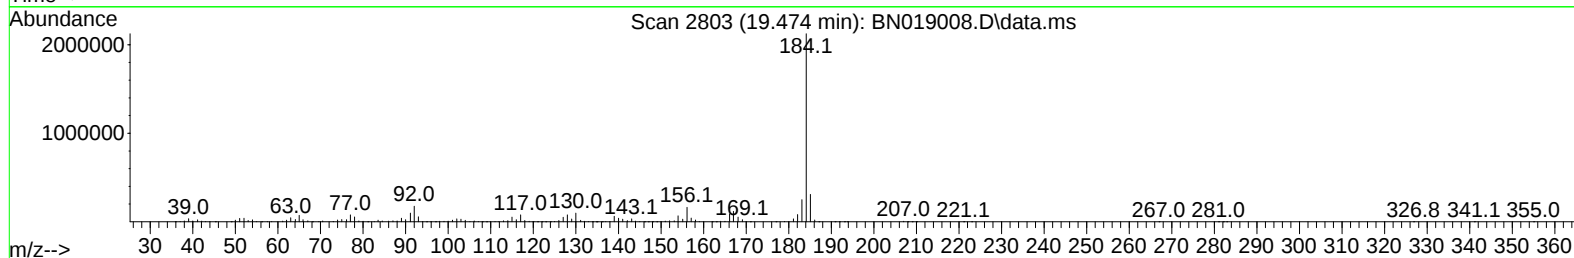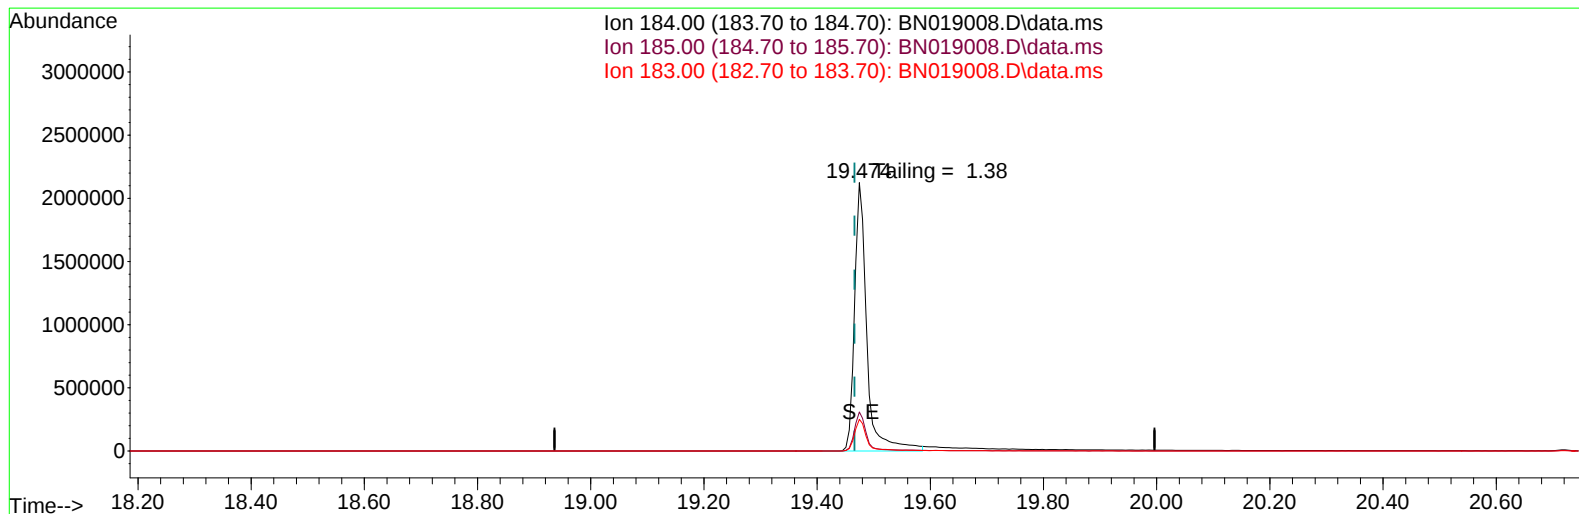

TIC: BN019008.D\data.ms

(77) Benzidine**19.474min (+ 0.009) 0.00 ng****response 3320510**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.58
183.00	13.20	11.80
0.00	0.00	0.00