
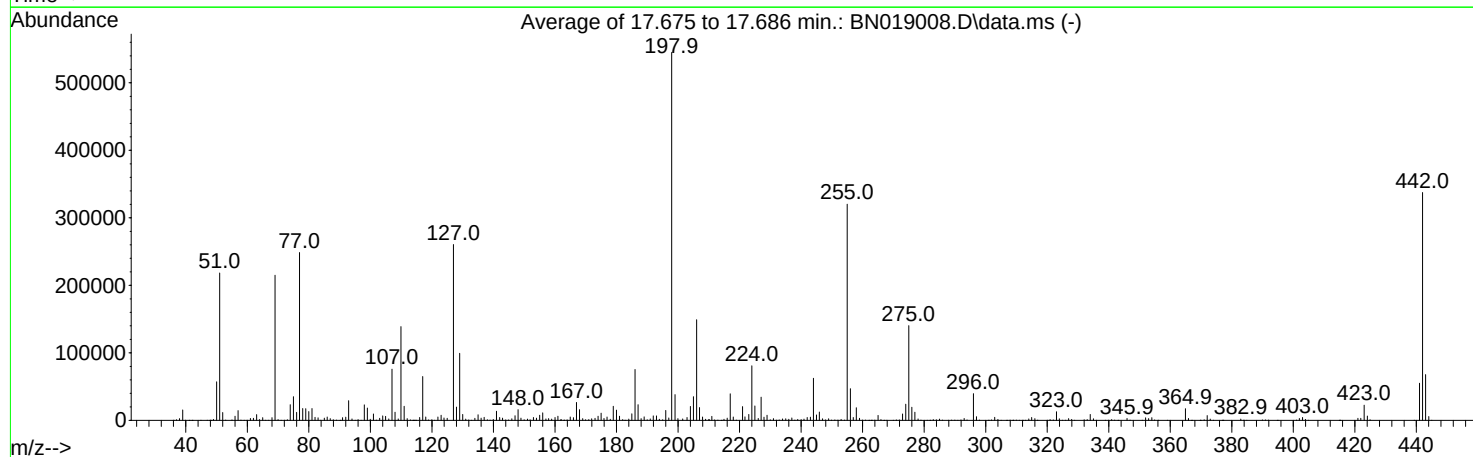


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031822\
 Data File : BN019008.D
 Acq On : 18 Mar 2022 08:51
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN031722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Mar 17 13:18:23 2022

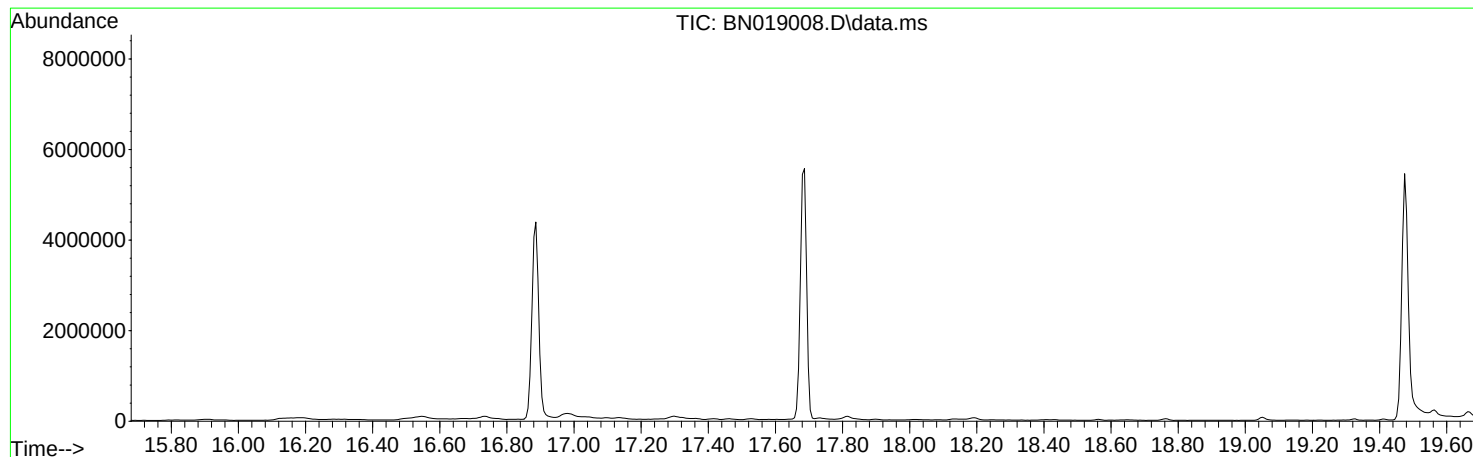

AutoFind: Scans 2497, 2498, 2499; Background Corrected with Scan 2490

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.1	218384	PASS
68	69	0.00	2	1.9	4085	PASS
69	198	0.00	100	39.5	215002	PASS
70	69	0.00	2	0.5	1113	PASS
127	198	10	80	47.8	260565	PASS
197	198	0.00	2	0.6	3486	PASS
198	198	100	100	100.0	544939	PASS
199	198	5	9	7.0	38085	PASS
275	198	10	60	25.7	140248	PASS
365	198	1	100	3.2	17350	PASS
441	198	0.01	100	10.1	54960	PASS
442	442	50	100	100.0	337600	PASS
443	442	15	24	20.1	67824	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
3/18/2022	BNA_N	<u>BN019008.D</u>
Compound Name	Response	Retention Time
DDT	1954994	20.72
DDD	25832	20.28
DDE	1012	19.77
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
26844	1981838	1.35

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031822\
Data File : BN019008.D
Acq On : 18 Mar 2022 08:51
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 18 15:17:30 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 14 15:11:57 2022
Response via : Initial Calibration

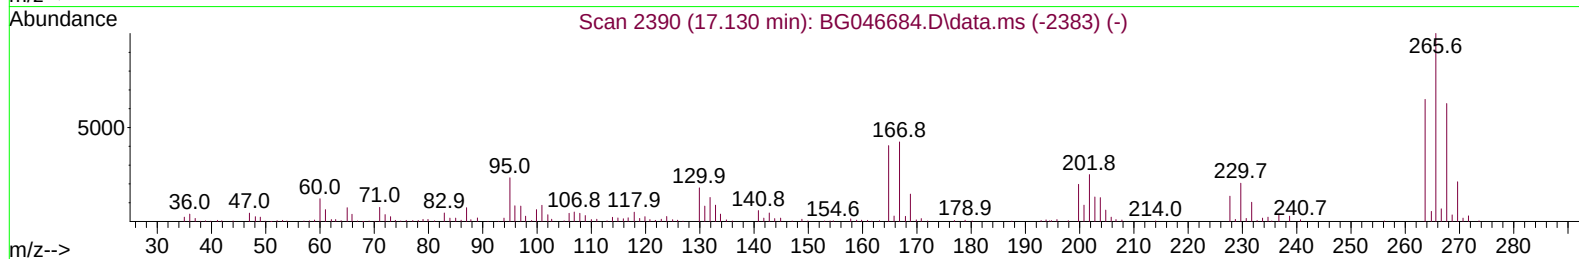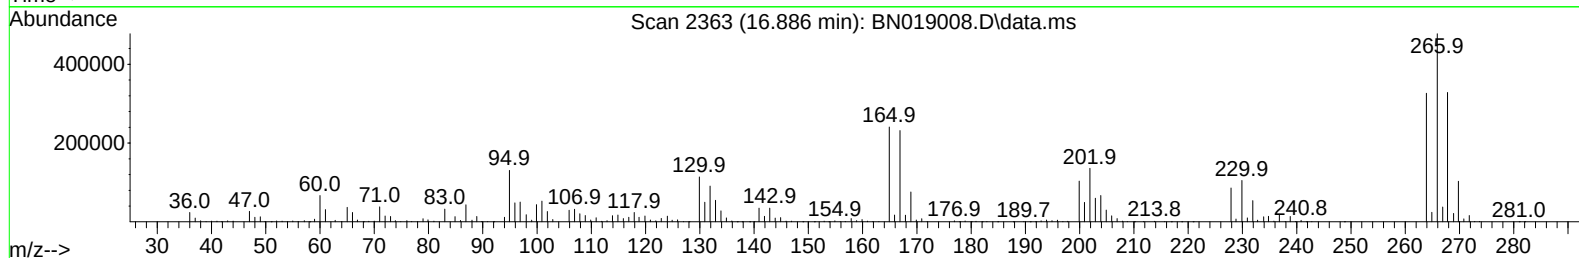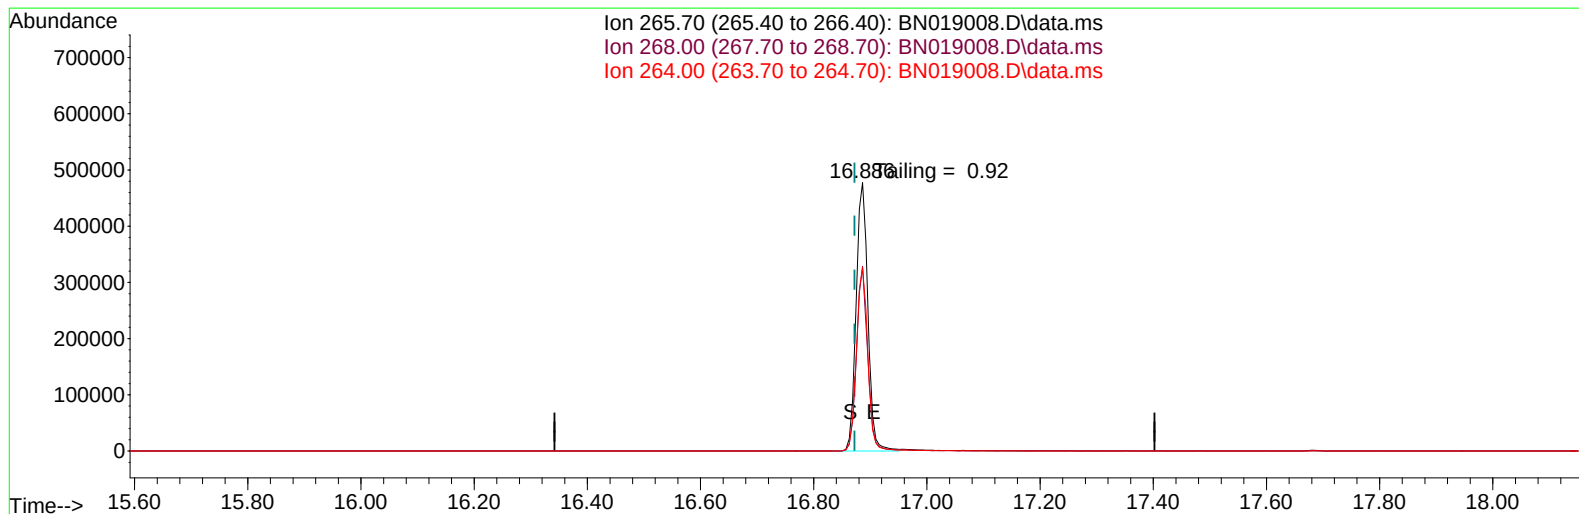

TIC: BN019008.D\data.ms

(70) Pentachlorophenol (C)

16.886min (+ 0.014) 22341.54 ng




response 694836

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	68.78
264.00	61.60	68.34
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031822\
Data File : BN019008.D
Acq On : 18 Mar 2022 08:51
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 18 15:17:30 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 14 15:11:57 2022
Response via : Initial Calibration

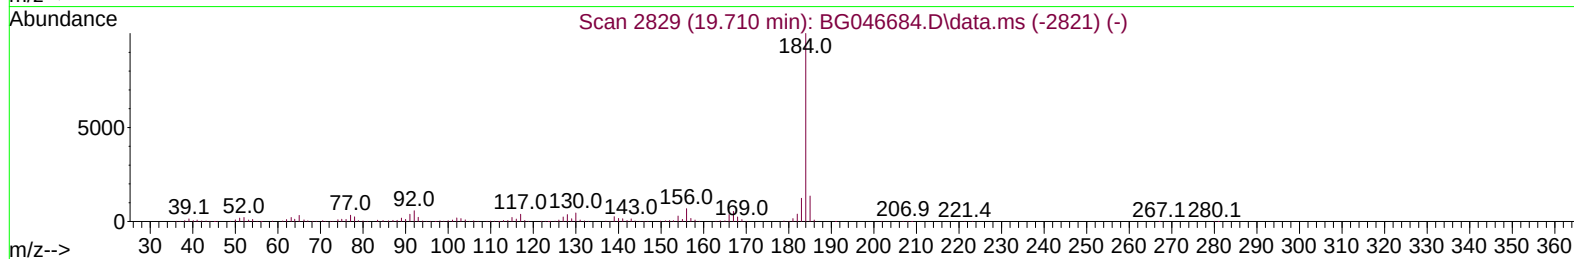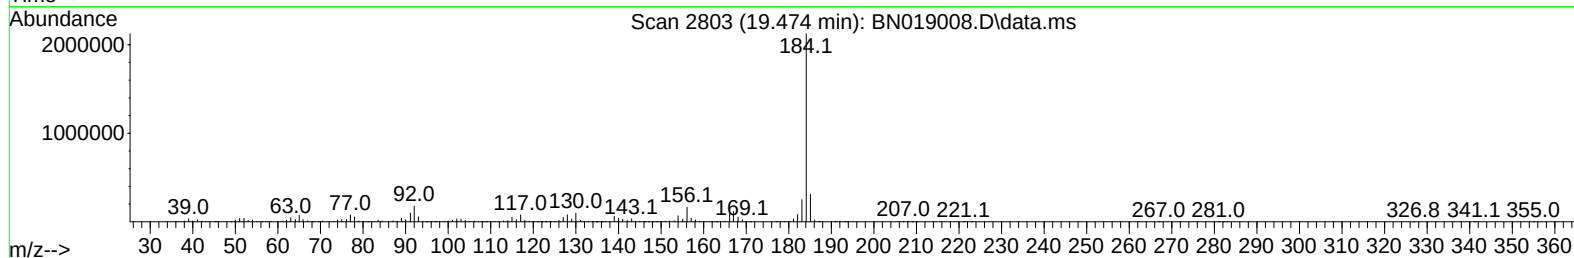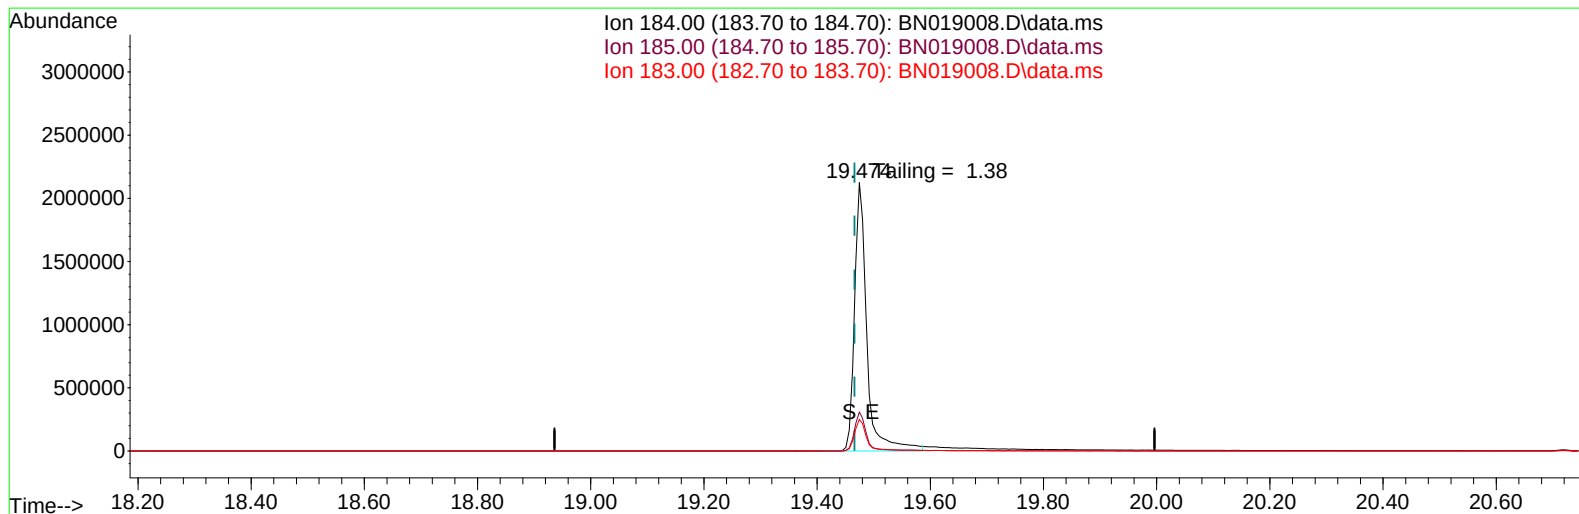

TIC: BN019008.D\data.ms

(77) Benzidine

19.474min (+ 0.009) 0.00 ng

response 3320510

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.58
183.00	13.20	11.80
0.00	0.00	0.00