
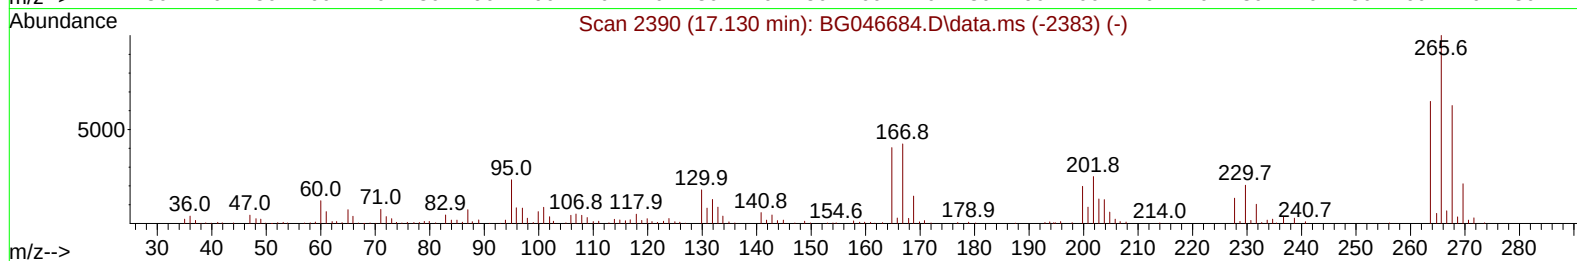
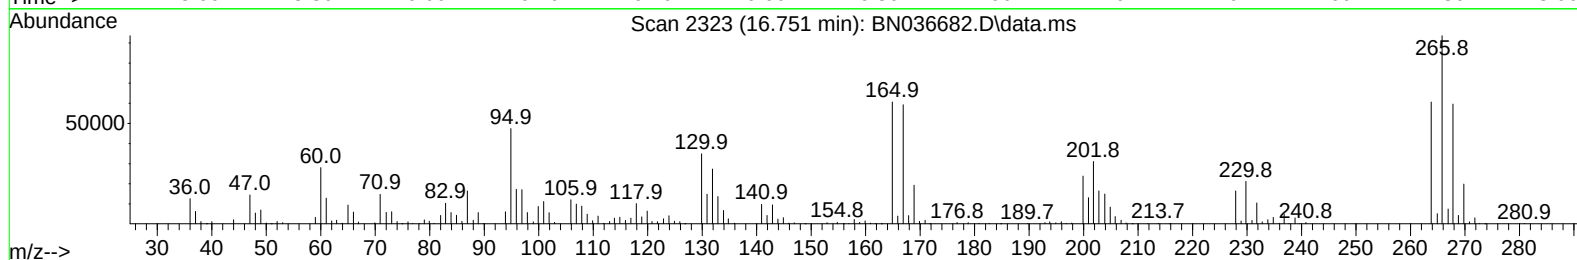


Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN031825\  
Data File : BN036682.D  
Acq On : 18 Mar 2025 08:42  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 18 13:19:40 2025  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Mar 18 01:27:23 2025  
Response via : Initial Calibration

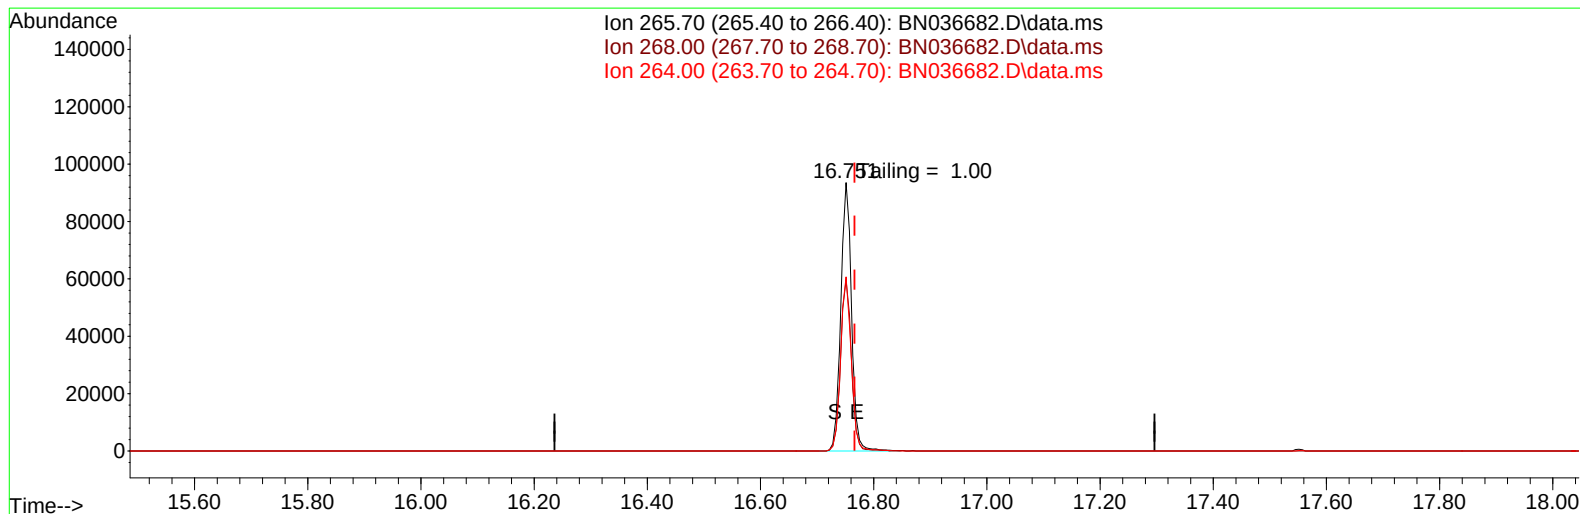

TIC: BN036682.D\data.ms

(70) Pentachlorophenol (C)

16.751min (-0.015) 15755.93 ng

```
response      123154
```

| Ion | Exp% | Act% |
|-----|------|------|
|-----|------|------|

|        |        |        |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
|--------|--------|--------|




|        |       |       |
|--------|-------|-------|
| 268.00 | 62.20 | 63.71 |
|--------|-------|-------|

|        |       |       |
|--------|-------|-------|
| 264.00 | 61.60 | 64.87 |
|--------|-------|-------|

0.00                      0.00                      0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN031825\  
Data File : BN036682.D  
Acq On : 18 Mar 2025 08:42  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 18 13:19:40 2025  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Mar 18 01:27:23 2025  
Response via : Initial Calibration

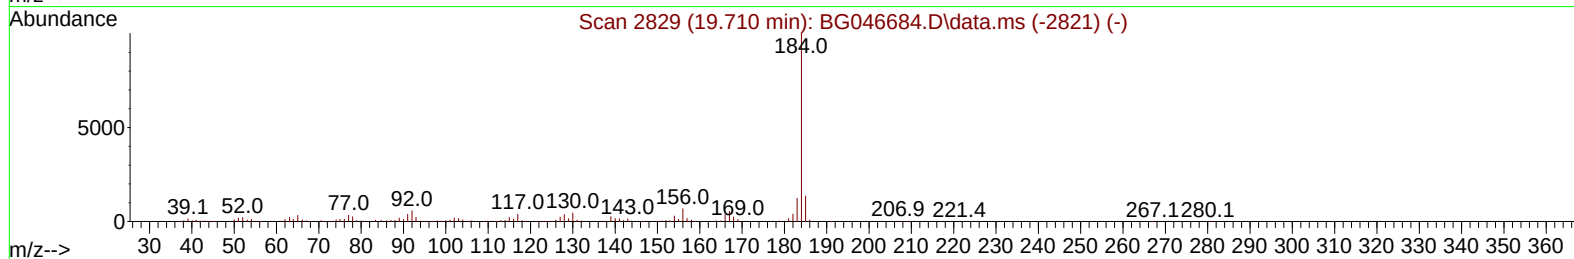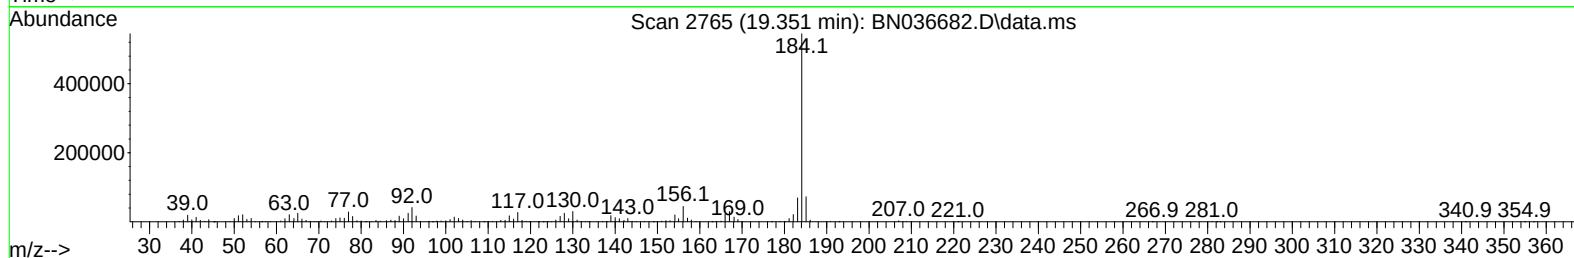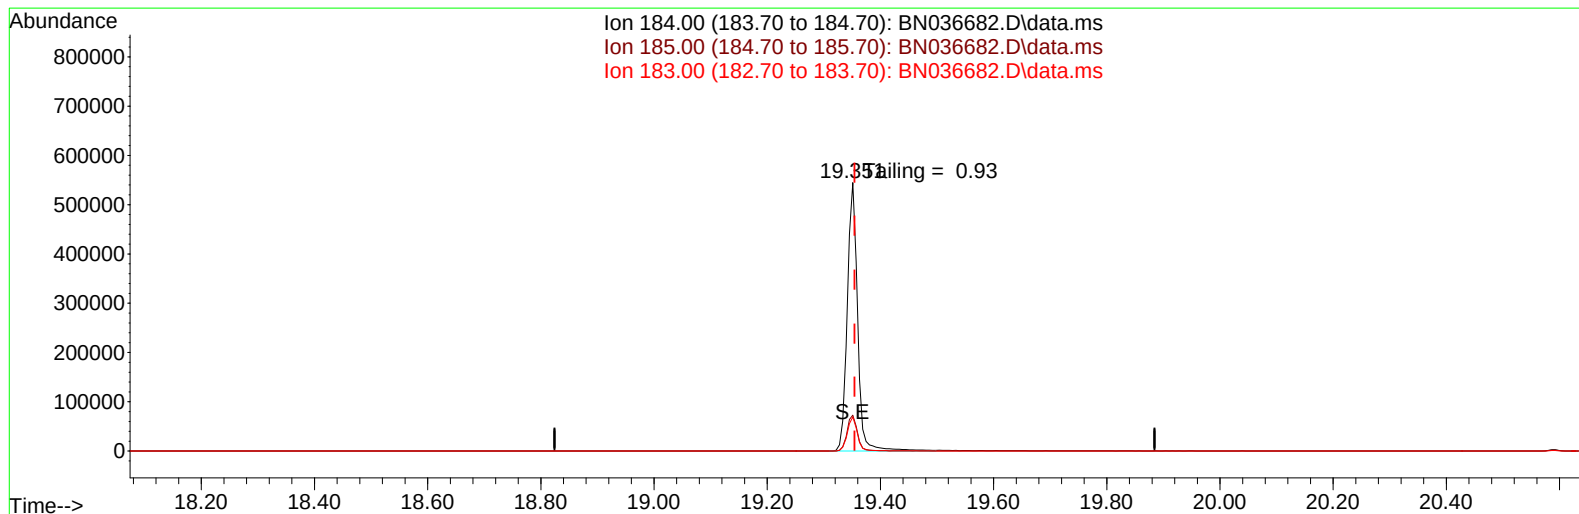

TIC: BN036682.D\data.ms

**(77) Benzidine**

**19.351min (-0.003) 0.00 ng**

**response 688778**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 15.50  | 13.35  |
| 183.00 | 13.20  | 12.70  |
| 0.00   | 0.00   | 0.00   |