


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN031920\
 Data File : BN010282.D
 Acq On : 19 Mar 2020 09:52
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN031920.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Mar 19 15:26:45 2020

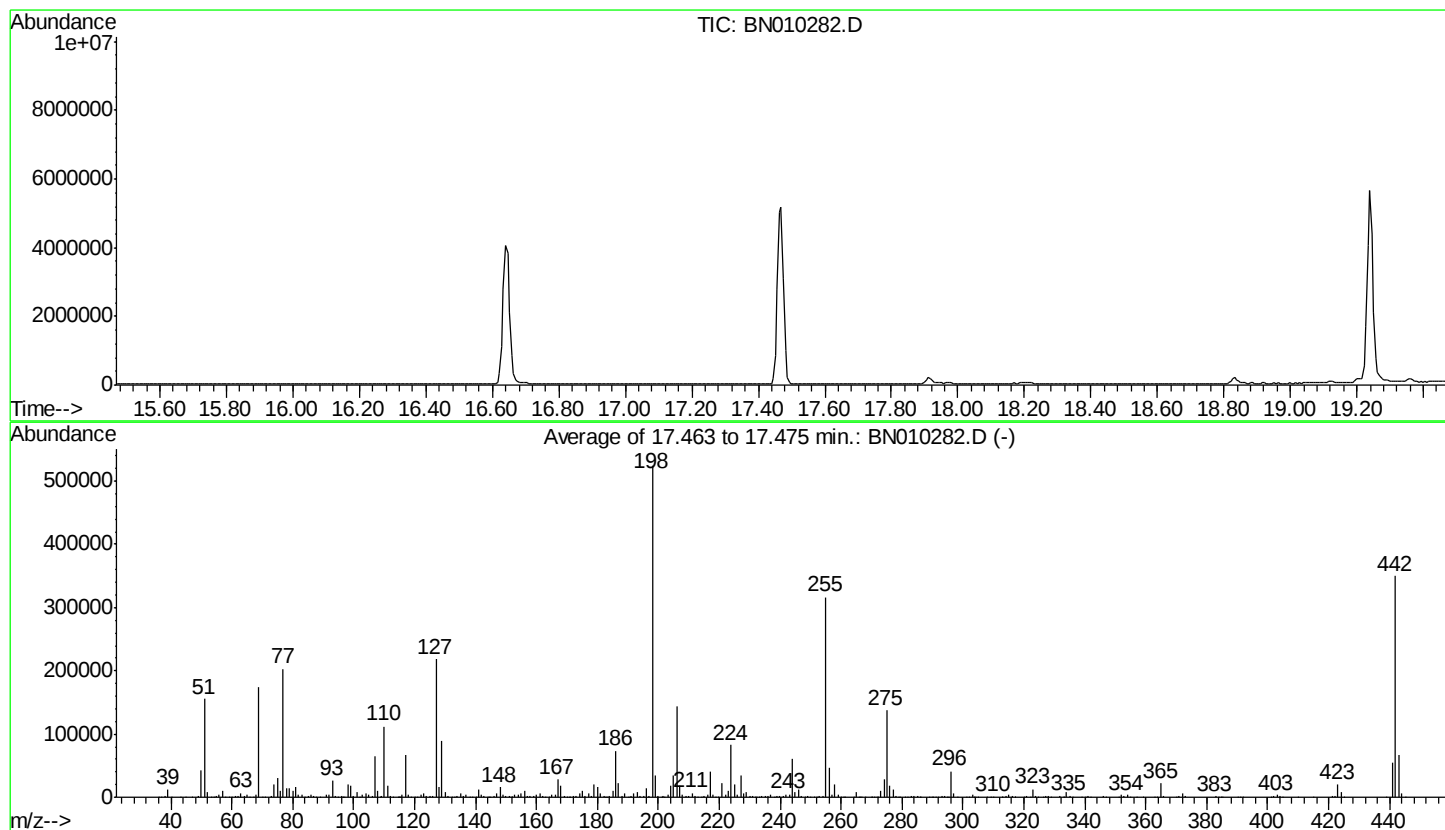

AutoFind: Scans 2495, 2496, 2497; Background Corrected with Scan 2488

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.6	155385	PASS
68	69	0.00	2	2.0	3420	PASS
69	198	0.00	100	33.1	173861	PASS
70	69	0.00	2	0.6	1039	PASS
127	198	10	80	41.7	218688	PASS
197	198	0.00	2	0.4	2274	PASS
198	198	100	100	100.0	524586	PASS
199	198	5	9	6.5	34245	PASS
275	198	10	60	26.1	136845	PASS
365	198	1	100	4.1	21610	PASS
441	198	0.01	100	10.6	55496	PASS
442	198	50	100	66.6	349397	PASS
443	442	15	24	19.2	67058	PASS