
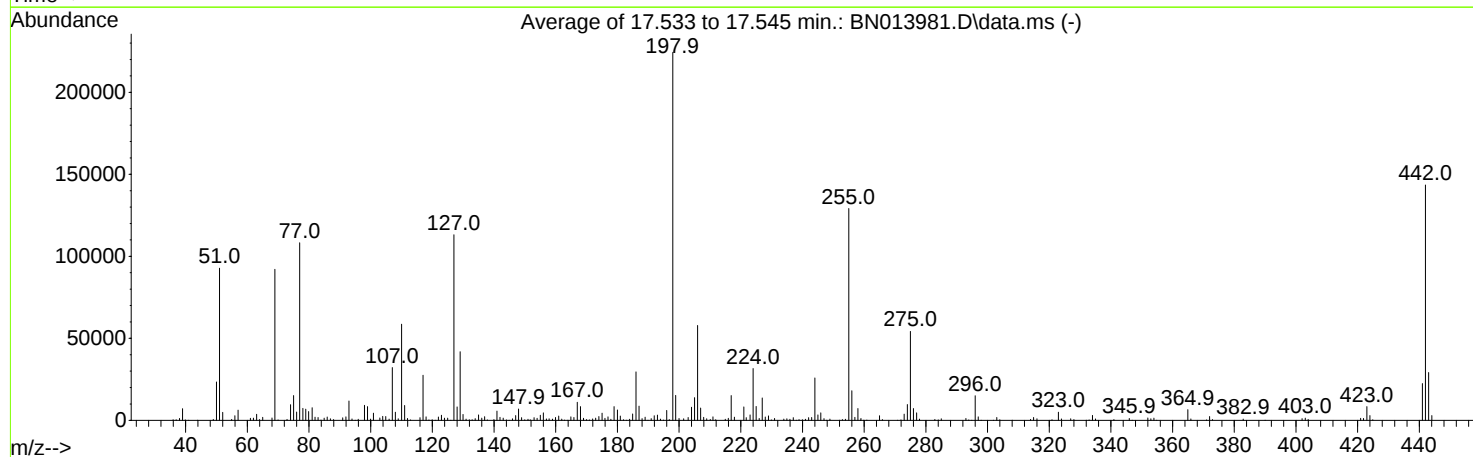


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031921\
 Data File : BN013981.D
 Acq On : 18 Mar 2021 14:31
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN022421.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Mar 18 15:58:40 2021

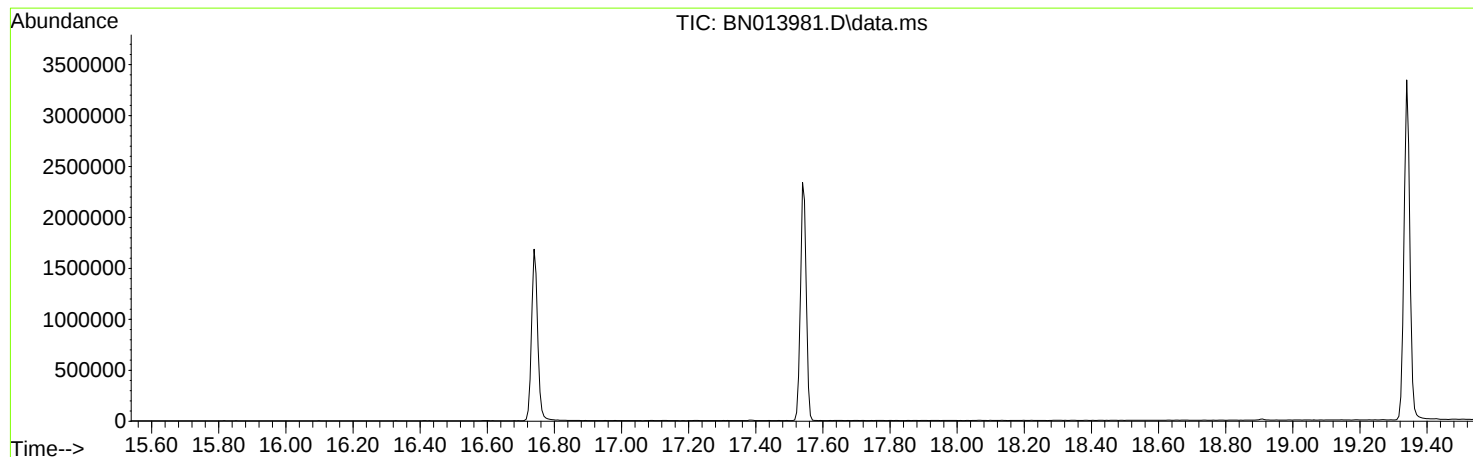

AutoFind: Scans 2456, 2457, 2458; Background Corrected with Scan 2450

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.4	92763	PASS
68	69	0.00	2	1.6	1482	PASS
69	198	0.00	100	41.1	92088	PASS
70	69	0.00	2	0.4	338	PASS
127	198	10	80	50.5	113181	PASS
197	198	0.00	2	0.2	434	PASS
198	198	100	100	100.0	224277	PASS
199	198	5	9	6.8	15207	PASS
275	198	10	60	24.2	54261	PASS
365	198	1	100	2.9	6516	PASS
441	198	0.01	100	10.0	22495	PASS
442	442	50	100	100.0	143517	PASS
443	442	15	24	20.3	29199	PASS




DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/19/2021	BNA_N	<u>BN013981.D</u>
Compound Name	Response	Retention Time
DDT	816997	20.57
DDD	4782	20.13
DDE	811	19.62
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5593	822590	0.68

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031921\
Data File : BN013981.D
Acq On : 18 Mar 2021 14:31
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 18 15:06:12 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 05 13:12:06 2021
Response via : Initial Calibration

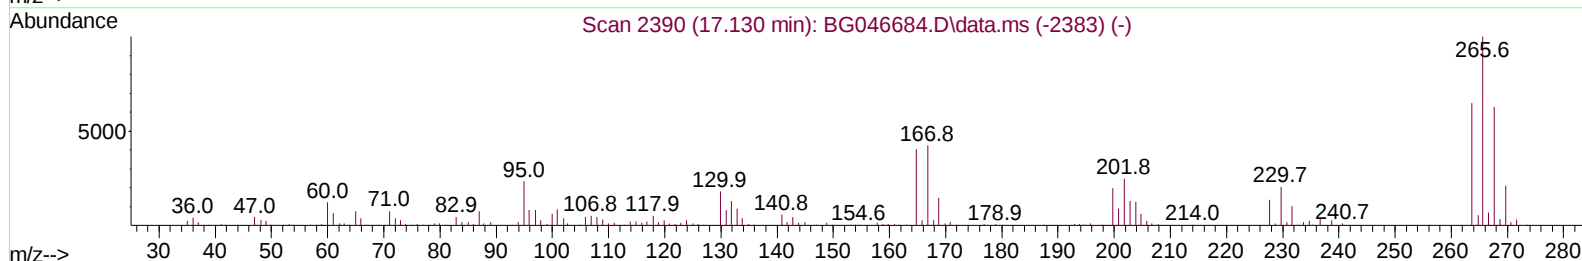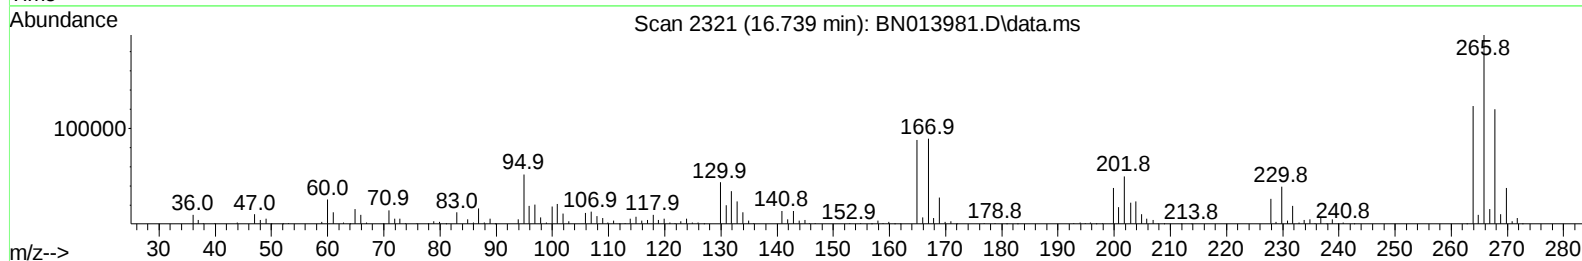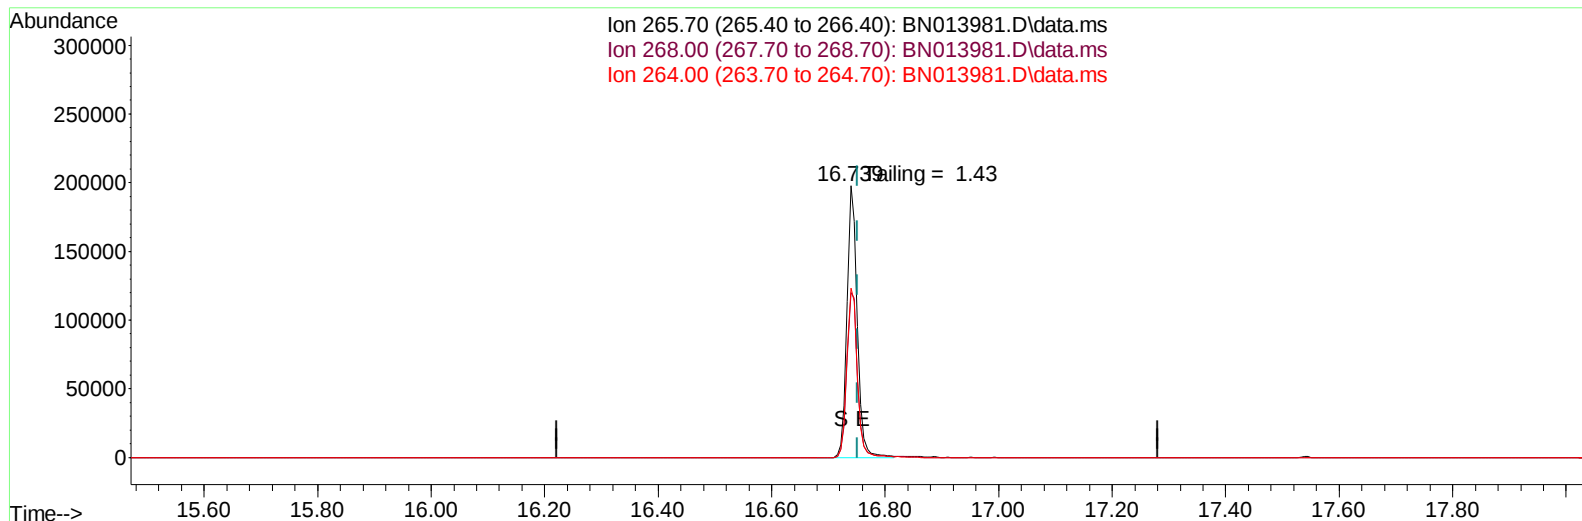

TIC: BN013981.D\data.ms

(70) Pentachloropheno1 (C)

16.739min (-0.012) 22405.73 ng




response 248630

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	60.64
264.00	61.60	62.39
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031921\
Data File : BN013981.D
Acq On : 18 Mar 2021 14:31
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 18 15:06:12 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 05 13:12:06 2021
Response via : Initial Calibration

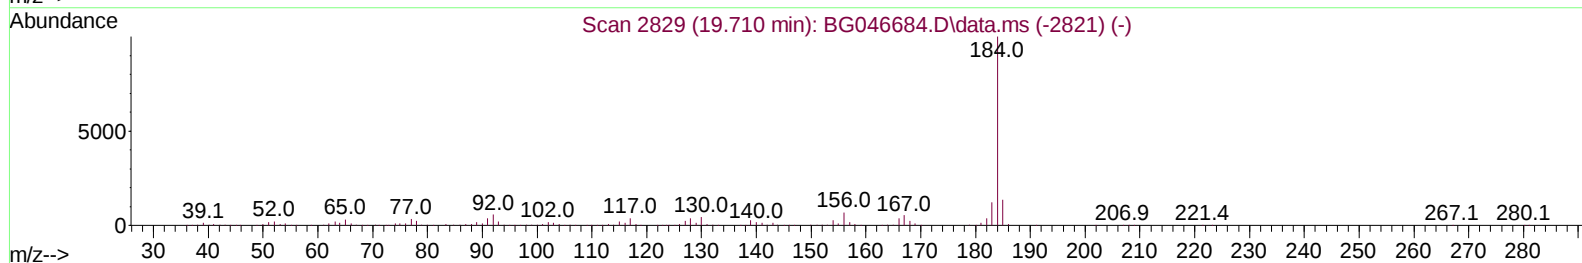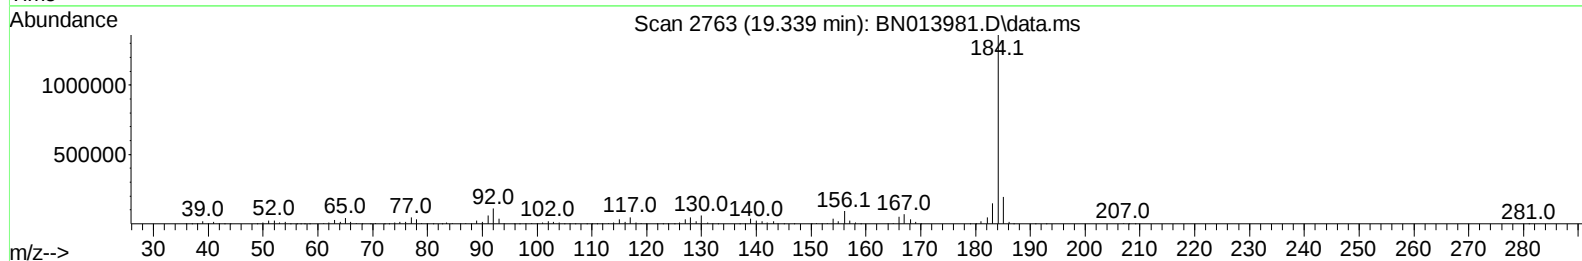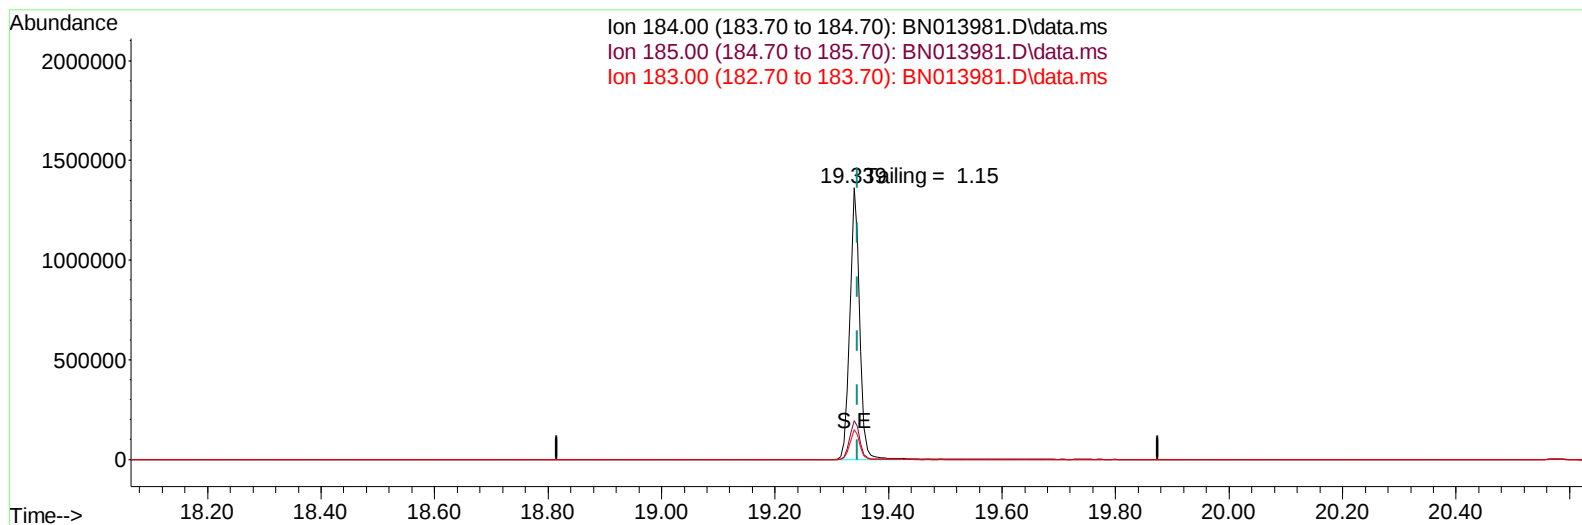

TIC: BN013981.D\data.ms

(77) Benzidine

19.339min (-0.006) 63553.22 ng

response 1629931

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.27
183.00	13.20	10.99
0.00	0.00	0.00