
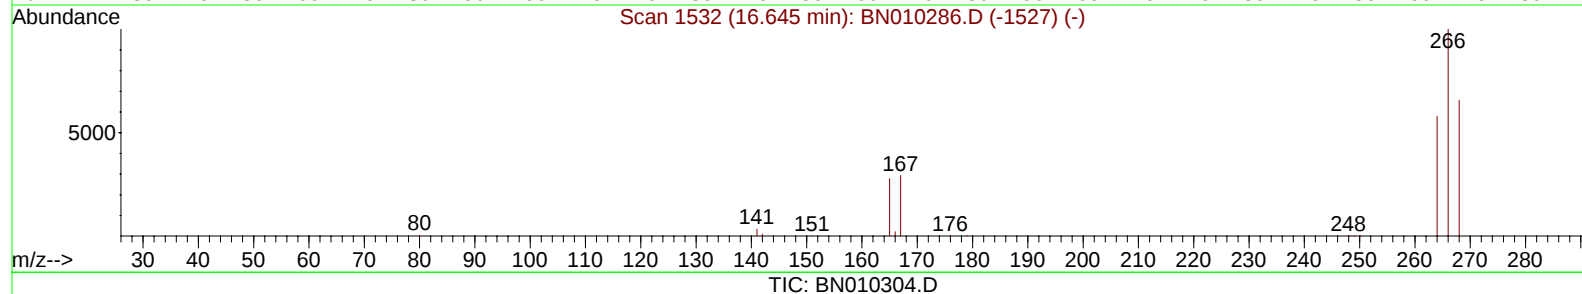
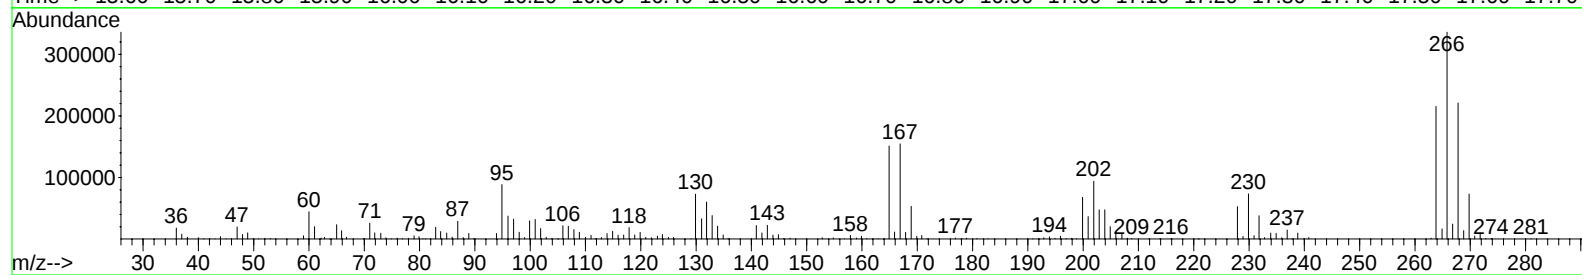


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN032020\
 Data File : BN010304.D
 Acq On : 20 Mar 2020 09:52
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 20 17:57:37 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN031920.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 19 15:26:45 2020
 Response via : Initial Calibration

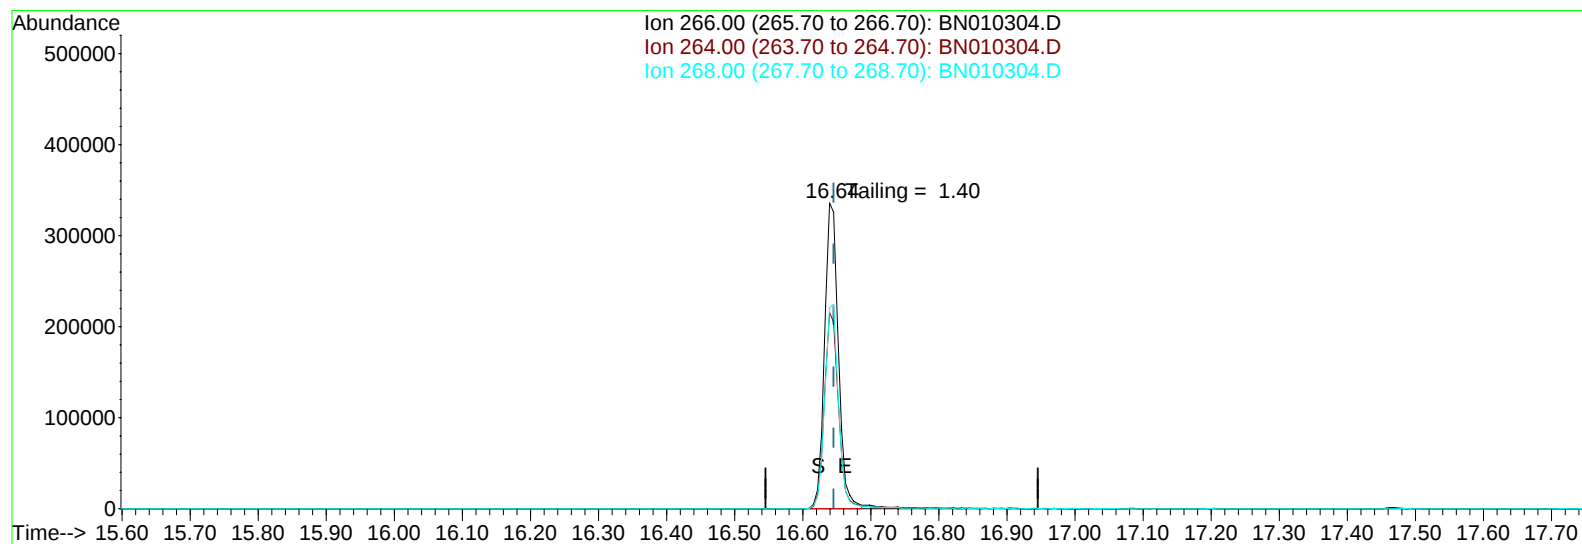

(22) Pentachlorophenol

16.639min (-0.006) 0.00ng

response 481296

Ion	Exp%	Act%
266.00	100	100
264.00	59.60	64.15
268.00	68.60	65.80
0.00	0.00	0.00