


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032020\
 Data File : BN010304.D
 Acq On : 20 Mar 2020 09:52
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN031920.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Mar 19 15:26:45 2020

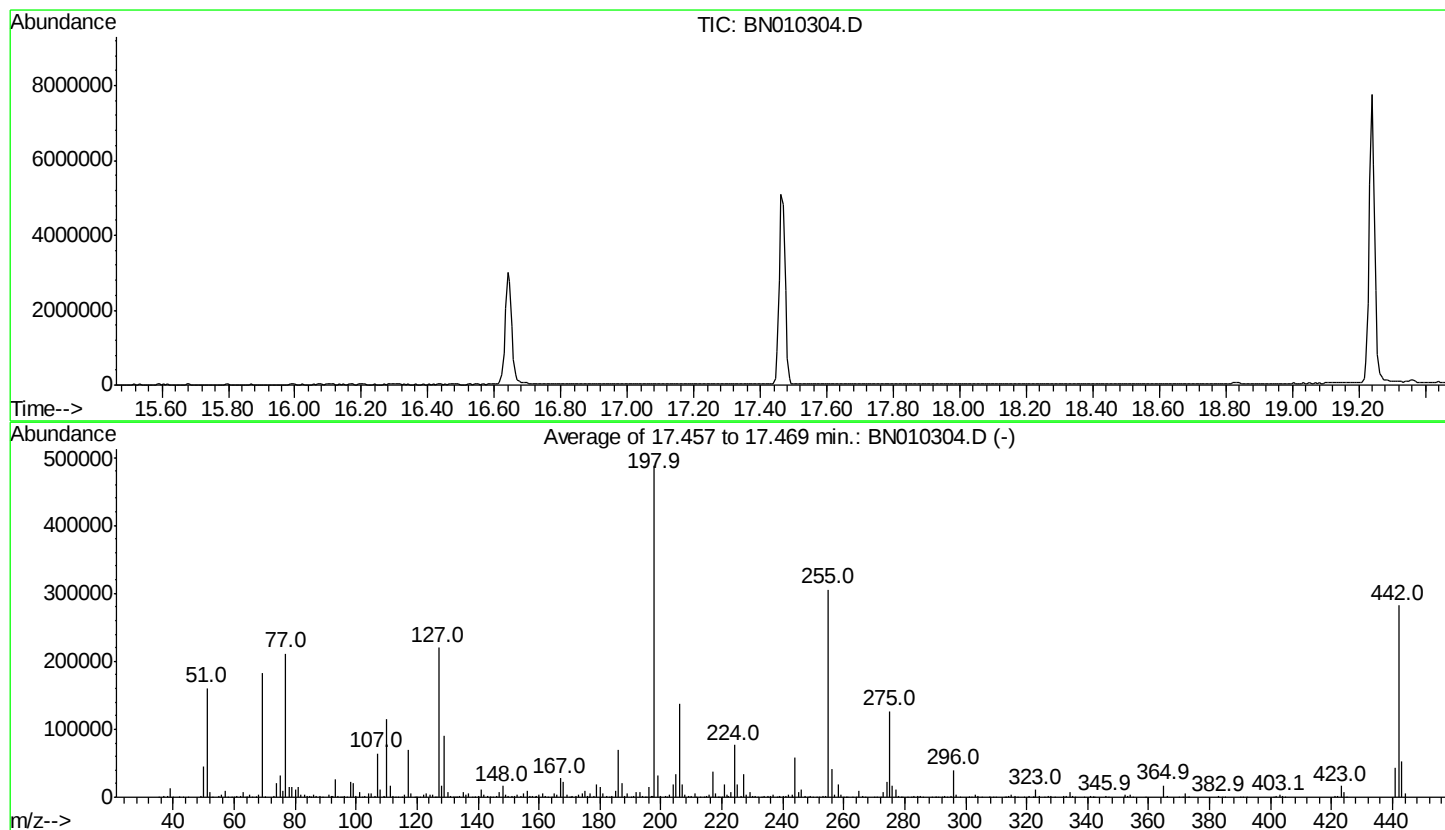

AutoFind: Scans 2494, 2495, 2496; Background Corrected with Scan 2488

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.9	160496	PASS
68	69	0.00	2	2.0	3580	PASS
69	198	0.00	100	37.4	182528	PASS
70	69	0.00	2	0.5	901	PASS
127	198	10	80	45.0	219626	PASS
197	198	0.00	2	0.3	1361	PASS
198	198	100	100	100.0	487850	PASS
199	198	5	9	6.8	32952	PASS
275	198	10	60	26.1	127101	PASS
365	198	1	100	3.5	17138	PASS
441	198	0.01	100	9.1	44266	PASS
442	198	50	100	57.8	282090	PASS
443	442	15	24	19.0	53605	PASS